

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072318\
 Data File : P0047057.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 3:07
 Operator : SM/SJ
 Sample : AR1232 MDL WATER
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1232 MDL WATER

Manual Integrations
 APPROVED

Sohil
 7/24/2018 1:42:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:57:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.650	3242749	3495952	19.340	18.227
2) SA Decachlor...	10.088	8.656	2357436	2142760	21.534	23.331m
Target Compounds						
11) L3 AR-1232-1	5.105	4.326	41608	48580	27.781	30.907m
12) L3 AR-1232-2	5.565	4.736	69694	72746	34.204	36.482m
13) L3 AR-1232-3	5.585	4.755	85209	102692	29.301m	33.221m
14) L3 AR-1232-4	5.651	4.809	51178	46864	28.683m	25.704m
15) L3 AR-1232-5	5.749	4.973	48993	43723	34.582m	43.502 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\PO072318\
Data File : PO047057.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 3:07
Operator : SM/SJ
Sample : AR1232 MDL WATER
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1232 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 06:57:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

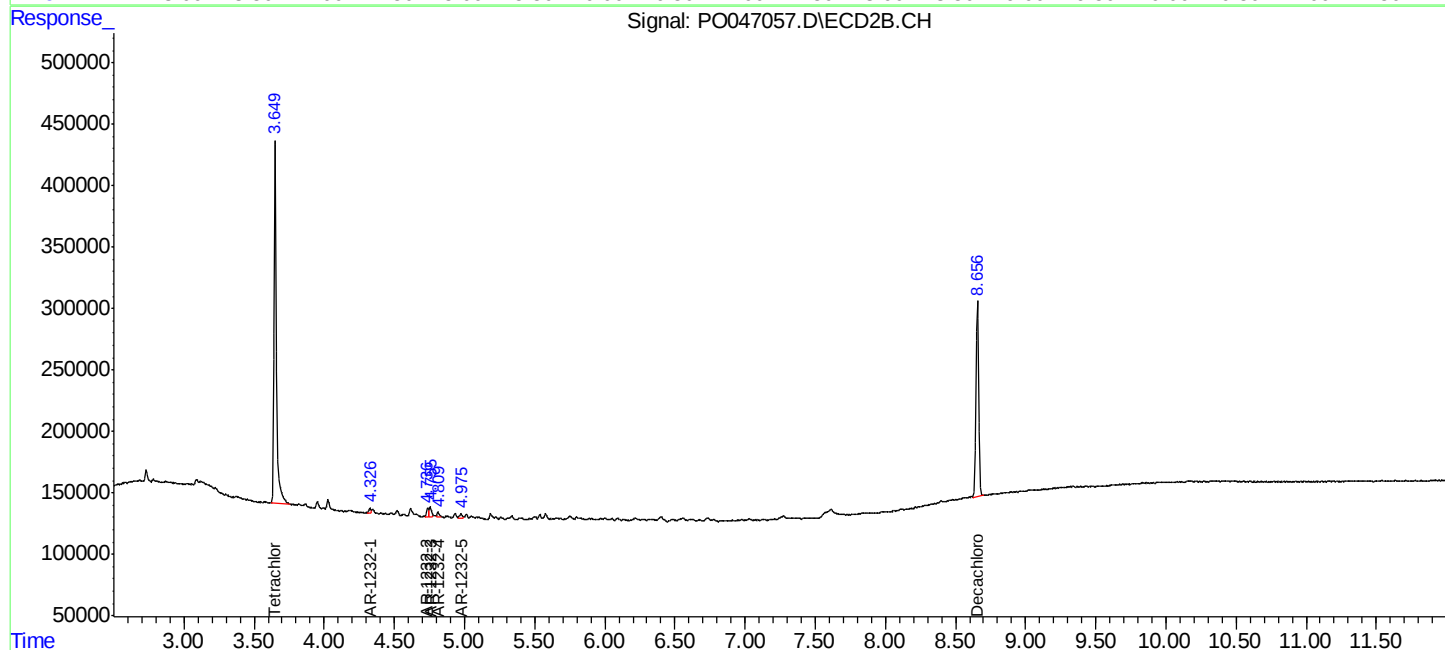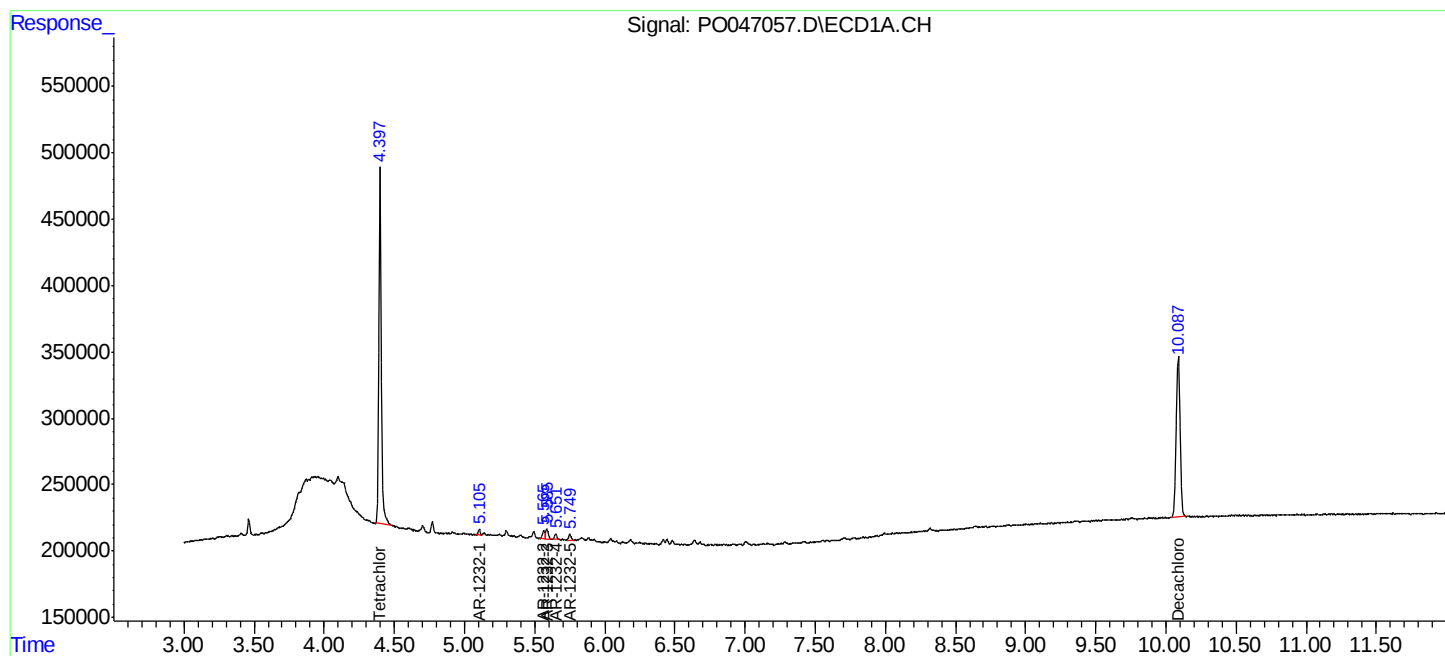

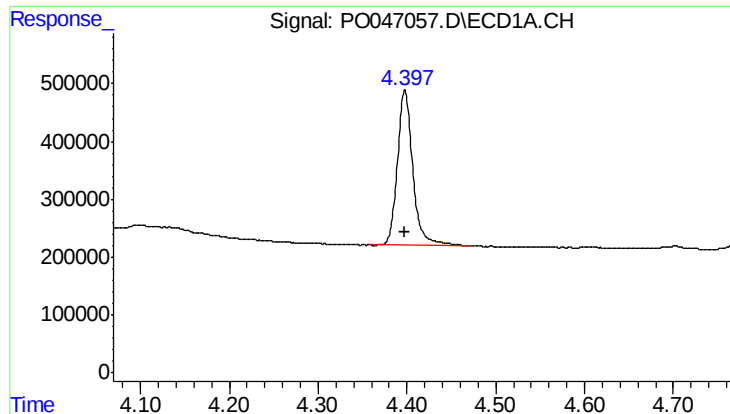


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 3242749
Conc: 19.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1232 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:11 PM

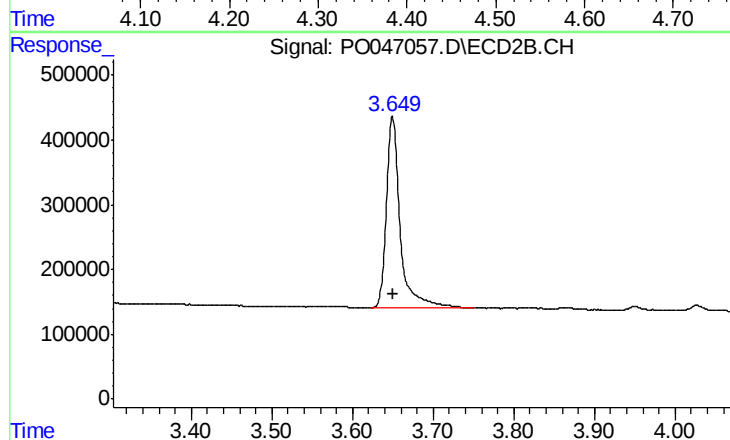


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: -0.001 min
Response: 3495952
Conc: 18.23 ng/ml

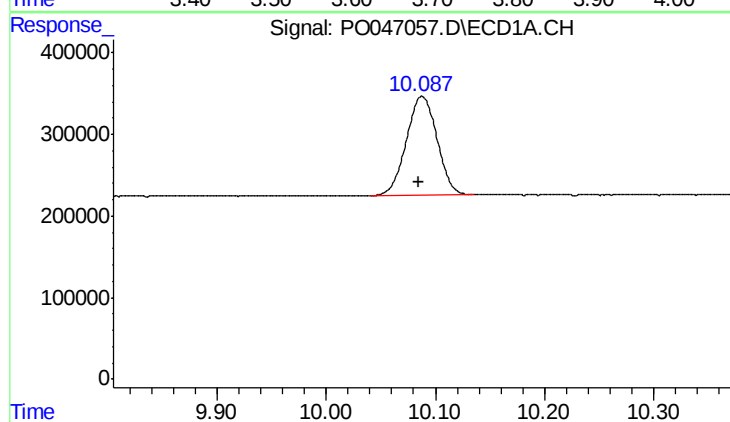


#2 Decachlorobiphenyl

R.T.: 10.088 min
Delta R.T.: 0.004 min
Response: 2357436
Conc: 21.53 ng/ml

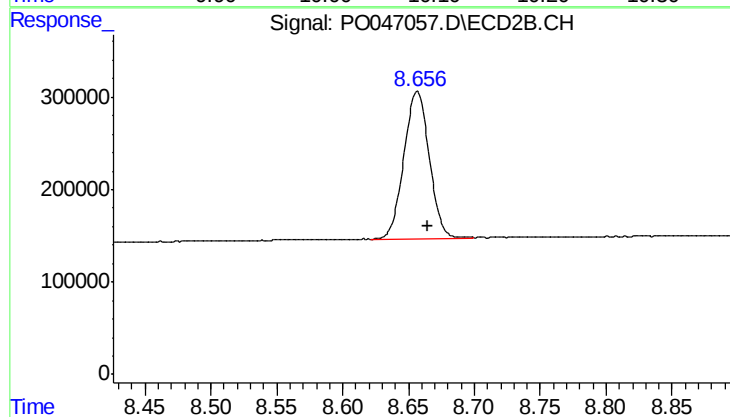

#2 Decachlorobiphenyl

R.T.: 8.656 min
Delta R.T.: -0.008 min
Response: 2142760
Conc: 23.33 ng/ml m

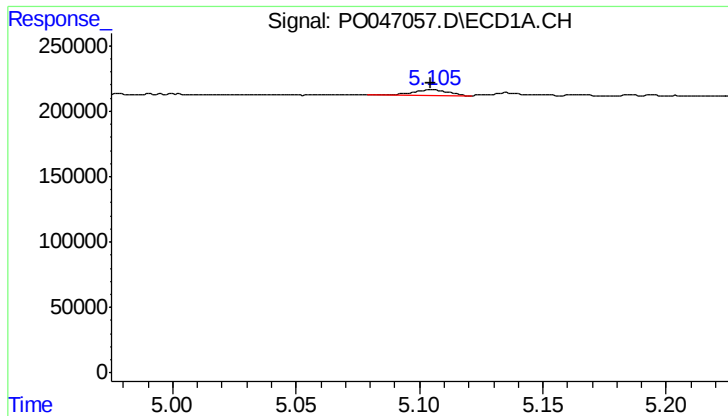


#11 AR-1232-1

R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 41608
Conc: 27.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1232 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:11 PM

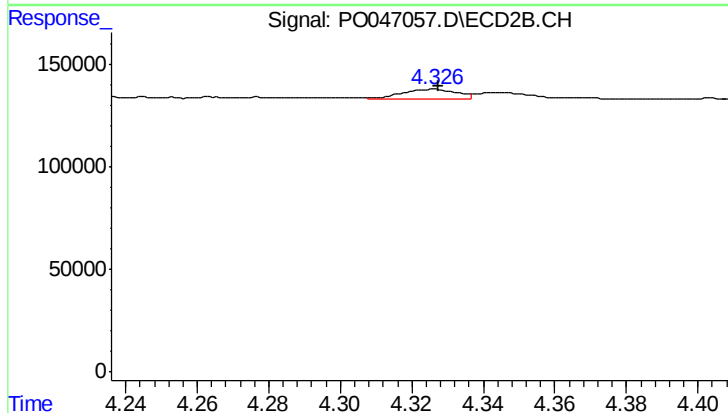


#11 AR-1232-1

R.T.: 4.326 min
Delta R.T.: -0.001 min
Response: 48580
Conc: 30.91 ng/ml m

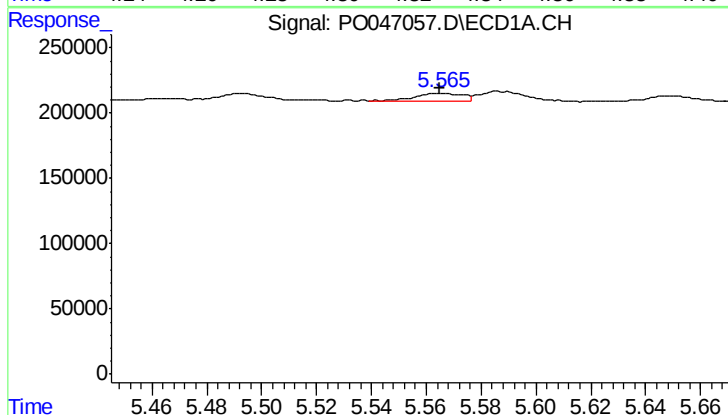


#12 AR-1232-2

R.T.: 5.565 min
Delta R.T.: 0.000 min
Response: 69694
Conc: 34.20 ng/ml

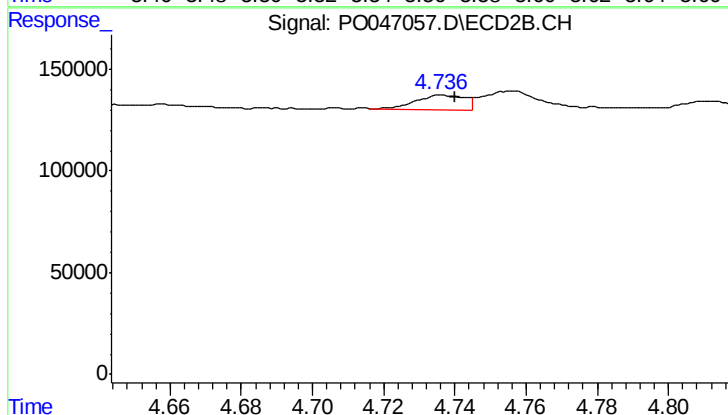

#12 AR-1232-2

R.T.: 4.736 min
Delta R.T.: -0.005 min
Response: 72746
Conc: 36.48 ng/ml m

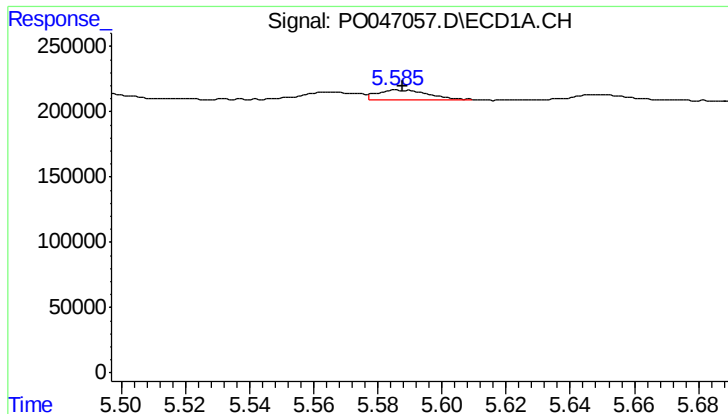


#13 AR-1232-3

R.T.: 5.585 min
Delta R.T.: -0.002 min
Response: 85209
Conc: 29.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1232 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:11 PM

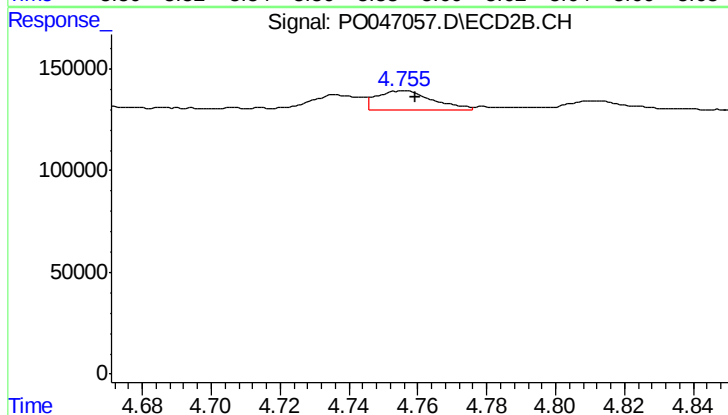


#13 AR-1232-3

R.T.: 4.755 min
Delta R.T.: -0.004 min
Response: 102692
Conc: 33.22 ng/ml m

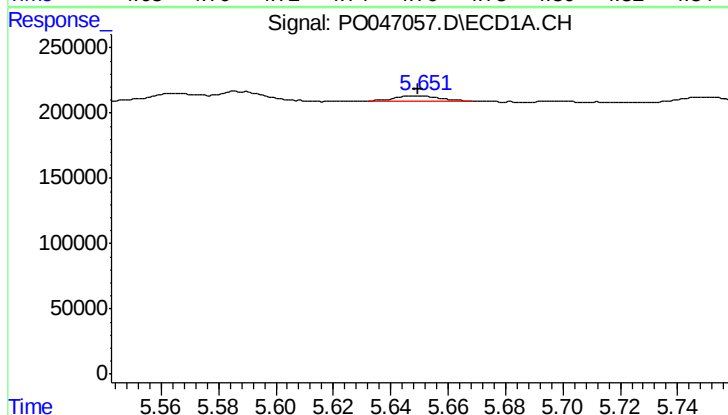


#14 AR-1232-4

R.T.: 5.651 min
Delta R.T.: 0.002 min
Response: 51178
Conc: 28.68 ng/ml m

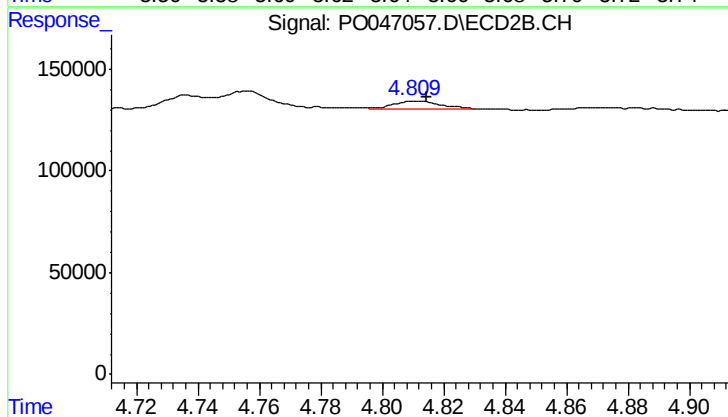

#14 AR-1232-4

R.T.: 4.809 min
Delta R.T.: -0.005 min
Response: 46864
Conc: 25.70 ng/ml m

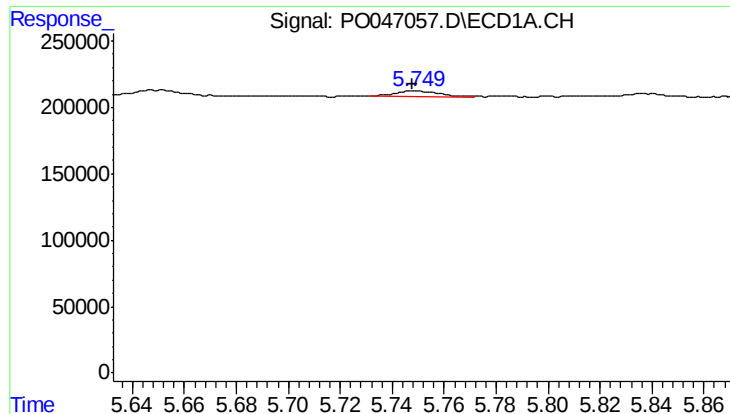


#15 AR-1232-5

R.T.: 5.749 min
Delta R.T.: 0.001 min
Response: 48993
Conc: 34.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1232 MDL WATER

Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:11 PM

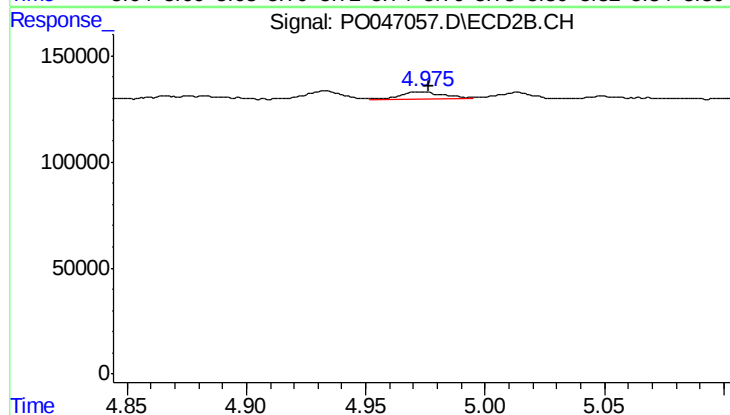

#15 AR-1232-5

R.T.: 4.973 min
Delta R.T.: -0.003 min
Response: 43723
Conc: 43.50 ng/ml