

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072318\
 Data File : P0047066.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 5:30
 Operator : SM/SJ
 Sample : AR1254 MDL WATER
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1254 MDL WATER

Manual Integrations
 APPROVED

Sohil
 7/24/2018 1:42:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 07:36:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.649	3278384	3589580	19.553	18.716
2) SA Decachlor...	10.085	8.653	2510256	2260822	22.930	24.617m
Target Compounds						
26) L6 AR-1254-1	6.634	5.537	298089	260744	36.253	36.501
27) L6 AR-1254-2	6.914	5.683	175359	243093	35.712	40.134
28) L6 AR-1254-3	6.999	6.087	325013	346062	37.817	36.756
29) L6 AR-1254-4	7.284	6.314	267400	226643	41.869	39.296
30) L6 AR-1254-5	7.556	6.629	173869	138890	36.616m	34.984

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072318\
Data File : P0047066.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 5:30
Operator : SM/SJ
Sample : AR1254 MDL WATER
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 07:36:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

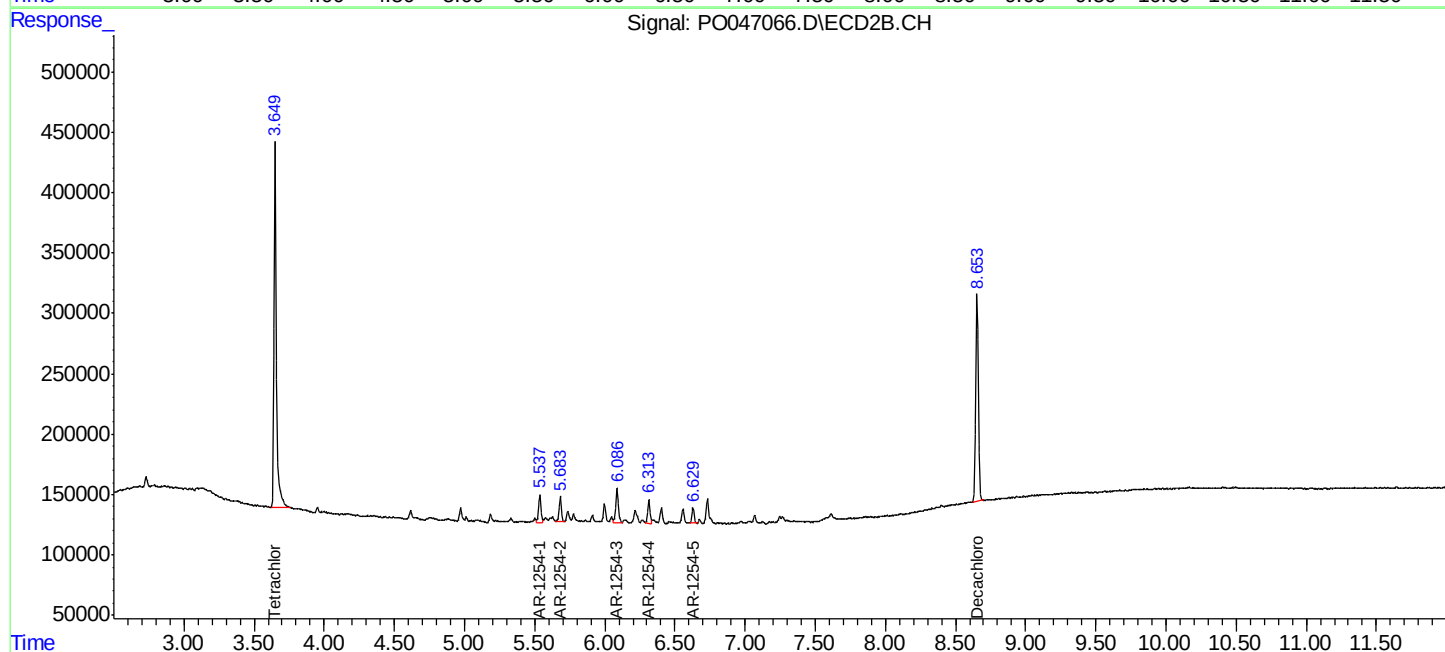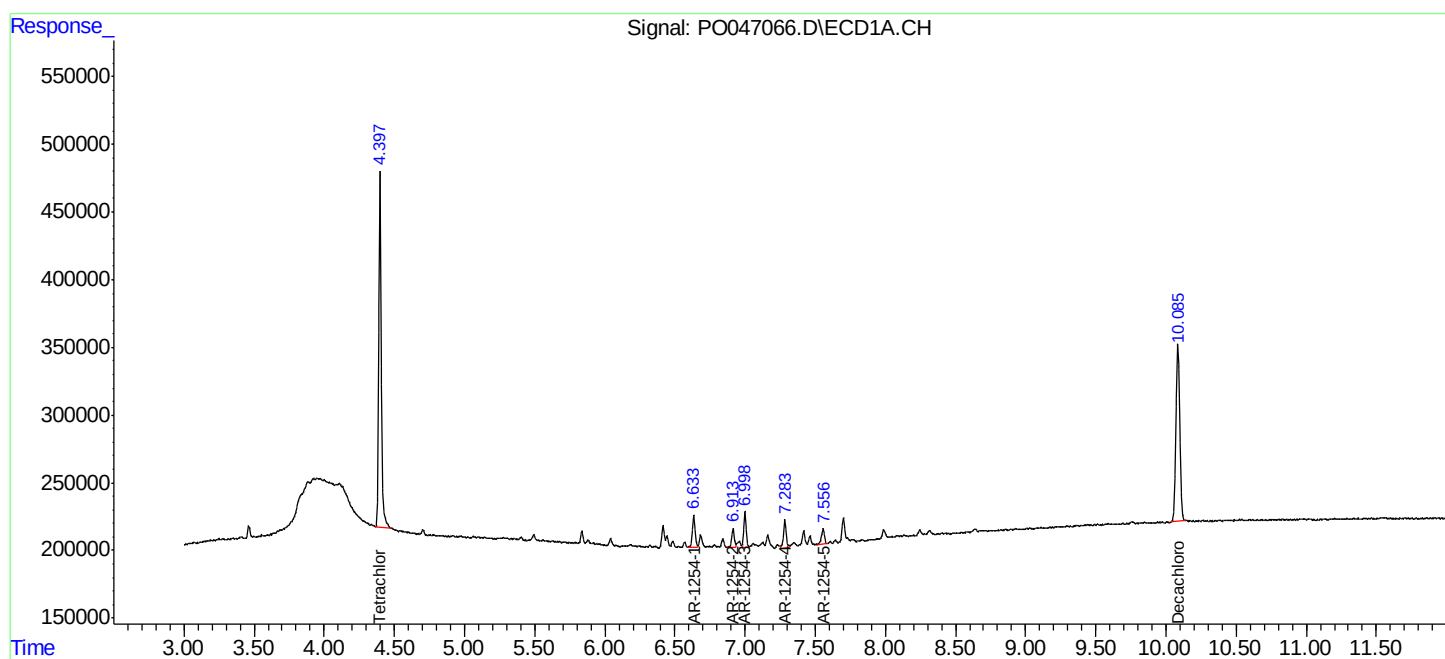

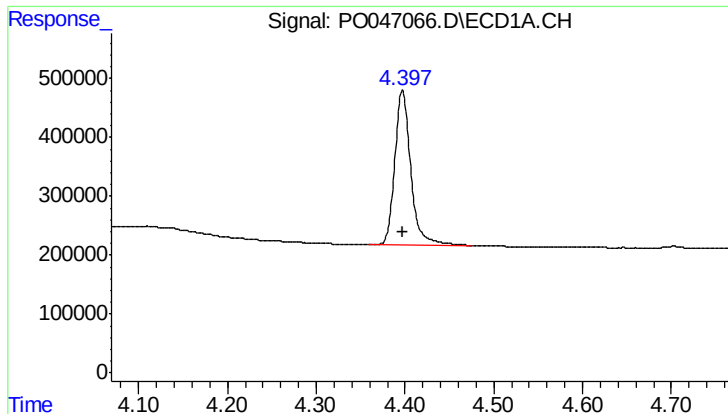


#1 Tetrachloro-m-xylene

R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 3278384
Conc: 19.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:40 PM

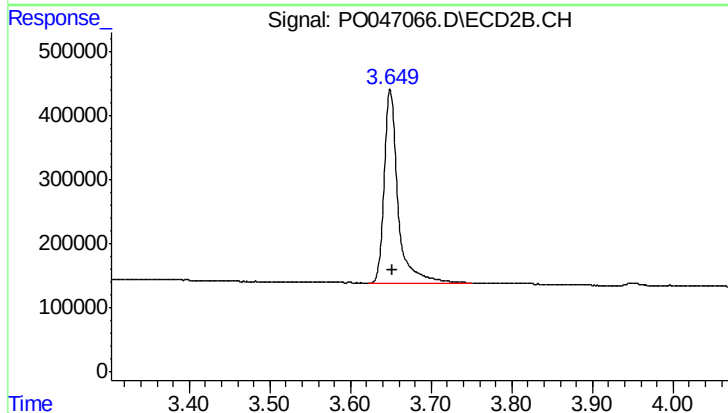


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 3589580
Conc: 18.72 ng/ml

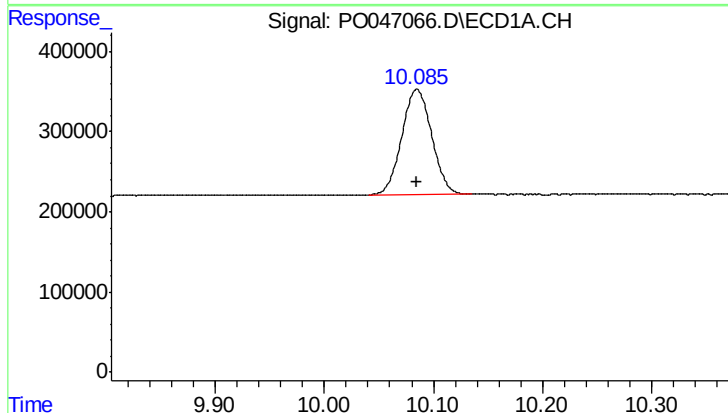


#2 Decachlorobiphenyl

R.T.: 10.085 min
Delta R.T.: 0.000 min
Response: 2510256
Conc: 22.93 ng/ml

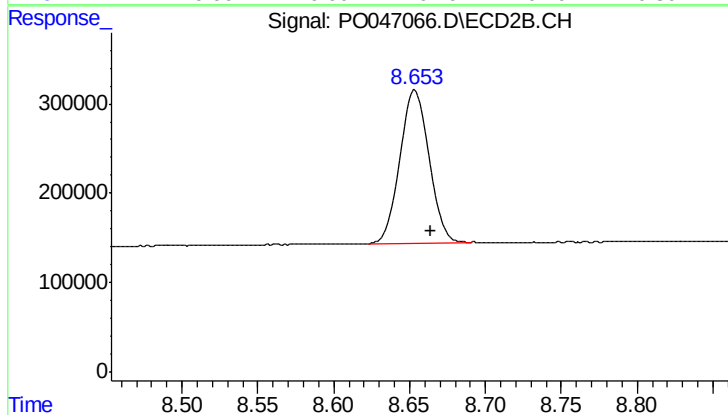

#2 Decachlorobiphenyl

R.T.: 8.653 min
Delta R.T.: -0.011 min
Response: 2260822
Conc: 24.62 ng/ml m

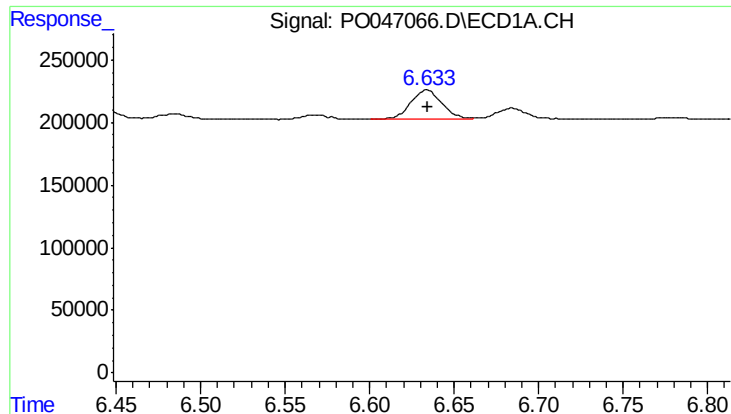


#26 AR-1254-1

R.T.: 6.634 min
Delta R.T.: 0.000 min
Response: 298089
Conc: 36.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:40 PM

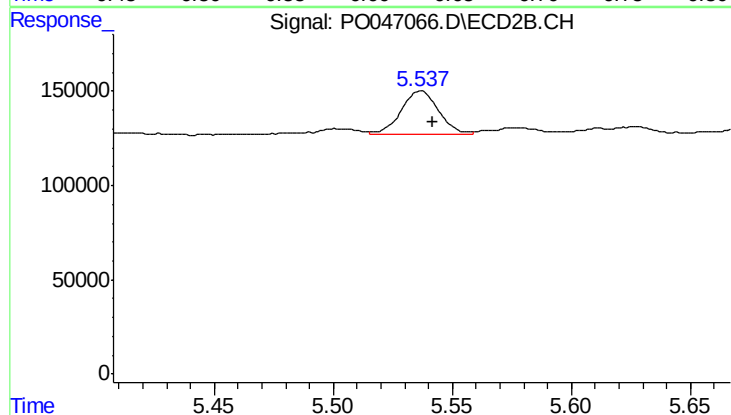


#26 AR-1254-1

R.T.: 5.537 min
Delta R.T.: -0.005 min
Response: 260744
Conc: 36.50 ng/ml

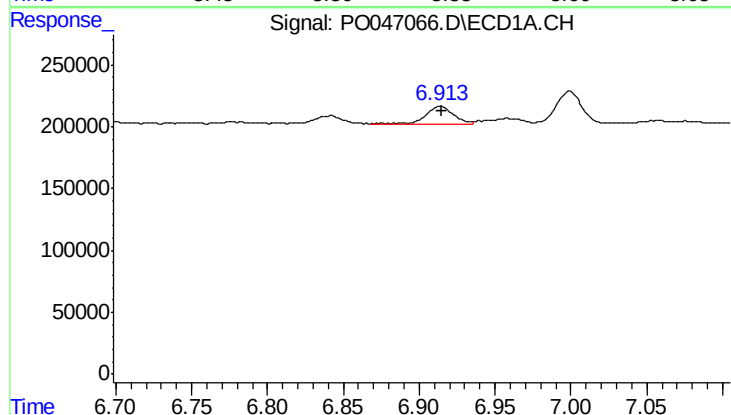


#27 AR-1254-2

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 175359
Conc: 35.71 ng/ml

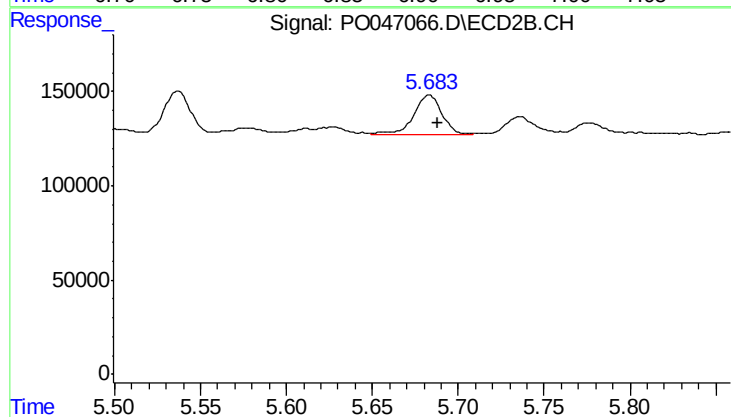

#27 AR-1254-2

R.T.: 5.683 min
Delta R.T.: -0.005 min
Response: 243093
Conc: 40.13 ng/ml

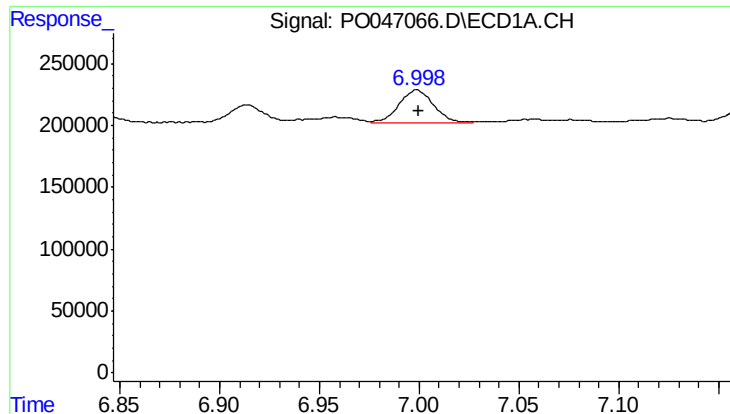


#28 AR-1254-3

R.T.: 6.999 min
Delta R.T.: 0.000 min
Response: 325013
Conc: 37.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:40 PM

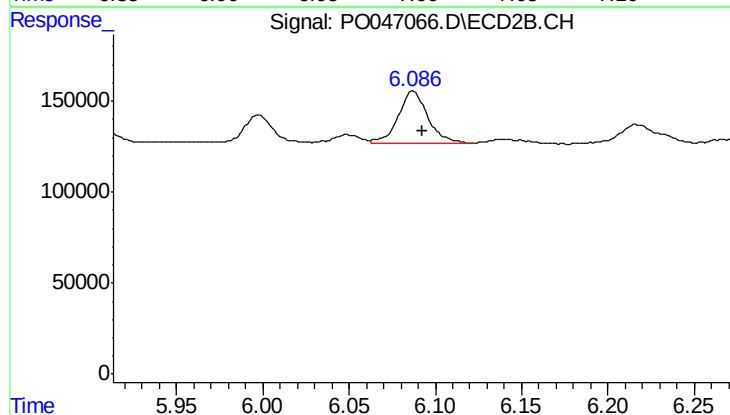


#28 AR-1254-3

R.T.: 6.087 min
Delta R.T.: -0.006 min
Response: 346062
Conc: 36.76 ng/ml

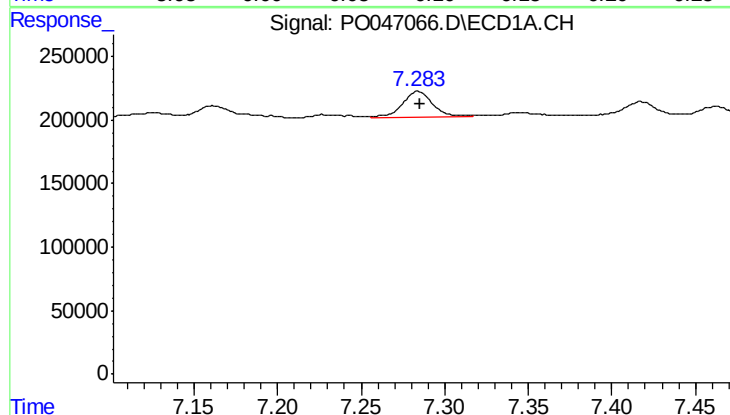


#29 AR-1254-4

R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 267400
Conc: 41.87 ng/ml

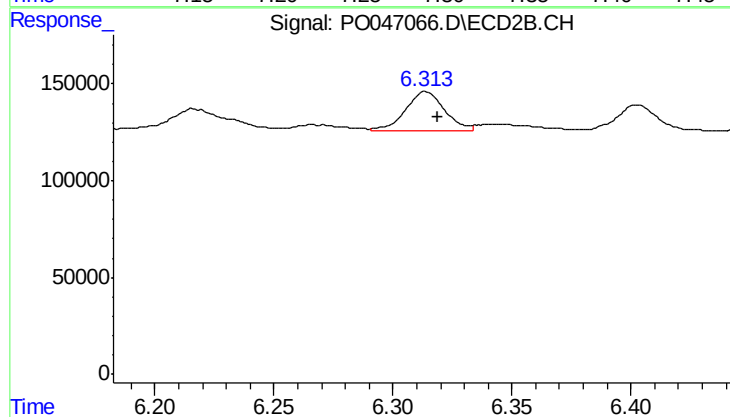

#29 AR-1254-4

R.T.: 6.314 min
Delta R.T.: -0.005 min
Response: 226643
Conc: 39.30 ng/ml

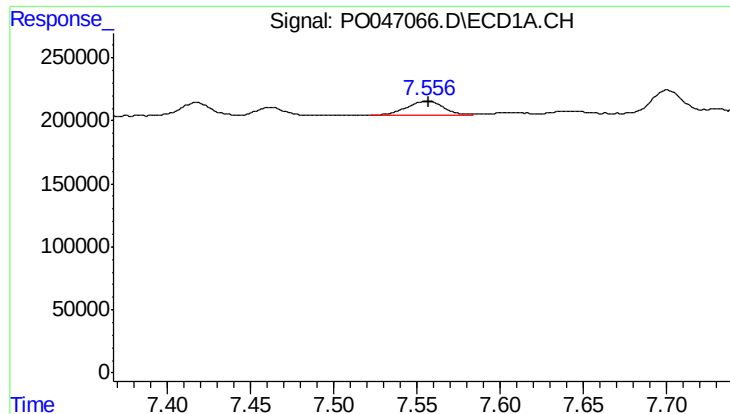


#30 AR-1254-5

R.T.: 7.556 min
Delta R.T.: -0.001 min
Response: 173869
Conc: 36.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254 MDL WATER

Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:40 PM

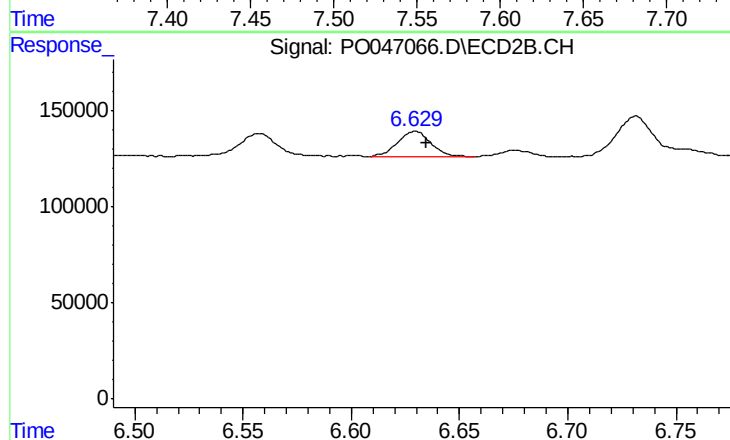

#30 AR-1254-5

R.T.: 6.629 min
Delta R.T.: -0.006 min
Response: 138890
Conc: 34.98 ng/ml