

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072318\
 Data File : P0047072.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 7:06
 Operator : SM/SJ
 Sample : AR1262 MDL WATER
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1262 MDL WATER

Manual Integrations
 APPROVED

Sohil
 7/24/2018 1:42:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 07:41:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.649	3460292	3758507	20.638	19.596
2) SA Decachlor...	10.086	8.653	2869377	2590247	26.211	28.204m
Target Compounds						
41) L9 AR-1268-1	8.619	7.552	535376	564936	34.182	41.462m
42) L9 AR-1268-2	8.711	7.616	477300	538374	34.060	42.896m#
43) L9 AR-1268-3	8.934	7.825	394815	393286	33.852	39.092m
44) L9 AR-1268-4	9.353	8.108	169315	156690	33.506	35.773
45) L9 AR-1268-5	9.757	8.398	1269073	1194898	34.682	39.801m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072318\
Data File : P0047072.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 7:06
Operator : SM/SJ
Sample : AR1262 MDL WATER
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 07:41:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

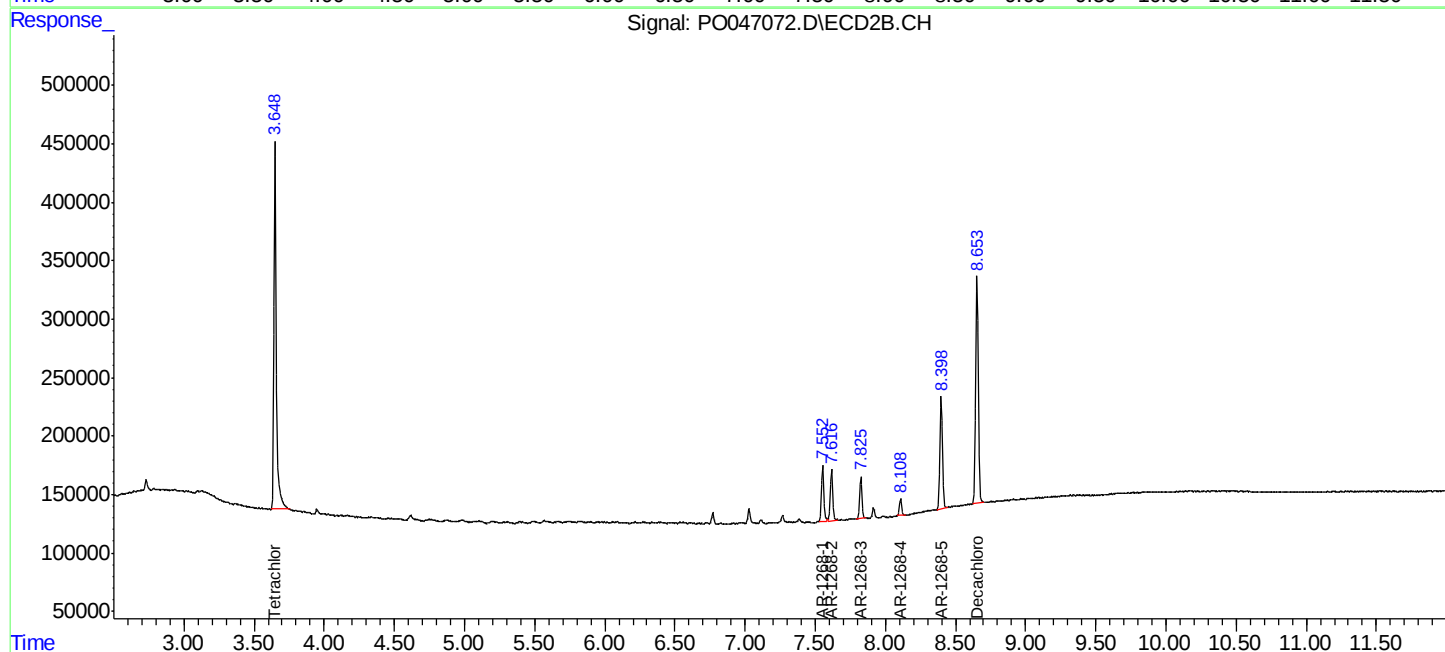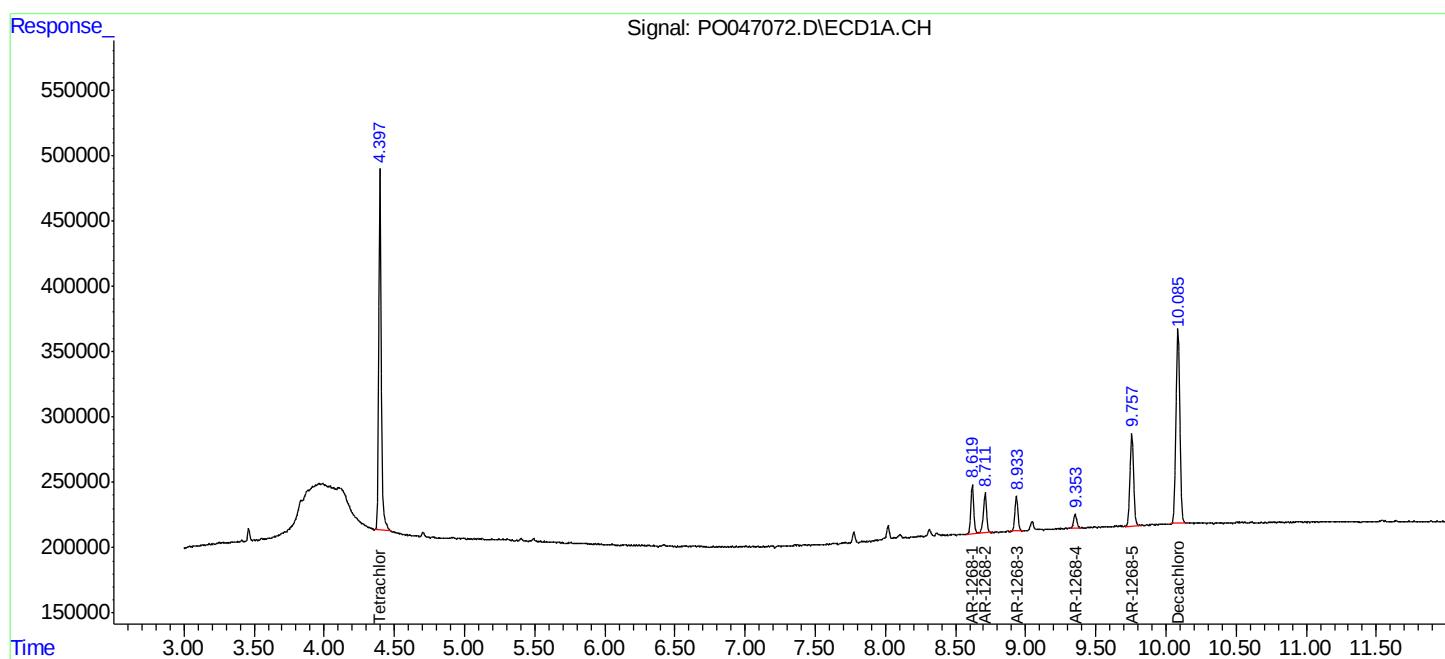

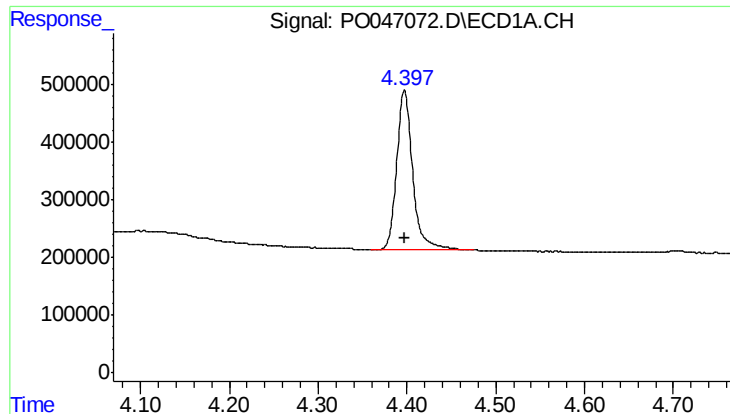


#1 Tetrachloro-m-xylene

R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 3460292
Conc: 20.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:59 PM

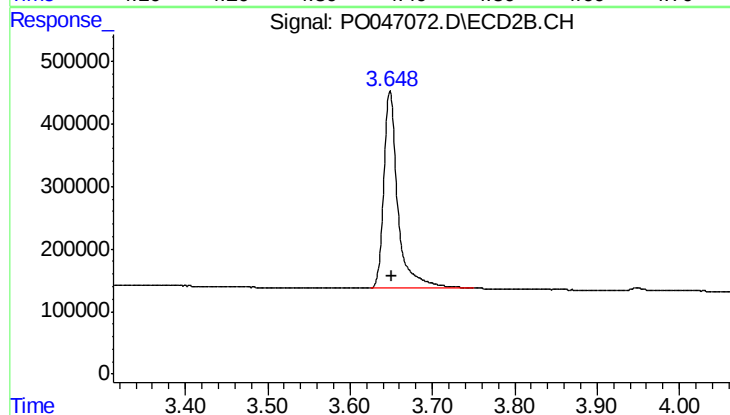


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 3758507
Conc: 19.60 ng/ml

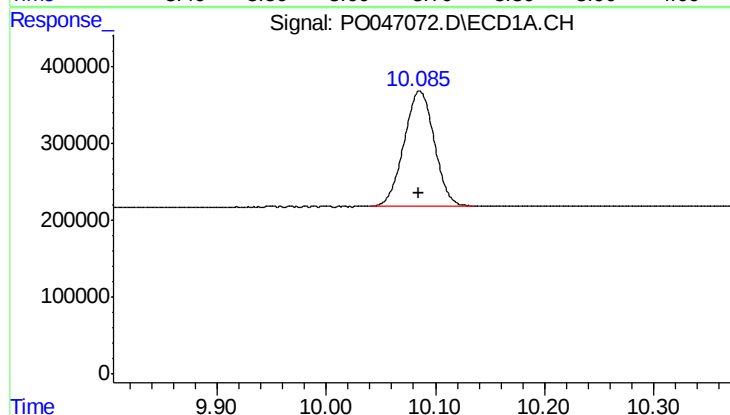


#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: 0.002 min
Response: 2869377
Conc: 26.21 ng/ml

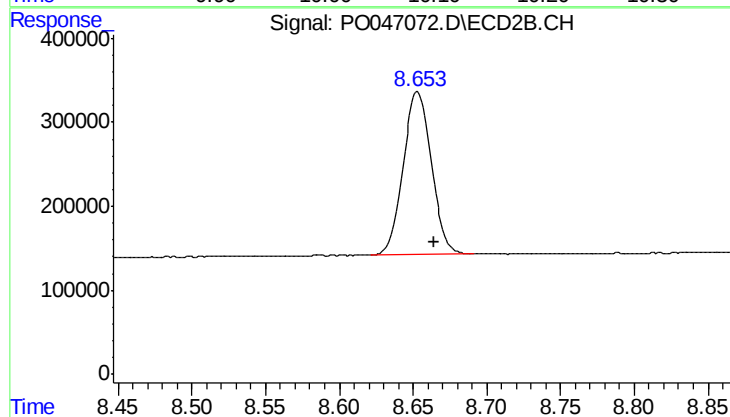

#2 Decachlorobiphenyl

R.T.: 8.653 min
Delta R.T.: -0.012 min
Response: 2590247
Conc: 28.20 ng/ml m

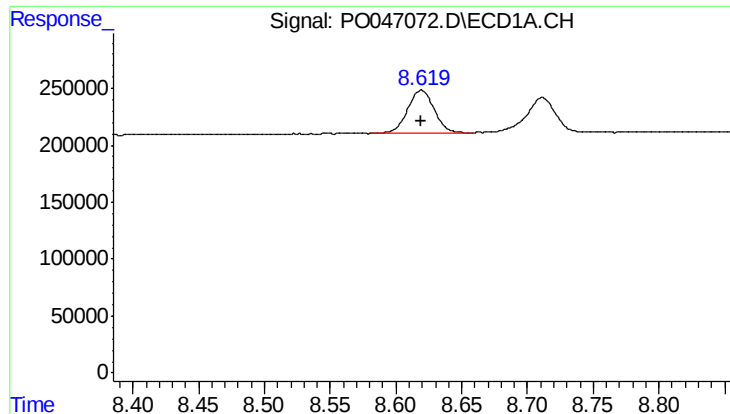


#41 AR-1268-1

R.T.: 8.619 min
Delta R.T.: 0.000 min
Response: 535376
Conc: 34.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:59 PM

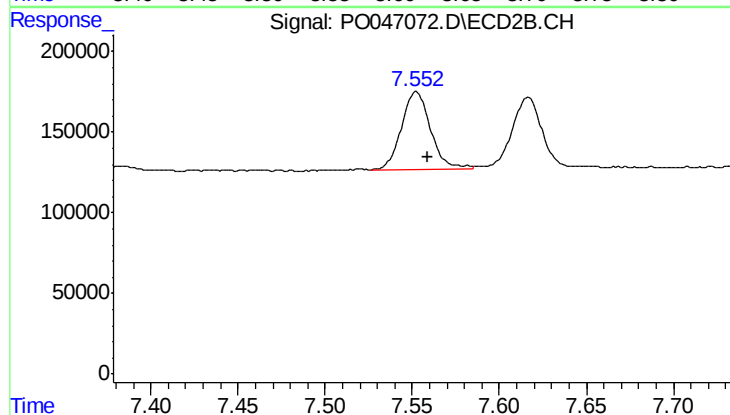


#41 AR-1268-1

R.T.: 7.552 min
Delta R.T.: -0.007 min
Response: 564936
Conc: 41.46 ng/ml m

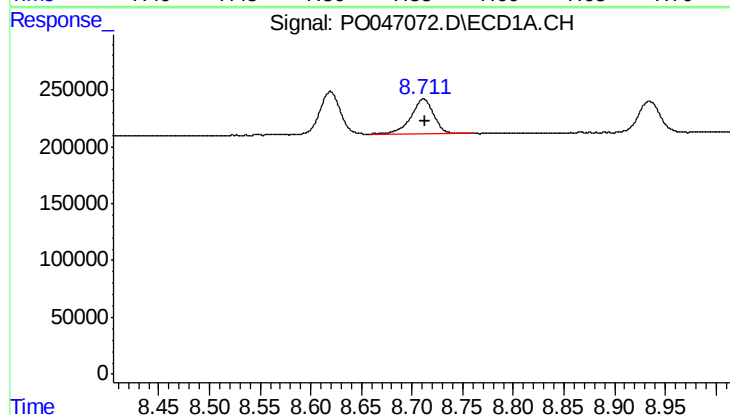


#42 AR-1268-2

R.T.: 8.711 min
Delta R.T.: -0.002 min
Response: 477300
Conc: 34.06 ng/ml

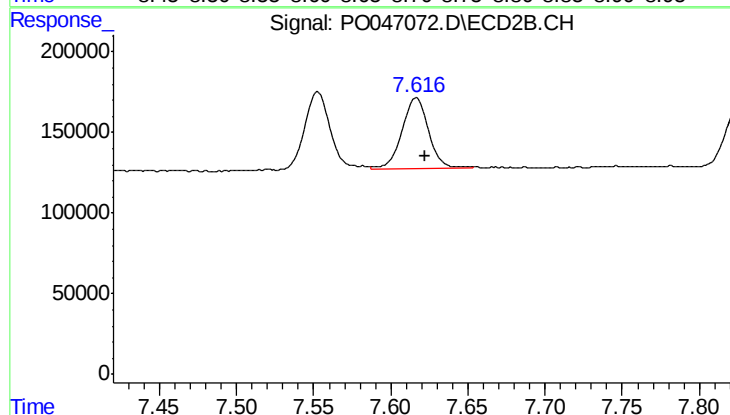

#42 AR-1268-2

R.T.: 7.616 min
Delta R.T.: -0.006 min
Response: 538374
Conc: 42.90 ng/ml m

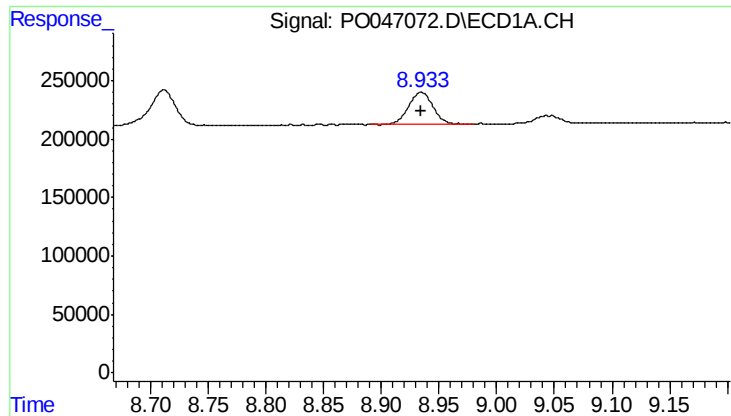


#43 AR-1268-3

R.T.: 8.934 min
Delta R.T.: 0.000 min
Response: 394815
Conc: 33.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER


Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:59 PM

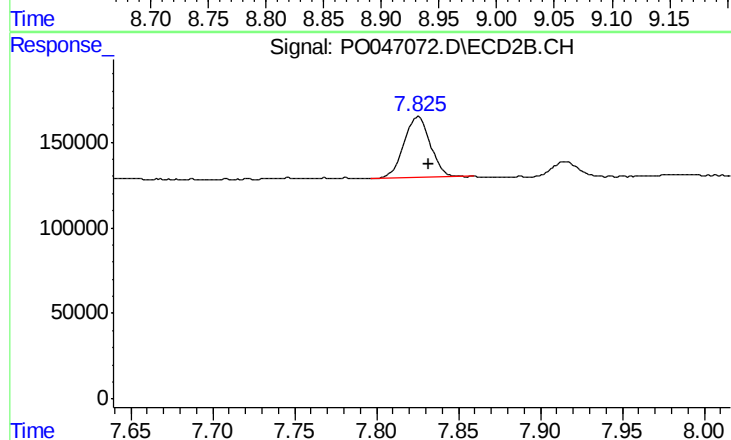


#43 AR-1268-3

R.T.: 7.825 min
Delta R.T.: -0.007 min
Response: 393286
Conc: 39.09 ng/ml m

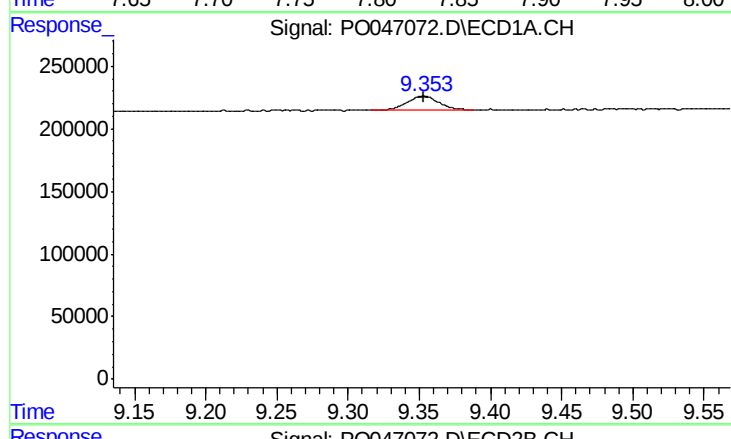


#44 AR-1268-4

R.T.: 9.353 min
Delta R.T.: 0.000 min
Response: 169315
Conc: 33.51 ng/ml

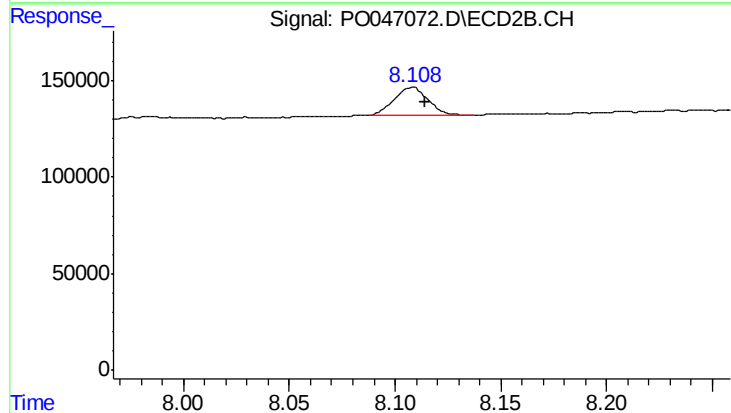

#44 AR-1268-4

R.T.: 8.108 min
Delta R.T.: -0.006 min
Response: 156690
Conc: 35.77 ng/ml

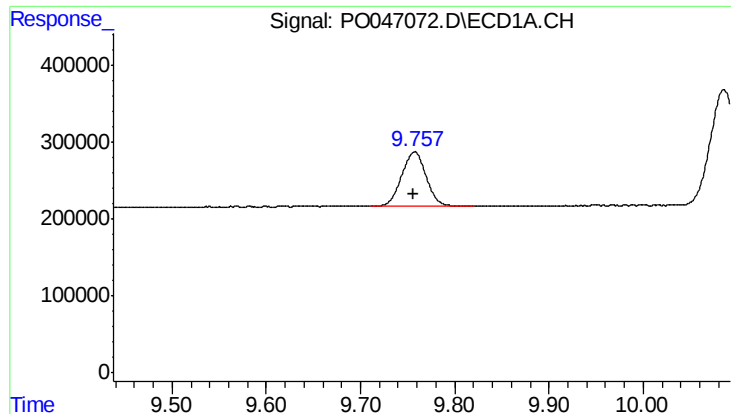


#45 AR-1268-5

R.T.: 9.757 min
Delta R.T.: 0.000 min
Response: 1269073
Conc: 34.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

Manual Integrations
APPROVED

Sohil
7/24/2018 1:42:59 PM

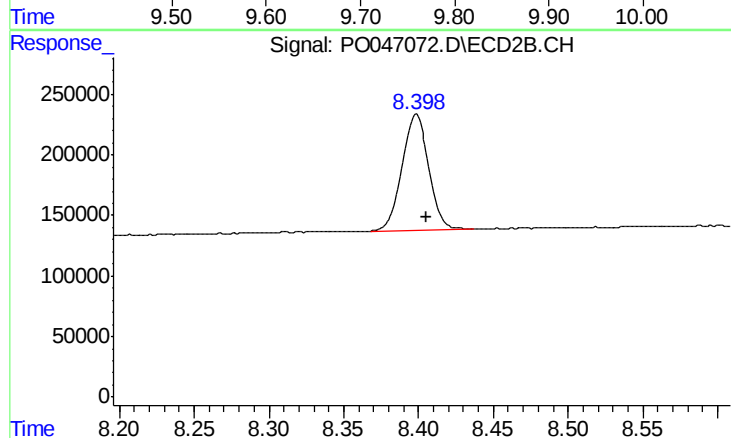

#45 AR-1268-5

R.T.: 8.398 min
Delta R.T.: -0.007 min
Response: 1194898
Conc: 39.80 ng/ml m