

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072321\
 Data File : P0079813.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 21:13
 Operator : DD\AJ
 Sample : PB137892BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB137892BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:34:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 23 05:30:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.001	4.120	949576	391765	16.792	17.621
2)	SA Decachlor...	11.113	9.533	760187	378888	19.236	22.091

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072321\
Data File : PO079813.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 21:13
Operator : DD\AJ
Sample : PB137892BL
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB137892BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:34:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 23 05:30:42 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

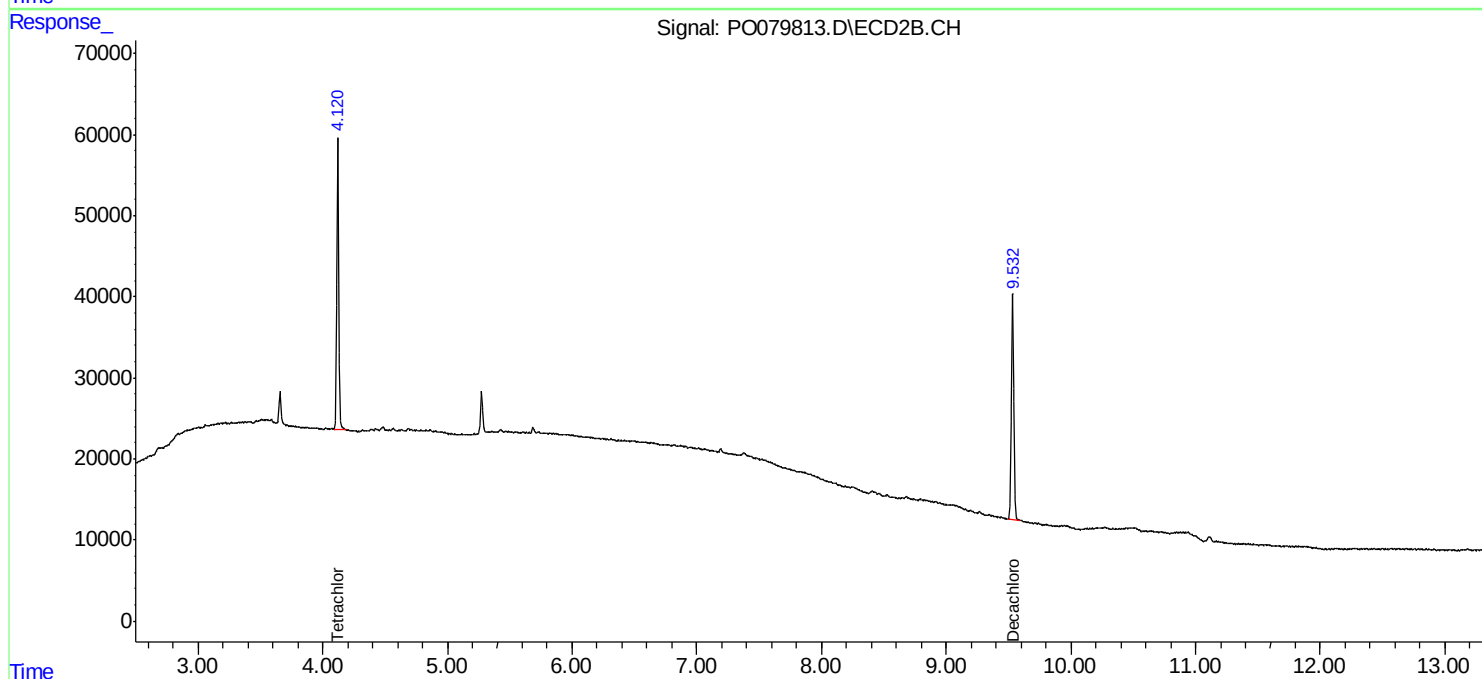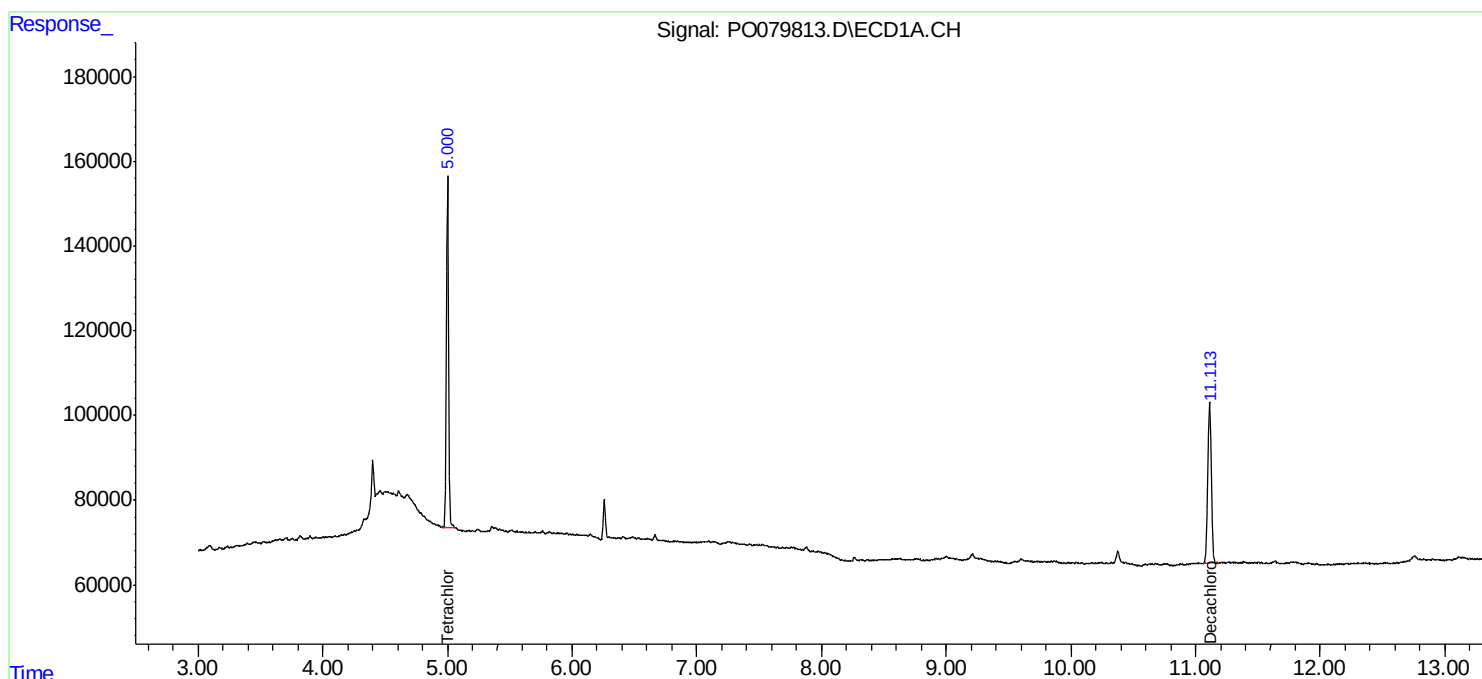


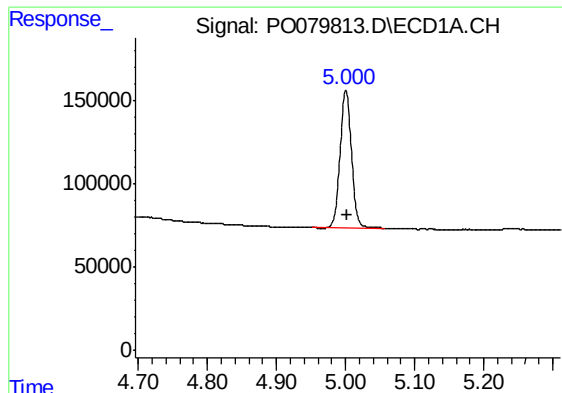

#1 Tetrachloro-m-xylene


R.T.: 5.001 min
Delta R.T.: -0.001 min
Response: 949576
Conc: 16.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB137892BL

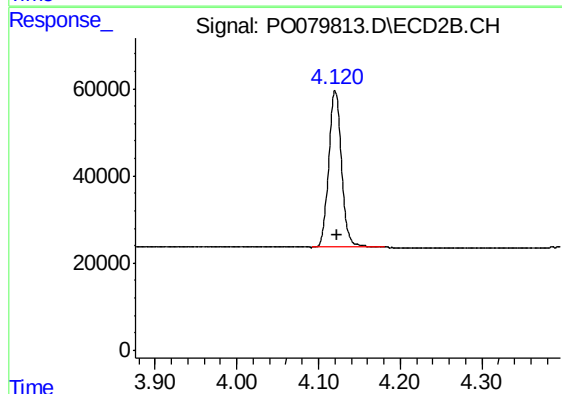


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: -0.002 min
Response: 391765
Conc: 17.62 ng/ml

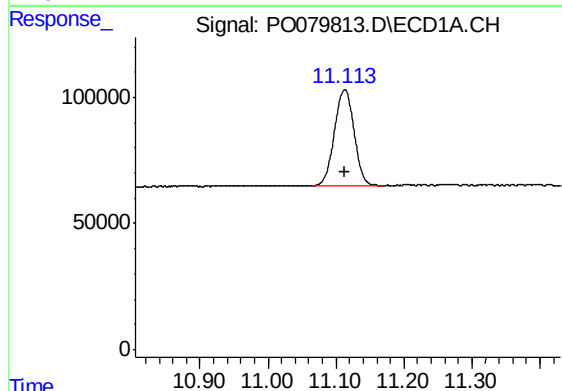

#2 Decachlorobiphenyl

R.T.: 11.113 min
Delta R.T.: 0.001 min
Response: 760187
Conc: 19.24 ng/ml

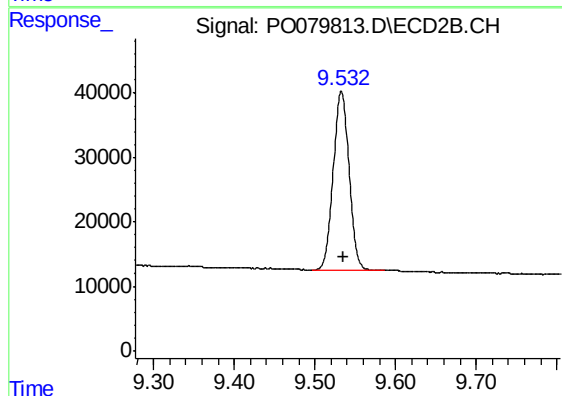

#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.003 min
Response: 378888
Conc: 22.09 ng/ml