

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072321\
 Data File : P0079794.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 15:28
 Operator : DD\AJ
 Sample : M3132-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 55-ST-32

Manual Integrations
 APPROVED

mohammad
 7/26/2021 11:57:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:22:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 23 05:30:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.000	4.120	1077317	462064	19.051m	20.783m
2) SA Decachlor...	11.111	9.532	1228883	365979	31.096	21.338 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072321\
Data File : P0079794.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 15:28
Operator : DD\AJ
Sample : M3132-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
55-ST-32


Manual Integrations
APPROVED

mohammad
7/26/2021 11:57:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:22:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 23 05:30:42 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

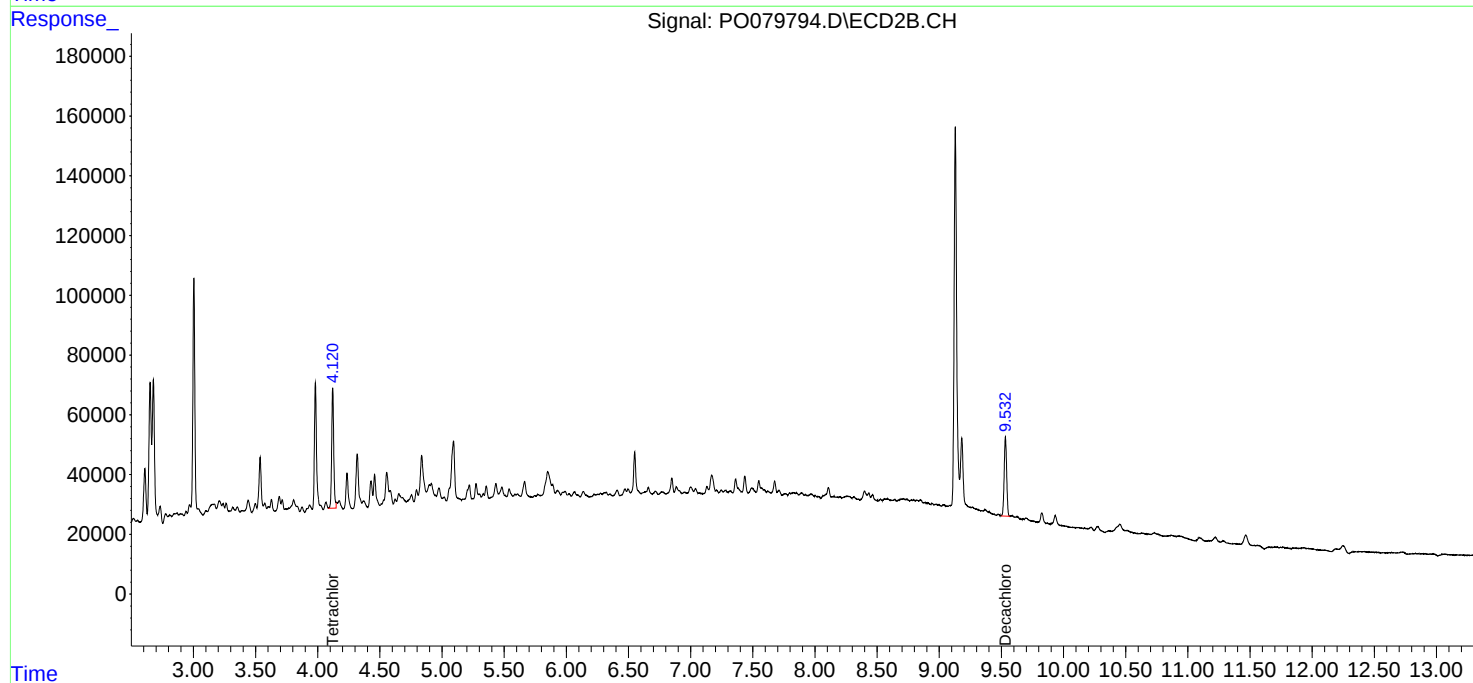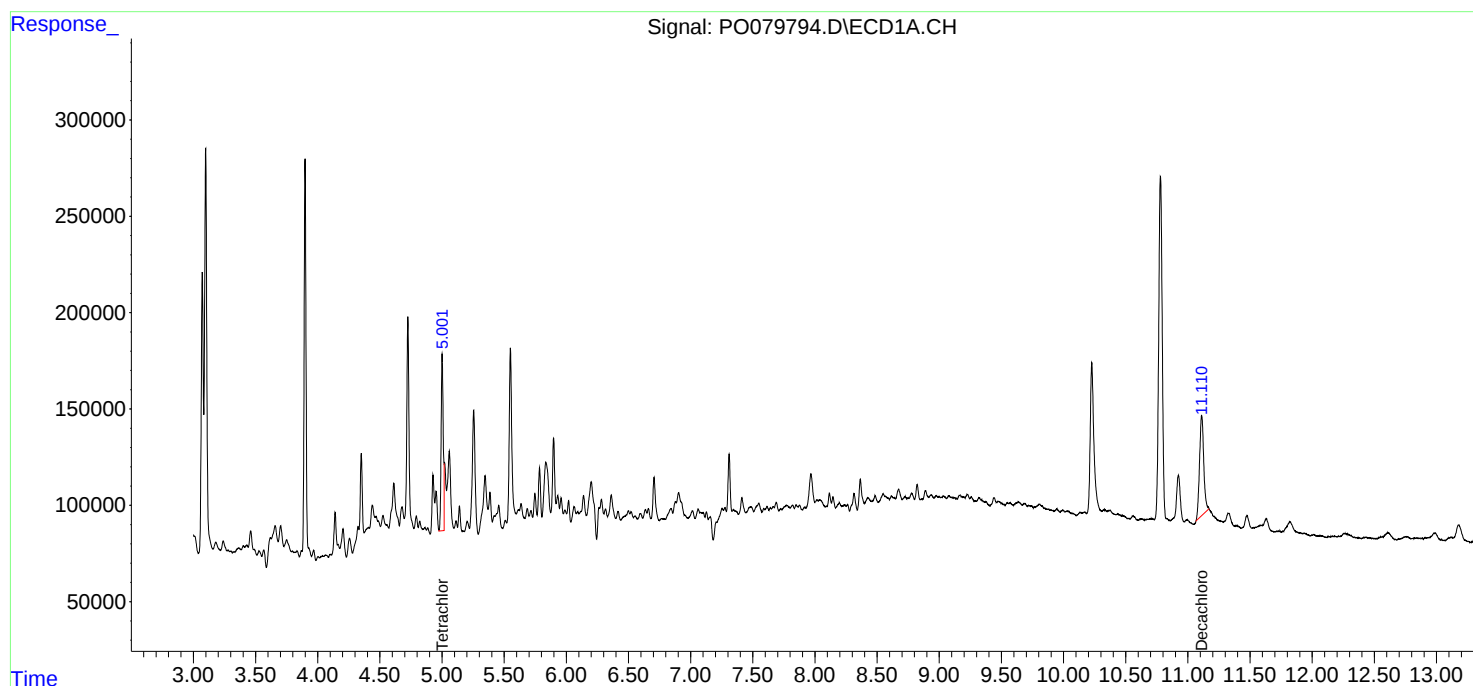

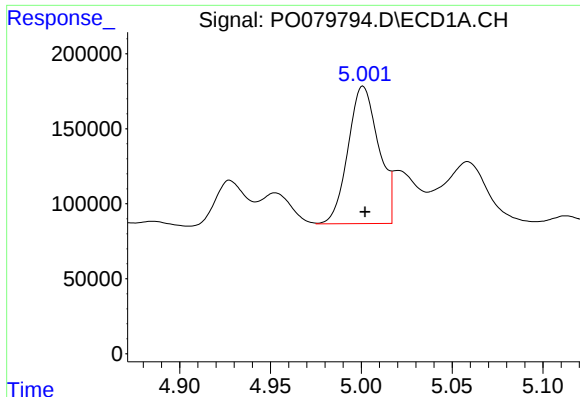


#1 Tetrachloro-m-xylene

R.T.: 5.000 min
Delta R.T.: -0.002 min
Response: 1077317
Conc: 19.05 ng/ml m

Instrument :
ECD_O
ClientSampleId :
55-ST-32


Manual Integrations
APPROVED

mohammad
7/26/2021 11:57:37 AM

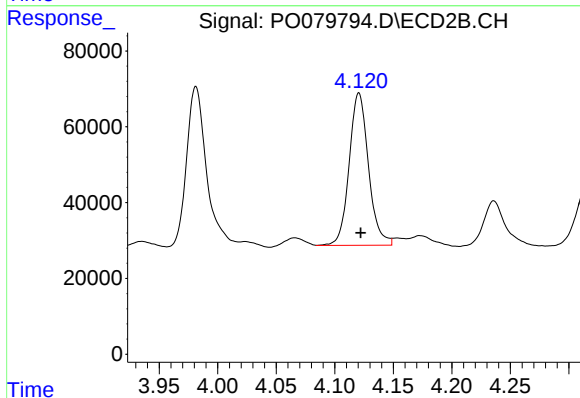


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: -0.002 min
Response: 462064
Conc: 20.78 ng/ml m

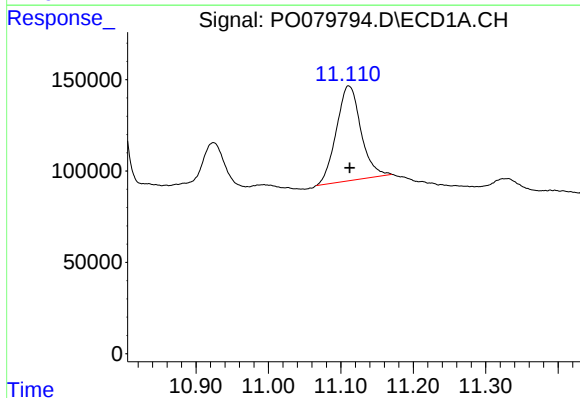

#2 Decachlorobiphenyl

R.T.: 11.111 min
Delta R.T.: -0.001 min
Response: 1228883
Conc: 31.10 ng/ml

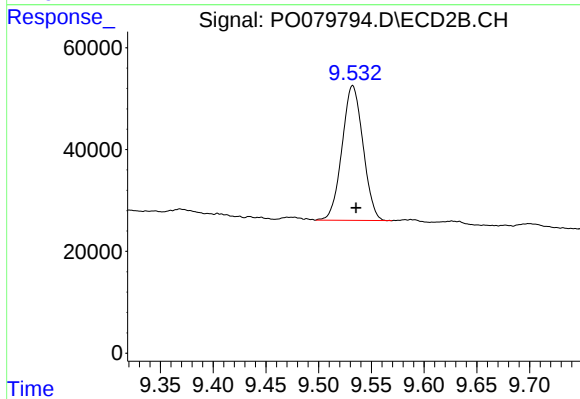

#2 Decachlorobiphenyl

R.T.: 9.532 min
Delta R.T.: -0.003 min
Response: 365979
Conc: 21.34 ng/ml