

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072321\
 Data File : P0079795.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2021 15:45
 Operator : DD\AJ
 Sample : M3130-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SVE-03-AQ

Manual Integrations
 APPROVED

mohammad
 7/26/2021 11:57:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 02:23:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 23 05:30:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.004	4.124	714905	346336	12.642	15.578
2) SA Decachlor...	11.112	9.534	984249	335552	24.906m	19.564

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072321\
Data File : P0079795.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2021 15:45
Operator : DD\AJ
Sample : M3130-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SVE-03-AQ


Manual Integrations
APPROVED

mohammad
7/26/2021 11:57:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 02:23:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 23 05:30:42 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

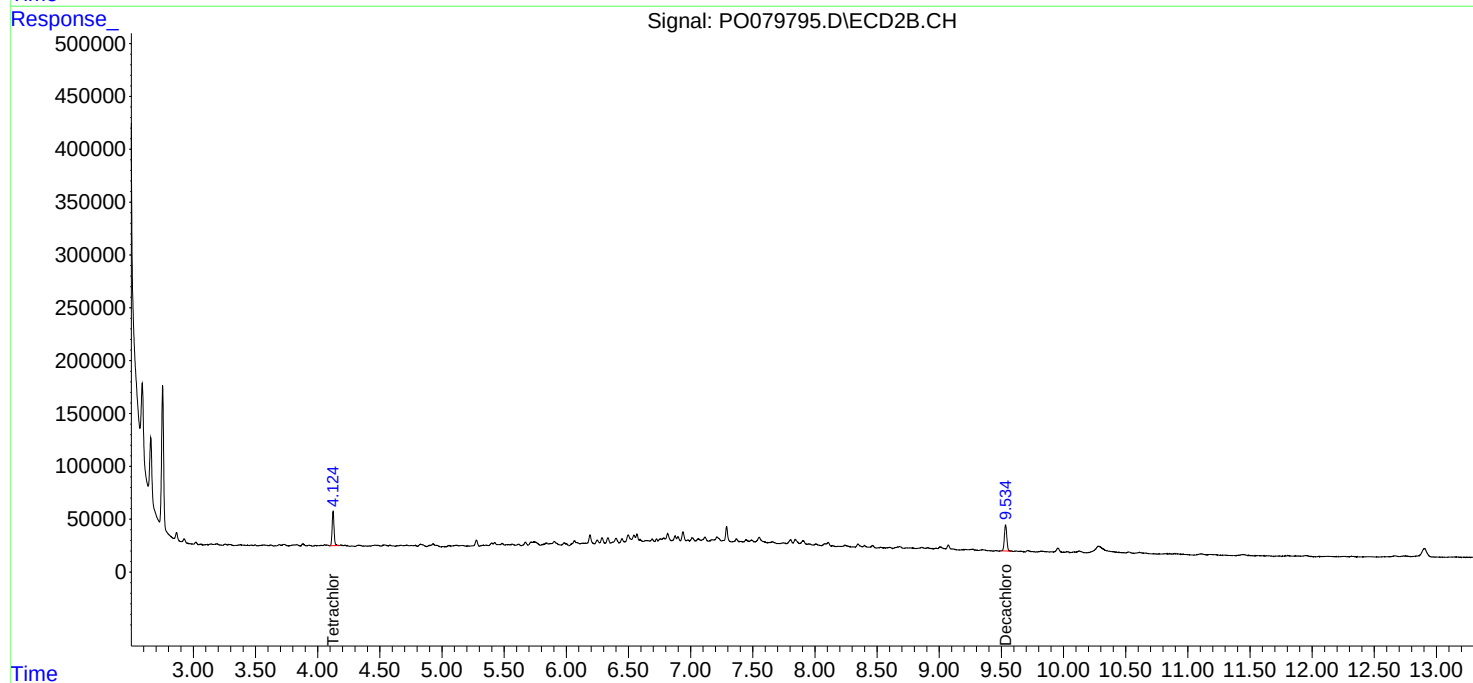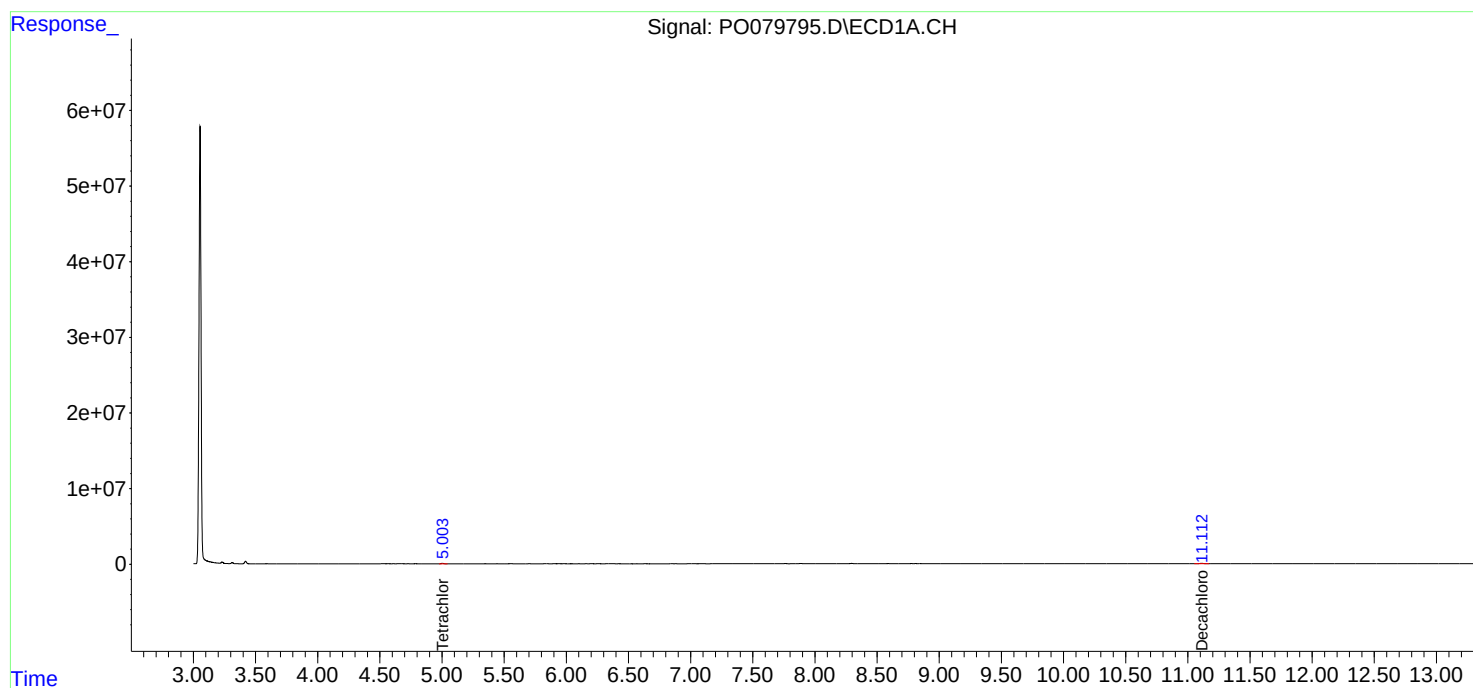

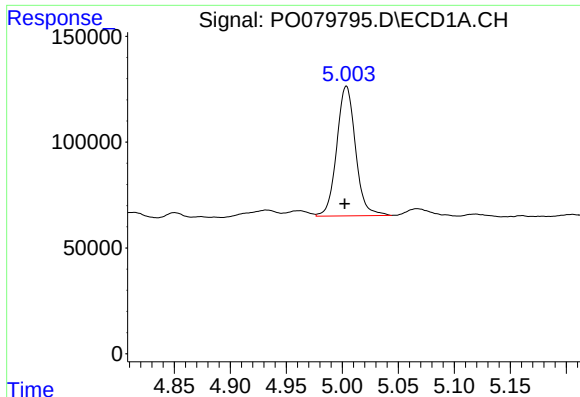


#1 Tetrachloro-m-xylene

R.T.: 5.004 min
Delta R.T.: 0.002 min
Response: 714905
Conc: 12.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
SVE-03-AQ


Manual Integrations
APPROVED

mohammad
7/26/2021 11:57:38 AM

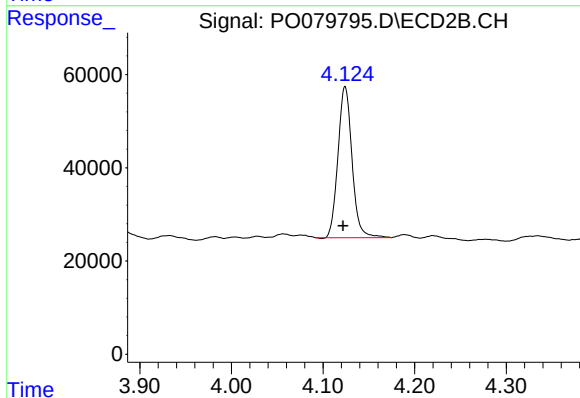


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.002 min
Response: 346336
Conc: 15.58 ng/ml

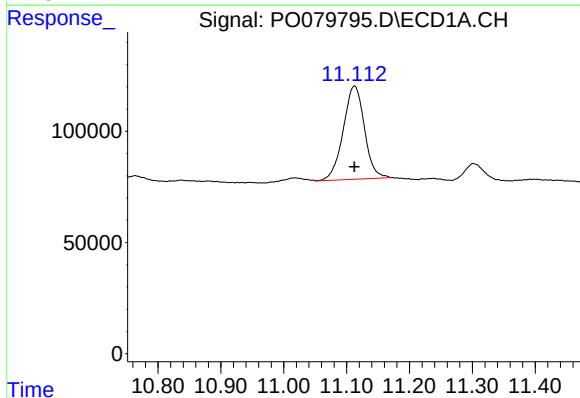

#2 Decachlorobiphenyl

R.T.: 11.112 min
Delta R.T.: 0.000 min
Response: 984249
Conc: 24.91 ng/ml m

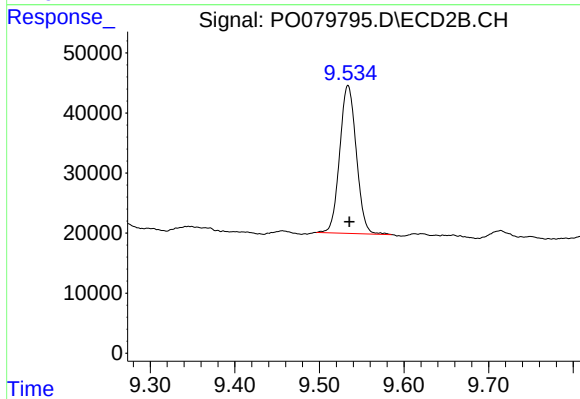

#2 Decachlorobiphenyl

R.T.: 9.534 min
Delta R.T.: -0.002 min
Response: 335552
Conc: 19.56 ng/ml