

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072321\
 Data File : P0079822.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2021 00:06
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 03:37:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 23 05:30:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.002	4.121	1015529	419487	17.959	18.868
2)	SA Decachlor...	11.114	9.533	815730	405020	20.641	23.614

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072321\
Data File : P0079822.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2021 00:06
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 03:37:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 23 05:30:42 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

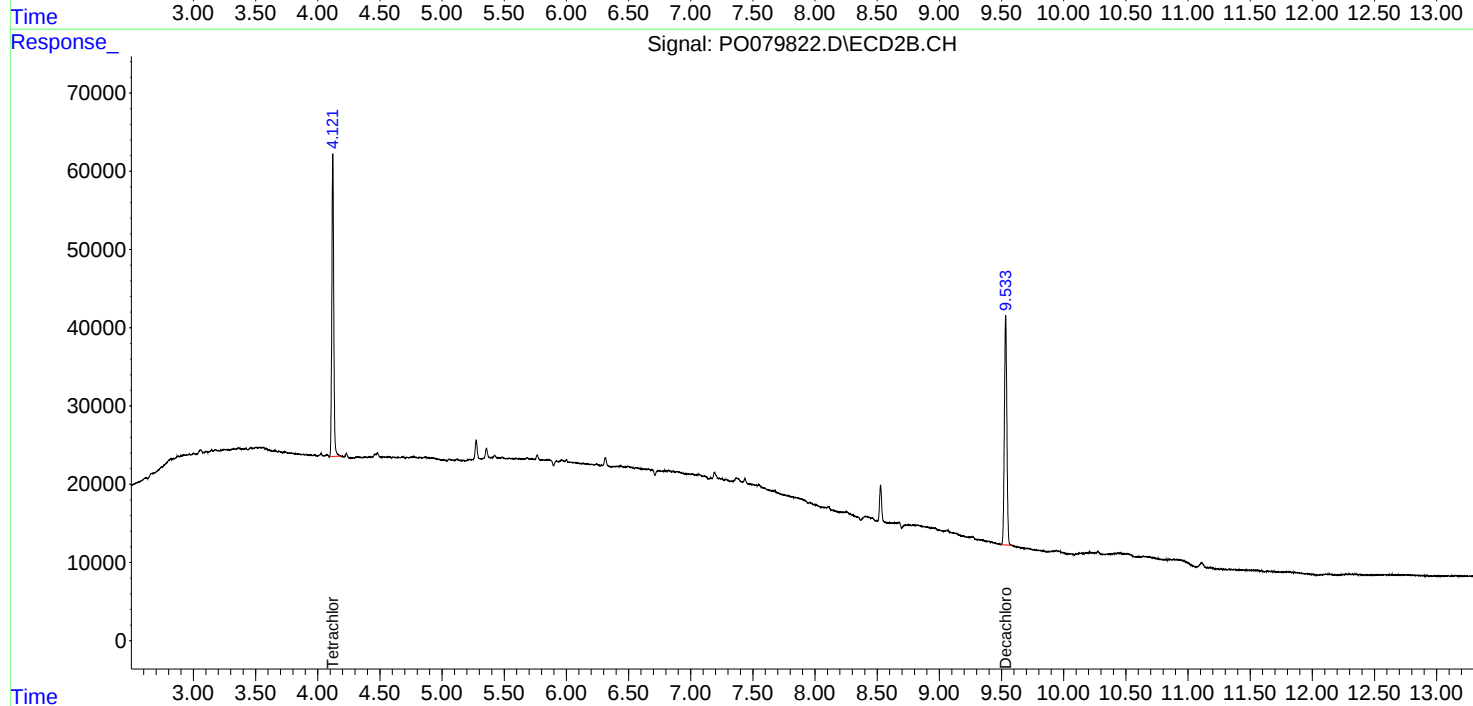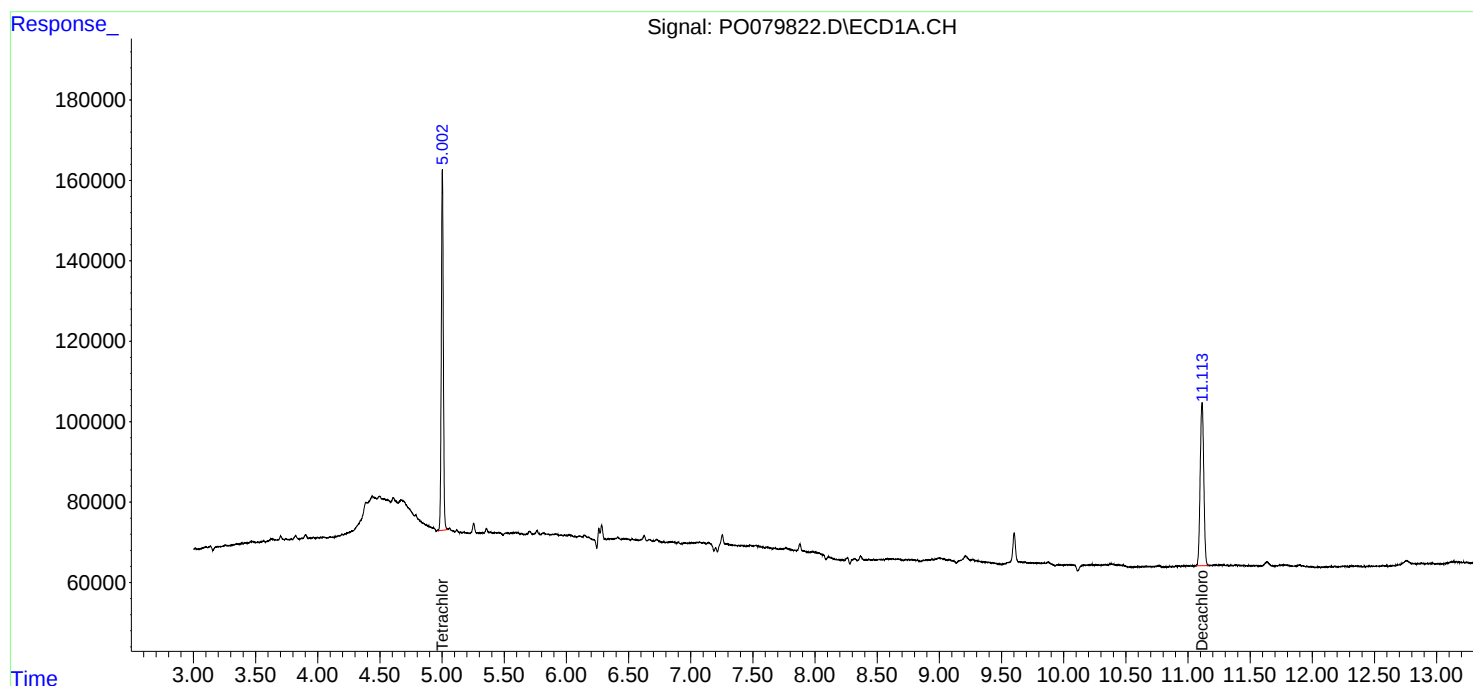


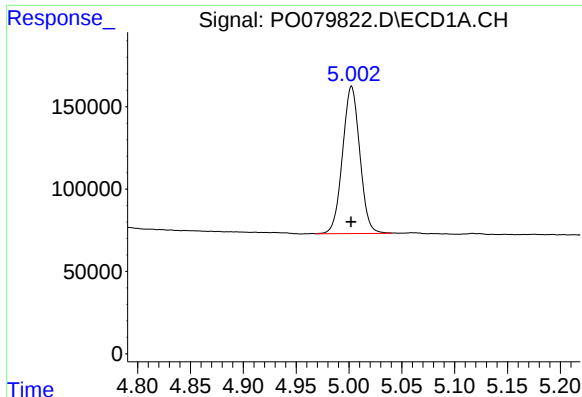

#1 Tetrachloro-m-xylene


R.T.: 5.002 min
Delta R.T.: 0.000 min
Response: 1015529
Conc: 17.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

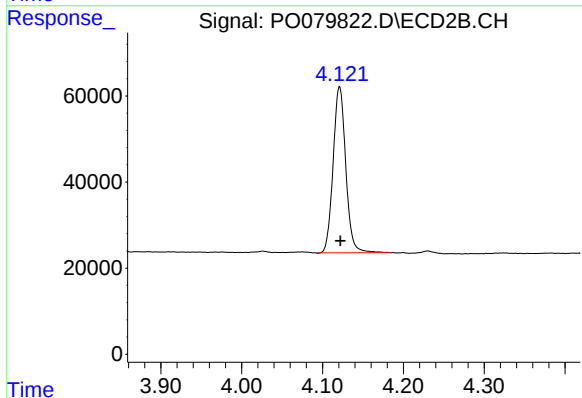


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: 0.000 min
Response: 419487
Conc: 18.87 ng/ml

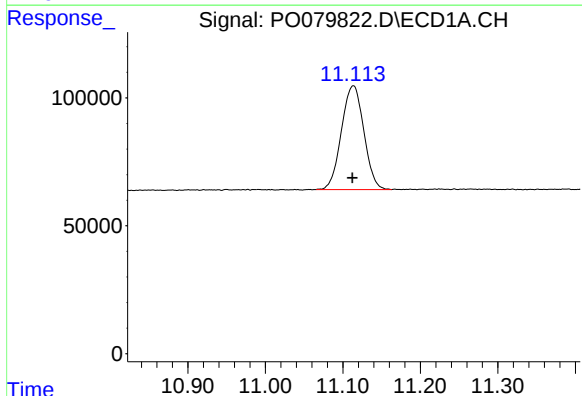

#2 Decachlorobiphenyl

R.T.: 11.114 min
Delta R.T.: 0.001 min
Response: 815730
Conc: 20.64 ng/ml

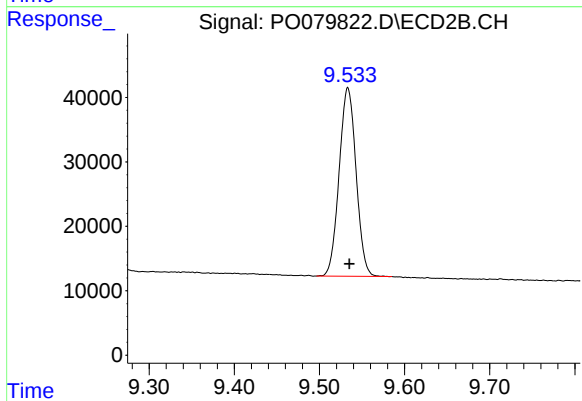

#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.002 min
Response: 405020
Conc: 23.61 ng/ml