

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072324\
 Data File : P0104914.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 12:49
 Operator : YP/AJ
 Sample : P3330-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KKA1110-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/24/2024
 Supervised By :Ankita Jodhani 07/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:50:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.540	11346810	4470639	1.267	1.370
2) SA Decachlor...	10.215	8.435	9296133	3129143	1.516	1.492m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072324\
Data File : PO104914.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 12:49
Operator : YP/AJ
Sample : P3330-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KKA1110-1-1


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 07/24/2024
Supervised By : Ankita Jodhani 07/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 01:50:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

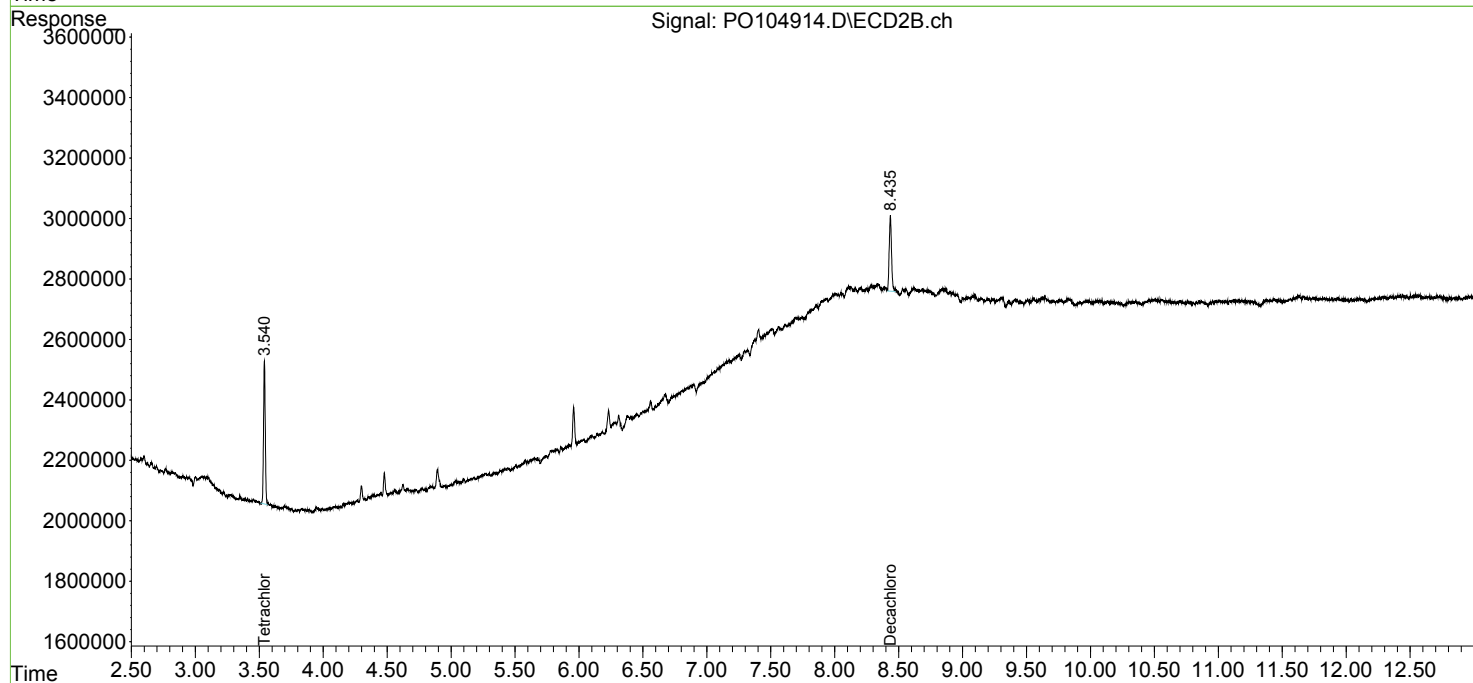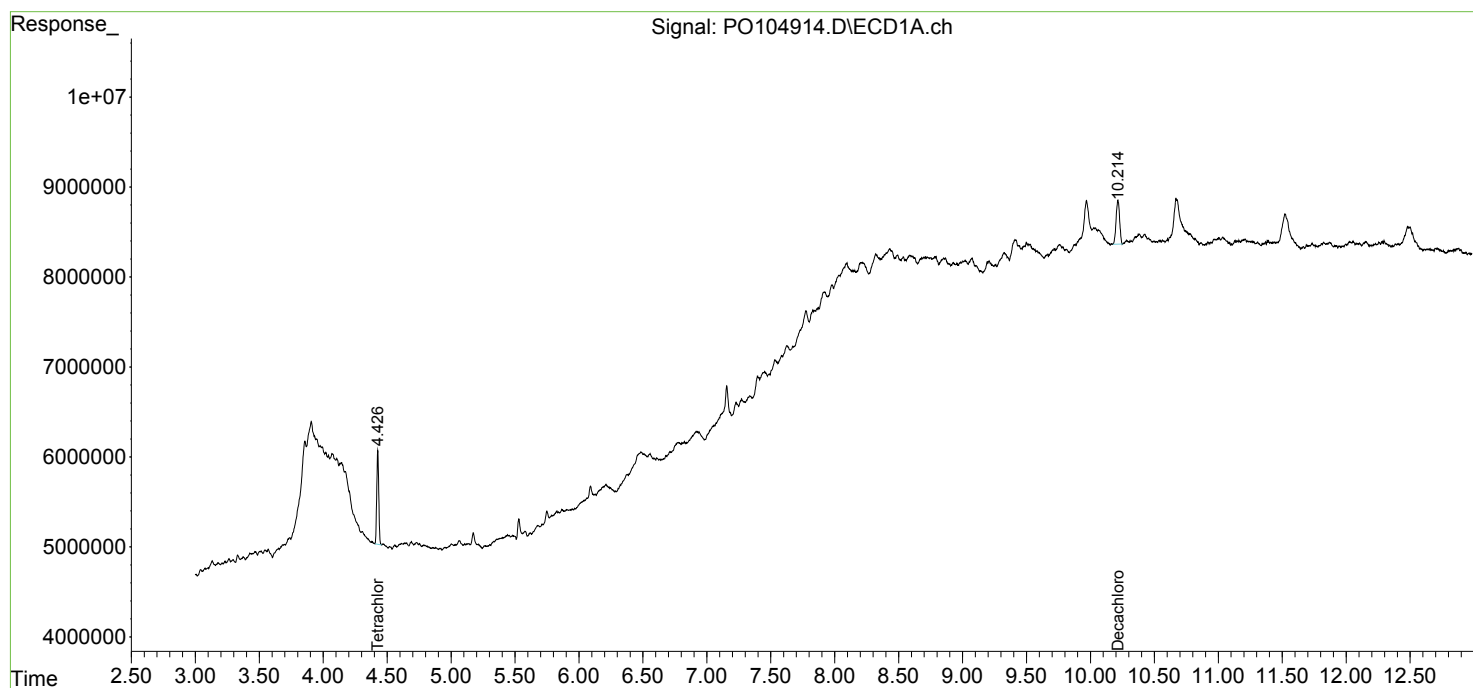

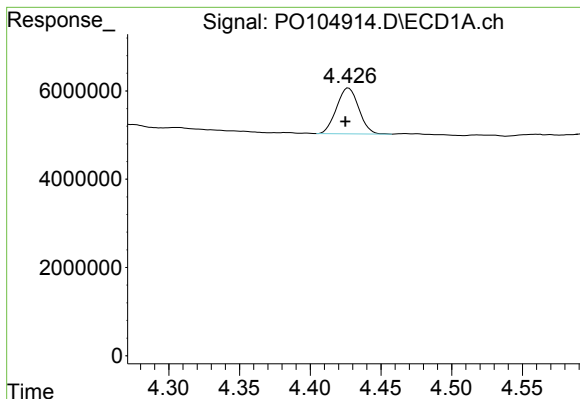


#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: 0.002 min
Response: 11346810
Conc: 1.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
KKA1110-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2024
Supervised By :Ankita Jodhani 07/24/2024

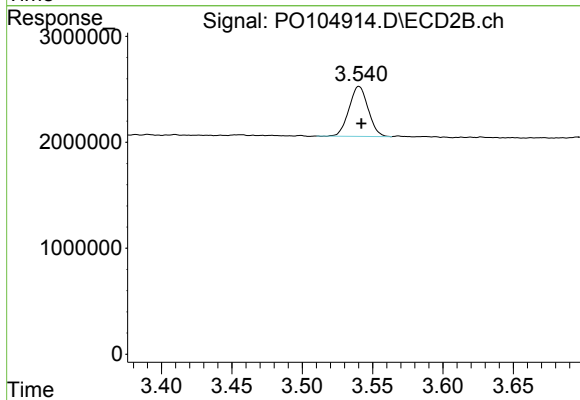


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.002 min
Response: 4470639
Conc: 1.37 ng/ml

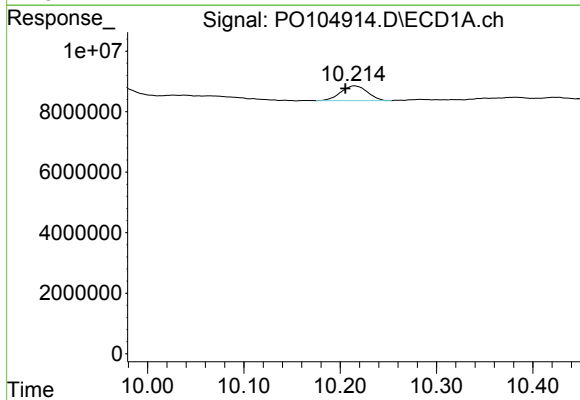

#2 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: 0.009 min
Response: 9296133
Conc: 1.52 ng/ml

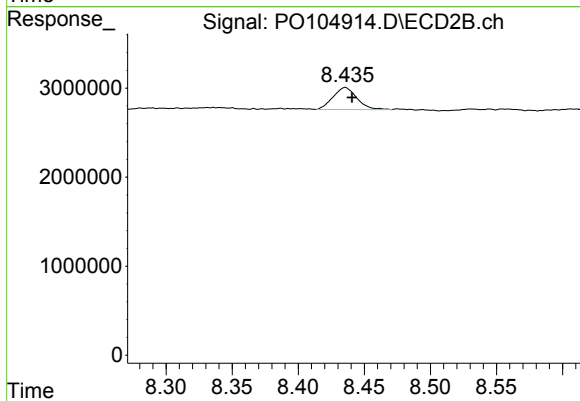

#2 Decachlorobiphenyl

R.T.: 8.435 min
Delta R.T.: -0.006 min
Response: 3129143
Conc: 1.49 ng/ml m