

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072324\
 Data File : P0104918.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2024 13:58
 Operator : YP/AJ
 Sample : P3331-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2310-0320-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/24/2024
 Supervised By :Ankita Jodhani 07/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 01:51:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.539	14460433	5062032	1.615	1.552
2) SA Decachlor...	10.216	8.436	10242291	2657725	1.670m	1.267m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072324\
Data File : PO104918.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2024 13:58
Operator : YP/AJ
Sample : P3331-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2310-0320-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2024
Supervised By :Ankita Jodhani 07/24/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 01:51:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

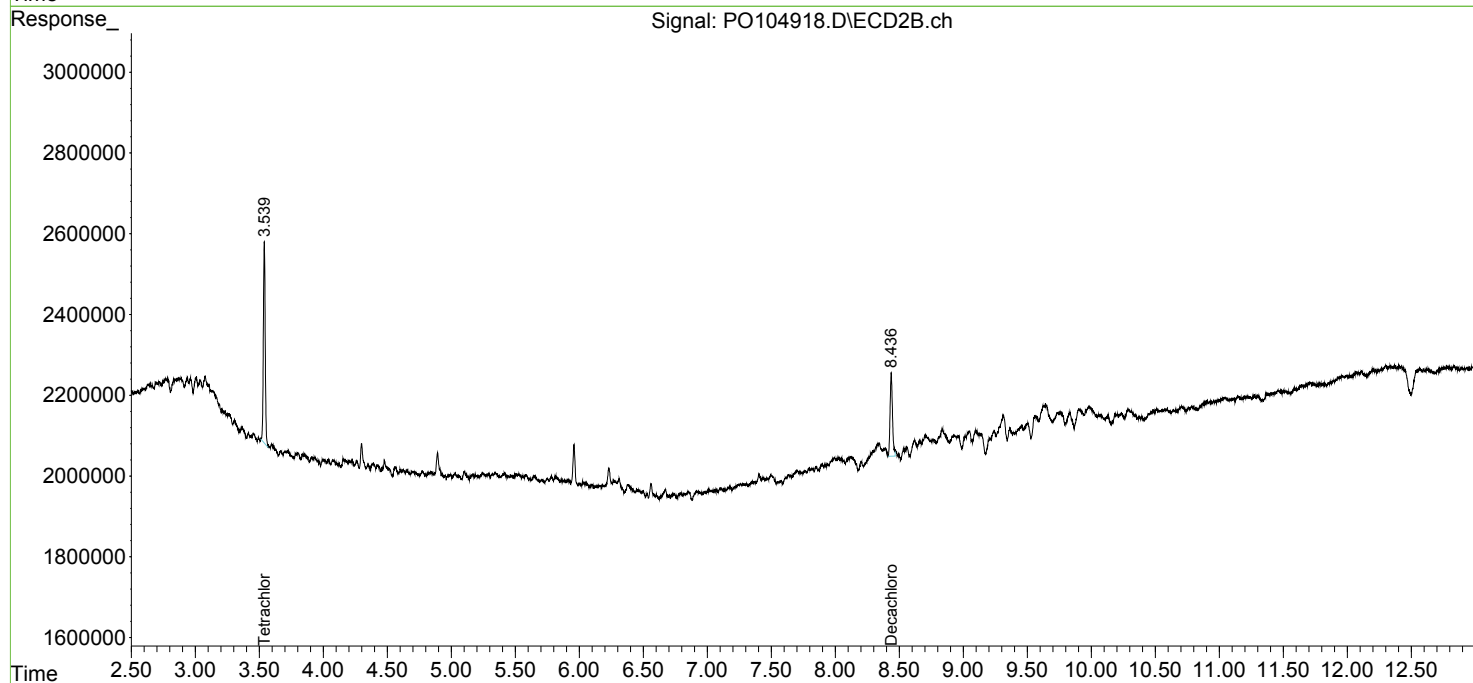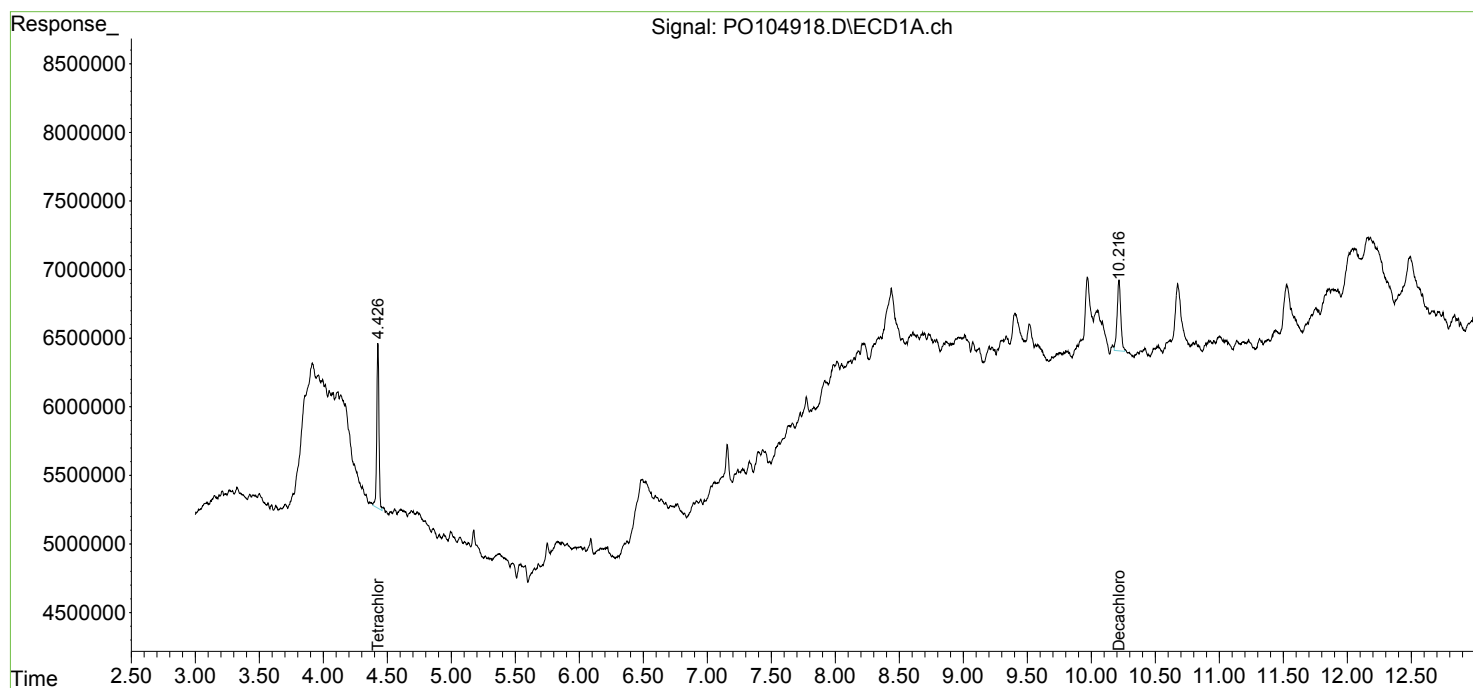

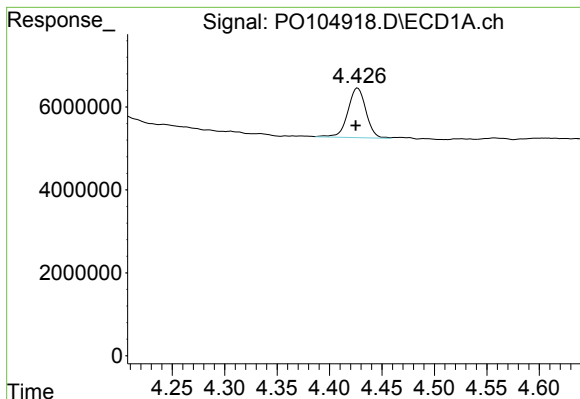


#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: 0.002 min
Response: 14460433
Conc: 1.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2310-0320-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2024
Supervised By :Ankita Jodhani 07/24/2024

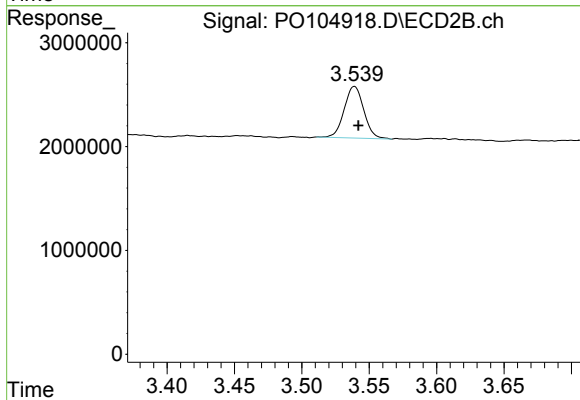


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.003 min
Response: 5062032
Conc: 1.55 ng/ml

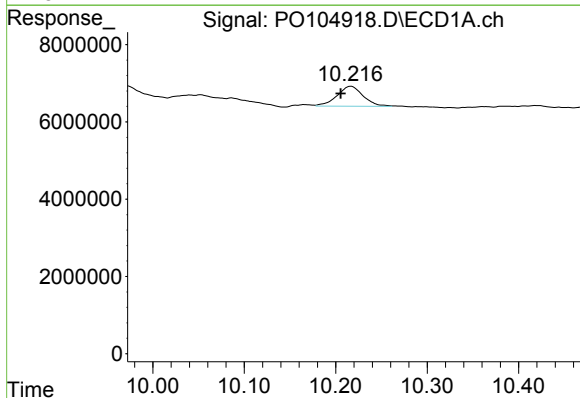

#2 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: 0.011 min
Response: 10242291
Conc: 1.67 ng/ml m

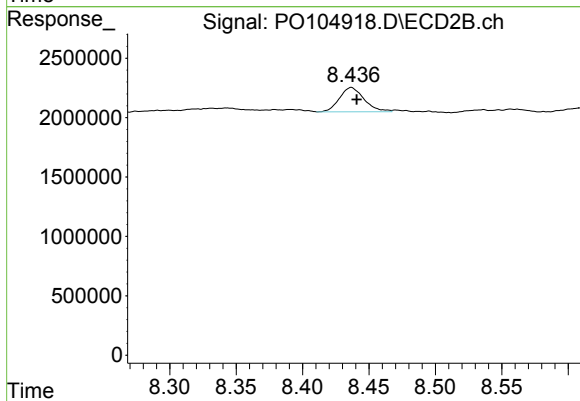

#2 Decachlorobiphenyl

R.T.: 8.436 min
Delta R.T.: -0.004 min
Response: 2657725
Conc: 1.27 ng/ml m