

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072325\
 Data File : P0112447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 23:07
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:05:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	0.000	3.669	0	52514	N.D.	0.011 #
2) SA Decachlor...	8.691	8.636	538381	99499	0.074	0.056
Target Compounds						
3) L1 AR-1016-1	4.758	4.738	512596	211473	1.910	1.208 #
4) L1 AR-1016-2	4.777	4.757	303839	174741	0.748	0.671
5) L1 AR-1016-3	4.840	4.924	783736	245799	2.995	1.808 #
6) L1 AR-1016-4	4.960	4.978	3409355	1275763	16.094	11.485 #
7) L1 AR-1016-5	5.218	5.183	5056651	540796	23.040	3.774 #
8) L2 AR-1221-1	3.830f	3.868	299361	38267	3.097	0.569 #
9) L2 AR-1221-2	0.000	3.962	0	248584	N.D.	4.900 #
10) L2 AR-1221-3	0.000	4.031	0	83310	N.D.	0.526 #
11) L3 AR-1232-1	0.000	4.031	0	83310	N.D.	0.658 #
12) L3 AR-1232-2	4.540	4.757	1272252	174741	11.821	1.332 #
13) L3 AR-1232-3	4.777	4.924	303839	245799	1.469	3.658 #
14) L3 AR-1232-4	4.960	5.017	3409355	419225	32.551	7.007 #
15) L3 AR-1232-5	5.010	5.183	4963111	540796	73.115	8.294 #
16) L4 AR-1242-1	4.758	4.738	512596	211473	2.070	1.335 #
17) L4 AR-1242-2	4.777	4.757	303839	174741	0.822	0.748
18) L4 AR-1242-3	4.840	4.924	783736	245799	3.312	2.028 #
19) L4 AR-1242-4	4.960	5.017	3409355	419225	17.549	3.416 #
20) L4 AR-1242-5	5.614	5.543	7124997	1056460	33.308	6.563 #
21) L5 AR-1248-1	4.758	4.738	512596	211473	2.738	1.740 #
22) L5 AR-1248-2	5.010	4.978	4963111	1275763	19.455	7.536 #
23) L5 AR-1248-3	5.218	5.017	5056651	419225	14.712	2.360 #
24) L5 AR-1248-4	5.571	5.183	5015131	540796	9.871	2.596 #
25) L5 AR-1248-5	5.614	5.578	7124997	877829	20.381	4.087 #
26) L6 AR-1254-1	5.571	5.543	5015131	1056460	9.136	3.215 #
27) L6 AR-1254-2	5.733	5.675	32146463	246716	66.156	0.852 #
28) L6 AR-1254-3	6.101	6.100	832937	13802808	1.119	32.290 #
29) L6 AR-1254-4	6.325	6.317	4423459	387388	8.047	1.419 #
30) L6 AR-1254-5	6.759	6.725	3823.7E6	1892.4E6	5402.088	5665.465
31) L7 AR-1260-1	6.238	6.217	459345	1056241	1.046	4.250 #
32) L7 AR-1260-2	6.437	6.405	7089425	4079277	10.306	12.380
33) L7 AR-1260-3	6.833	6.620f	1377006	186154	2.342	0.725 #
34) L7 AR-1260-4	7.061	7.035	4158557	227850	9.221	1.191 #
35) L7 AR-1260-5	7.306	7.262	2280827	395290	1.841	0.959 #
36) L8 AR-1262-1	6.833	6.725f	1377006	1892.4E6	1.482	4561.835 #
37) L8 AR-1262-2	7.306	7.262	2280827	395290	1.534	0.767 #
38) L8 AR-1262-3	7.592	7.544	556382	87646	0.943	0.470 #
39) L8 AR-1262-4	7.647	7.619	591400	91132	0.595	0.316 #
40) L8 AR-1262-5	8.137	8.104	54490	58456	0.126	0.587 #
41) L9 AR-1268-1	7.592	7.544	556382	87646	0.318	0.169 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072325\
 Data File : P0112447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 23:07
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:05:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.647	7.619	591400	91132	0.401	0.214 #
43) L9	AR-1268-3	7.851	7.835	2507568	35708	2.002	0.111 #
44) L9	AR-1268-4	8.137	8.104	54490	58456	0.113	0.525 #
45) L9	AR-1268-5	8.440	8.395	1143419	33716	0.341	0.046 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072325\
Data File : P0112447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2025 23:07
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 05:05:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

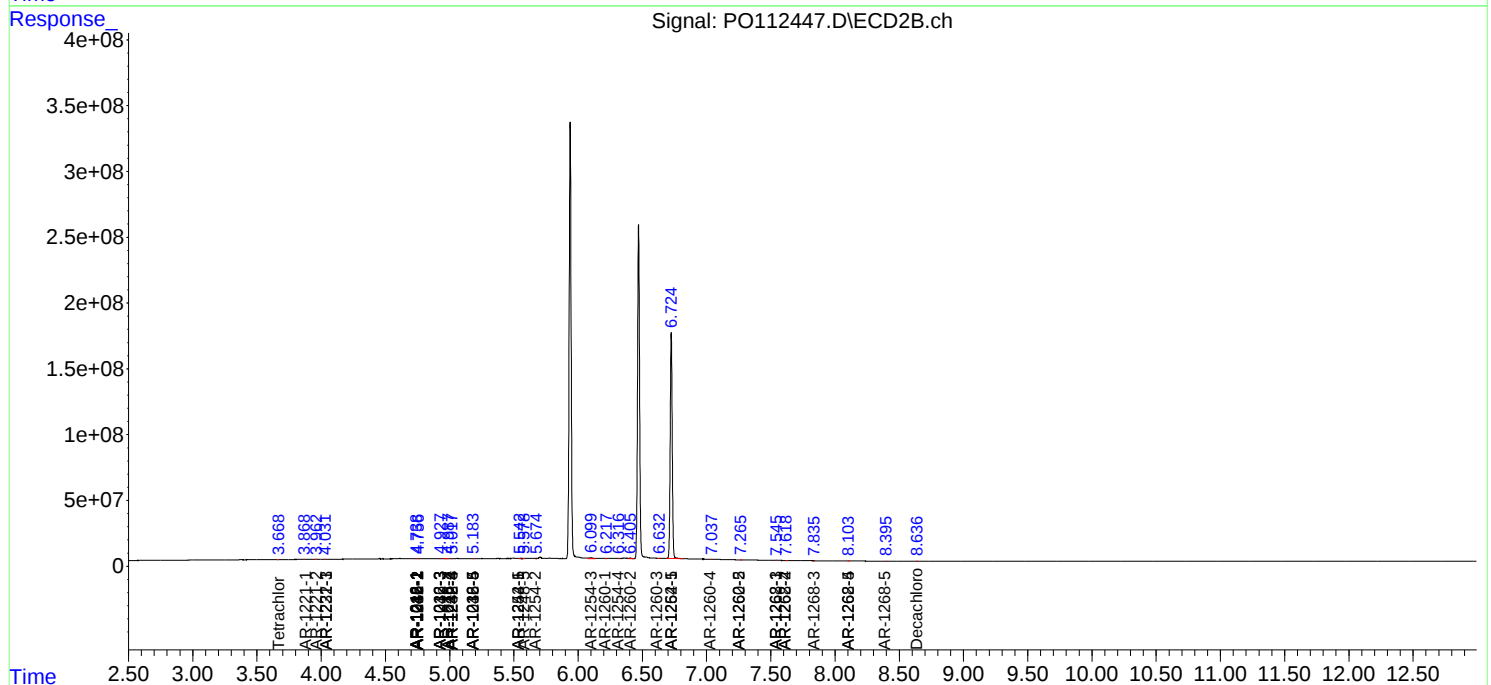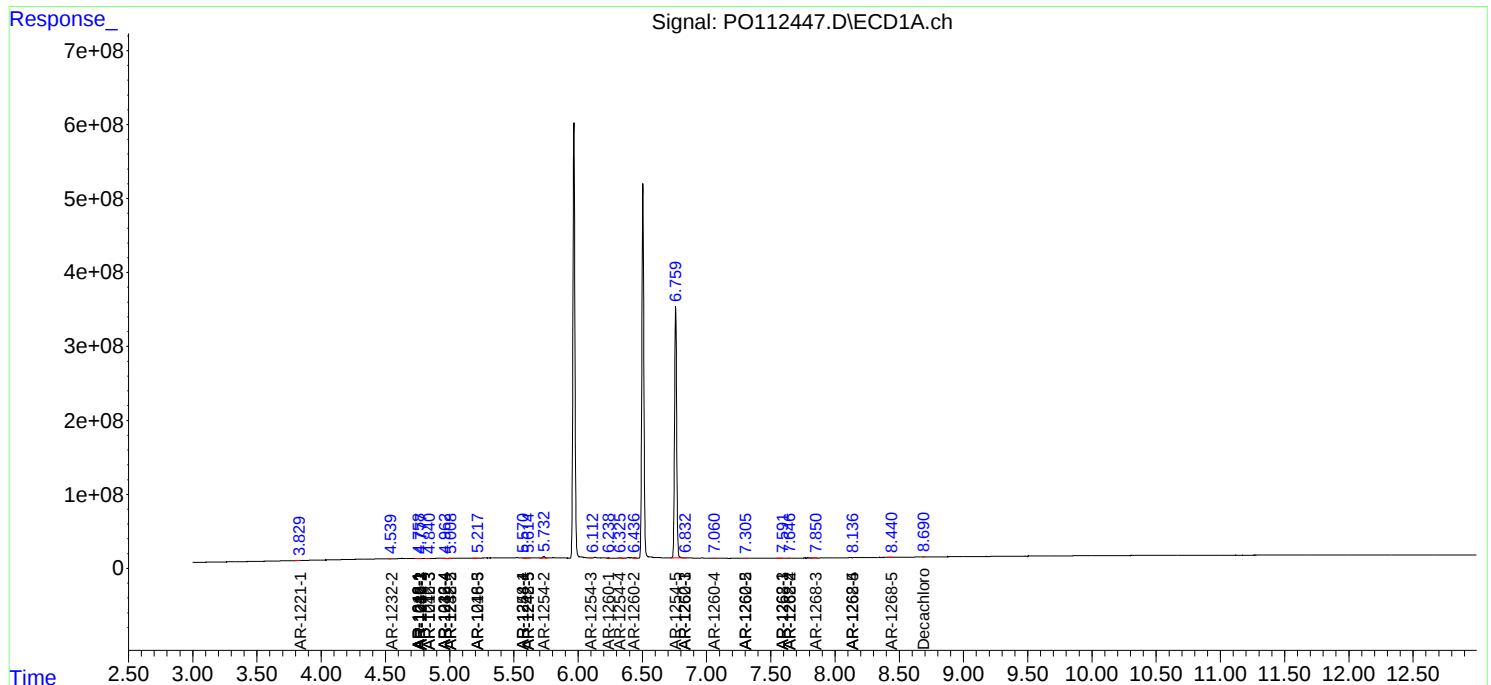


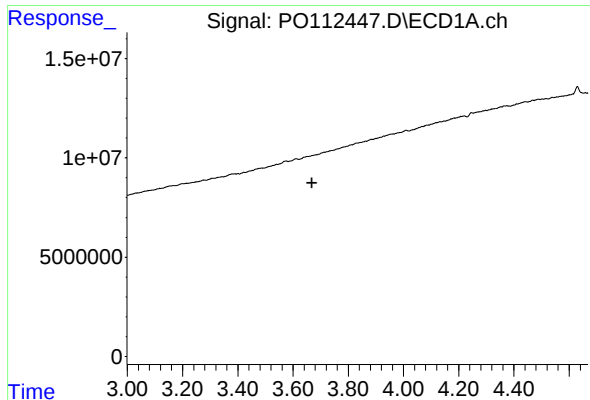

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.669 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

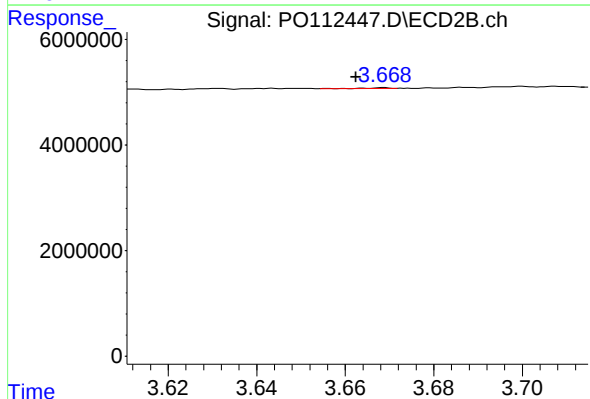


#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: 0.006 min
Response: 52514
Conc: 0.01 ng/ml

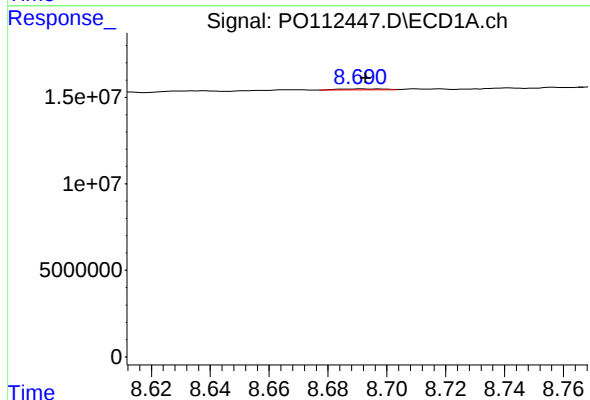


#2 Decachlorobiphenyl

R.T.: 8.691 min
Delta R.T.: -0.002 min
Response: 538381
Conc: 0.07 ng/ml

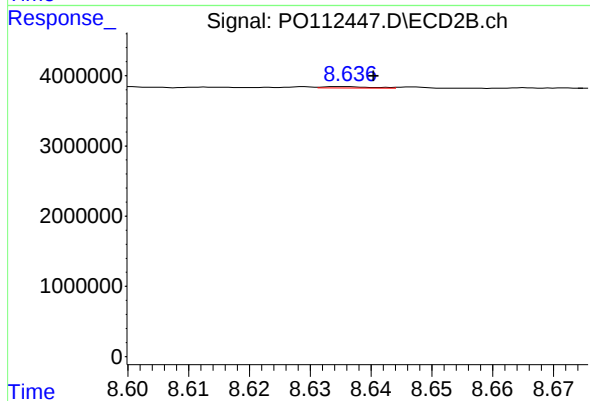

#2 Decachlorobiphenyl


R.T.: 8.636 min
Delta R.T.: -0.004 min
Response: 99499
Conc: 0.06 ng/ml

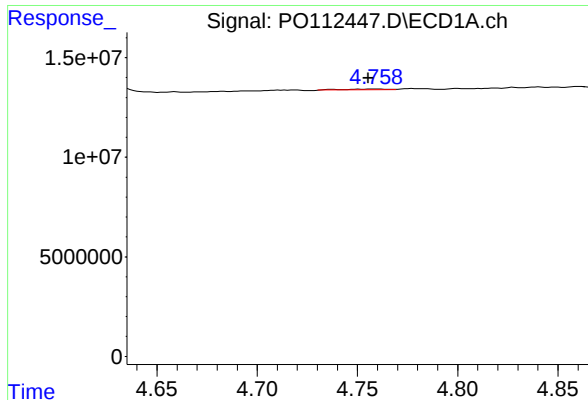

#3 AR-1016-1


R.T.: 4.758 min
Delta R.T.: 0.003 min
Response: 512596
Conc: 1.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

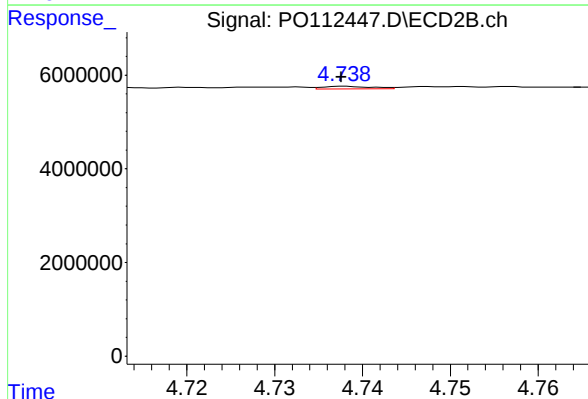


#3 AR-1016-1

R.T.: 4.738 min
Delta R.T.: 0.000 min
Response: 211473
Conc: 1.21 ng/ml

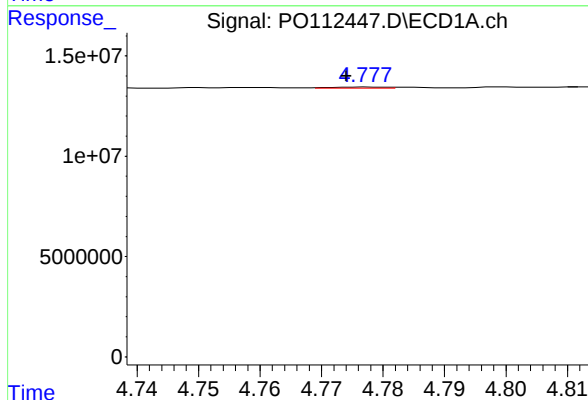


#4 AR-1016-2

R.T.: 4.777 min
Delta R.T.: 0.003 min
Response: 303839
Conc: 0.75 ng/ml

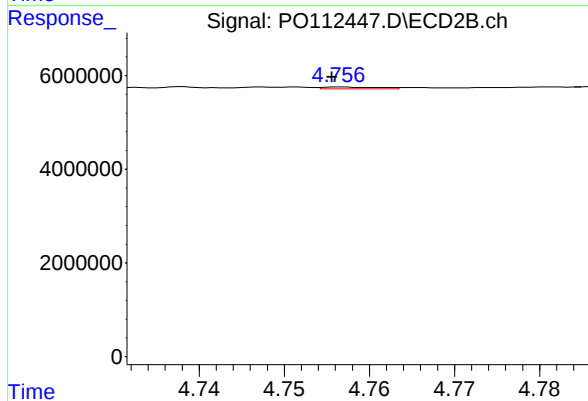

#4 AR-1016-2


R.T.: 4.757 min
Delta R.T.: 0.001 min
Response: 174741
Conc: 0.67 ng/ml

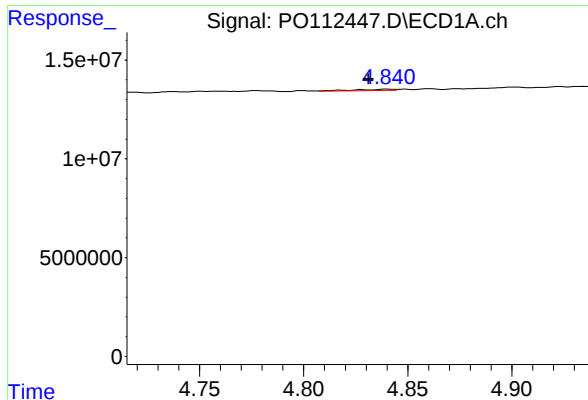

#5 AR-1016-3


R.T.: 4.840 min
Delta R.T.: 0.009 min
Response: 783736
Conc: 3.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

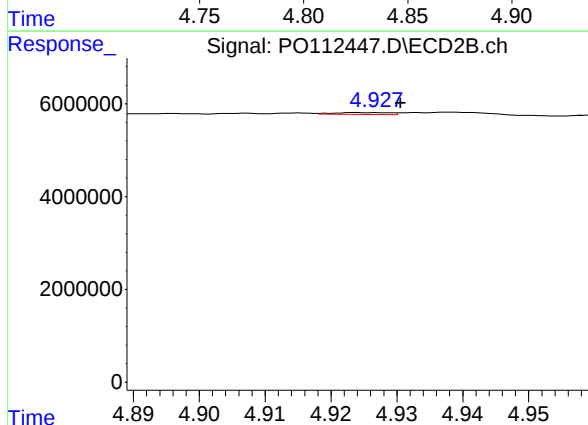


#5 AR-1016-3

R.T.: 4.924 min
Delta R.T.: -0.007 min
Response: 245799
Conc: 1.81 ng/ml

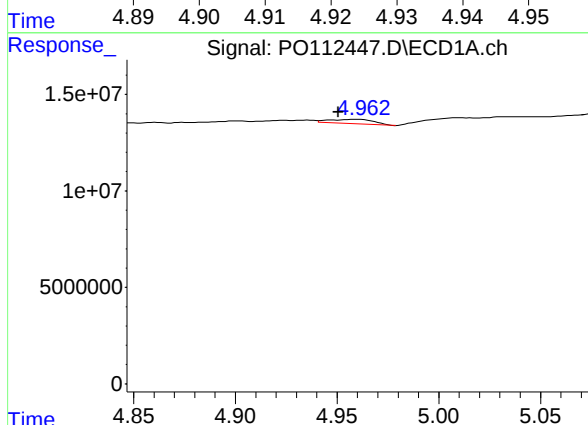


#6 AR-1016-4

R.T.: 4.960 min
Delta R.T.: 0.010 min
Response: 3409355
Conc: 16.09 ng/ml

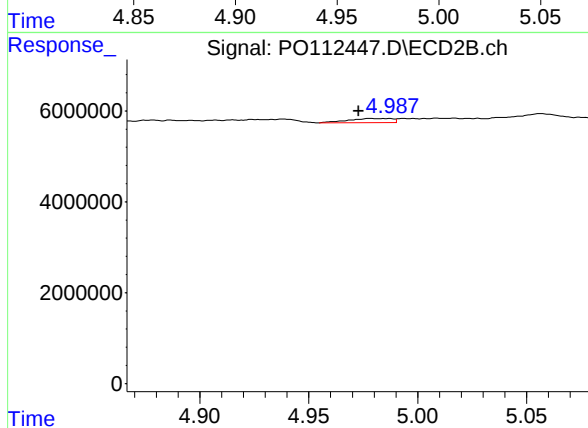

#6 AR-1016-4


R.T.: 4.978 min
Delta R.T.: 0.005 min
Response: 1275763
Conc: 11.48 ng/ml

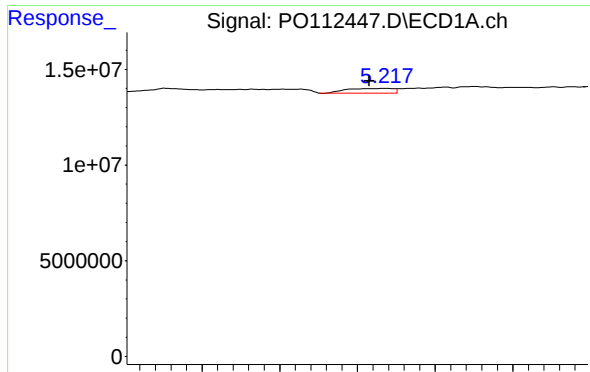

#7 AR-1016-5


R.T.: 5.218 min
Delta R.T.: 0.010 min
Response: 5056651
Conc: 23.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

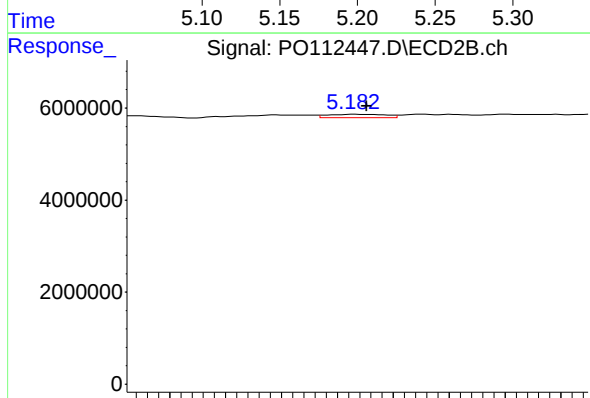


#7 AR-1016-5

R.T.: 5.183 min
Delta R.T.: -0.002 min
Response: 540796
Conc: 3.77 ng/ml

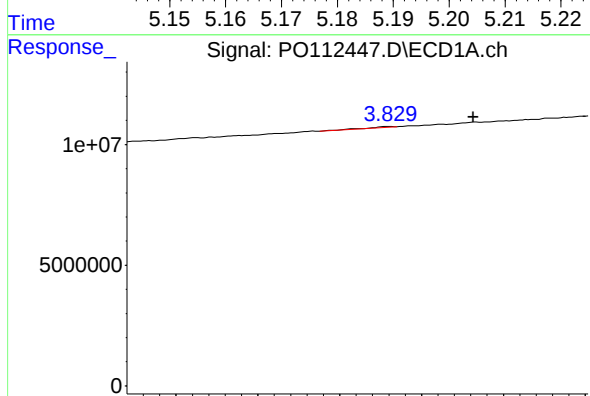


#8 AR-1221-1

R.T.: 3.830 min
Delta R.T.: -0.052 min
Response: 299361
Conc: 3.10 ng/ml

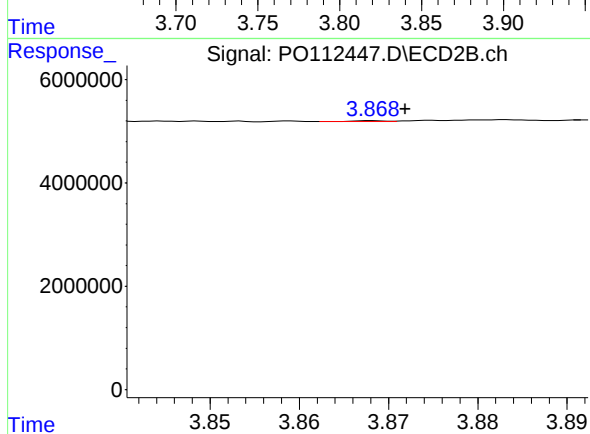

#8 AR-1221-1


R.T.: 3.868 min
Delta R.T.: -0.004 min
Response: 38267
Conc: 0.57 ng/ml

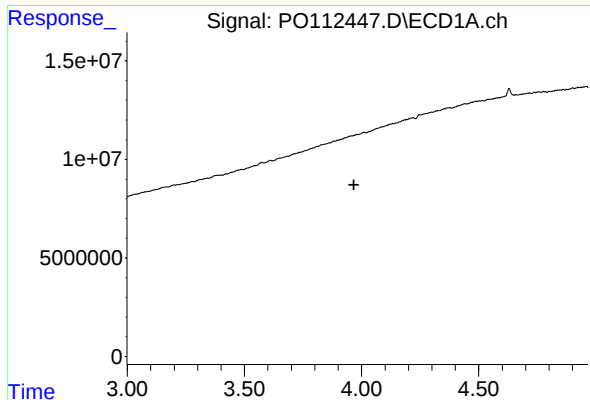

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 3.967 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

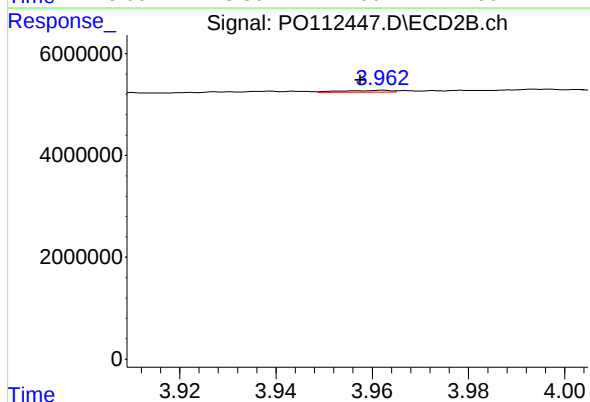


#9 AR-1221-2

R.T.: 3.962 min
Delta R.T.: 0.005 min
Response: 248584
Conc: 4.90 ng/ml

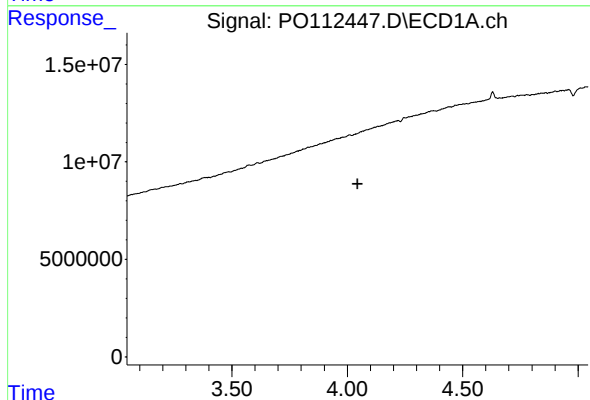


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 4.044 min
Response: 0
Conc: N.D.

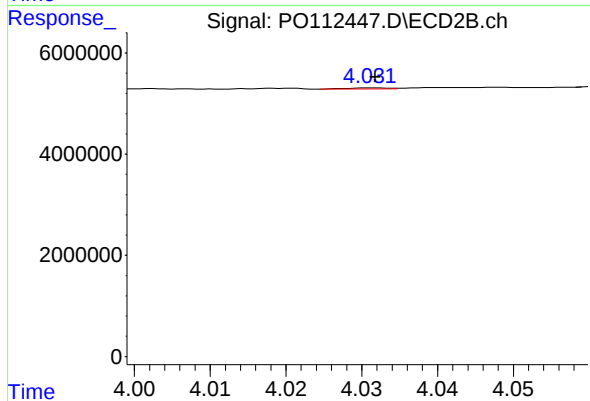

#10 AR-1221-3


R.T.: 4.031 min
Delta R.T.: 0.000 min
Response: 83310
Conc: 0.53 ng/ml

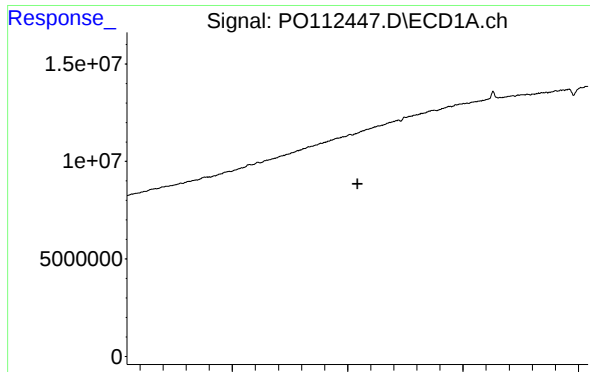

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

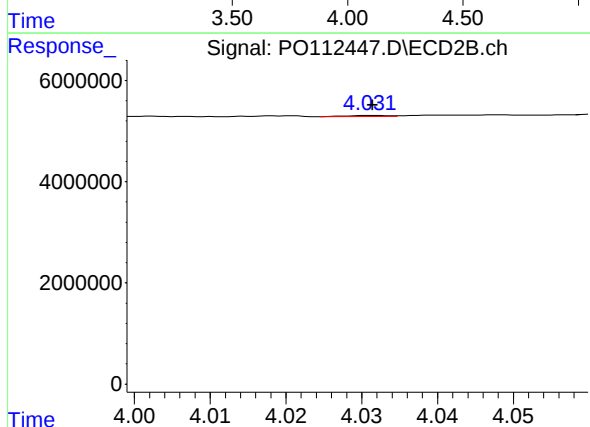


#11 AR-1232-1

R.T.: 4.031 min
Delta R.T.: 0.000 min
Response: 83310
Conc: 0.66 ng/ml

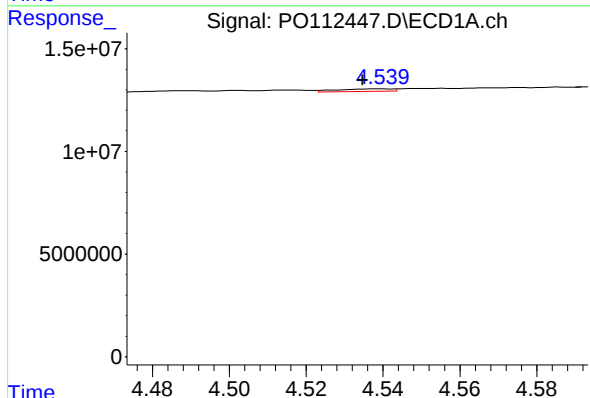


#12 AR-1232-2

R.T.: 4.540 min
Delta R.T.: 0.005 min
Response: 1272252
Conc: 11.82 ng/ml

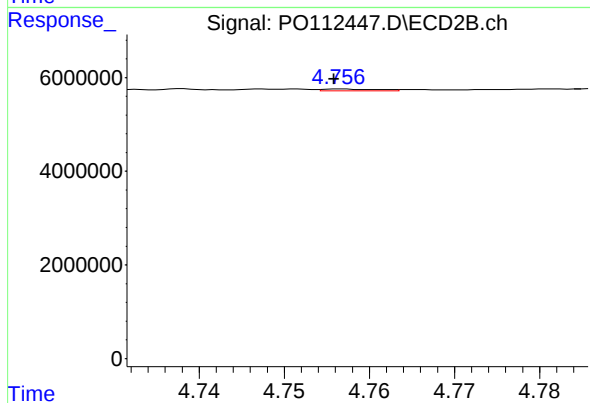

#12 AR-1232-2


R.T.: 4.757 min
Delta R.T.: 0.000 min
Response: 174741
Conc: 1.33 ng/ml

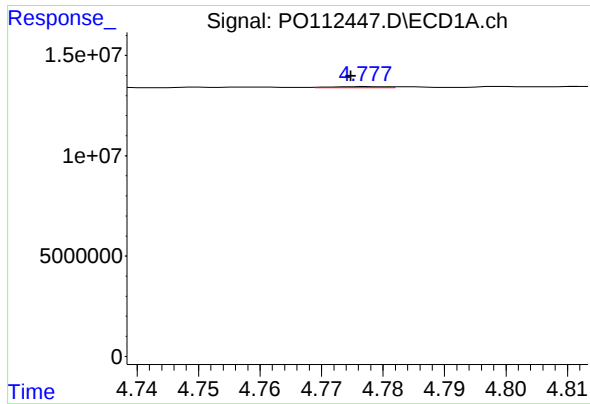

#13 AR-1232-3


R.T.: 4.777 min
Delta R.T.: 0.002 min
Response: 303839
Conc: 1.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

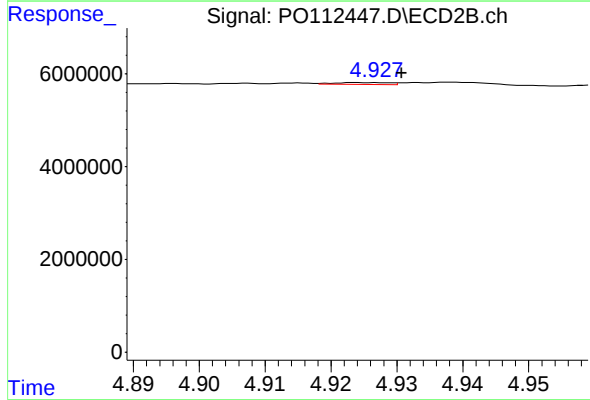


#13 AR-1232-3

R.T.: 4.924 min
Delta R.T.: -0.007 min
Response: 245799
Conc: 3.66 ng/ml

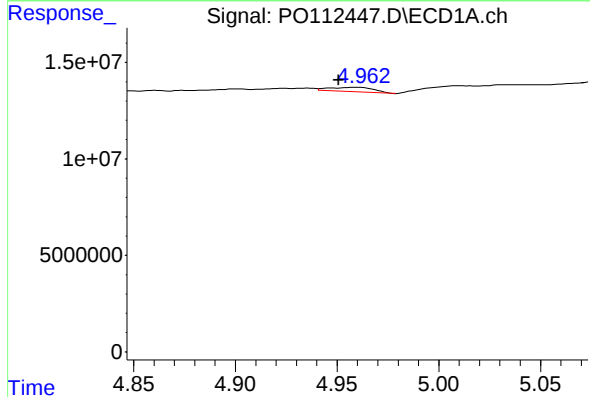


#14 AR-1232-4

R.T.: 4.960 min
Delta R.T.: 0.010 min
Response: 3409355
Conc: 32.55 ng/ml

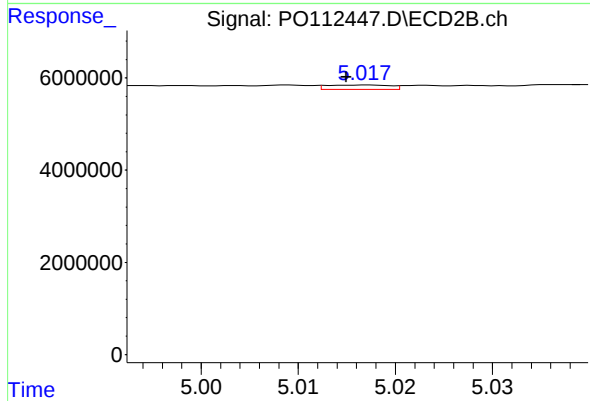

#14 AR-1232-4


R.T.: 5.017 min
Delta R.T.: 0.002 min
Response: 419225
Conc: 7.01 ng/ml

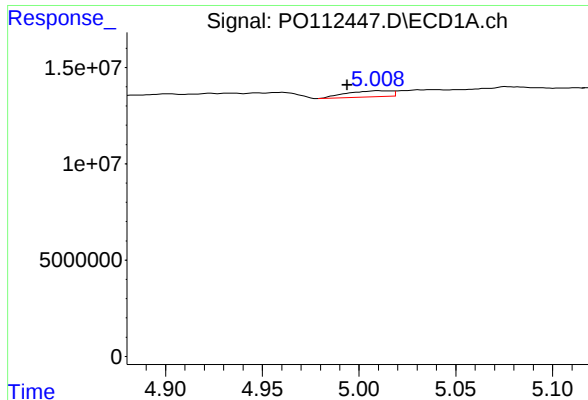

#15 AR-1232-5


R.T.: 5.010 min
Delta R.T.: 0.016 min
Response: 4963111
Conc: 73.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

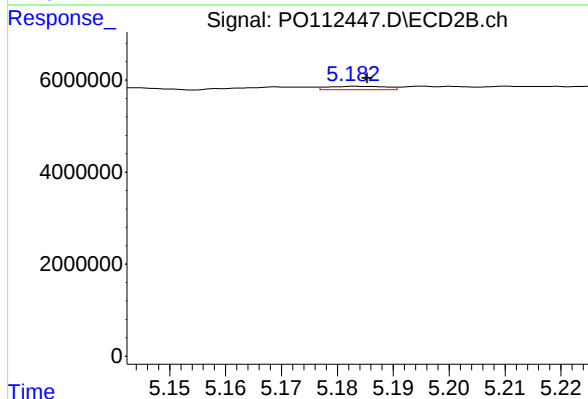


#15 AR-1232-5

R.T.: 5.183 min
Delta R.T.: -0.002 min
Response: 540796
Conc: 8.29 ng/ml

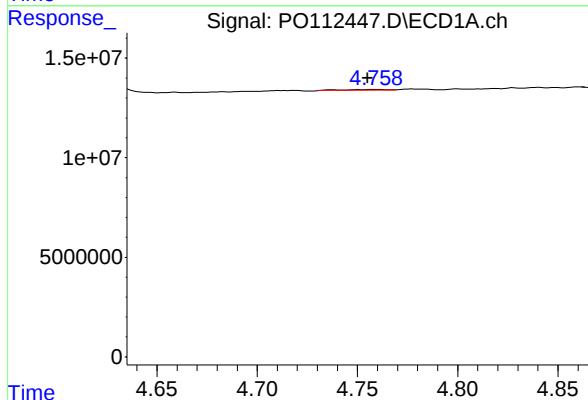


#16 AR-1242-1

R.T.: 4.758 min
Delta R.T.: 0.003 min
Response: 512596
Conc: 2.07 ng/ml

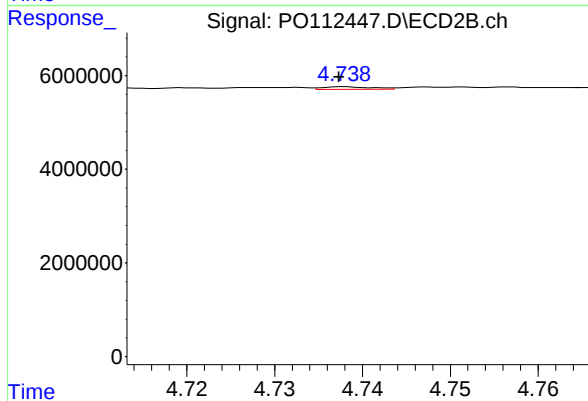

#16 AR-1242-1


R.T.: 4.738 min
Delta R.T.: 0.000 min
Response: 211473
Conc: 1.34 ng/ml

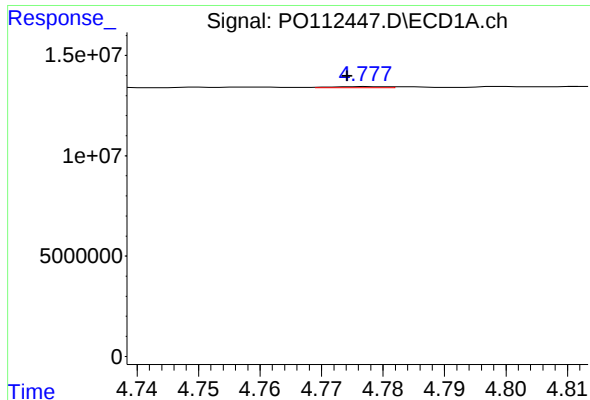

#17 AR-1242-2


R.T.: 4.777 min
Delta R.T.: 0.003 min
Response: 303839
Conc: 0.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

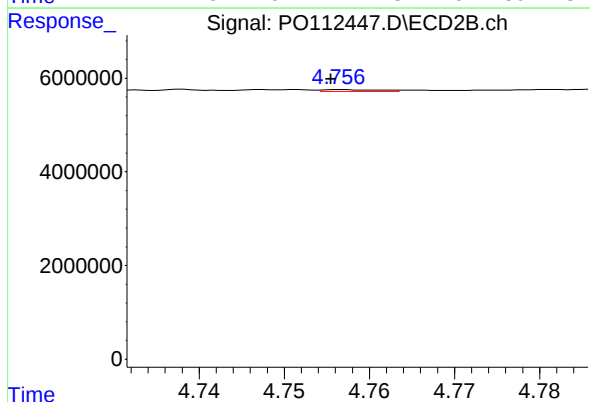


#17 AR-1242-2

R.T.: 4.757 min
Delta R.T.: 0.001 min
Response: 174741
Conc: 0.75 ng/ml

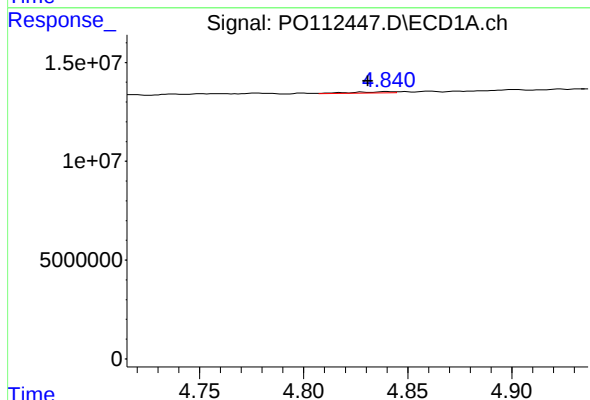


#18 AR-1242-3

R.T.: 4.840 min
Delta R.T.: 0.009 min
Response: 783736
Conc: 3.31 ng/ml

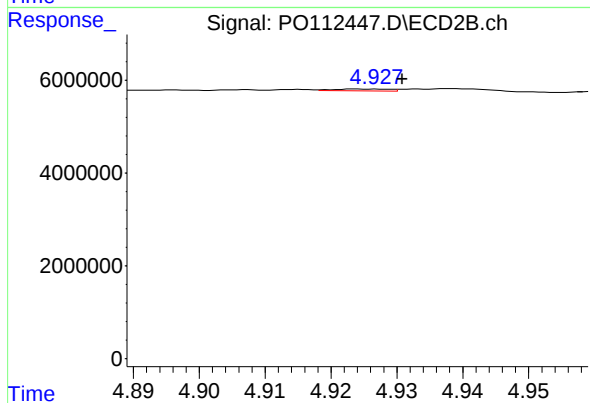

#18 AR-1242-3


R.T.: 4.924 min
Delta R.T.: -0.007 min
Response: 245799
Conc: 2.03 ng/ml

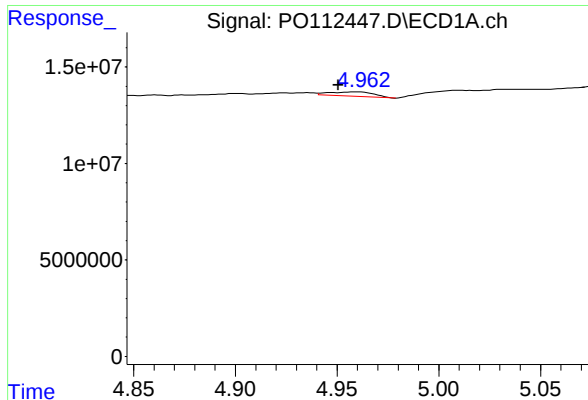

#19 AR-1242-4


R.T.: 4.960 min
Delta R.T.: 0.010 min
Response: 3409355
Conc: 17.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

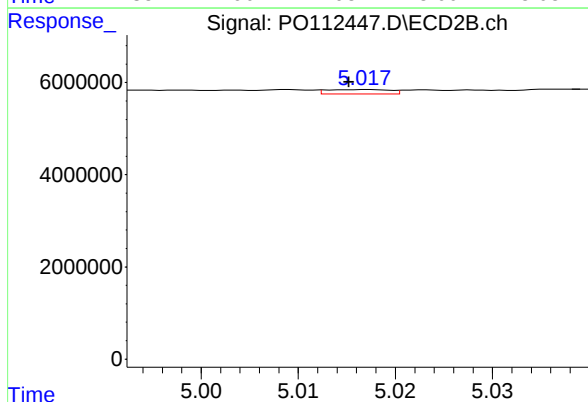


#19 AR-1242-4

R.T.: 5.017 min
Delta R.T.: 0.002 min
Response: 419225
Conc: 3.42 ng/ml

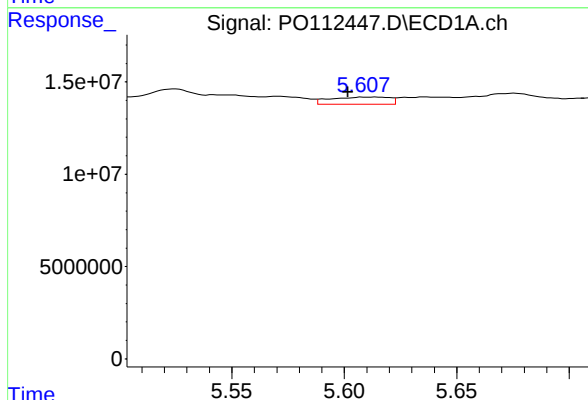


#20 AR-1242-5

R.T.: 5.614 min
Delta R.T.: 0.013 min
Response: 7124997
Conc: 33.31 ng/ml

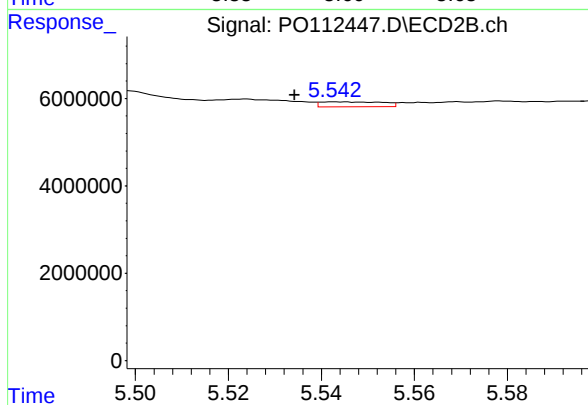

#20 AR-1242-5


R.T.: 5.543 min
Delta R.T.: 0.008 min
Response: 1056460
Conc: 6.56 ng/ml

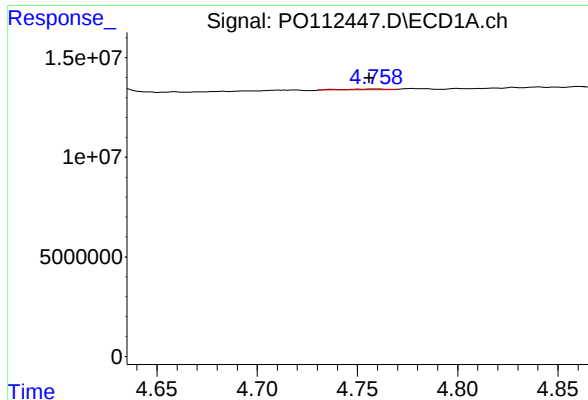

#21 AR-1248-1


R.T.: 4.758 min
Delta R.T.: 0.003 min
Response: 512596
Conc: 2.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

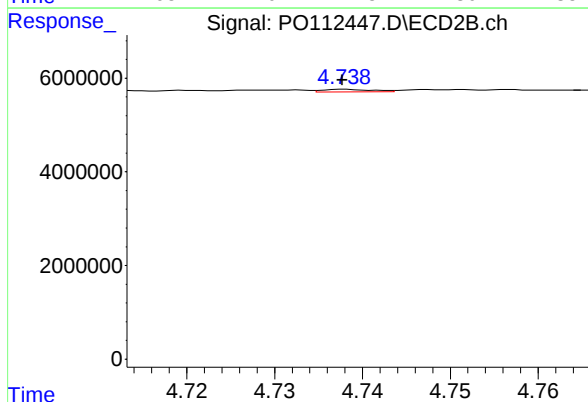


#21 AR-1248-1

R.T.: 4.738 min
Delta R.T.: 0.000 min
Response: 211473
Conc: 1.74 ng/ml

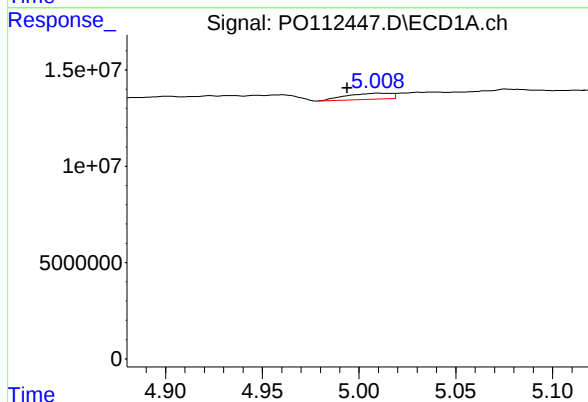


#22 AR-1248-2

R.T.: 5.010 min
Delta R.T.: 0.016 min
Response: 4963111
Conc: 19.45 ng/ml

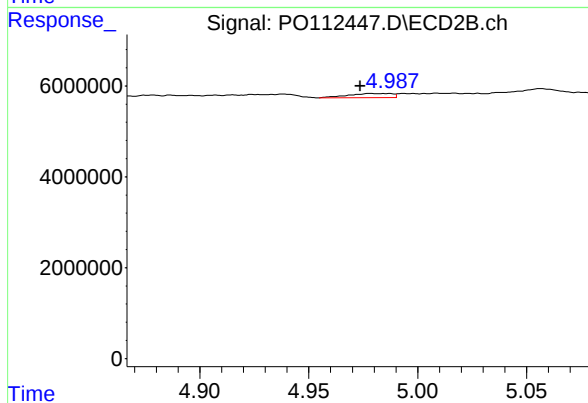

#22 AR-1248-2


R.T.: 4.978 min
Delta R.T.: 0.005 min
Response: 1275763
Conc: 7.54 ng/ml

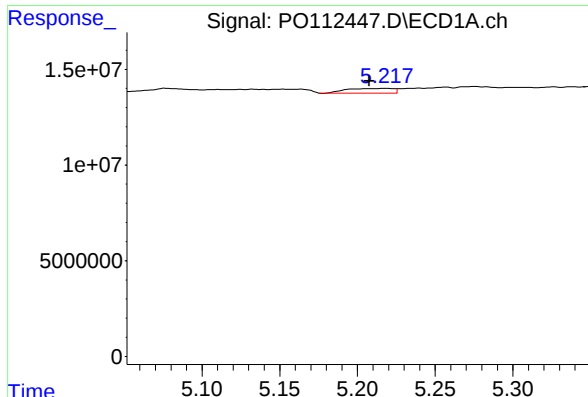

#23 AR-1248-3


R.T.: 5.218 min
Delta R.T.: 0.010 min
Response: 5056651
Conc: 14.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

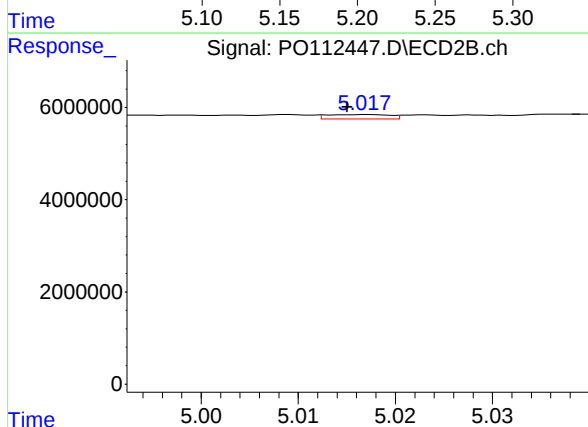


#23 AR-1248-3

R.T.: 5.017 min
Delta R.T.: 0.002 min
Response: 419225
Conc: 2.36 ng/ml

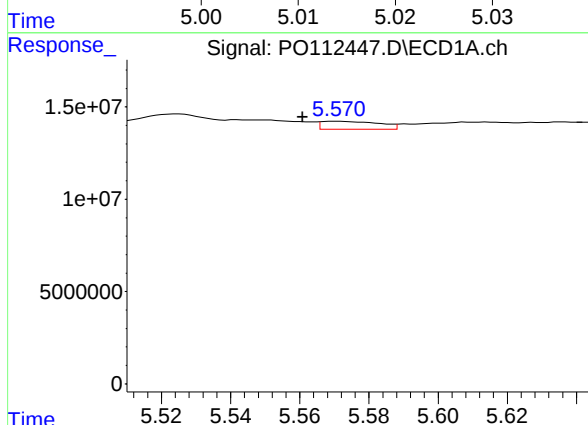


#24 AR-1248-4

R.T.: 5.571 min
Delta R.T.: 0.010 min
Response: 5015131
Conc: 9.87 ng/ml

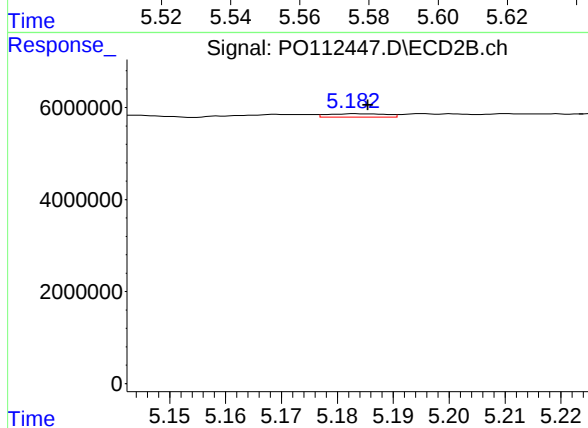

#24 AR-1248-4


R.T.: 5.183 min
Delta R.T.: -0.002 min
Response: 540796
Conc: 2.60 ng/ml

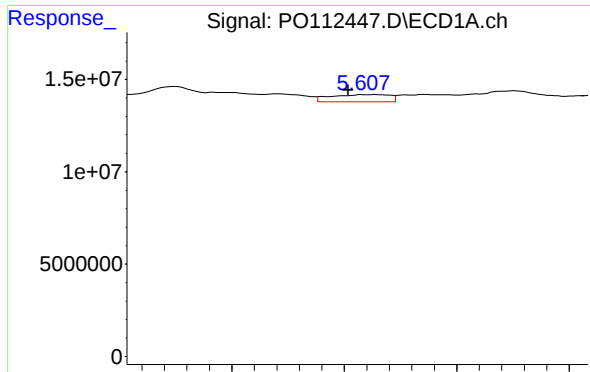

#25 AR-1248-5


R.T.: 5.614 min
Delta R.T.: 0.013 min
Response: 7124997
Conc: 20.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

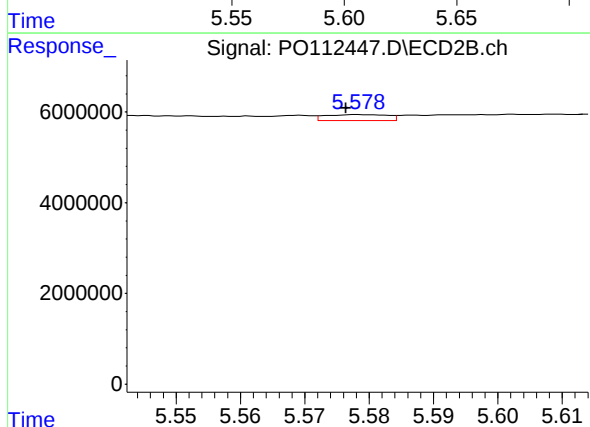


#25 AR-1248-5

R.T.: 5.578 min
Delta R.T.: 0.002 min
Response: 877829
Conc: 4.09 ng/ml

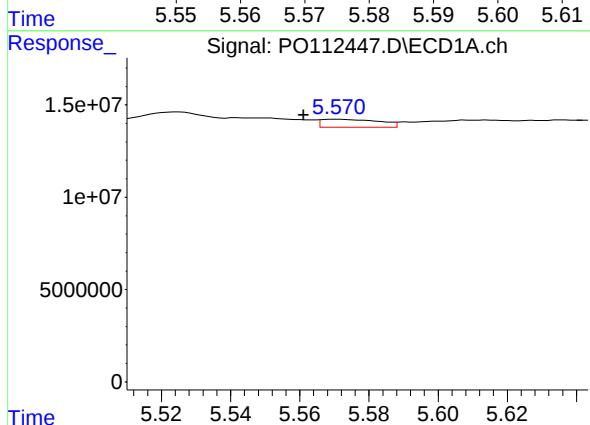


#26 AR-1254-1

R.T.: 5.571 min
Delta R.T.: 0.010 min
Response: 5015131
Conc: 9.14 ng/ml

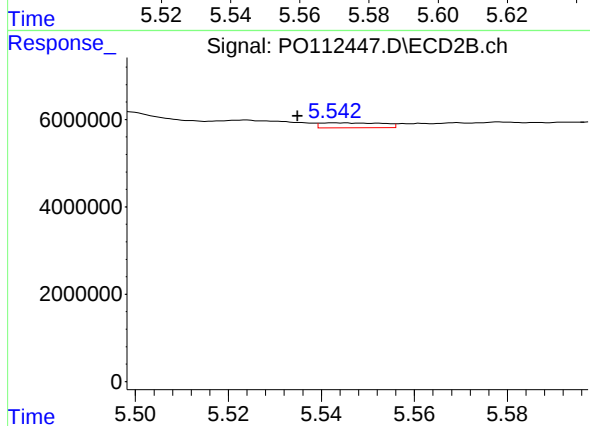

#26 AR-1254-1


R.T.: 5.543 min
Delta R.T.: 0.008 min
Response: 1056460
Conc: 3.21 ng/ml

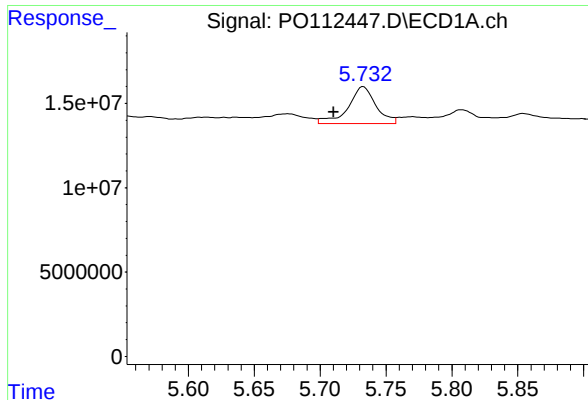

#27 AR-1254-2


R.T.: 5.733 min
Delta R.T.: 0.022 min
Response: 32146463
Conc: 66.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

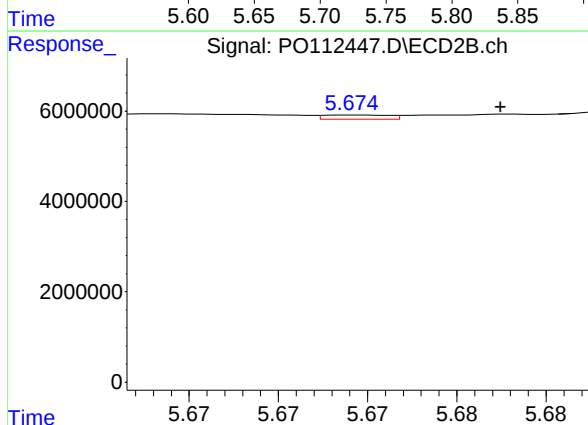


#27 AR-1254-2

R.T.: 5.675 min
Delta R.T.: -0.008 min
Response: 246716
Conc: 0.85 ng/ml

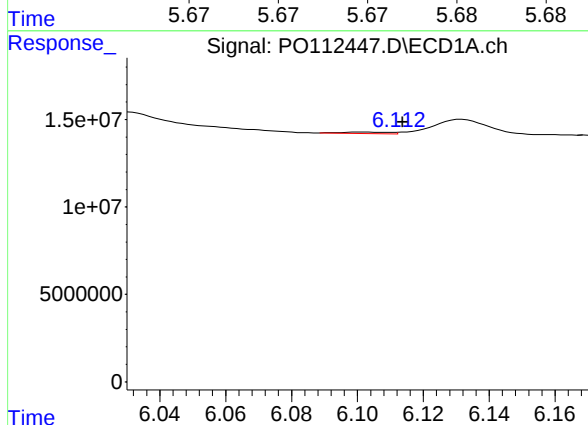


#28 AR-1254-3

R.T.: 6.101 min
Delta R.T.: -0.013 min
Response: 832937
Conc: 1.12 ng/ml

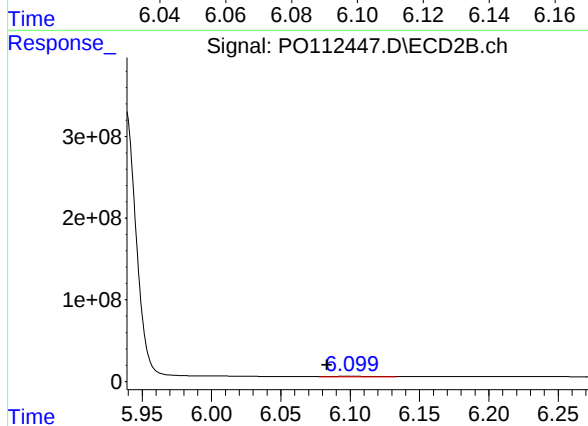

#28 AR-1254-3


R.T.: 6.100 min
Delta R.T.: 0.016 min
Response: 13802808
Conc: 32.29 ng/ml

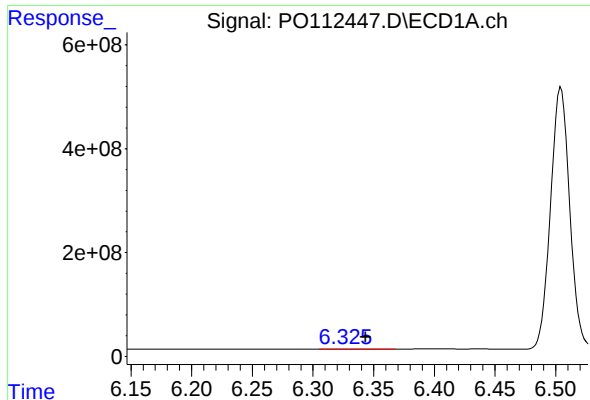

#29 AR-1254-4


R.T.: 6.325 min
Delta R.T.: -0.018 min
Response: 4423459
Conc: 8.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

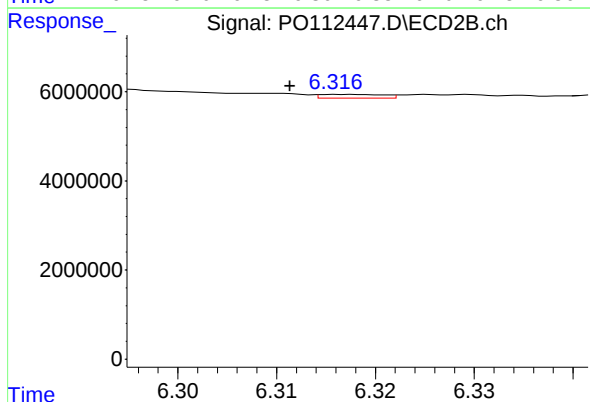


#29 AR-1254-4

R.T.: 6.317 min
Delta R.T.: 0.005 min
Response: 387388
Conc: 1.42 ng/ml

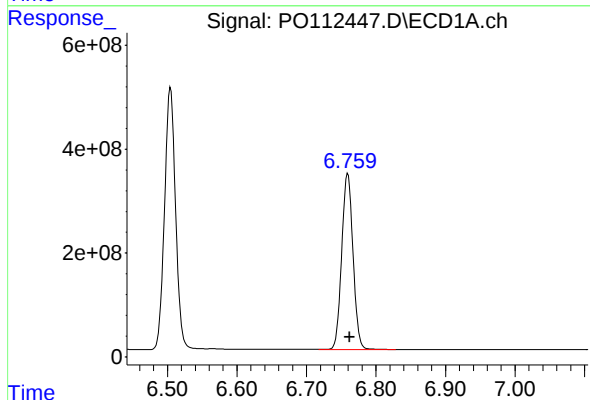


#30 AR-1254-5

R.T.: 6.759 min
Delta R.T.: -0.003 min
Response: 3823728738
Conc: 5402.09 ng/ml

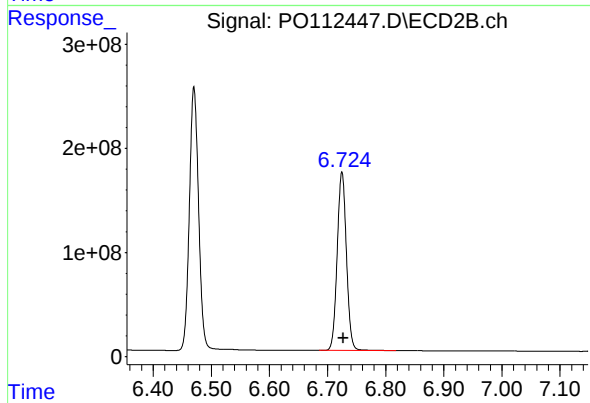

#30 AR-1254-5


R.T.: 6.725 min
Delta R.T.: -0.002 min
Response: 1892376626
Conc: 5665.46 ng/ml

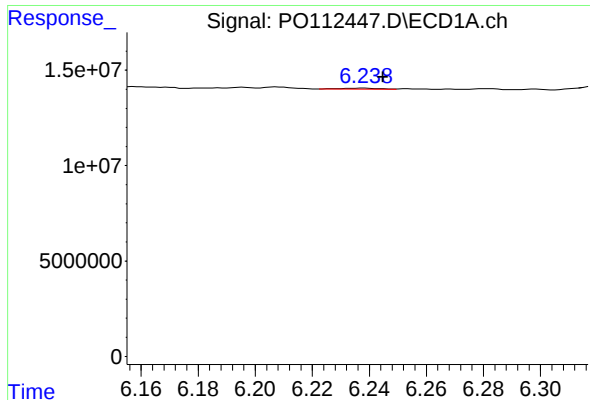

#31 AR-1260-1


R.T.: 6.238 min
Delta R.T.: -0.006 min
Response: 459345
Conc: 1.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

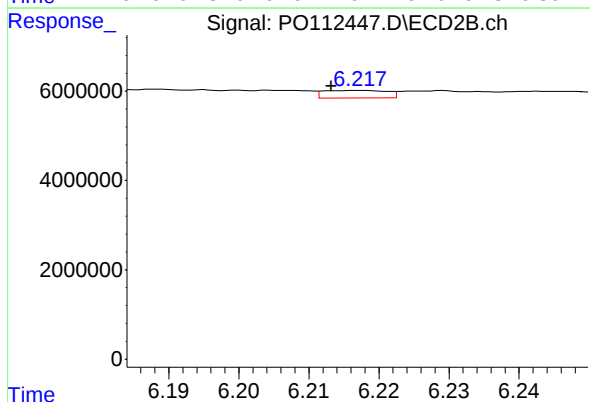


#31 AR-1260-1

R.T.: 6.217 min
Delta R.T.: 0.004 min
Response: 1056241
Conc: 4.25 ng/ml

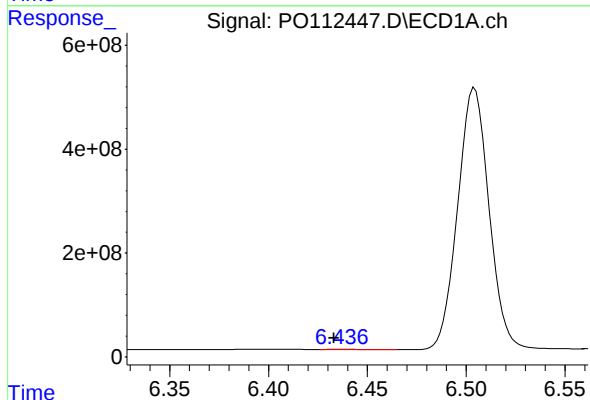


#32 AR-1260-2

R.T.: 6.437 min
Delta R.T.: 0.003 min
Response: 7089425
Conc: 10.31 ng/ml

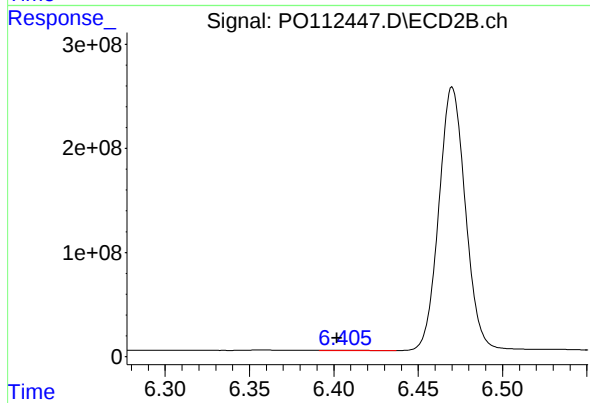

#32 AR-1260-2


R.T.: 6.405 min
Delta R.T.: 0.003 min
Response: 4079277
Conc: 12.38 ng/ml

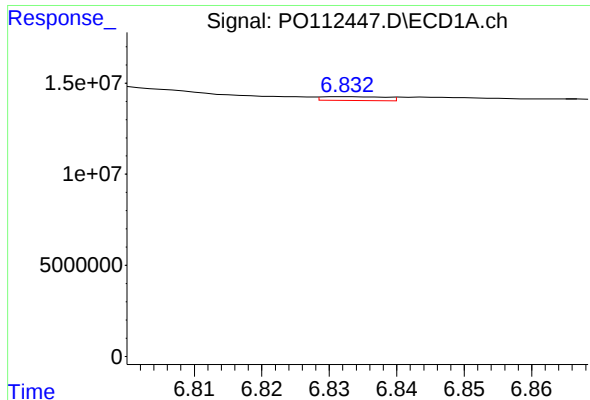

#33 AR-1260-3


R.T.: 6.833 min
Delta R.T.: 0.033 min
Response: 1377006
Conc: 2.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

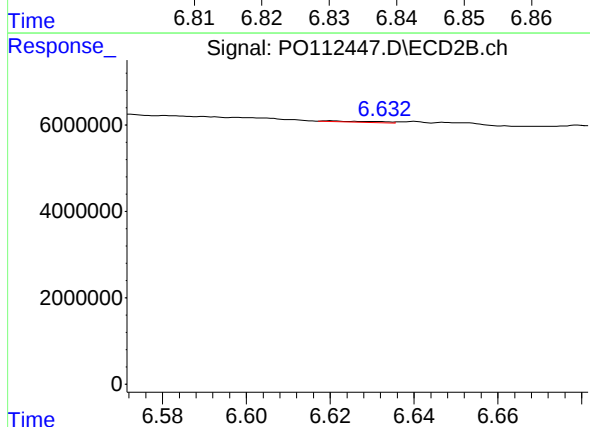


#33 AR-1260-3

R.T.: 6.620 min
Delta R.T.: 0.067 min
Response: 186154
Conc: 0.72 ng/ml

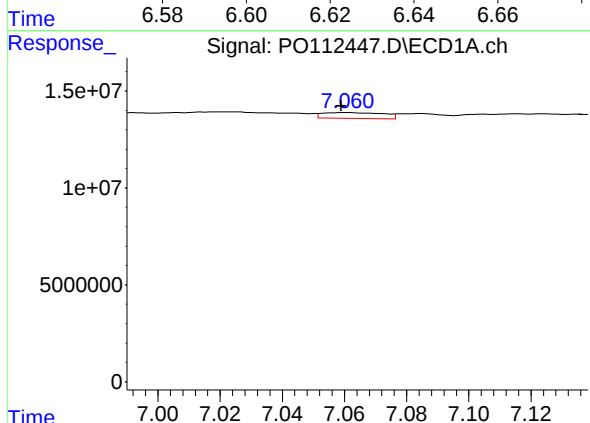


#34 AR-1260-4

R.T.: 7.061 min
Delta R.T.: 0.002 min
Response: 4158557
Conc: 9.22 ng/ml

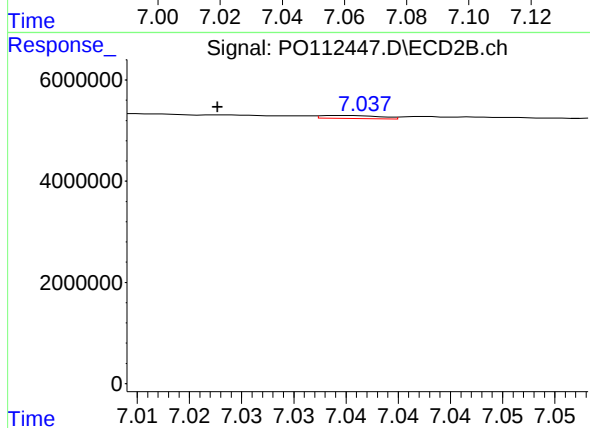

#34 AR-1260-4


R.T.: 7.035 min
Delta R.T.: 0.012 min
Response: 227850
Conc: 1.19 ng/ml

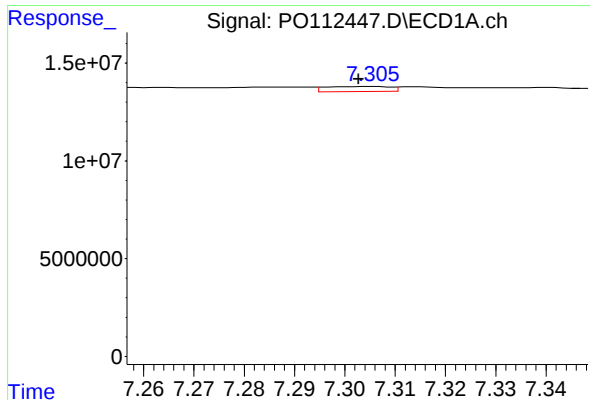

#35 AR-1260-5


R.T.: 7.306 min
Delta R.T.: 0.003 min
Response: 2280827
Conc: 1.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

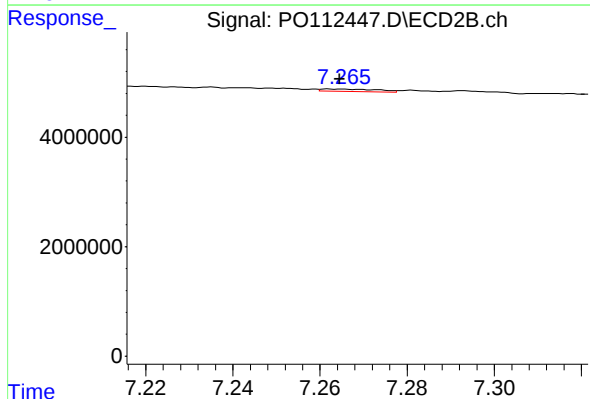


#35 AR-1260-5

R.T.: 7.262 min
Delta R.T.: -0.002 min
Response: 395290
Conc: 0.96 ng/ml

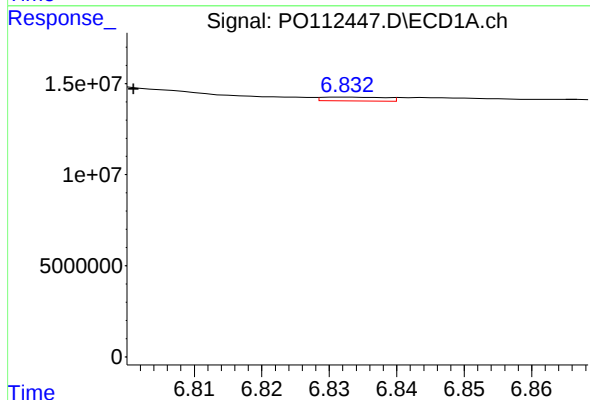


#36 AR-1262-1

R.T.: 6.833 min
Delta R.T.: 0.032 min
Response: 1377006
Conc: 1.48 ng/ml

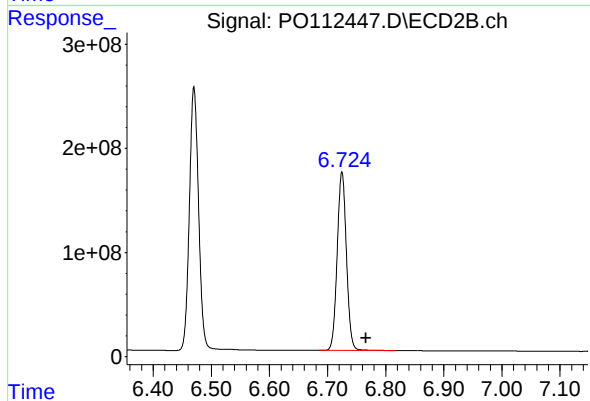

#36 AR-1262-1


R.T.: 6.725 min
Delta R.T.: -0.041 min
Response: 1892376626
Conc: 4561.83 ng/ml

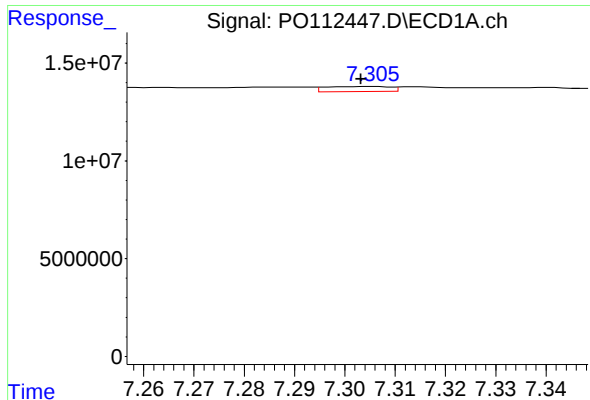

#37 AR-1262-2


R.T.: 7.306 min
Delta R.T.: 0.002 min
Response: 2280827
Conc: 1.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

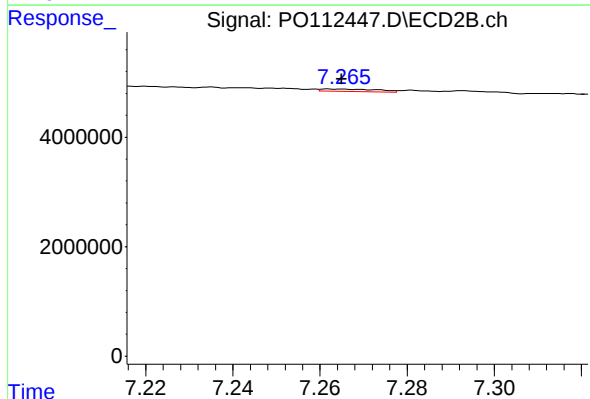


#37 AR-1262-2

R.T.: 7.262 min
Delta R.T.: -0.003 min
Response: 395290
Conc: 0.77 ng/ml

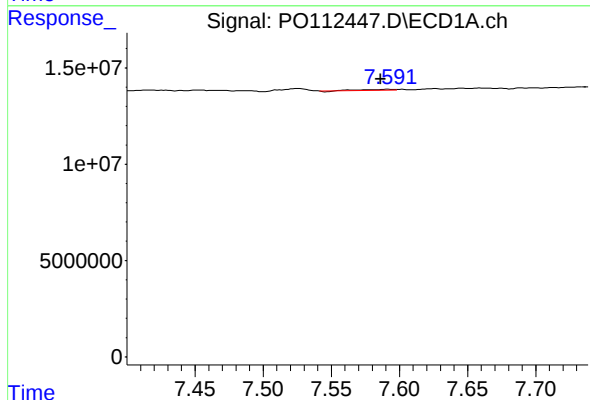


#38 AR-1262-3

R.T.: 7.592 min
Delta R.T.: 0.005 min
Response: 556382
Conc: 0.94 ng/ml

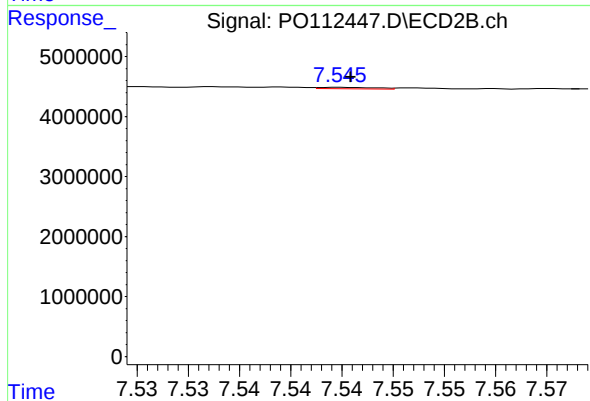

#38 AR-1262-3


R.T.: 7.544 min
Delta R.T.: -0.001 min
Response: 87646
Conc: 0.47 ng/ml

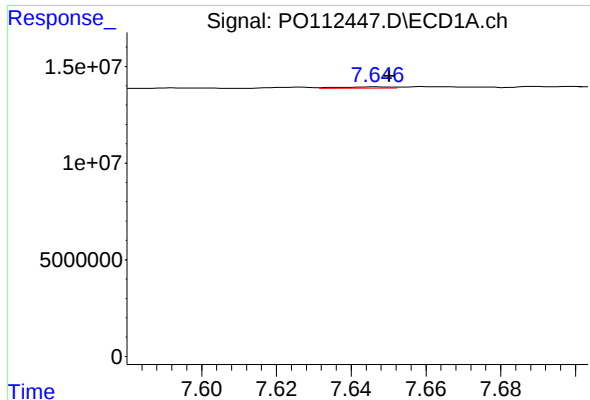

#39 AR-1262-4


R.T.: 7.647 min
Delta R.T.: -0.004 min
Response: 591400
Conc: 0.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

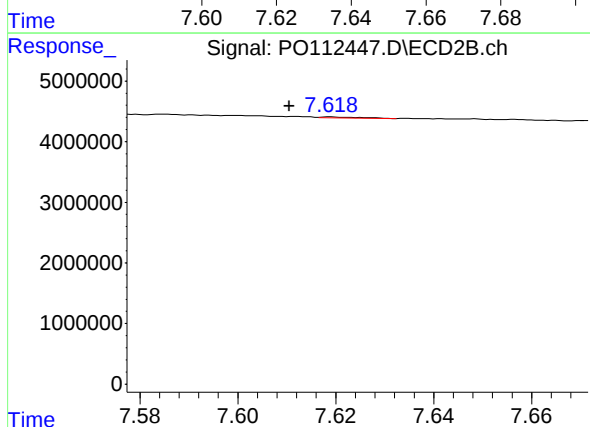


#39 AR-1262-4

R.T.: 7.619 min
Delta R.T.: 0.009 min
Response: 91132
Conc: 0.32 ng/ml

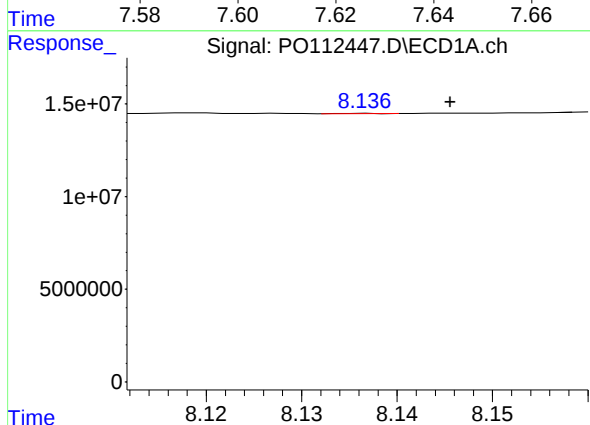


#40 AR-1262-5

R.T.: 8.137 min
Delta R.T.: -0.009 min
Response: 54490
Conc: 0.13 ng/ml

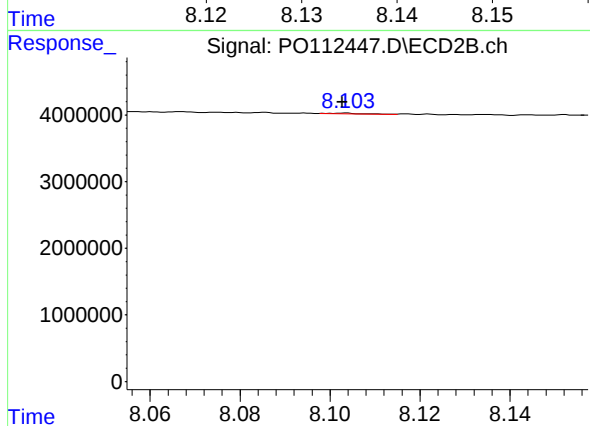

#40 AR-1262-5


R.T.: 8.104 min
Delta R.T.: 0.000 min
Response: 58456
Conc: 0.59 ng/ml

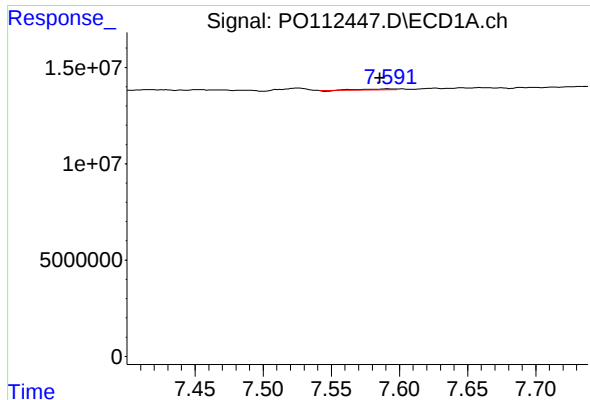

#41 AR-1268-1


R.T.: 7.592 min
Delta R.T.: 0.006 min
Response: 556382
Conc: 0.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

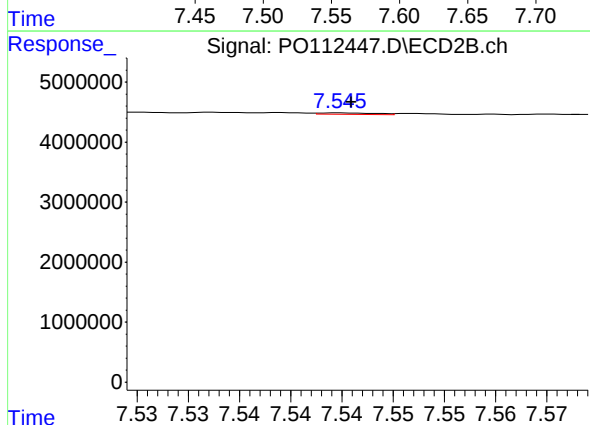


#41 AR-1268-1

R.T.: 7.544 min
Delta R.T.: -0.001 min
Response: 87646
Conc: 0.17 ng/ml

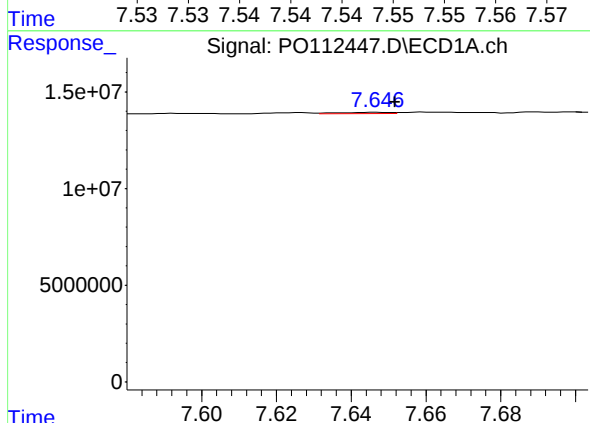


#42 AR-1268-2

R.T.: 7.647 min
Delta R.T.: -0.005 min
Response: 591400
Conc: 0.40 ng/ml

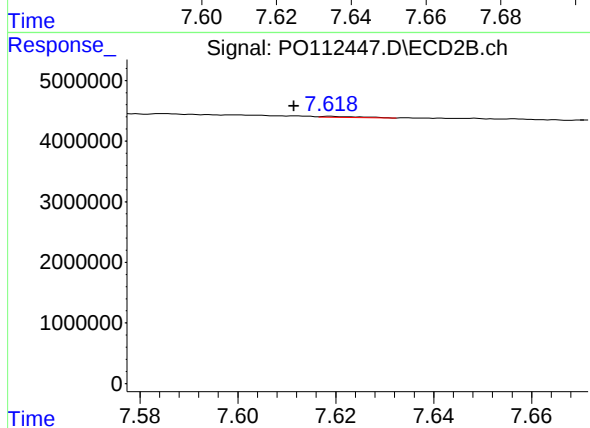

#42 AR-1268-2


R.T.: 7.619 min
Delta R.T.: 0.008 min
Response: 91132
Conc: 0.21 ng/ml

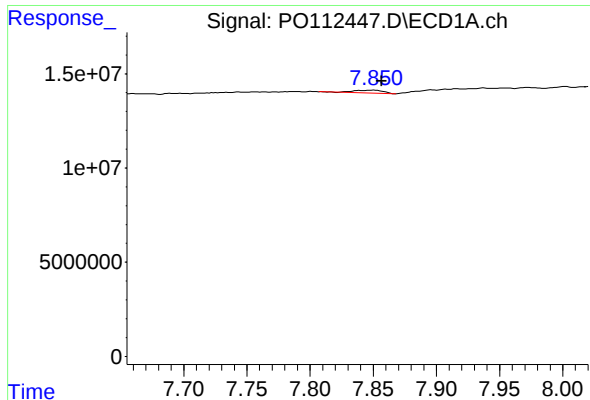

#43 AR-1268-3


R.T.: 7.851 min
Delta R.T.: -0.006 min
Response: 2507568
Conc: 2.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

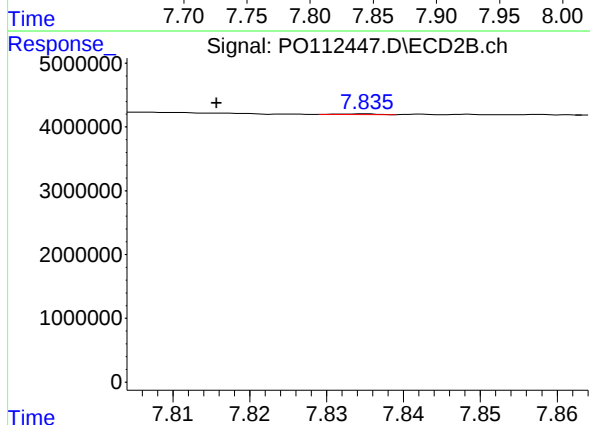


#43 AR-1268-3

R.T.: 7.835 min
Delta R.T.: 0.019 min
Response: 35708
Conc: 0.11 ng/ml

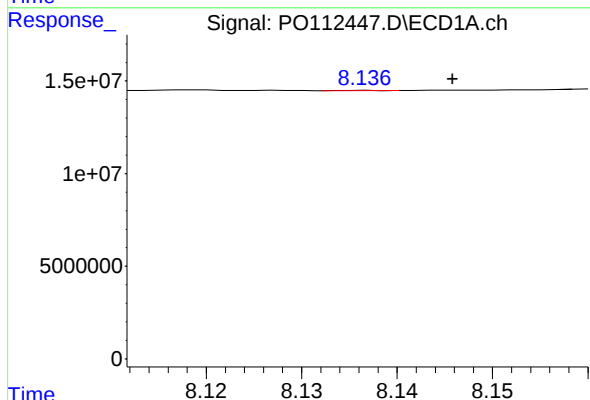


#44 AR-1268-4

R.T.: 8.137 min
Delta R.T.: -0.009 min
Response: 54490
Conc: 0.11 ng/ml

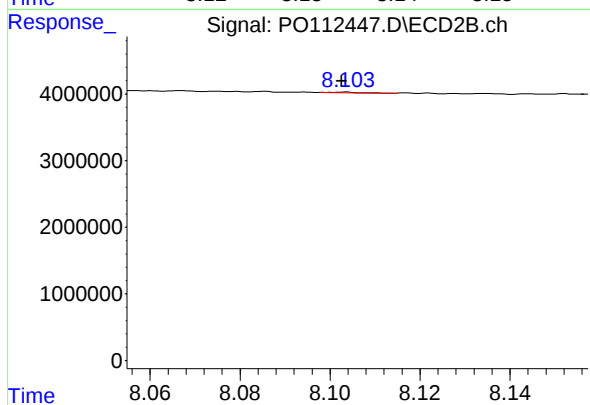

#44 AR-1268-4


R.T.: 8.104 min
Delta R.T.: 0.001 min
Response: 58456
Conc: 0.53 ng/ml

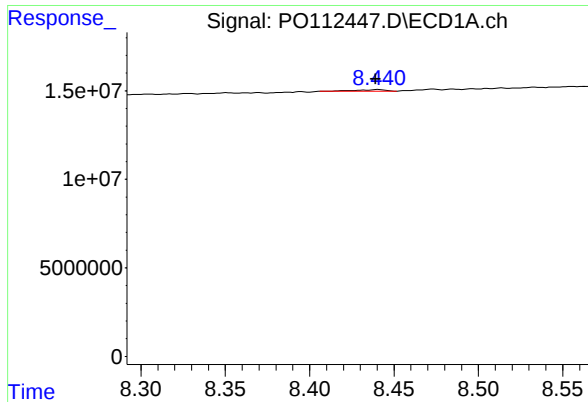

#45 AR-1268-5

R.T.: 8.440 min
Delta R.T.: 0.001 min
Response: 1143419
Conc: 0.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

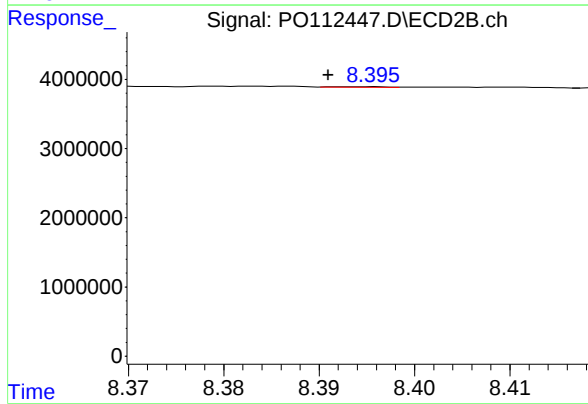

#45 AR-1268-5

R.T.: 8.395 min
Delta R.T.: 0.004 min
Response: 33716
Conc: 0.05 ng/ml