

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072418\
Data File : P0047089.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 12:54
Operator : SM/SJ
Sample : J4087-53
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ES-PILLAR-3-4

Manual Integrations
APPROVED

Sohil
7/25/2018 1:31:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 13:50:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.395	3.645	4310213	5056743	25.707	26.365
2) SA Decachlor...	10.082	8.650	3146248	2754343	28.740	29.990m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072418\
Data File : P0047089.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 12:54
Operator : SM/SJ
Sample : J4087-53
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ES-PILLAR-3-4


Manual Integrations
APPROVED

Sohil
7/25/2018 1:31:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 13:50:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

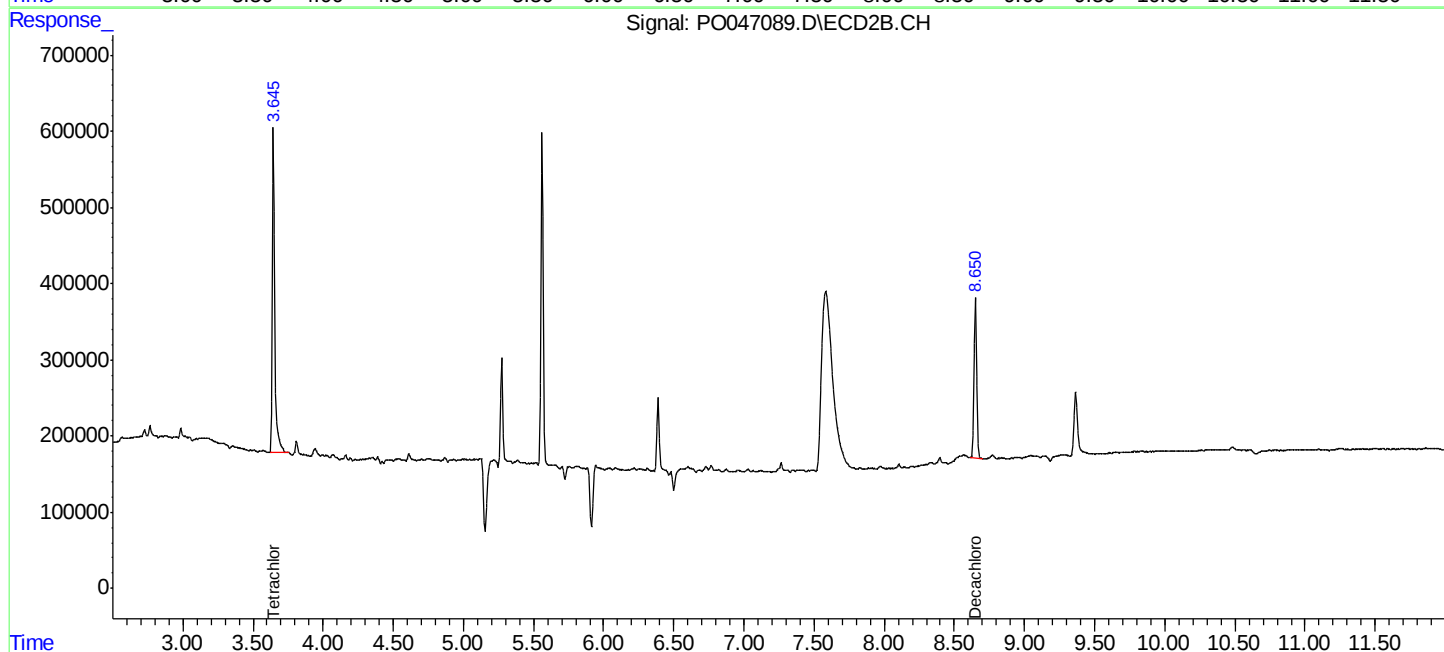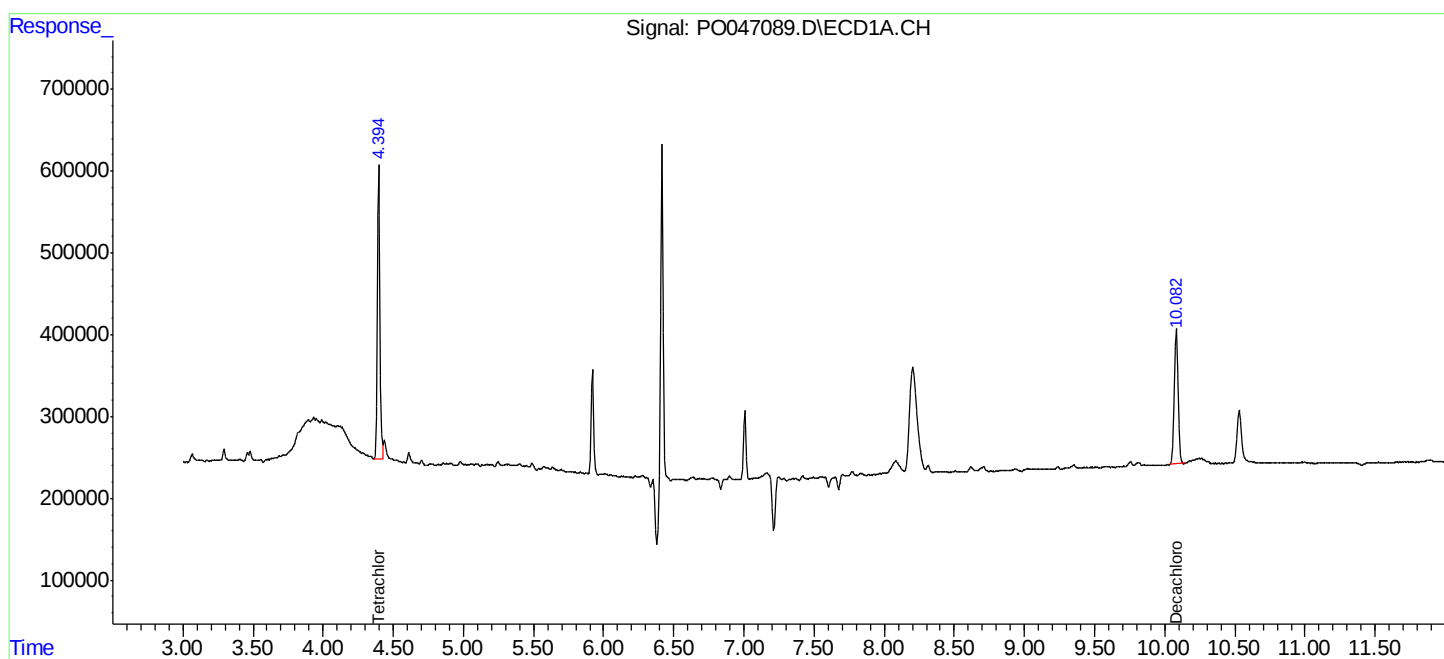

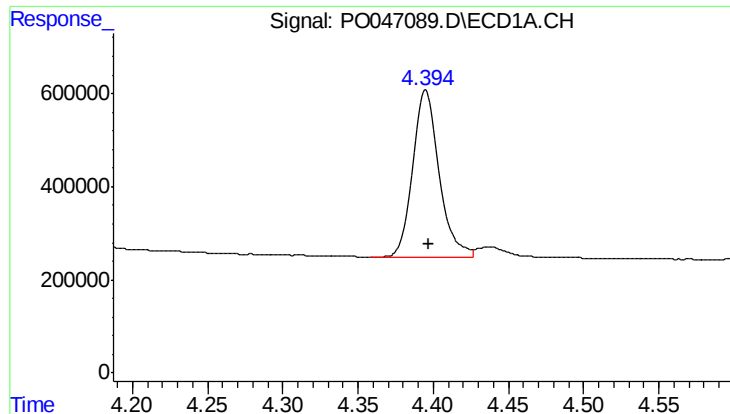


#1 Tetrachloro-m-xylene

R.T.: 4.395 min
Delta R.T.: -0.002 min
Response: 4310213
Conc: 25.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
ES-PILLAR-3-4


Manual Integrations
APPROVED

Sohil
7/25/2018 1:31:38 PM

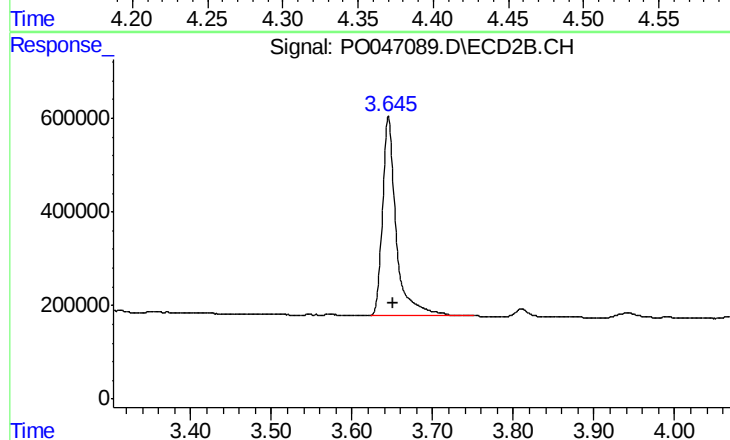


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.006 min
Response: 5056743
Conc: 26.37 ng/ml

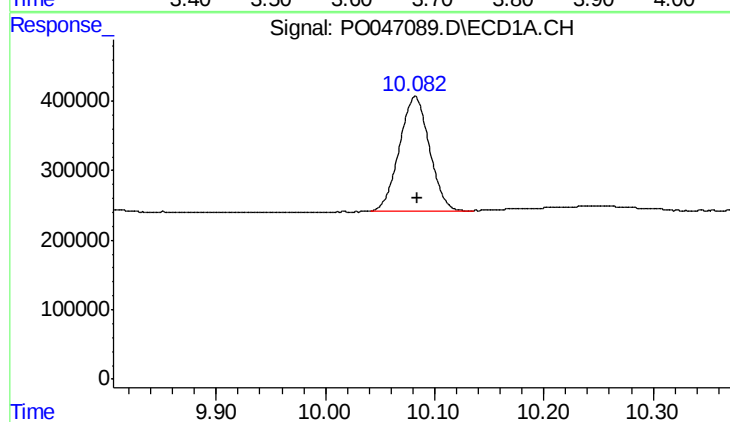

#2 Decachlorobiphenyl

R.T.: 10.082 min
Delta R.T.: -0.002 min
Response: 3146248
Conc: 28.74 ng/ml

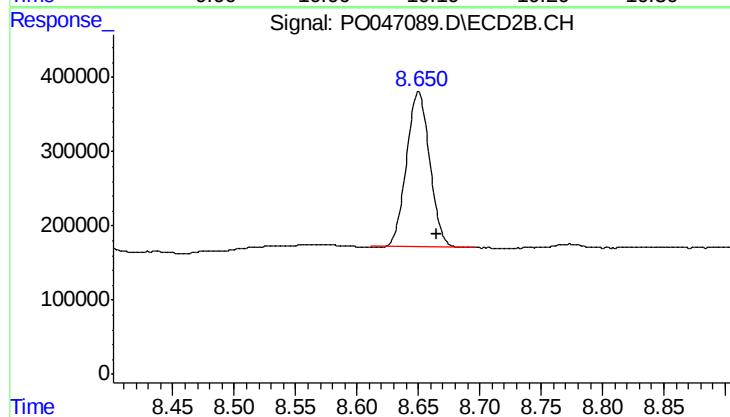

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: -0.015 min
Response: 2754343
Conc: 29.99 ng/ml m