

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072420\
 Data File : P0069944.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jul 2020 19:59
 Operator : DD\AJ
 Sample : L3216-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 02:10:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 23 02:12:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.378	3.555	622918	648160	18.146	17.982
2)	SA Decachlor...	10.021	8.757	1002706	978901	18.766	19.193
Target Compounds							
9)	L2 AR-1221-2	4.724	0.000	15062	0	49.699	N.D. #
10)	L2 AR-1221-3	4.815	3.989	25040	29673	24.863	28.512
11)	L3 AR-1232-1	4.815	3.989	25040	29673	30.044	34.104
20)	L4 AR-1242-5	6.630f	0.000	4637	0	4.036	N.D. #
24)	L5 AR-1248-4	6.616	0.000	6467	0	3.690	N.D. #
25)	L5 AR-1248-5	6.630f	0.000	4637	0	2.776	N.D. #
26)	L6 AR-1254-1	6.590	0.000	40348	0	22.862	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072420\
Data File : P0069944.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2020 19:59
Operator : DD\AJ
Sample : L3216-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 02:10:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 23 02:12:36 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

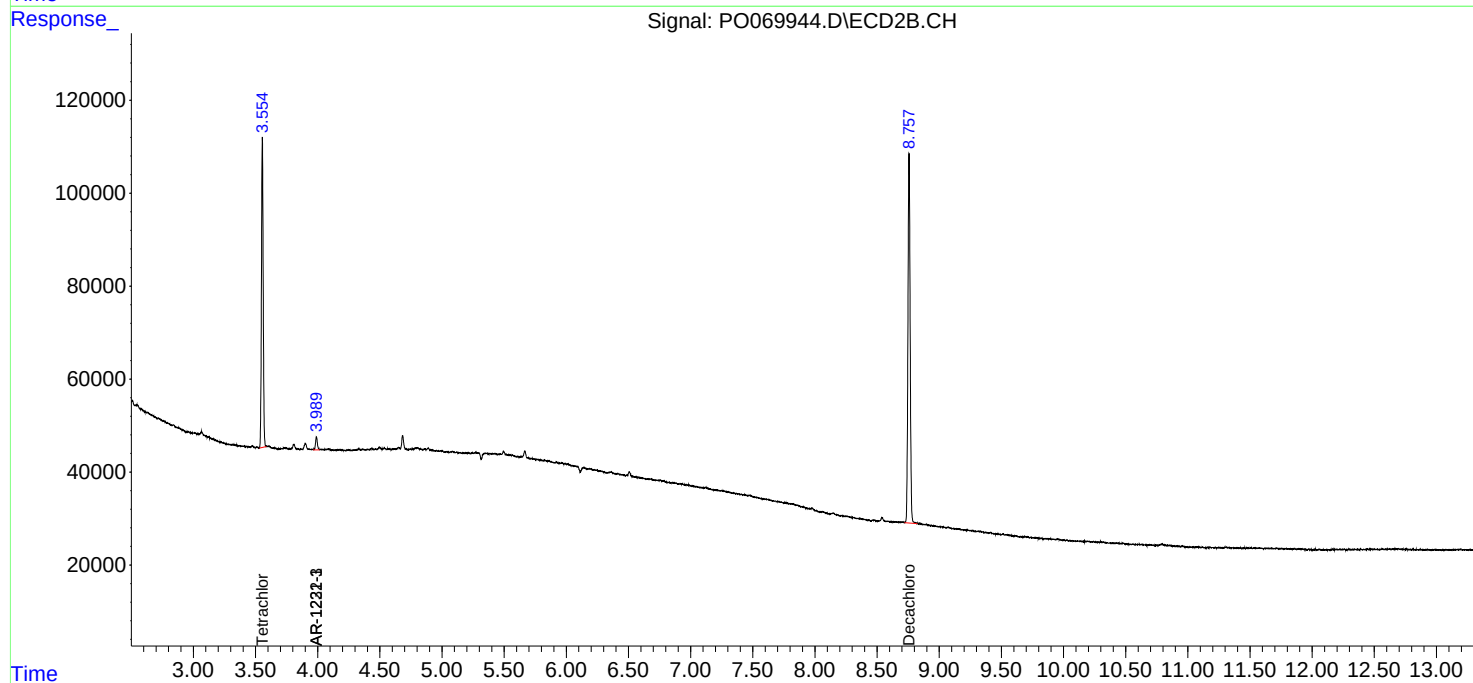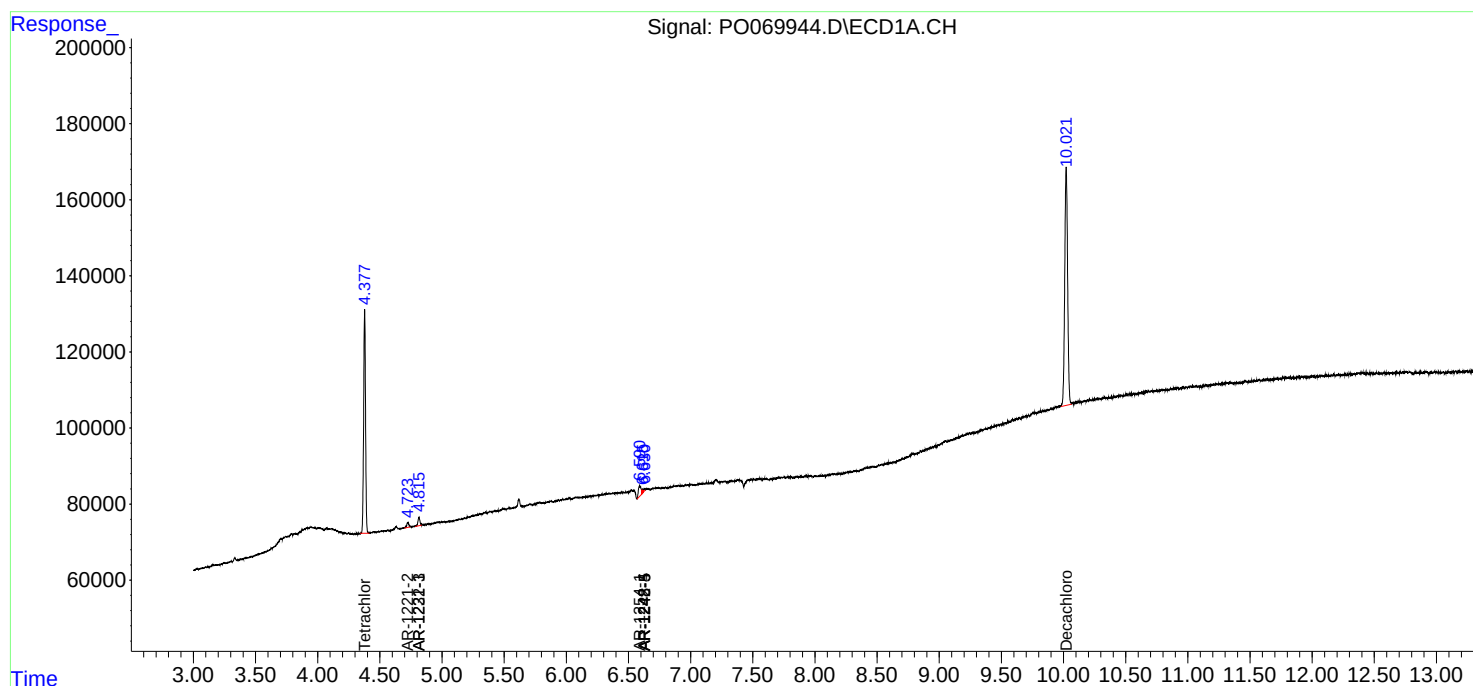


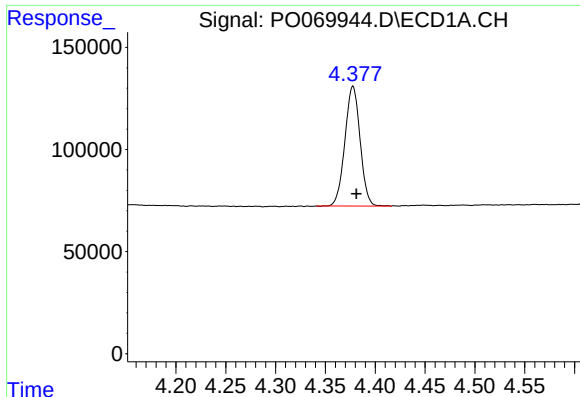

#1 Tetrachloro-m-xylene


R.T.: 4.378 min
Delta R.T.: -0.003 min
Response: 622918
Conc: 18.15 ng/ml

Instrument :
ECD_O
ClientSampleId :

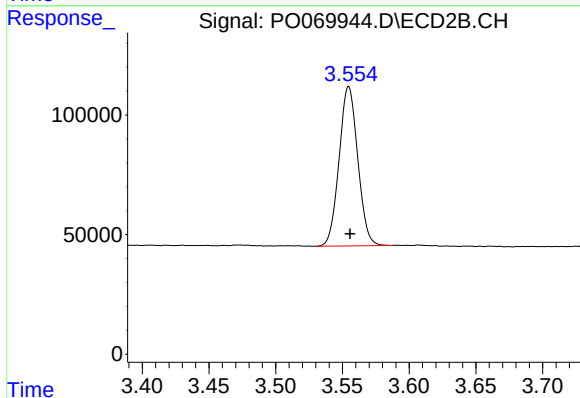


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 648160
Conc: 17.98 ng/ml

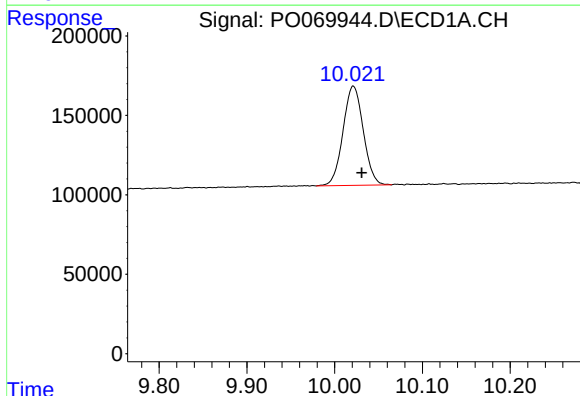


#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.010 min
Response: 1002706
Conc: 18.77 ng/ml

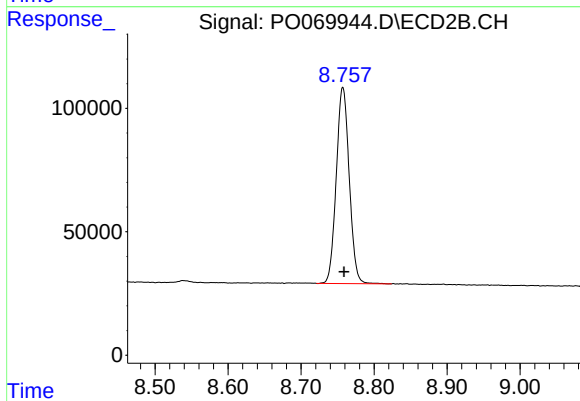

#2 Decachlorobiphenyl


R.T.: 8.757 min
Delta R.T.: -0.002 min
Response: 978901
Conc: 19.19 ng/ml

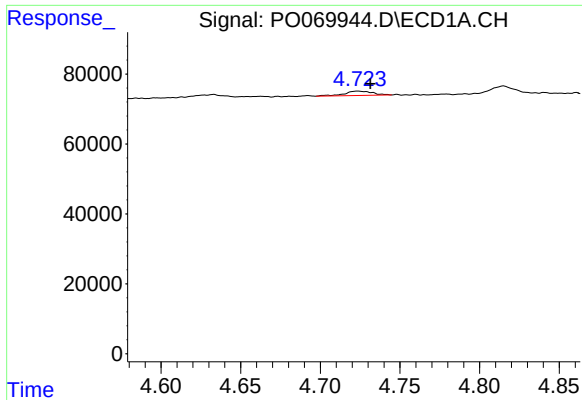

#9 AR-1221-2


R.T.: 4.724 min
Delta R.T.: -0.008 min
Response: 15062
Conc: 49.70 ng/ml

Instrument :
ECD_O
ClientSampleId :

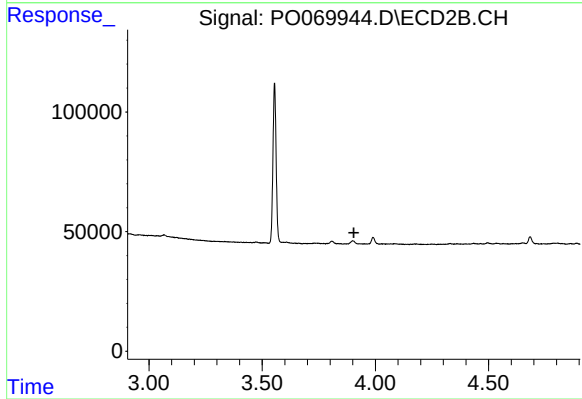


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.905 min
Response: 0
Conc: N.D.

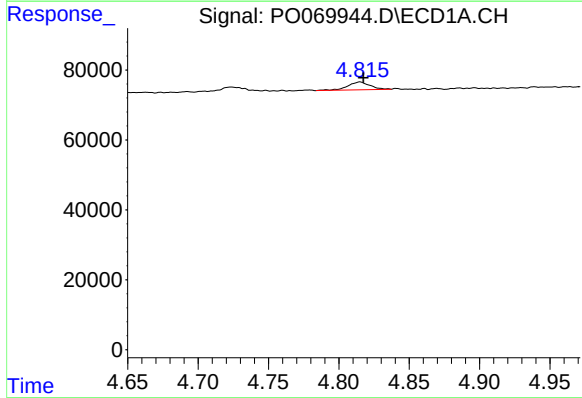


#10 AR-1221-3

R.T.: 4.815 min
Delta R.T.: -0.002 min
Response: 25040
Conc: 24.86 ng/ml

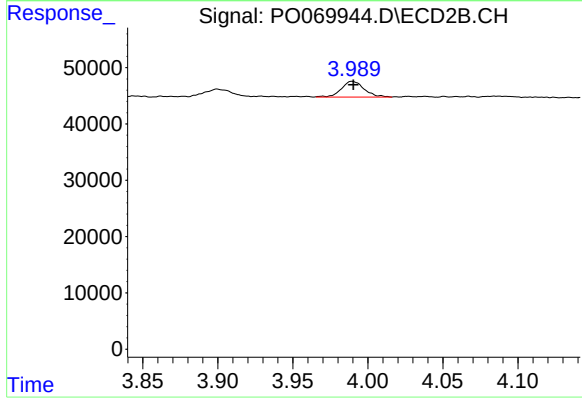

#10 AR-1221-3


R.T.: 3.989 min
Delta R.T.: 0.000 min
Response: 29673
Conc: 28.51 ng/ml

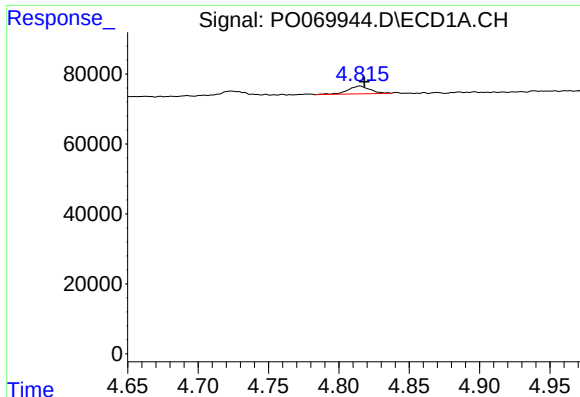

#11 AR-1232-1


R.T.: 4.815 min
Delta R.T.: -0.003 min
Response: 25040
Conc: 30.04 ng/ml

Instrument :
ECD_O
ClientSampleId :

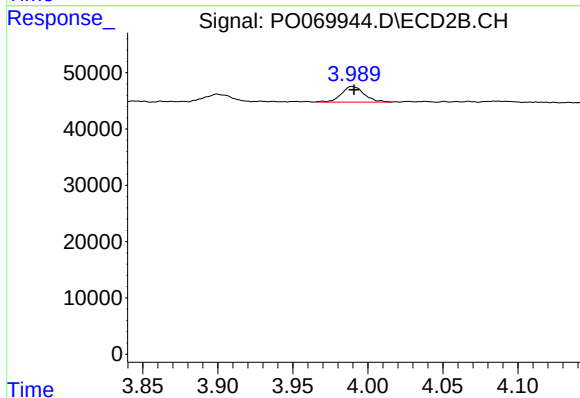


#11 AR-1232-1

R.T.: 3.989 min
Delta R.T.: -0.001 min
Response: 29673
Conc: 34.10 ng/ml

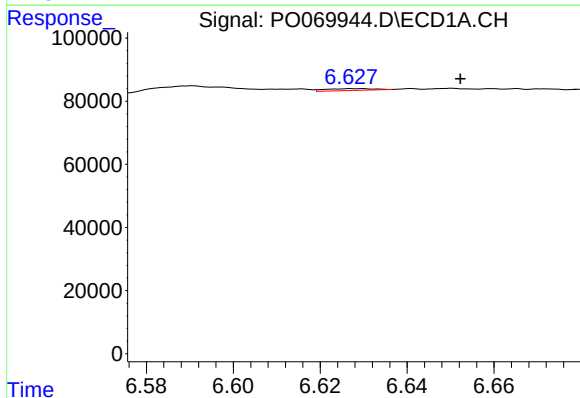


#20 AR-1242-5

R.T.: 6.630 min
Delta R.T.: -0.022 min
Response: 4637
Conc: 4.04 ng/ml

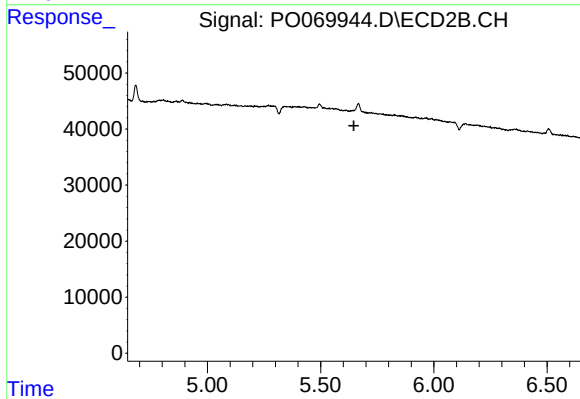

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 5.647 min
Response: 0
Conc: N.D.

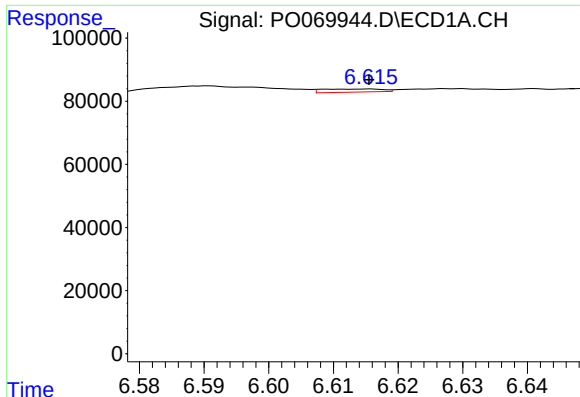

#24 AR-1248-4


R.T.: 6.616 min
Delta R.T.: 0.000 min
Response: 6467
Conc: 3.69 ng/ml

Instrument :
ECD_O
ClientSampleId :

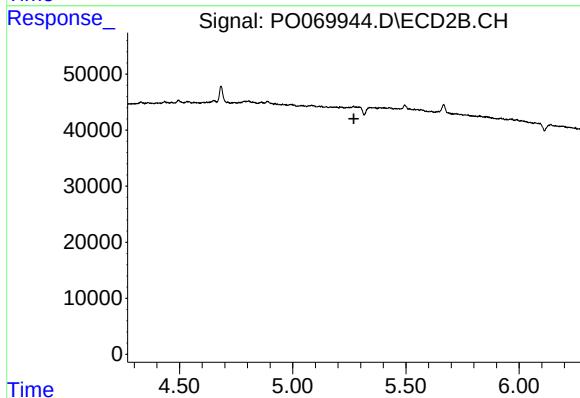


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.270 min
Response: 0
Conc: N.D.

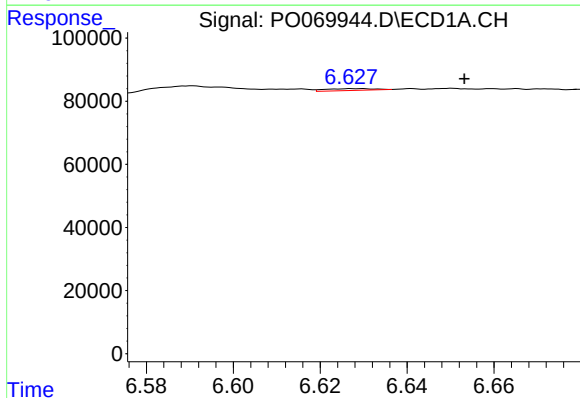


#25 AR-1248-5

R.T.: 6.630 min
Delta R.T.: -0.023 min
Response: 4637
Conc: 2.78 ng/ml

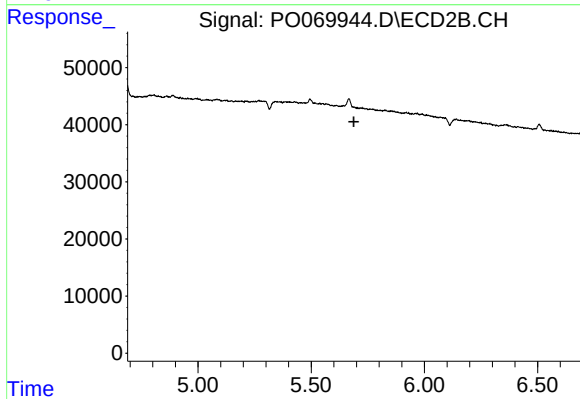

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.689 min
Response: 0
Conc: N.D.

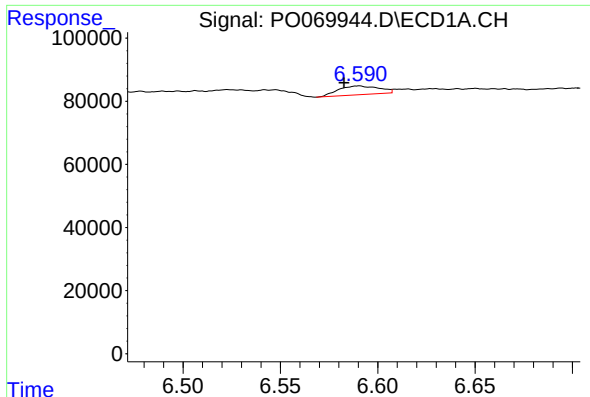

#26 AR-1254-1

R.T.: 6.590 min
Delta R.T.: 0.008 min
Response: 40348
Conc: 22.86 ng/ml

Instrument :
ECD_O
ClientSampleId :

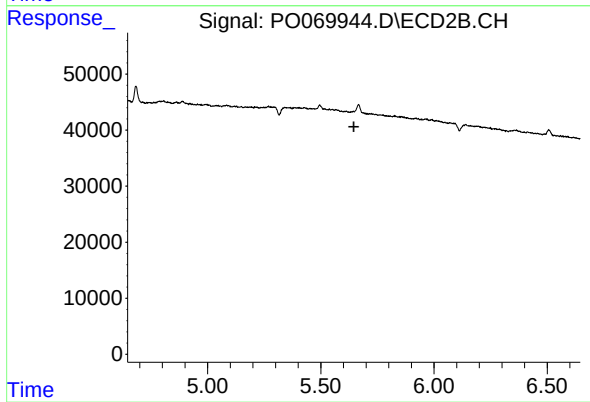

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.646 min
Response: 0
Conc: N.D.