

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072420\
Data File : P0069929.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2020 15:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 16:33:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 23 02:12:36 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.377	3.554	613701	675186	17.878	18.732
2) SA Decachlor...	10.022	8.757	1015782	1003713	19.011	19.680

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072420\
Data File : P0069929.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jul 2020 15:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 16:33:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 23 02:12:36 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

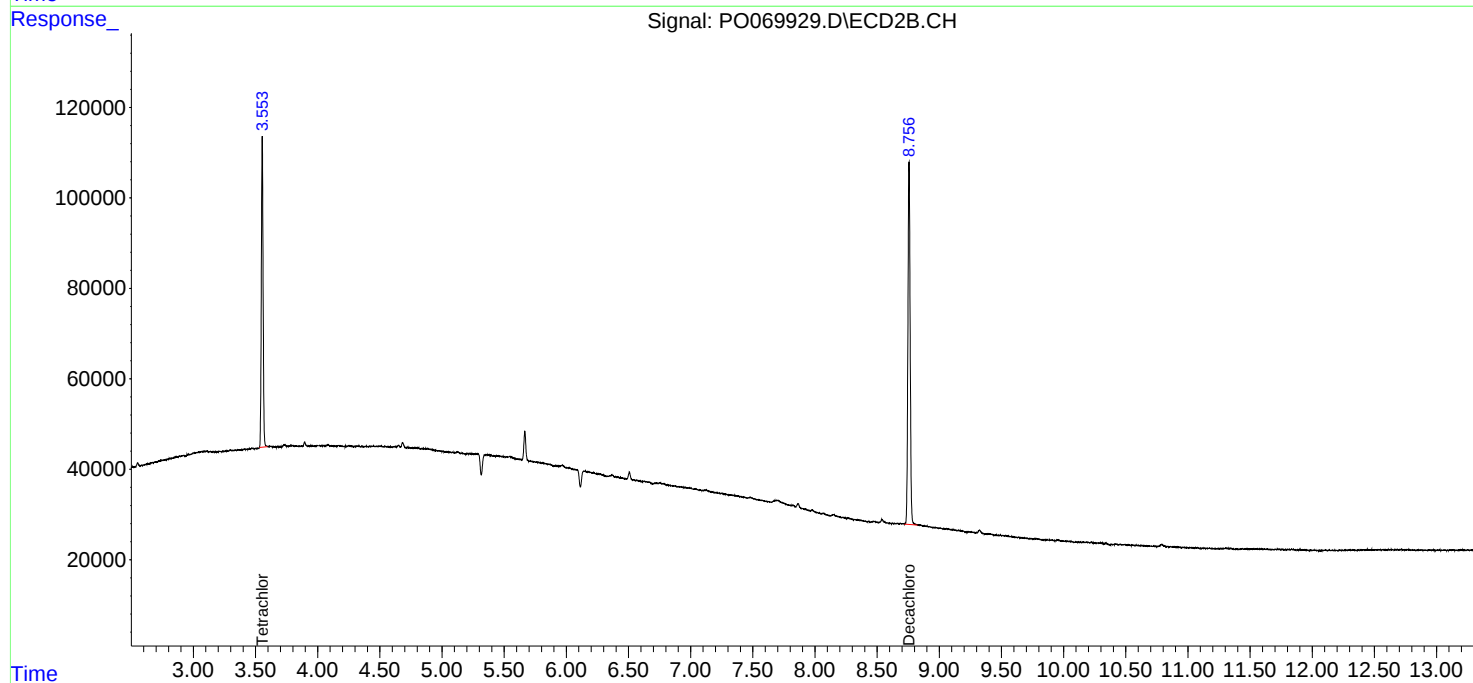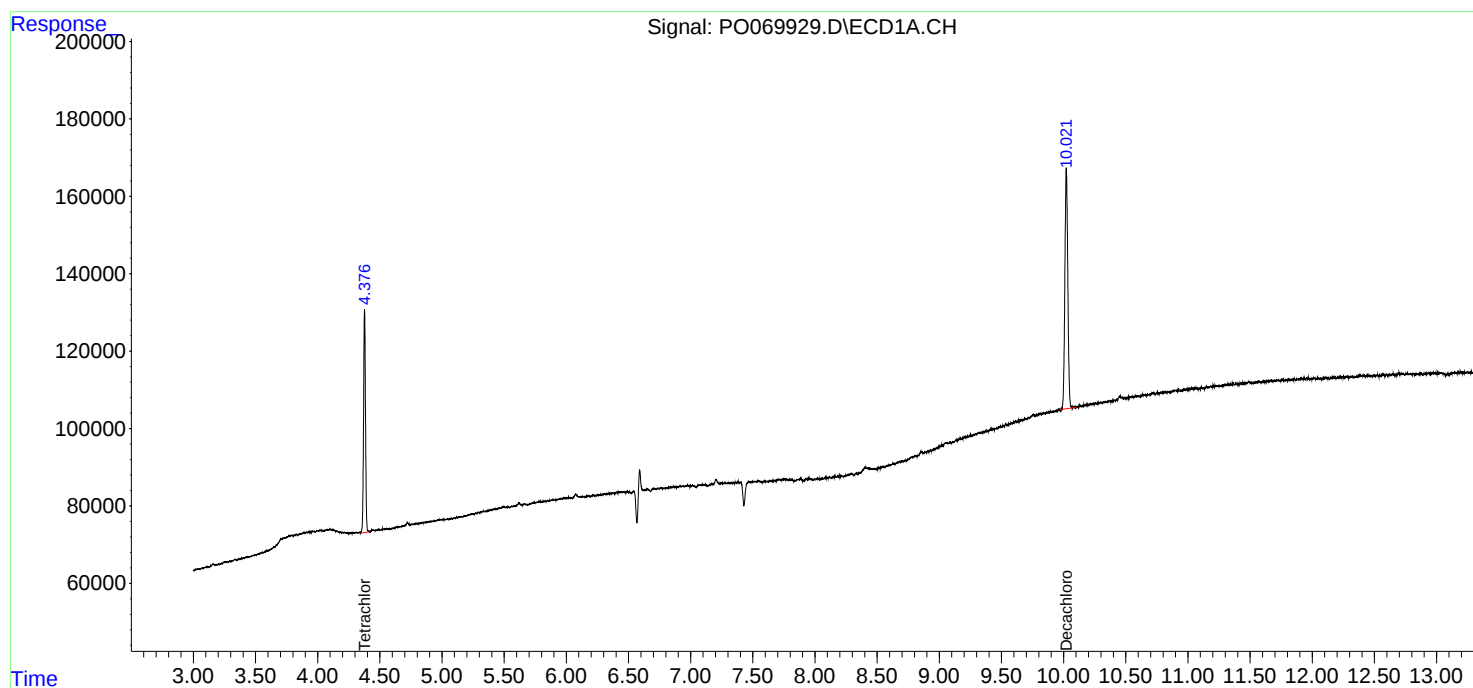


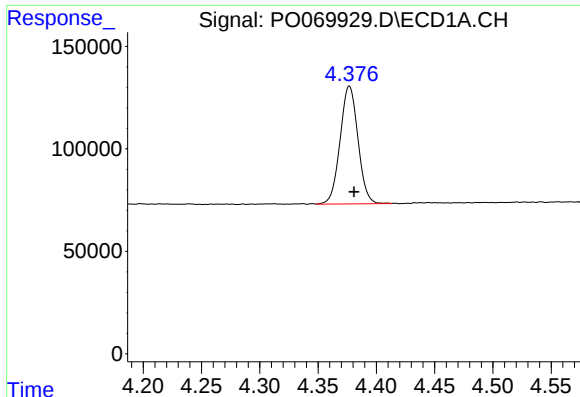

#1 Tetrachloro-m-xylene


R.T.: 4.377 min
Delta R.T.: -0.004 min
Response: 613701
Conc: 17.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

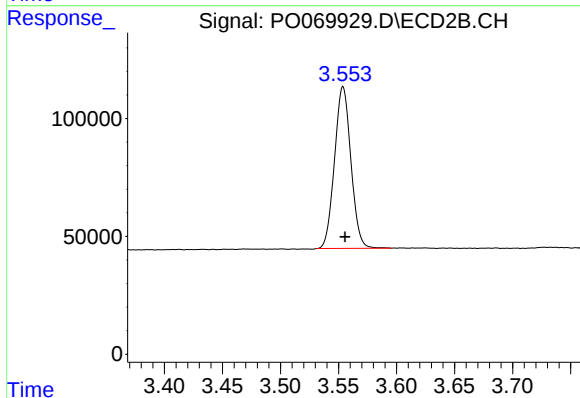


#1 Tetrachloro-m-xylene

R.T.: 3.554 min
Delta R.T.: -0.002 min
Response: 675186
Conc: 18.73 ng/ml

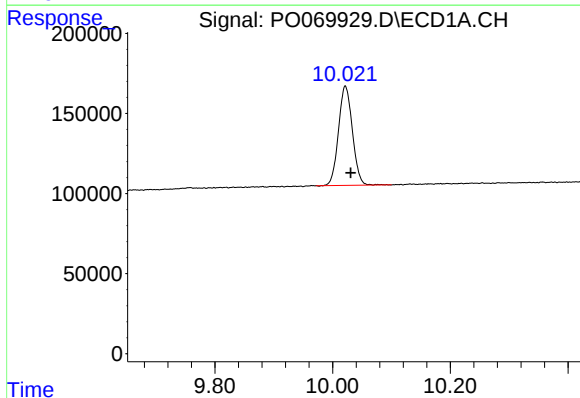

#2 Decachlorobiphenyl

R.T.: 10.022 min
Delta R.T.: -0.009 min
Response: 1015782
Conc: 19.01 ng/ml

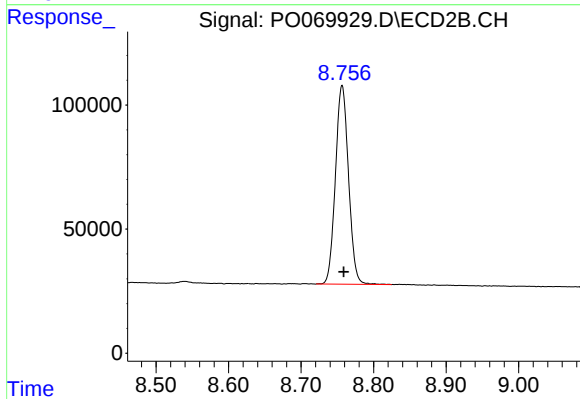

#2 Decachlorobiphenyl

R.T.: 8.757 min
Delta R.T.: -0.002 min
Response: 1003713
Conc: 19.68 ng/ml