

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072423\
 Data File : P0096268.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2023 11:55
 Operator : YP/AJ
 Sample : 03686-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-29-0-2-20230721

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2023
 Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 21:34:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 12:20:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.411	3.628	62534676	24800673	19.862	18.896
2) SA Decachlor...	10.233	8.658	43303173	22249926	22.006	20.423m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072423\
Data File : P0096268.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2023 11:55
Operator : YP/AJ
Sample : 03686-09
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-29-0-2-20230721


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 21:34:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 12:20:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

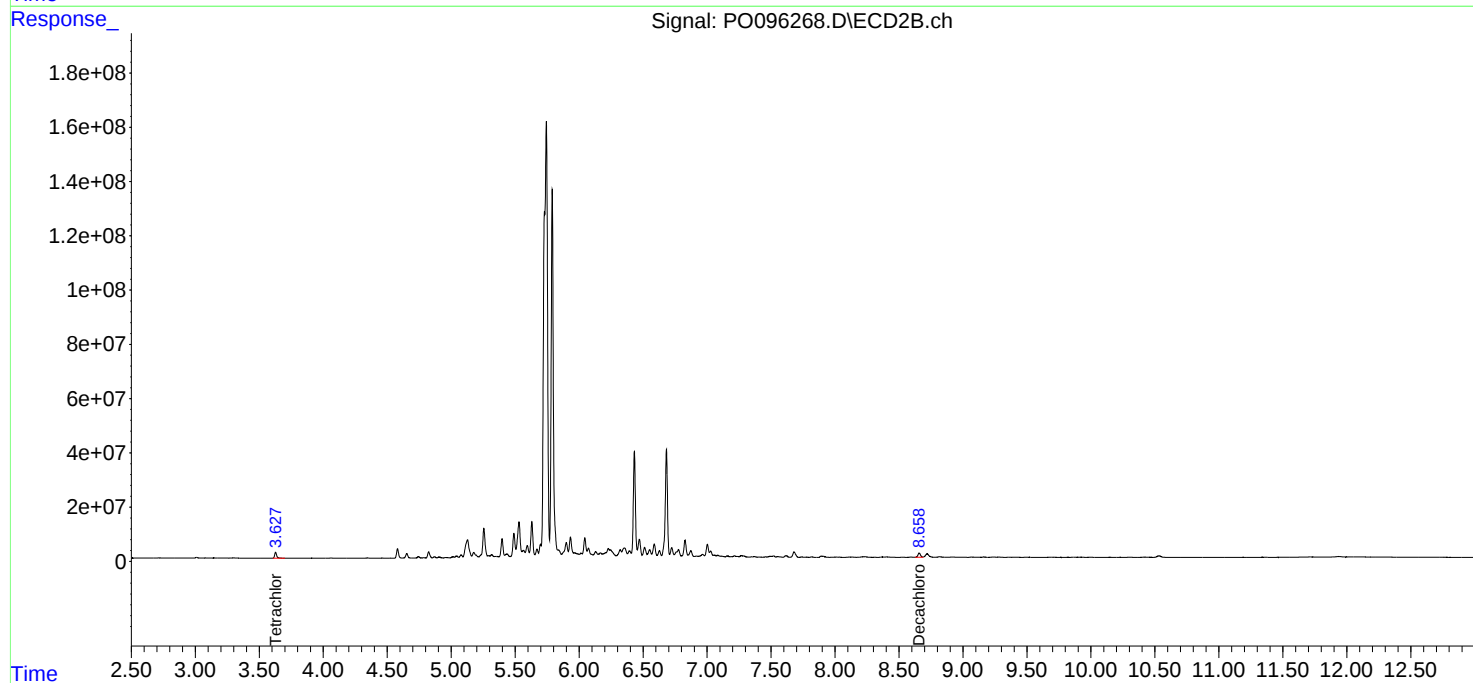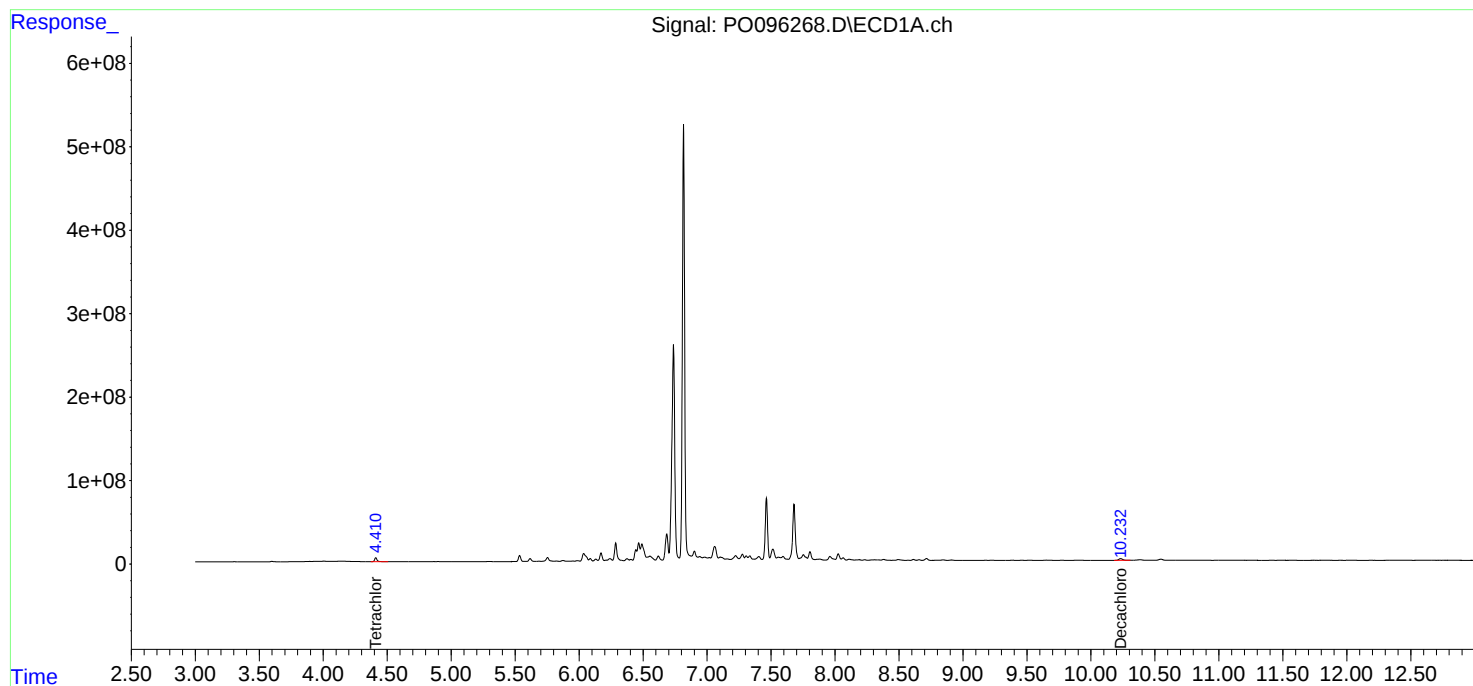

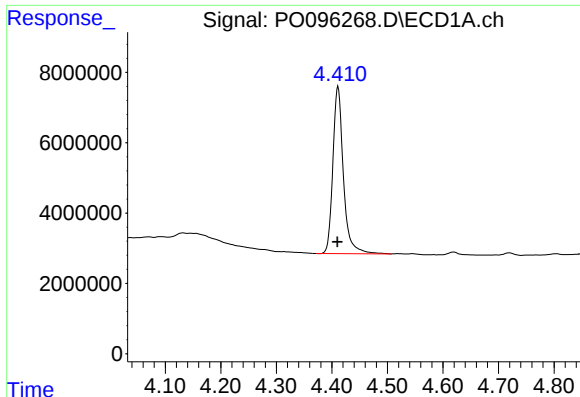


#1 Tetrachloro-m-xylene

R.T.: 4.411 min
Delta R.T.: 0.001 min
Response: 62534676
Conc: 19.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-29-0-2-20230721


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2023
Supervised By :Ankita Jodhani 07/25/2023

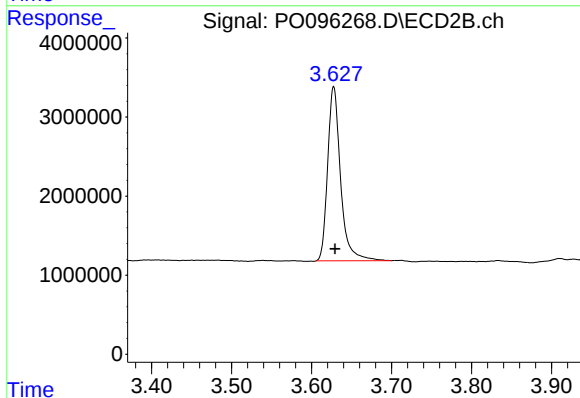


#1 Tetrachloro-m-xylene

R.T.: 3.628 min
Delta R.T.: -0.002 min
Response: 24800673
Conc: 18.90 ng/ml

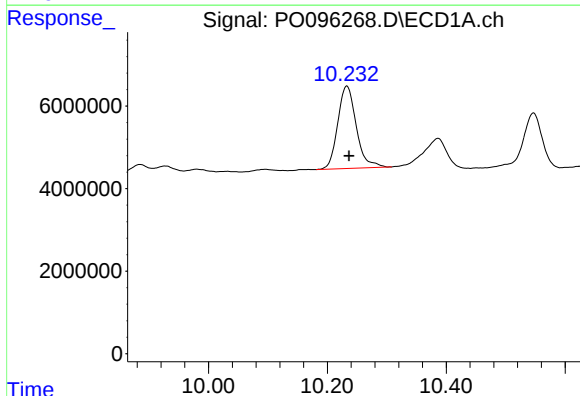

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: -0.004 min
Response: 43303173
Conc: 22.01 ng/ml

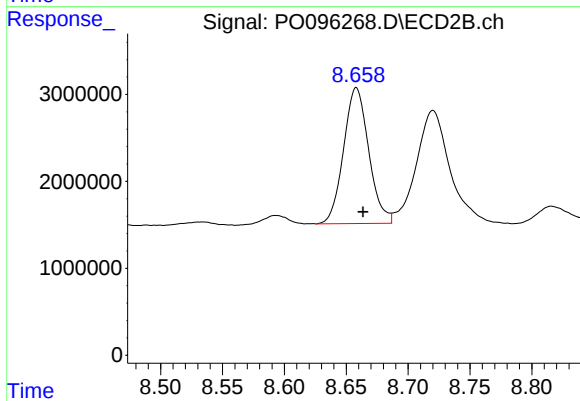

#2 Decachlorobiphenyl

R.T.: 8.658 min
Delta R.T.: -0.006 min
Response: 22249926
Conc: 20.42 ng/ml m