

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072424\
 Data File : P0104937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jul 2024 13:53
 Operator : YP/AJ
 Sample : P3341-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-05-072324

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2024
 Supervised By :Ankita Jodhani 07/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 14:14:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.426	3.539	124.9E6	44907038	13.955	13.764
2) SA Decachlor...	10.209	8.433	88449180	24032666	14.423m	11.460

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072424\
Data File : PO104937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jul 2024 13:53
Operator : YP/AJ
Sample : P3341-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AU-05-072324


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2024
Supervised By :Ankita Jodhani 07/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 14:14:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

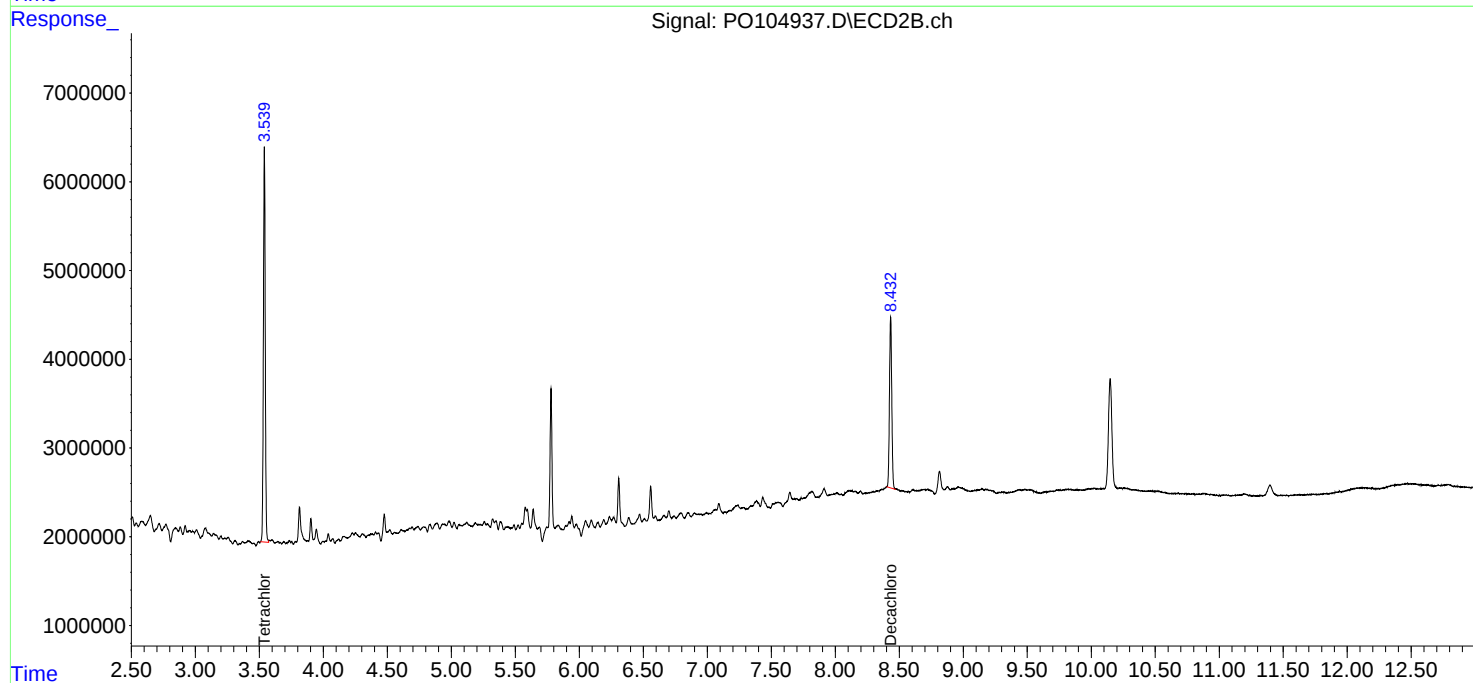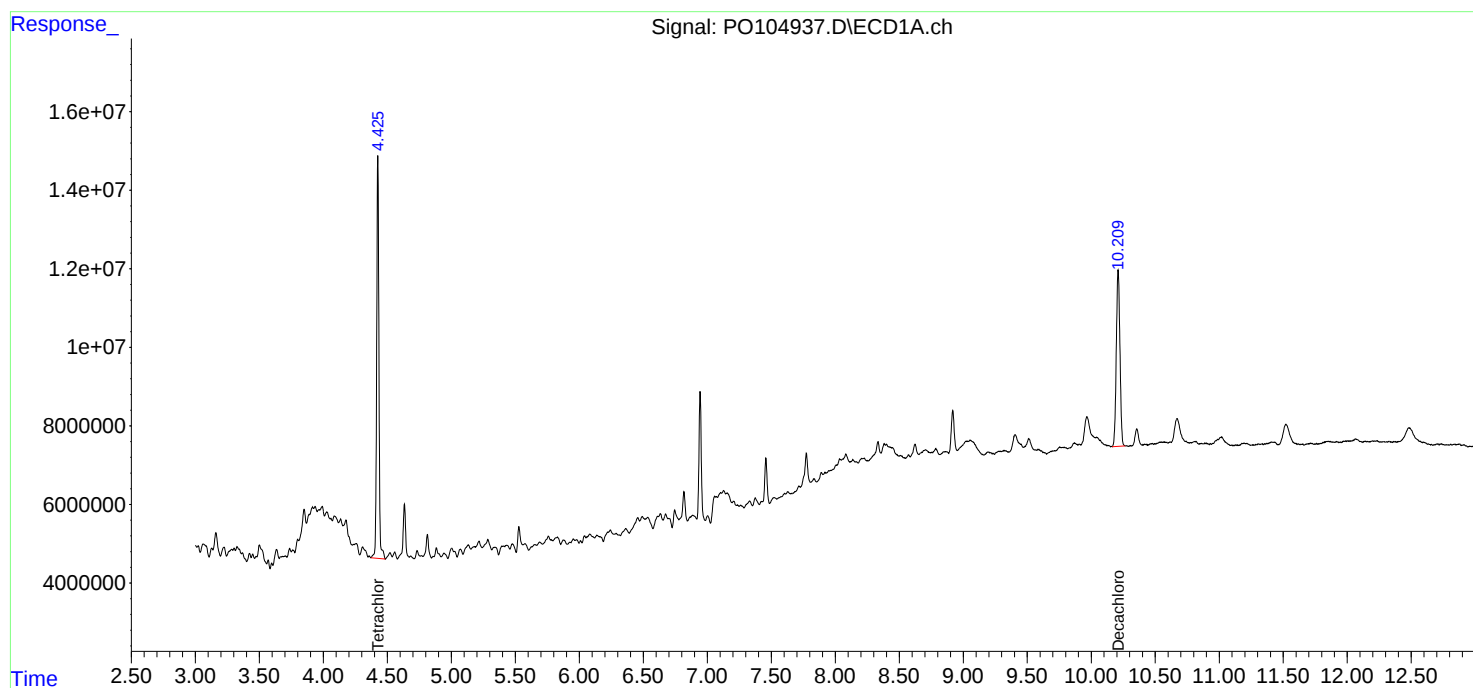

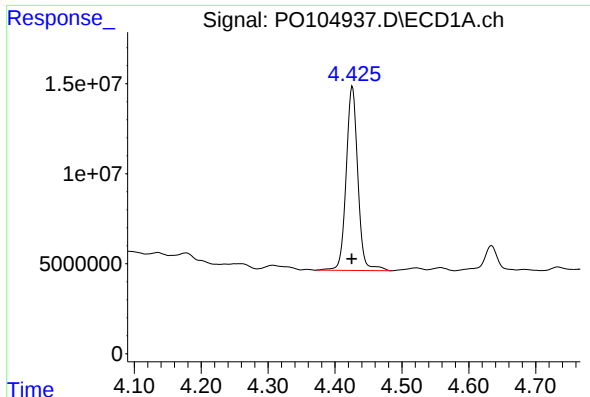


#1 Tetrachloro-m-xylene

R.T.: 4.426 min
Delta R.T.: 0.000 min
Response: 124945280
Conc: 13.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-072324


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2024
Supervised By :Ankita Jodhani 07/25/2024

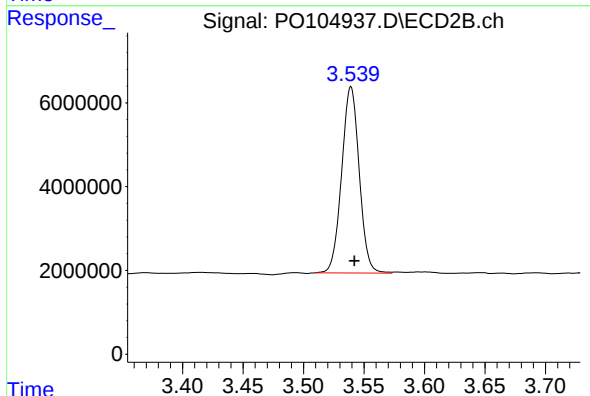


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.003 min
Response: 44907038
Conc: 13.76 ng/ml

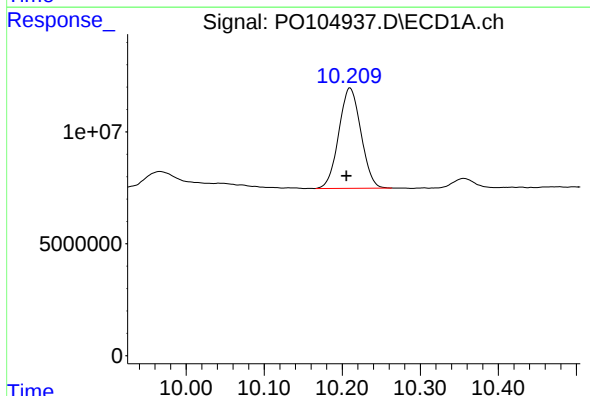

#2 Decachlorobiphenyl

R.T.: 10.209 min
Delta R.T.: 0.004 min
Response: 88449180
Conc: 14.42 ng/ml m

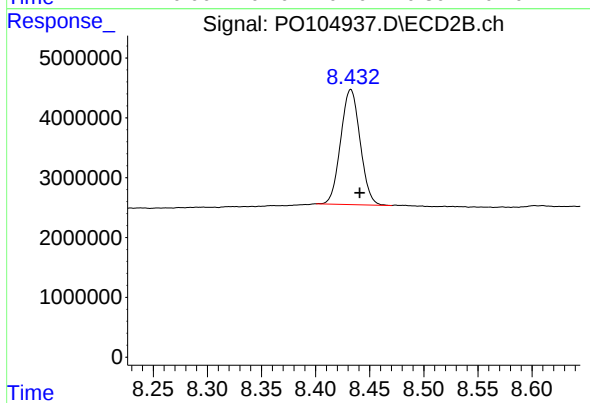

#2 Decachlorobiphenyl

R.T.: 8.433 min
Delta R.T.: -0.008 min
Response: 24032666
Conc: 11.46 ng/ml