

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072425\
 Data File : P0112491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2025 04:05
 Operator : YP/AJ
 Sample : Q2685-02 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/25/2025
 Supervised By :mohammad ahmed 07/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 06:25:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.671	3.664	5310762	4070841	0.653m	0.819m#
2) SA Decachlor...	8.697	8.642	5951839	2196389	0.814	1.243 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072425\
Data File : P0112491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2025 04:05
Operator : YP/AJ
Sample : Q2685-02 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 06:25:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

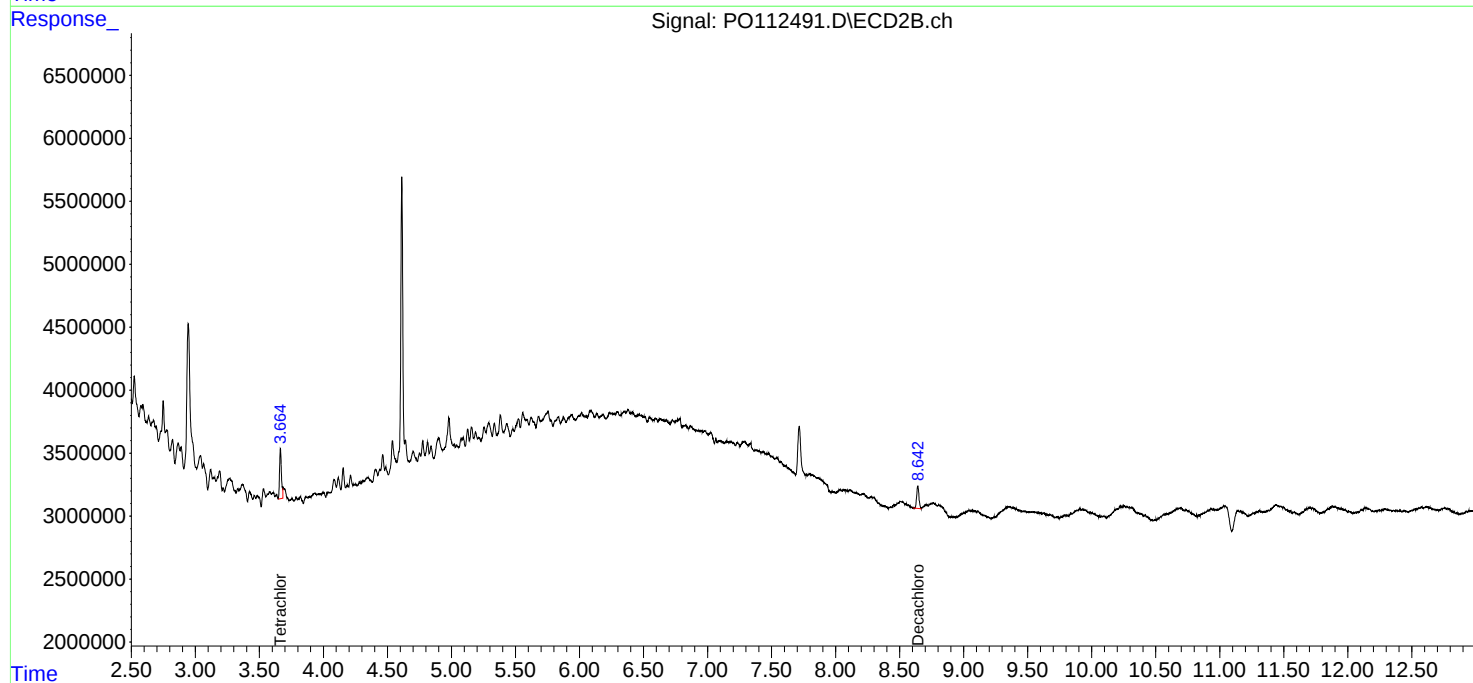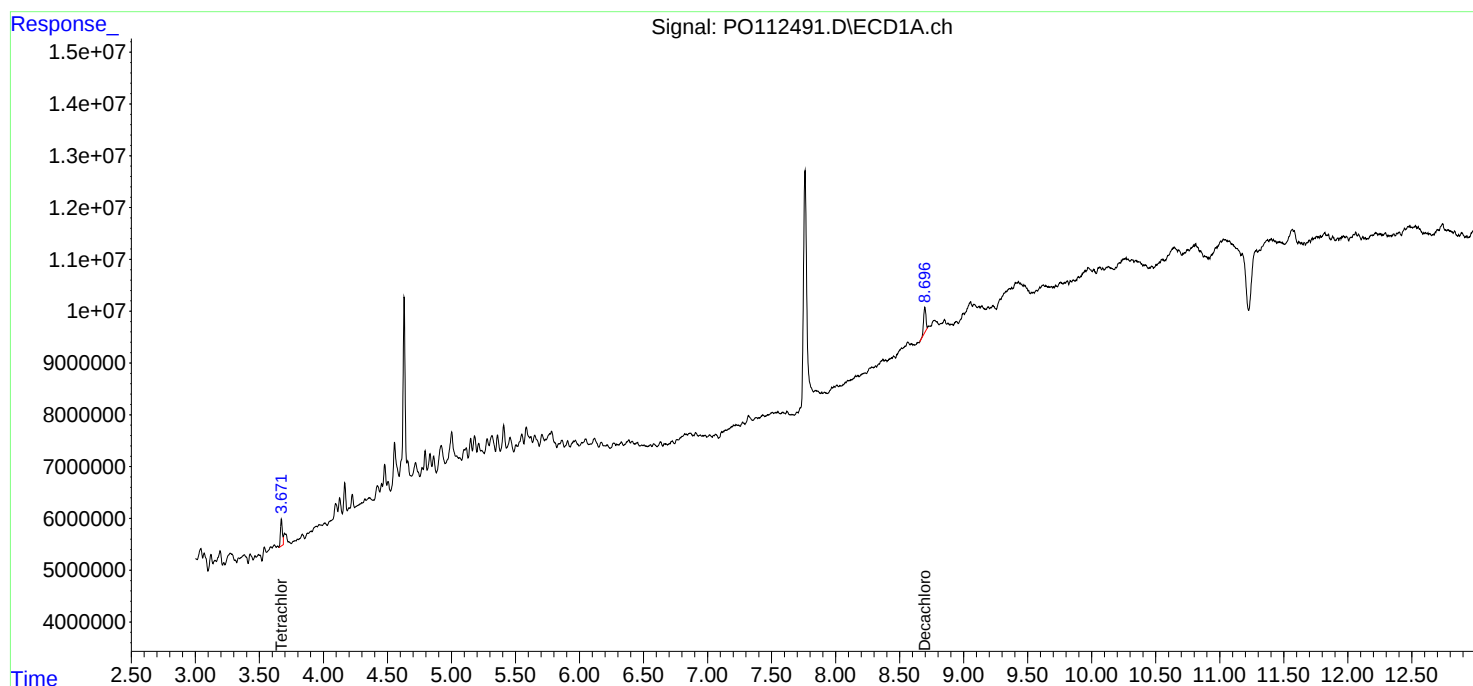

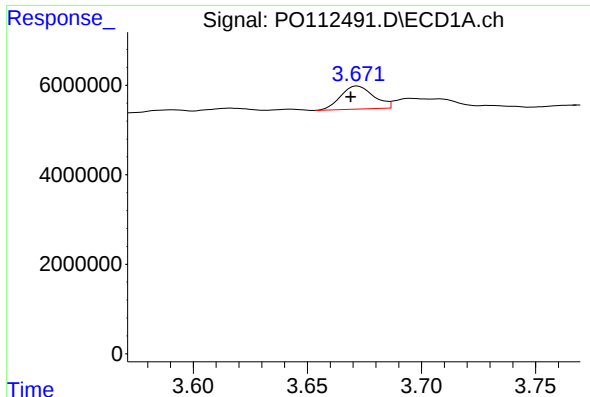


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: 0.002 min
Response: 5310762
Conc: 0.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/25/2025
Supervised By :mohammad ahmed 07/29/2025

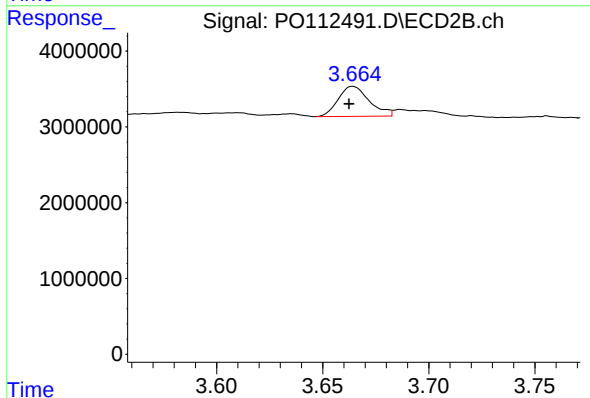


#1 Tetrachloro-m-xylene

R.T.: 3.664 min
Delta R.T.: 0.001 min
Response: 4070841
Conc: 0.82 ng/ml m

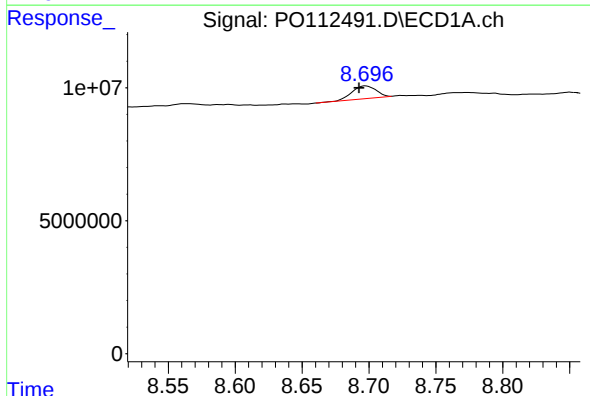

#2 Decachlorobiphenyl

R.T.: 8.697 min
Delta R.T.: 0.005 min
Response: 5951839
Conc: 0.81 ng/ml

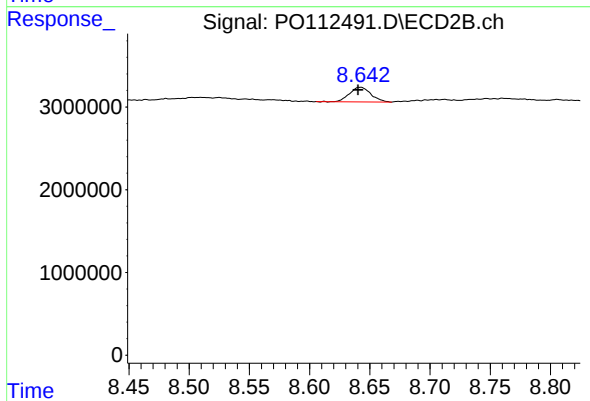

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: 0.002 min
Response: 2196389
Conc: 1.24 ng/ml