

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072520\
 Data File : P0070010.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2020 20:18
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 00:05:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 23 02:12:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.372	3.552	690881	758817	20.126	21.052
2)	SA Decachlor...	10.009	8.753	1105490	1019831	20.690	19.996
Target Compounds							
20)	L4 AR-1242-5	6.646	5.663f	76354	66923	66.463	54.471
24)	L5 AR-1248-4	6.617	0.000	41839	0	23.870	N.D. #
25)	L5 AR-1248-5	6.646	5.663f	76354	66923	45.718	42.385
26)	L6 AR-1254-1	6.583	5.663f	282278	66923	159.944	26.249 #
28)	L6 AR-1254-3	7.196	0.000	35866	0	11.811	N.D. #
29)	L6 AR-1254-4	7.485	0.000	3177	0	1.162	N.D. #
43)	L9 AR-1268-3	9.031f	0.000	2275	0	0.372	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072520\
Data File : P0070010.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2020 20:18
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 00:05:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 23 02:12:36 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

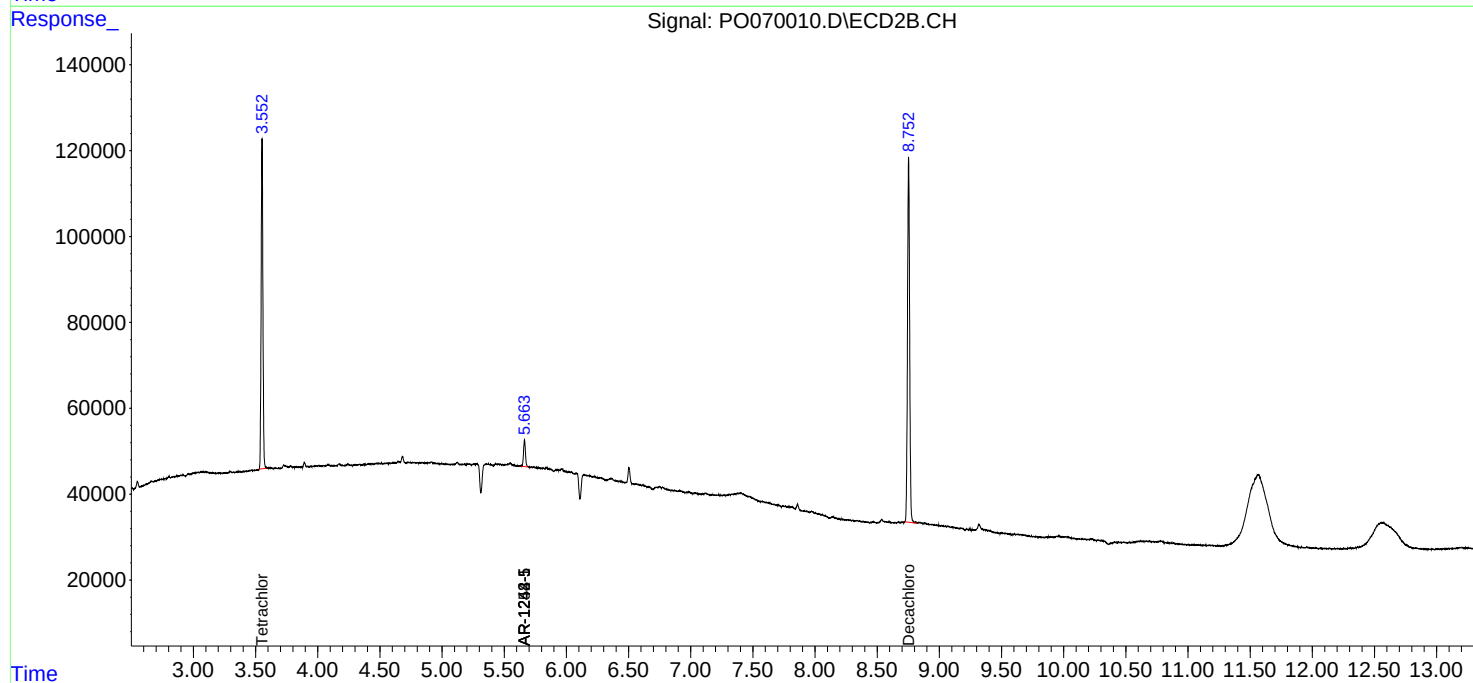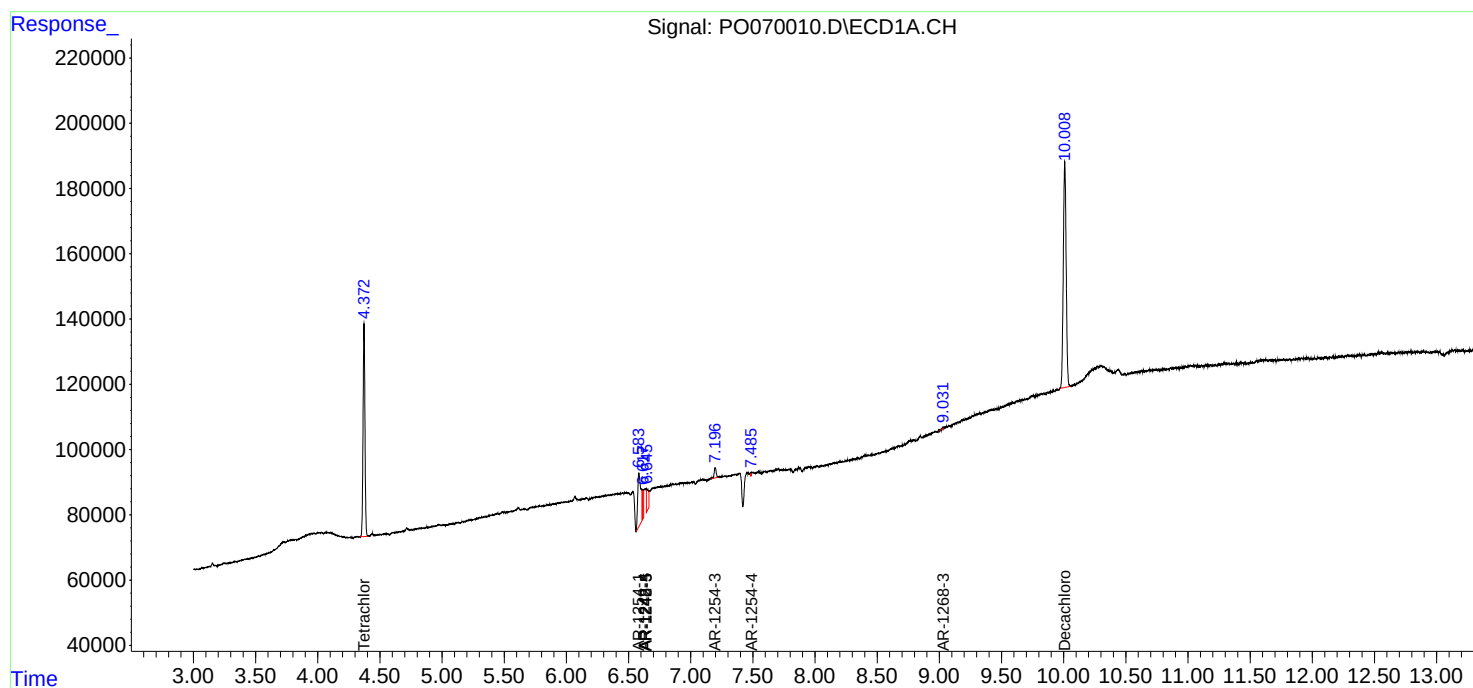


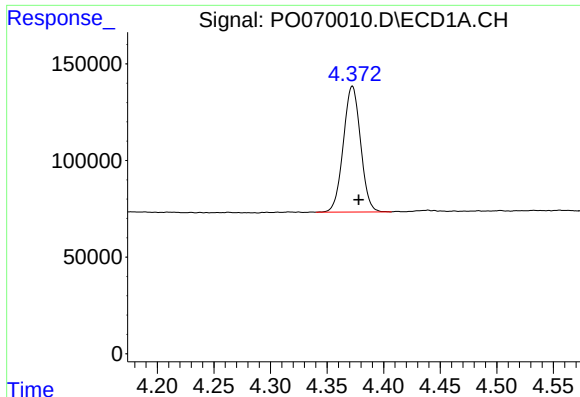

#1 Tetrachloro-m-xylene


R.T.: 4.372 min
Delta R.T.: -0.006 min
Response: 690881
Conc: 20.13 ng/ml

Instrument :
ECD_O
ClientSampleId :

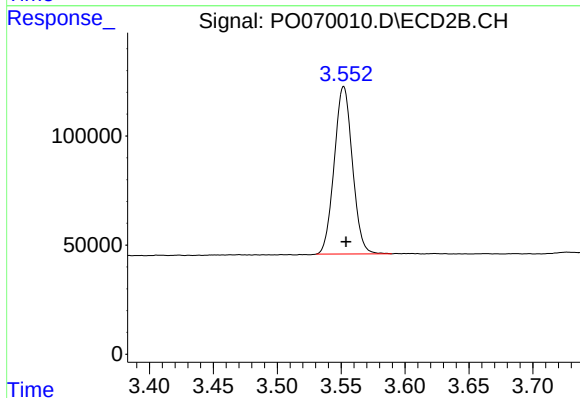


#1 Tetrachloro-m-xylene

R.T.: 3.552 min
Delta R.T.: -0.002 min
Response: 758817
Conc: 21.05 ng/ml

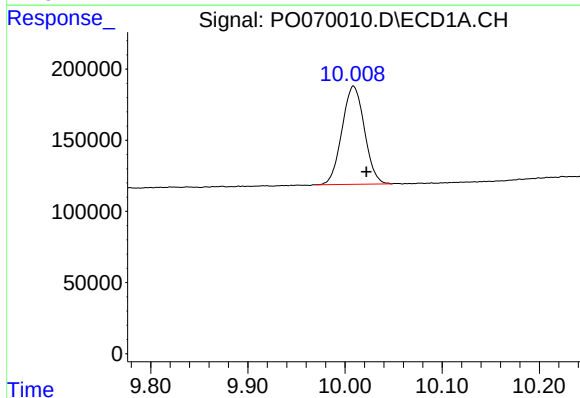


#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: -0.013 min
Response: 1105490
Conc: 20.69 ng/ml

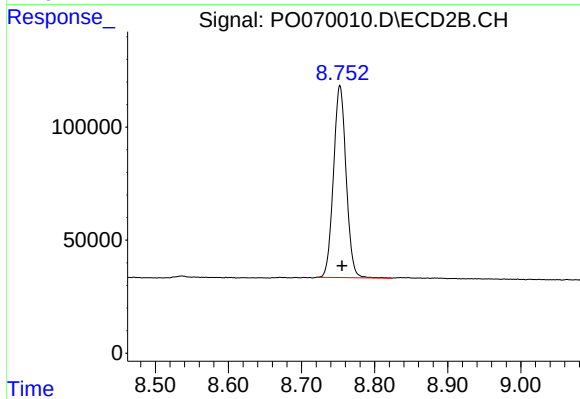

#2 Decachlorobiphenyl


R.T.: 8.753 min
Delta R.T.: -0.003 min
Response: 1019831
Conc: 20.00 ng/ml

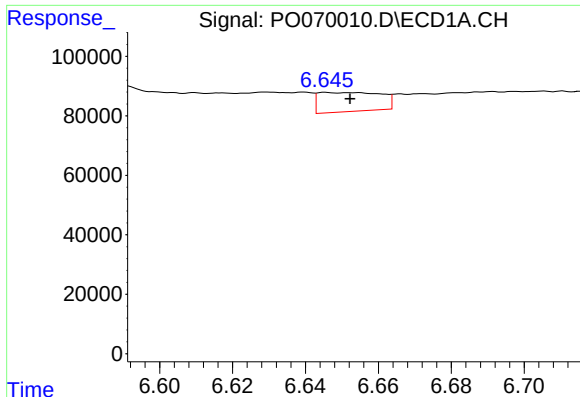

#20 AR-1242-5


R.T.: 6.646 min
Delta R.T.: -0.007 min
Response: 76354
Conc: 66.46 ng/ml

Instrument :
ECD_O
ClientSampleId :

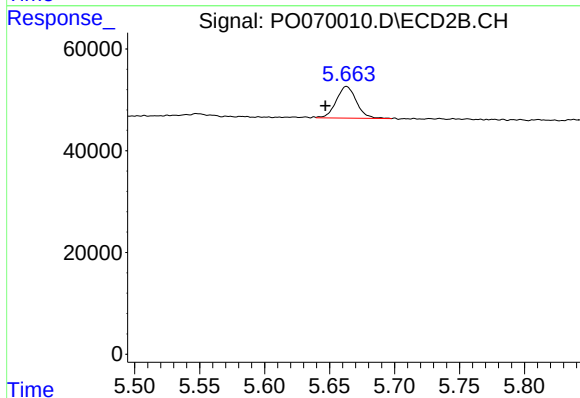


#20 AR-1242-5

R.T.: 5.663 min
Delta R.T.: 0.016 min
Response: 66923
Conc: 54.47 ng/ml

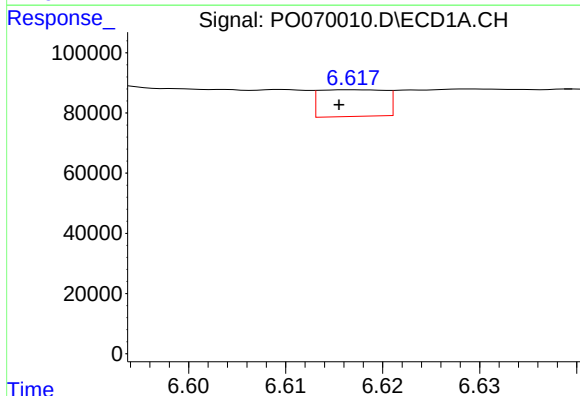


#24 AR-1248-4

R.T.: 6.617 min
Delta R.T.: 0.001 min
Response: 41839
Conc: 23.87 ng/ml

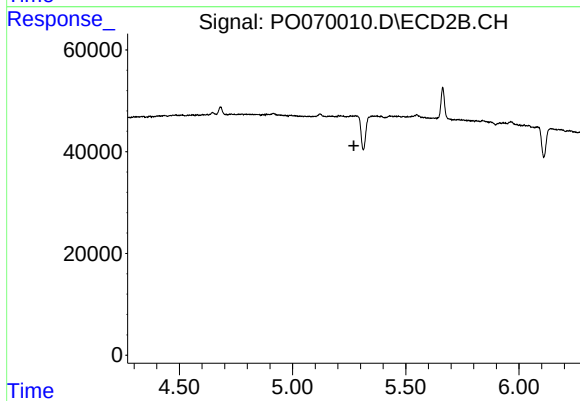

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.270 min
Response: 0
Conc: N.D.

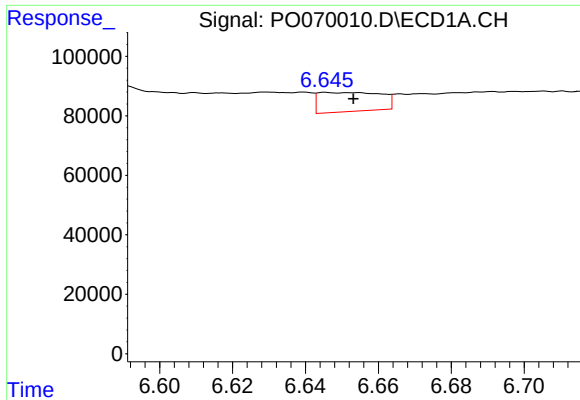

#25 AR-1248-5


R.T.: 6.646 min
Delta R.T.: -0.008 min
Response: 76354
Conc: 45.72 ng/ml

Instrument :
ECD_O
ClientSampleId :

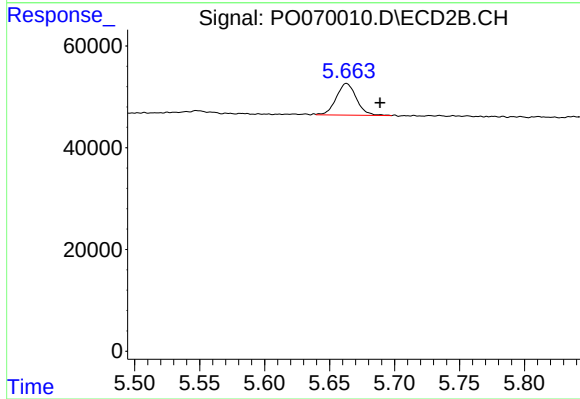


#25 AR-1248-5

R.T.: 5.663 min
Delta R.T.: -0.026 min
Response: 66923
Conc: 42.38 ng/ml

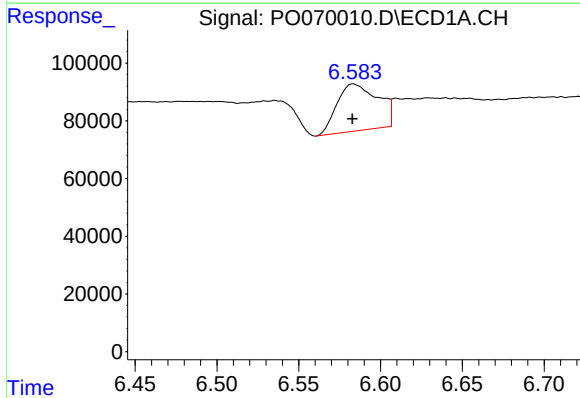


#26 AR-1254-1

R.T.: 6.583 min
Delta R.T.: 0.000 min
Response: 282278
Conc: 159.94 ng/ml

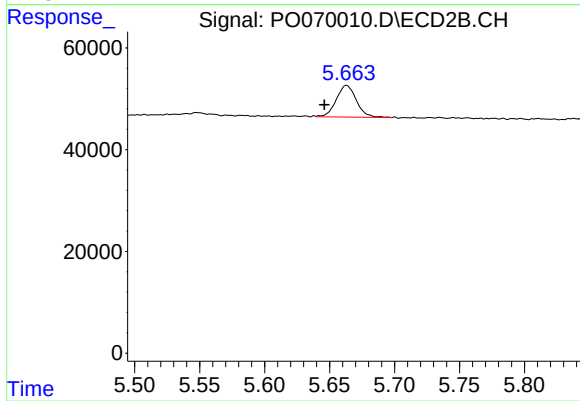

#26 AR-1254-1


R.T.: 5.663 min
Delta R.T.: 0.017 min
Response: 66923
Conc: 26.25 ng/ml

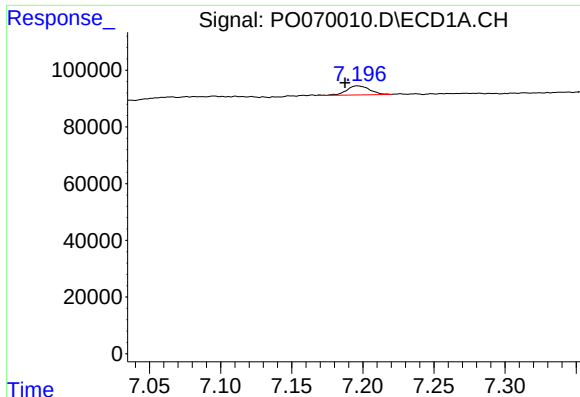

#28 AR-1254-3


R.T.: 7.196 min
Delta R.T.: 0.009 min
Response: 35866
Conc: 11.81 ng/ml

Instrument :
ECD_O
ClientSampleId :

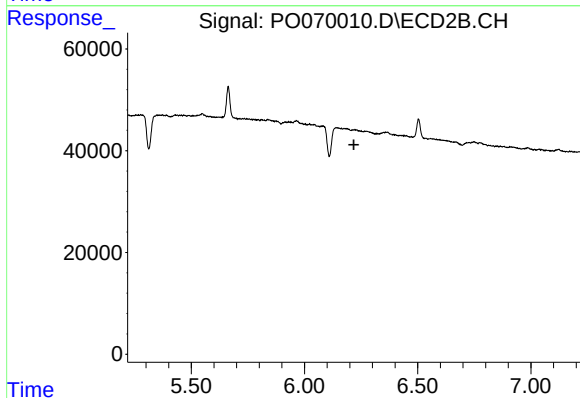


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.218 min
Response: 0
Conc: N.D.

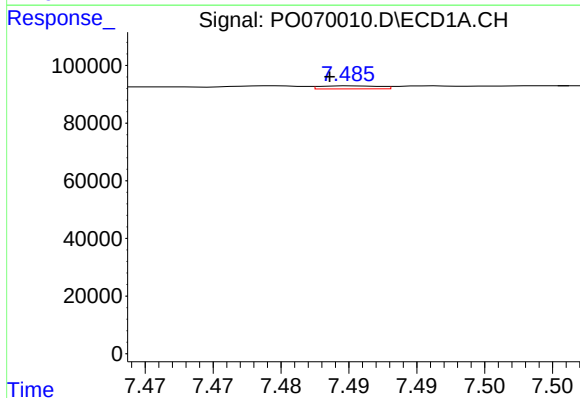


#29 AR-1254-4

R.T.: 7.485 min
Delta R.T.: 0.002 min
Response: 3177
Conc: 1.16 ng/ml

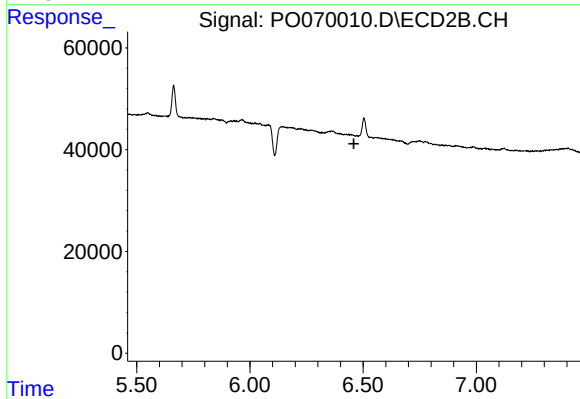

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.459 min
Response: 0
Conc: N.D.

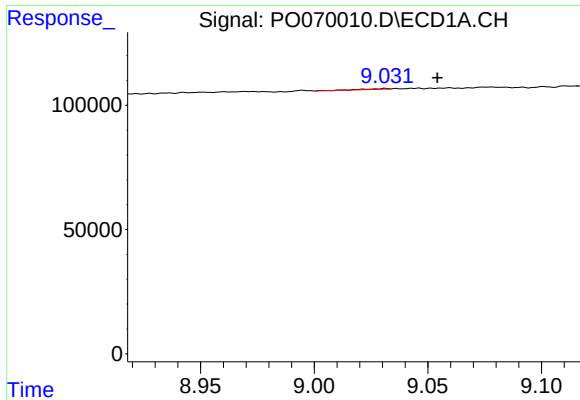

#43 AR-1268-3

R.T.: 9.031 min
Delta R.T.: -0.023 min
Response: 2275
Conc: 0.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

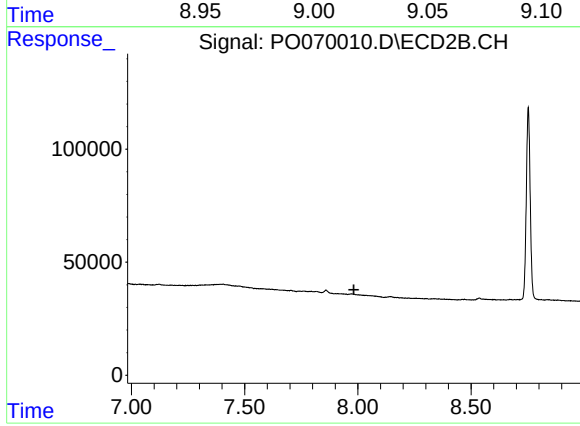

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.982 min
Response: 0
Conc: N.D.