

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072520\
 Data File : P0069981.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2020 11:58
 Operator : DD\AJ
 Sample : L3410-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FM-CON-A

Manual Integrations
 APPROVED

Ankita
 7/27/2020 12:25:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 14:03:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 23 02:12:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.389	3.557	895018	954213	26.073	26.473
2) SA Decachlor...	10.025	8.758	1945841	1718525	36.417	33.695
Target Compounds						
41) L9 AR-1268-1	8.784	7.713	1716828	1586161	214.321m	218.329
42) L9 AR-1268-2	8.868	7.778	2103622	2261734	298.422	337.660
43) L9 AR-1268-3	9.051	7.980	1082241	1271690	176.813	227.236 #
44) L9 AR-1268-4	9.425	8.273	744238	744788	279.448	283.578
45) L9 AR-1268-5	9.760	8.541	3552661	2960218	184.830	165.371

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072520\
Data File : PO069981.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2020 11:58
Operator : DD\AJ
Sample : L3410-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
FM-CON-A


Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 14:03:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 23 02:12:36 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

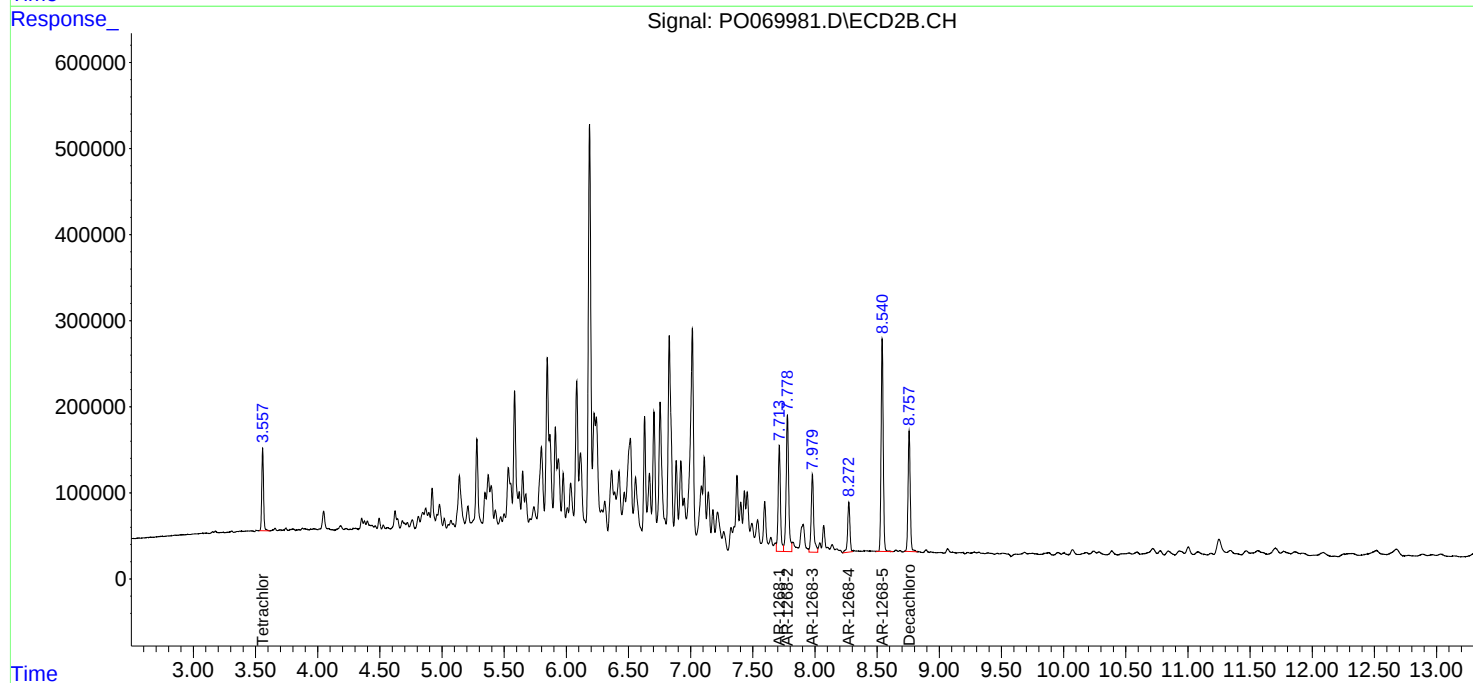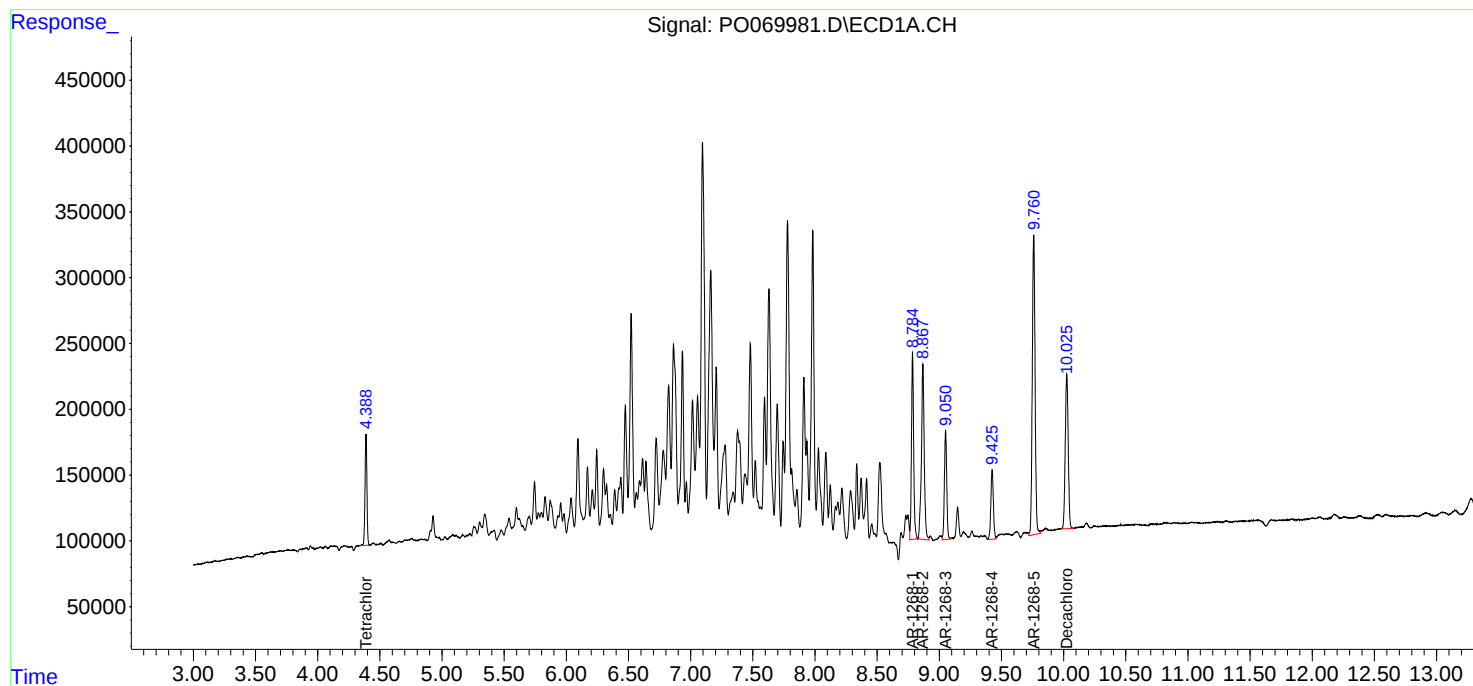

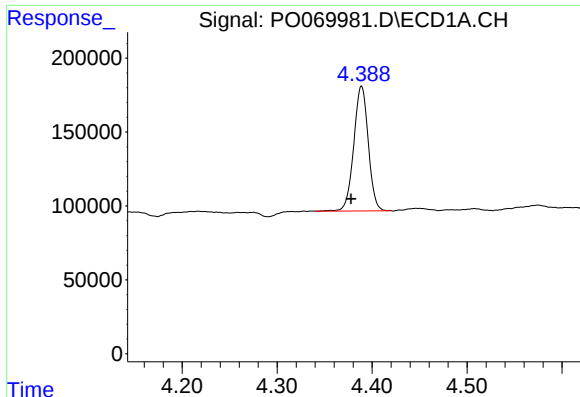


#1 Tetrachloro-m-xylene

R.T.: 4.389 min
Delta R.T.: 0.011 min
Response: 895018
Conc: 26.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
FM-CON-A


Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:00 PM

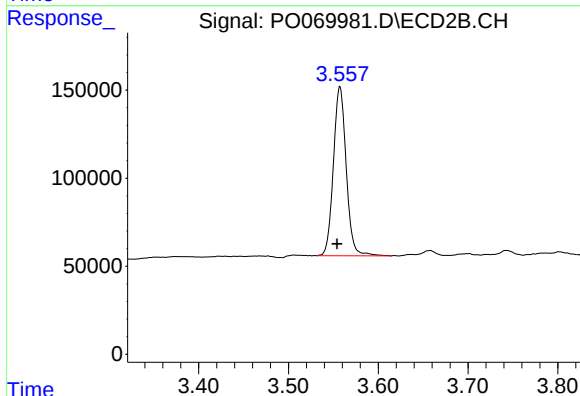


#1 Tetrachloro-m-xylene

R.T.: 3.557 min
Delta R.T.: 0.003 min
Response: 954213
Conc: 26.47 ng/ml

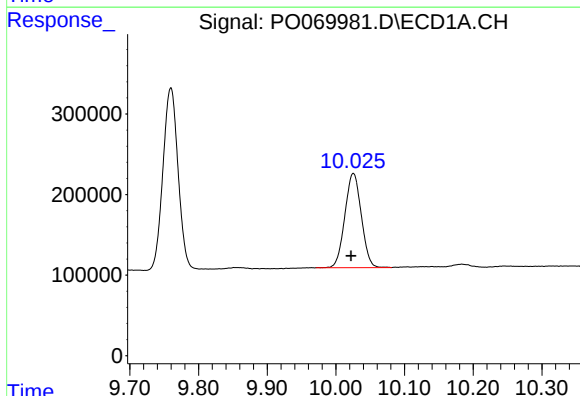


#2 Decachlorobiphenyl

R.T.: 10.025 min
Delta R.T.: 0.003 min
Response: 1945841
Conc: 36.42 ng/ml

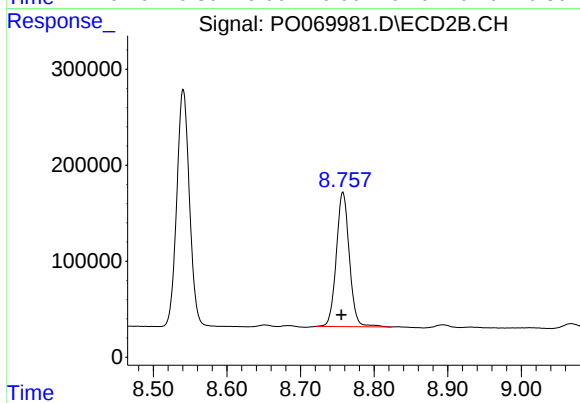

#2 Decachlorobiphenyl

R.T.: 8.758 min
Delta R.T.: 0.002 min
Response: 1718525
Conc: 33.70 ng/ml

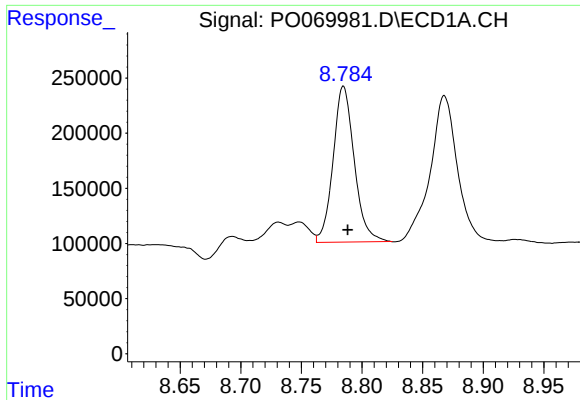


#41 AR-1268-1

R.T.: 8.784 min
Delta R.T.: -0.004 min
Response: 1716828
Conc: 214.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FM-CON-A


Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:00 PM

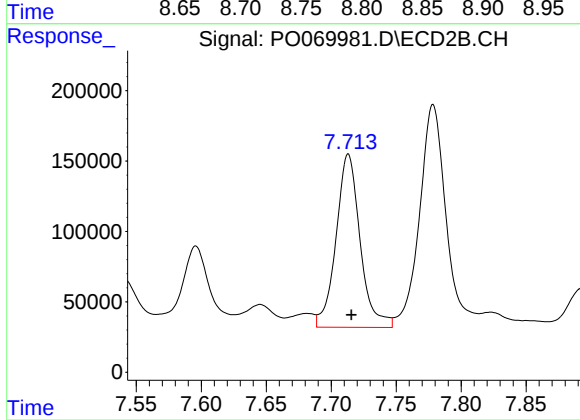


#41 AR-1268-1

R.T.: 7.713 min
Delta R.T.: -0.002 min
Response: 1586161
Conc: 218.33 ng/ml

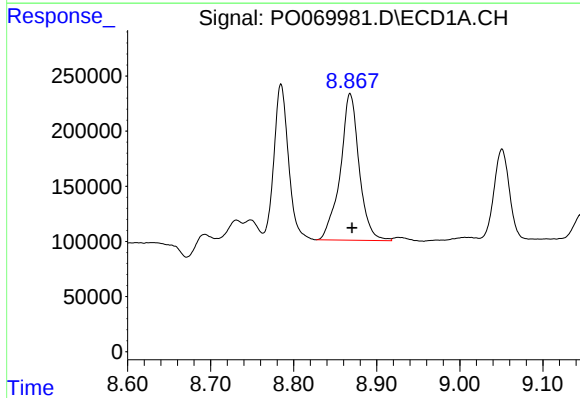


#42 AR-1268-2

R.T.: 8.868 min
Delta R.T.: -0.002 min
Response: 2103622
Conc: 298.42 ng/ml

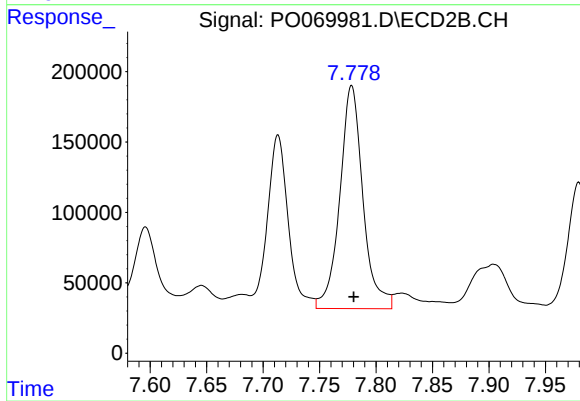

#42 AR-1268-2

R.T.: 7.778 min
Delta R.T.: -0.002 min
Response: 2261734
Conc: 337.66 ng/ml

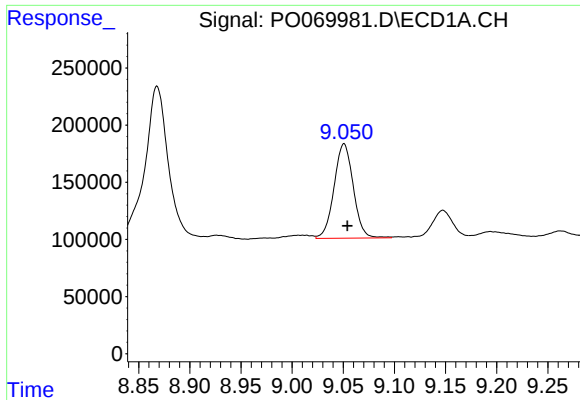


#43 AR-1268-3

R.T.: 9.051 min
Delta R.T.: -0.003 min
Response: 1082241
Conc: 176.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
FM-CON-A


Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:00 PM

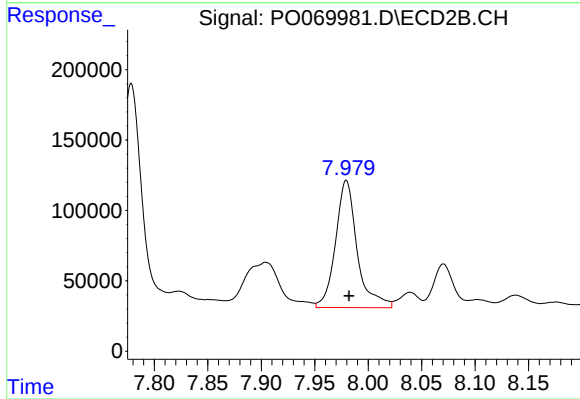


#43 AR-1268-3

R.T.: 7.980 min
Delta R.T.: -0.003 min
Response: 1271690
Conc: 227.24 ng/ml

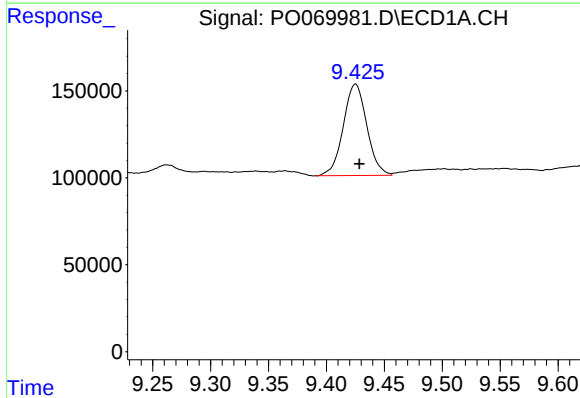


#44 AR-1268-4

R.T.: 9.425 min
Delta R.T.: -0.003 min
Response: 744238
Conc: 279.45 ng/ml

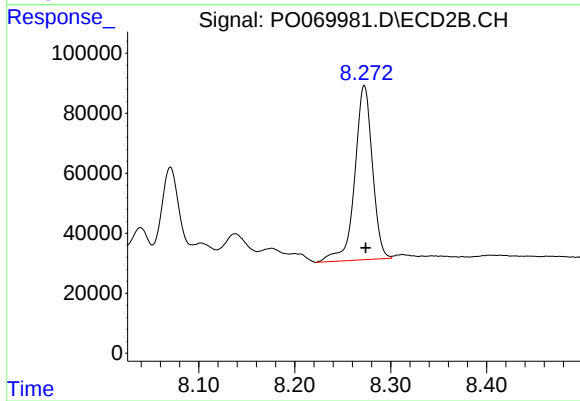

#44 AR-1268-4

R.T.: 8.273 min
Delta R.T.: -0.001 min
Response: 744788
Conc: 283.58 ng/ml

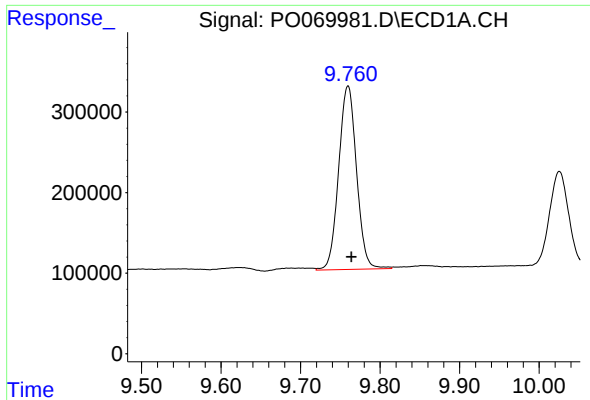


#45 AR-1268-5

R.T.: 9.760 min
Delta R.T.: -0.004 min
Response: 3552661
Conc: 184.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
FM-CON-A

Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:00 PM

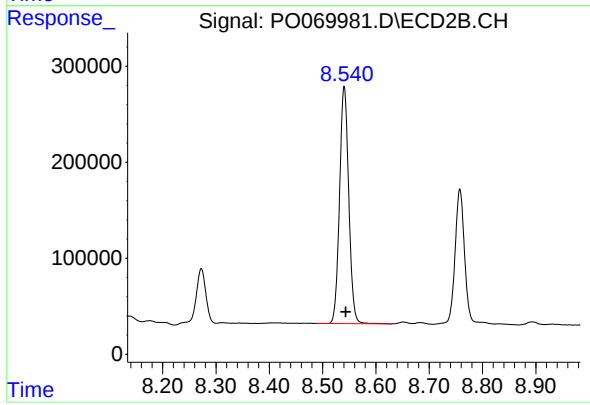

#45 AR-1268-5

R.T.: 8.541 min
Delta R.T.: -0.003 min
Response: 2960218
Conc: 165.37 ng/ml