

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072520\
 Data File : P0069998.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2020 16:53
 Operator : DD\AJ
 Sample : L3383-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CRT-018

Manual Integrations
 APPROVED

Ankita
 7/27/2020 12:25:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 00:00:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 23 02:12:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.380	3.555	939199	1015592	27.360	28.176
2) SA Decachlor...	10.014	8.755	1387751	1263831	25.973m	24.780m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072520\
Data File : PO069998.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2020 16:53
Operator : DD\AJ
Sample : L3383-05
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CRT-018


Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 00:00:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 23 02:12:36 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

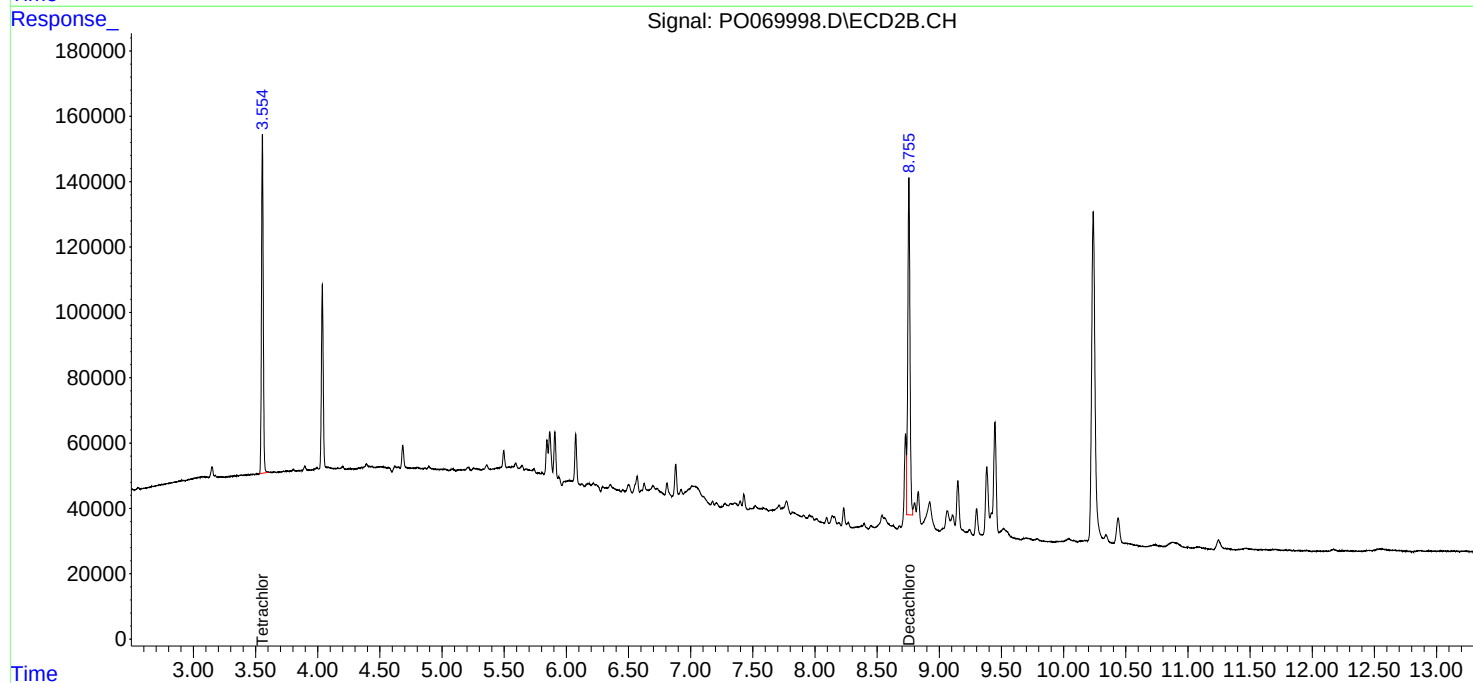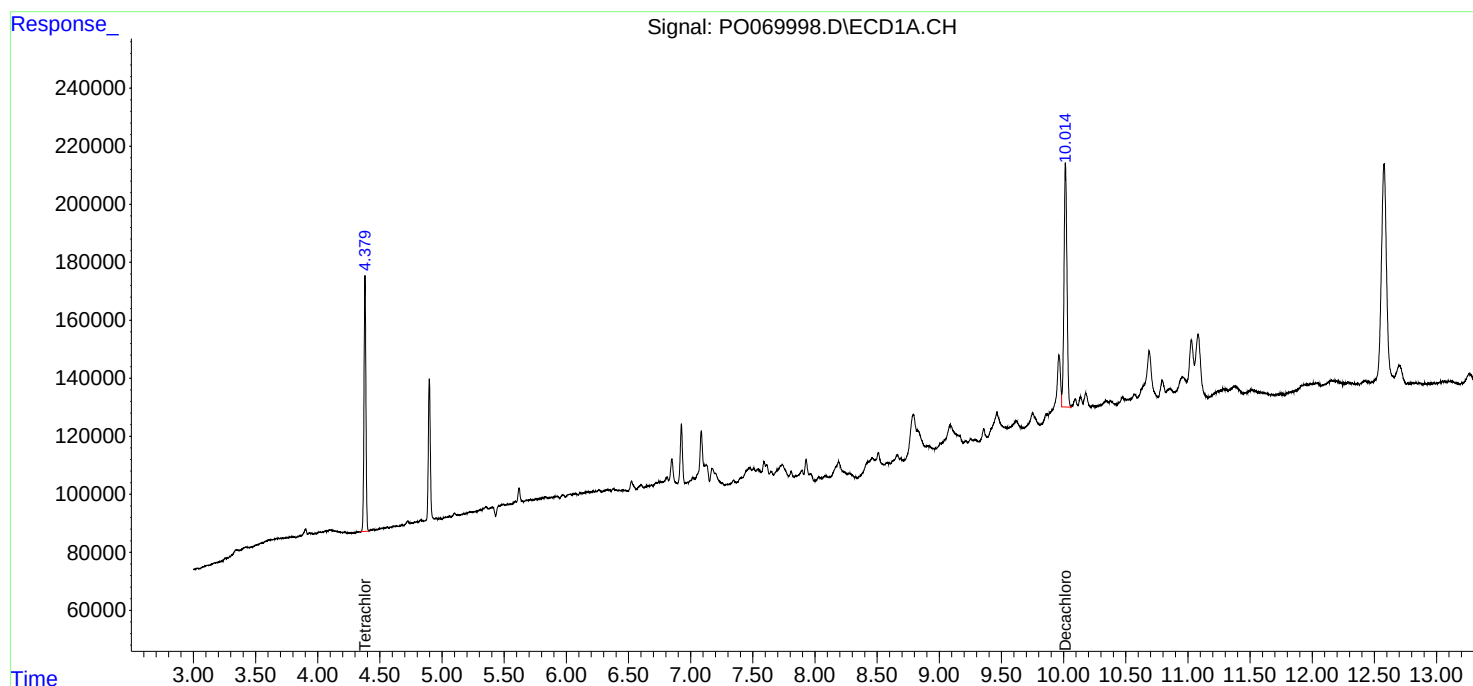

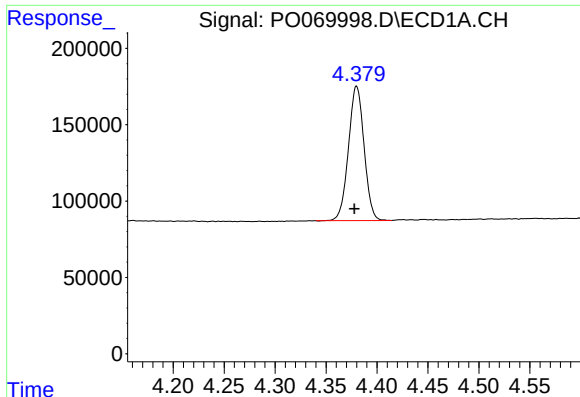


#1 Tetrachloro-m-xylene

R.T.: 4.380 min
Delta R.T.: 0.002 min
Response: 939199
Conc: 27.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
CRT-018


Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:42 PM

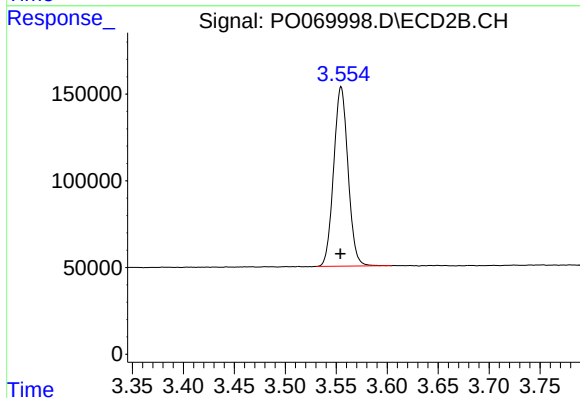


#1 Tetrachloro-m-xylene

R.T.: 3.555 min
Delta R.T.: 0.000 min
Response: 1015592
Conc: 28.18 ng/ml

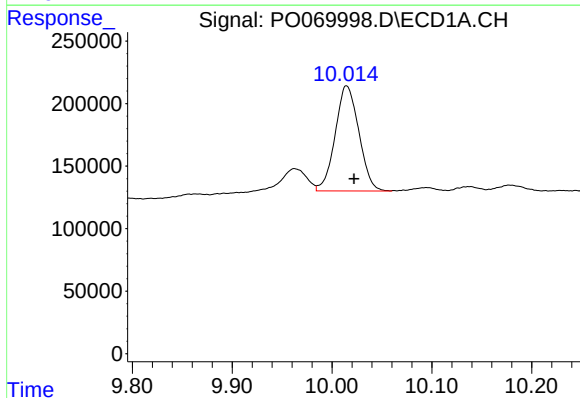

#2 Decachlorobiphenyl

R.T.: 10.014 min
Delta R.T.: -0.008 min
Response: 1387751
Conc: 25.97 ng/ml m

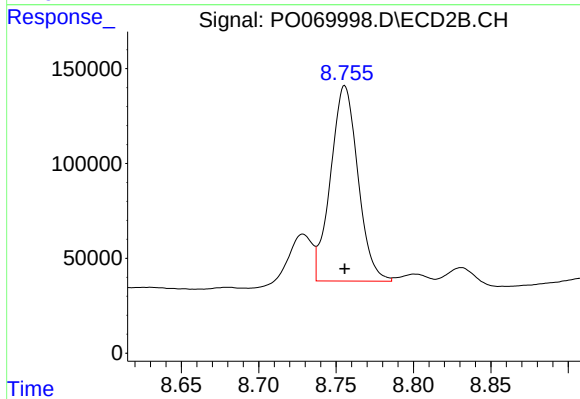

#2 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: 0.000 min
Response: 1263831
Conc: 24.78 ng/ml m