

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072520\
 Data File : P0069999.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2020 17:10
 Operator : DD\AJ
 Sample : L3383-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CRT-013

Manual Integrations
 APPROVED

Ankita
 7/27/2020 12:25:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 00:00:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 23 02:12:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.372	3.551	888905	990140	25.895	27.470
2) SA Decachlor...	10.009	8.752	1314793	1202104	24.607m	23.570m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072520\
Data File : P0069999.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2020 17:10
Operator : DD\AJ
Sample : L3383-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CRT-013


Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 00:00:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 23 02:12:36 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

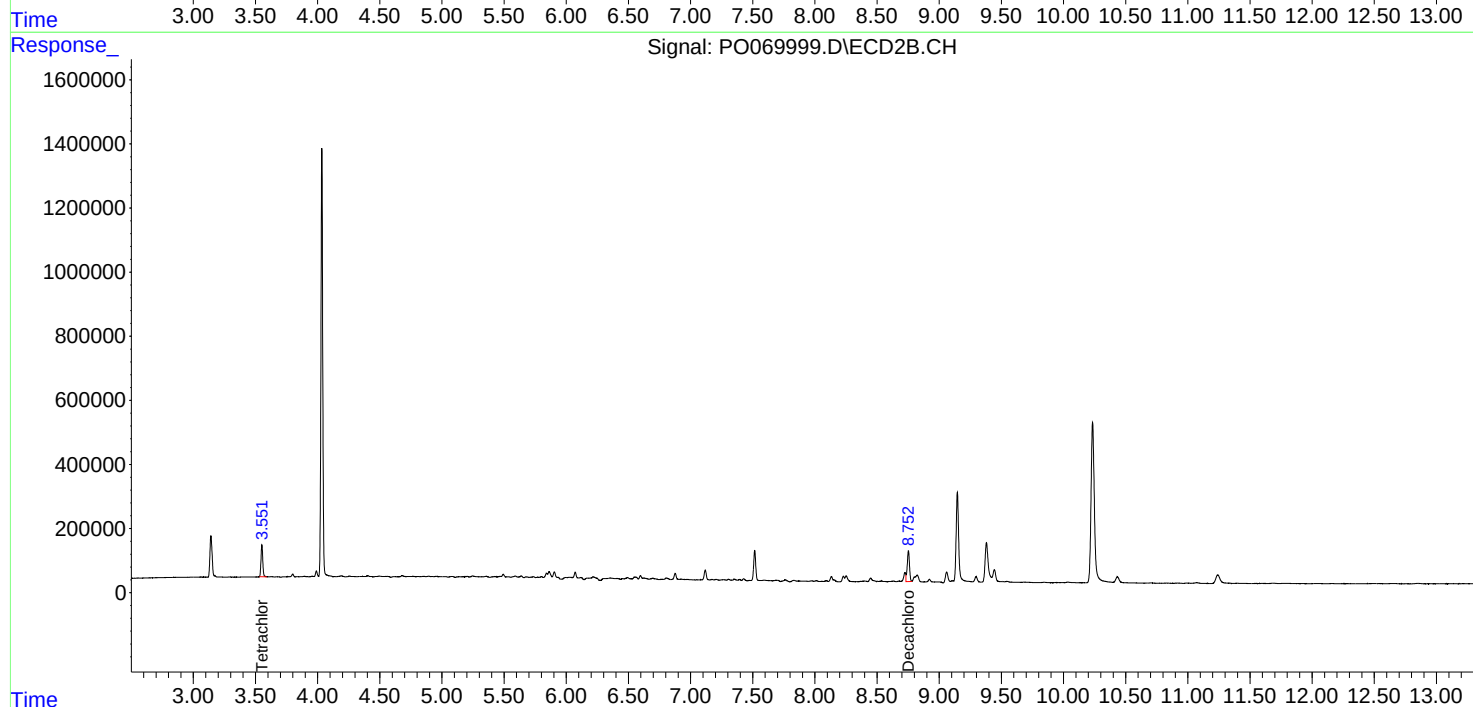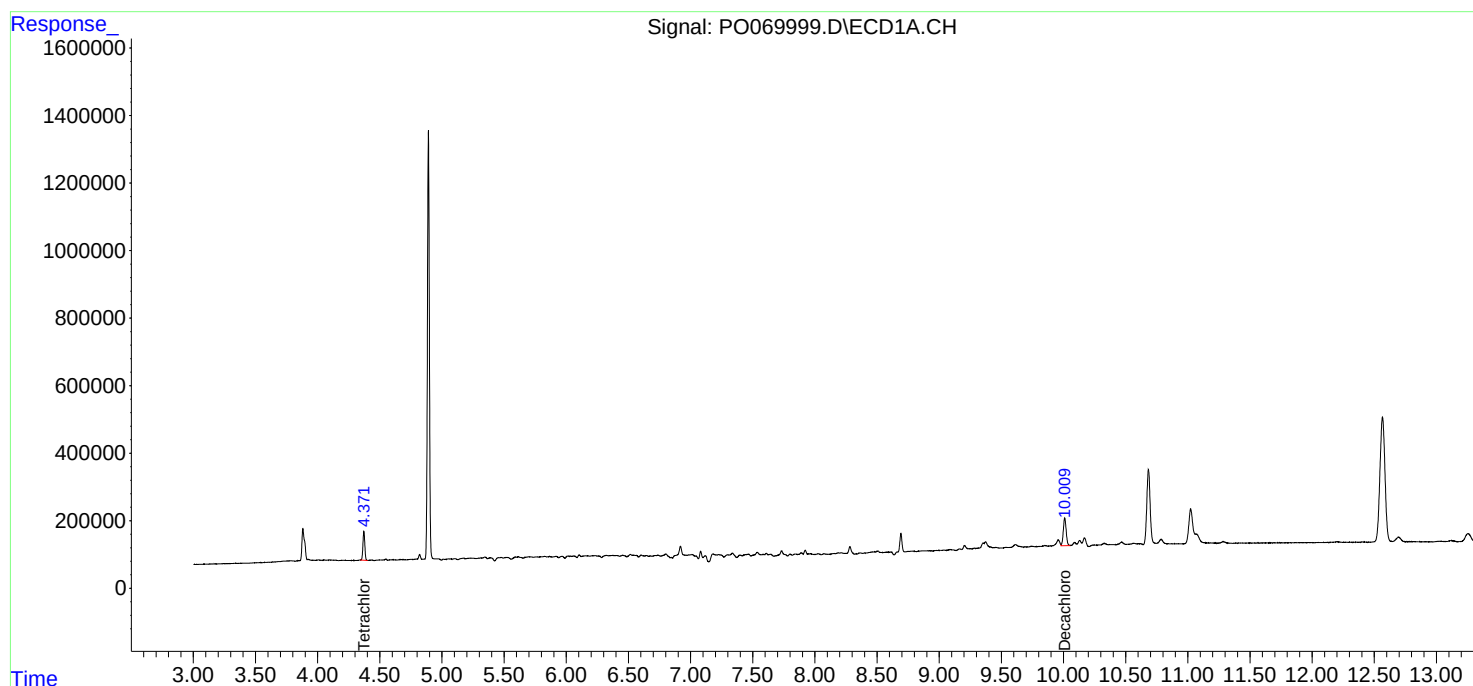

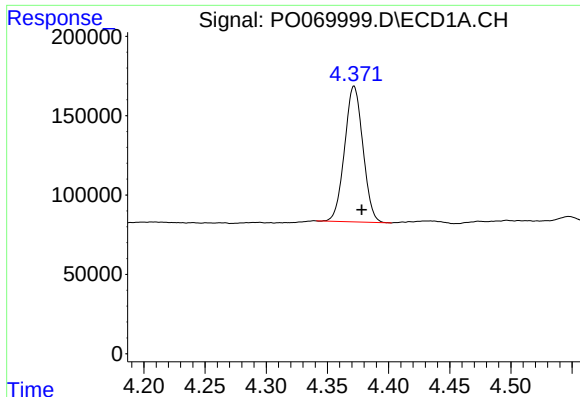


#1 Tetrachloro-m-xylene

R.T.: 4.372 min
Delta R.T.: -0.006 min
Response: 888905
Conc: 25.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
CRT-013


Manual Integrations
APPROVED

Ankita
7/27/2020 12:25:46 PM

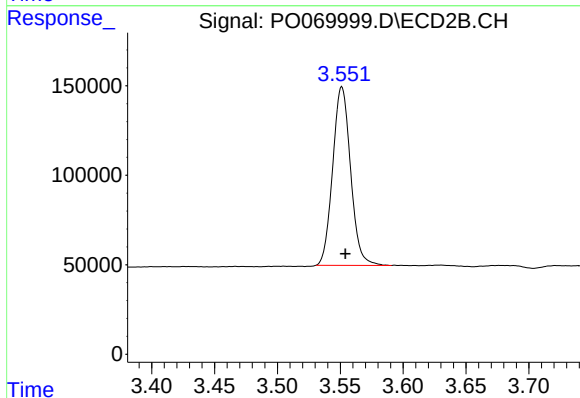


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: -0.003 min
Response: 990140
Conc: 27.47 ng/ml

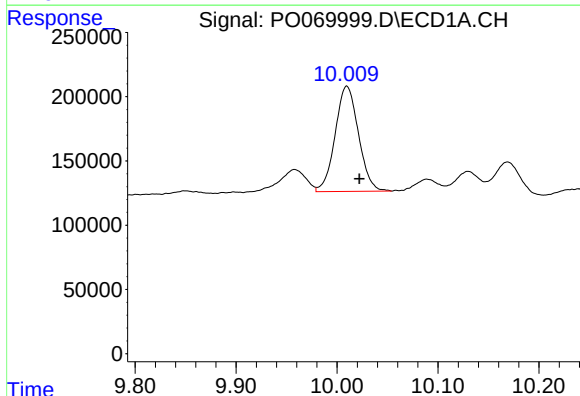

#2 Decachlorobiphenyl

R.T.: 10.009 min
Delta R.T.: -0.013 min
Response: 1314793
Conc: 24.61 ng/ml m

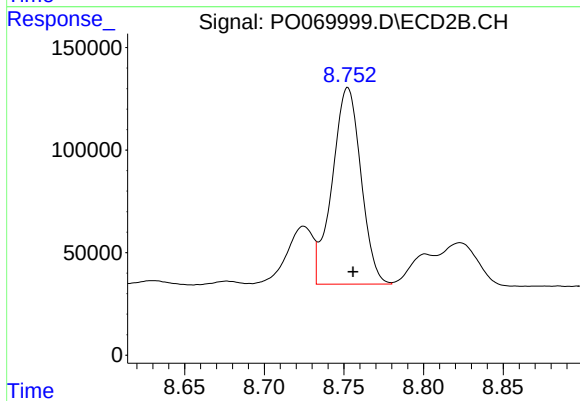

#2 Decachlorobiphenyl

R.T.: 8.752 min
Delta R.T.: -0.004 min
Response: 1202104
Conc: 23.57 ng/ml m