

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072520\
 Data File : P0070005.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2020 18:53
 Operator : DD\AJ
 Sample : L3383-29
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CRT-002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 25 00:03:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 23 02:12:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.373	3.552	724404	807170	21.103	22.394
2) SA Decachlor...	10.010	8.753	1139114	1065024	21.319	20.882

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072520\
Data File : P0070005.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2020 18:53
Operator : DD\AJ
Sample : L3383-29
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CRT-002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 25 00:03:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072320.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 23 02:12:36 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

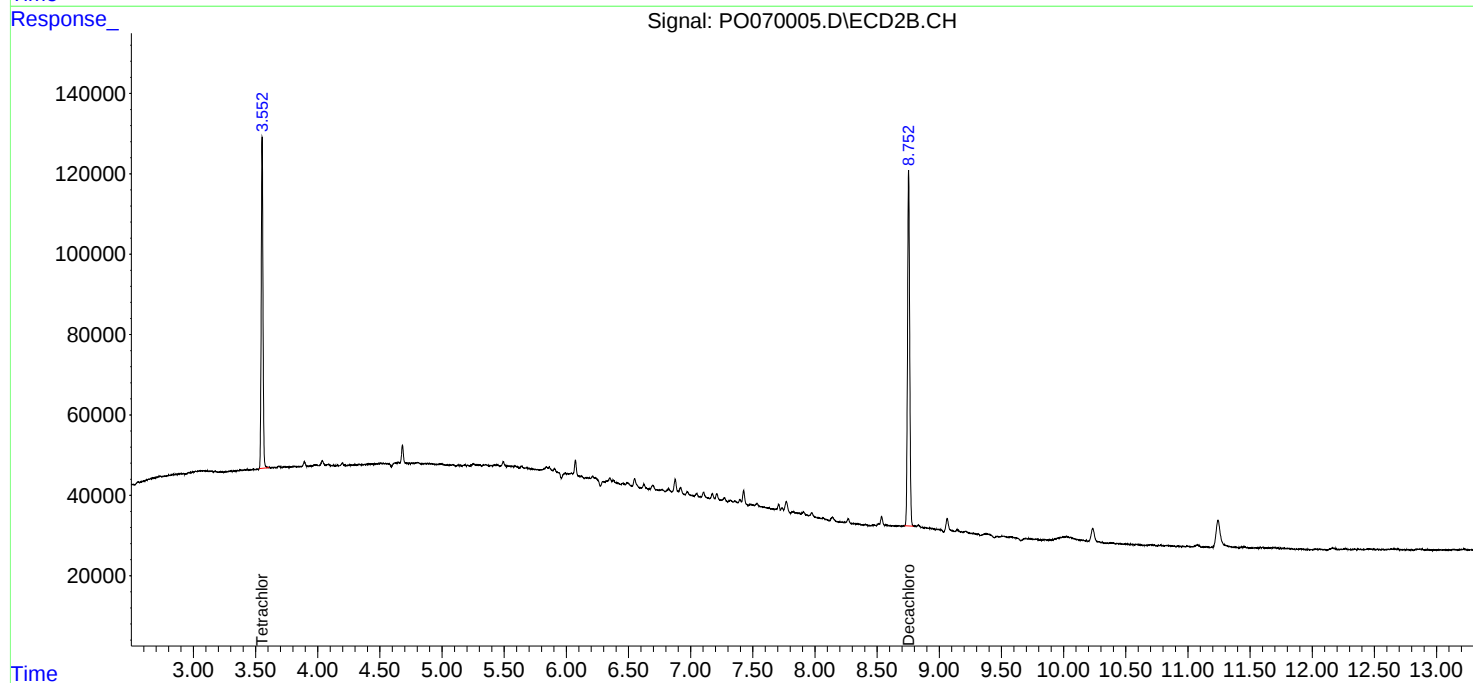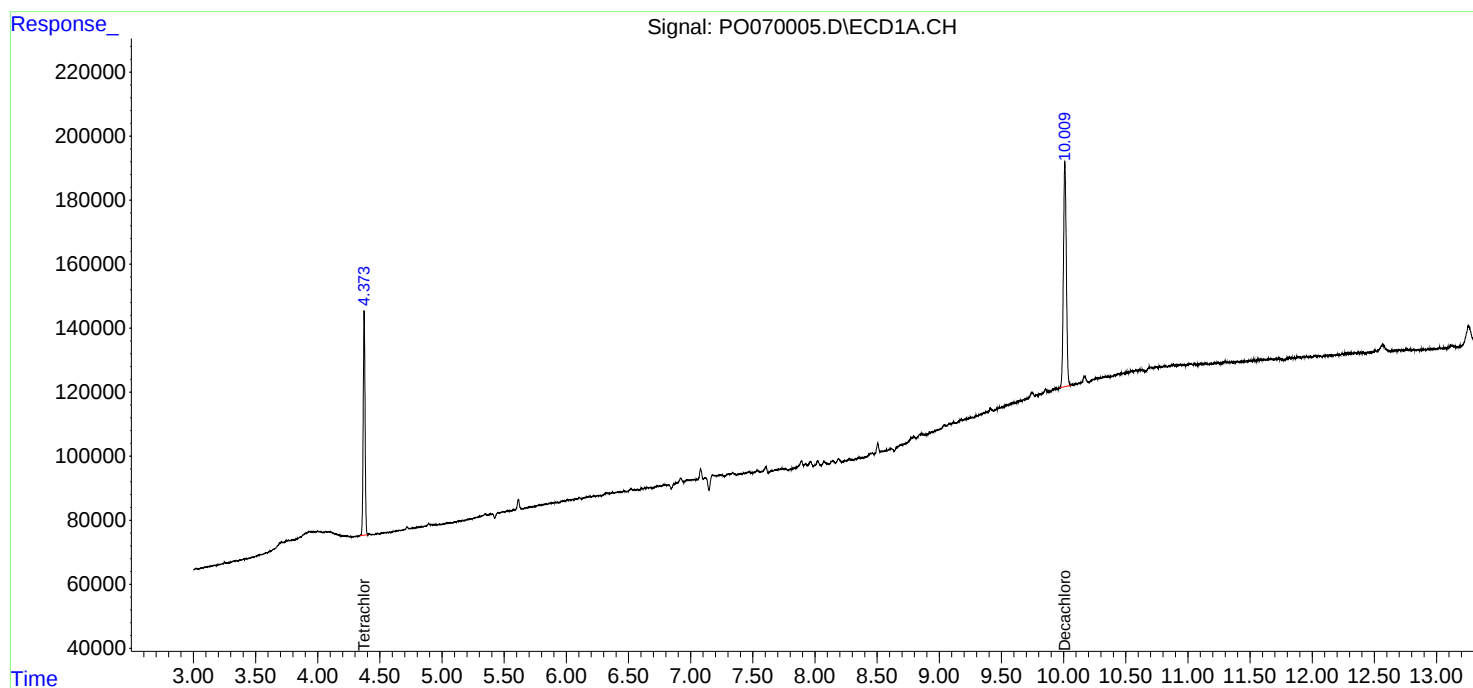


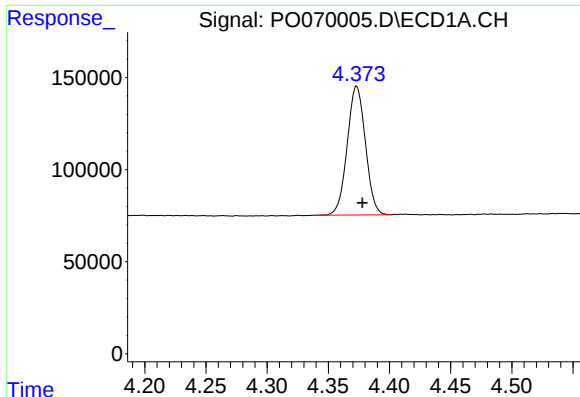

#1 Tetrachloro-m-xylene


R.T.: 4.373 min
Delta R.T.: -0.005 min
Response: 724404
Conc: 21.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
CRT-002

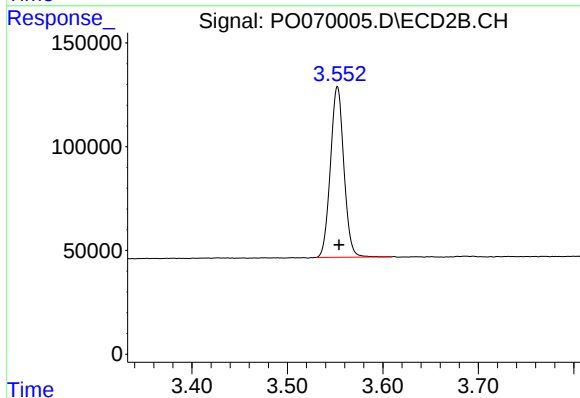


#1 Tetrachloro-m-xylene

R.T.: 3.552 min
Delta R.T.: -0.002 min
Response: 807170
Conc: 22.39 ng/ml

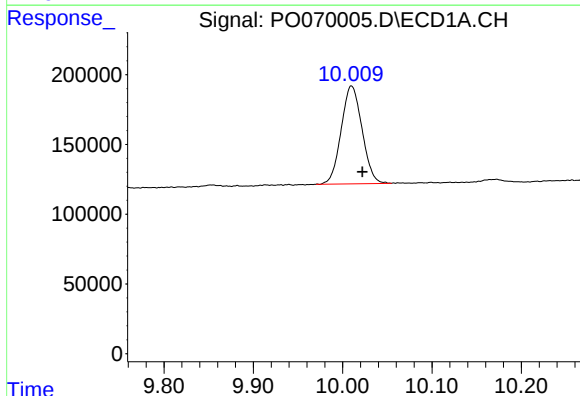

#2 Decachlorobiphenyl

R.T.: 10.010 min
Delta R.T.: -0.012 min
Response: 1139114
Conc: 21.32 ng/ml

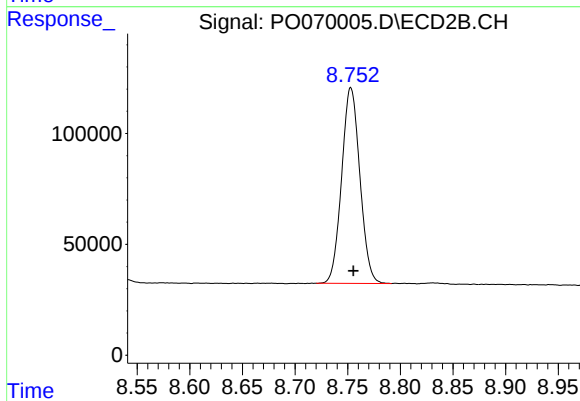

#2 Decachlorobiphenyl

R.T.: 8.753 min
Delta R.T.: -0.003 min
Response: 1065024
Conc: 20.88 ng/ml