

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072524\
 Data File : P0104953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2024 14:40
 Operator : YP/AJ
 Sample : P3353-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLEAN-PADS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/26/2024
 Supervised By :Ankita Jodhani 07/26/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 08:59:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.428	3.540	132.0E6	49597978	14.748	15.202
2) SA Decachlor...	10.214	8.435	90529254	24988410	14.762m	11.916

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072524\
Data File : PO104953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2024 14:40
Operator : YP/AJ
Sample : P3353-02
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CLEAN-PADS


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 07/26/2024
Supervised By : Ankita Jodhani 07/26/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 08:59:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

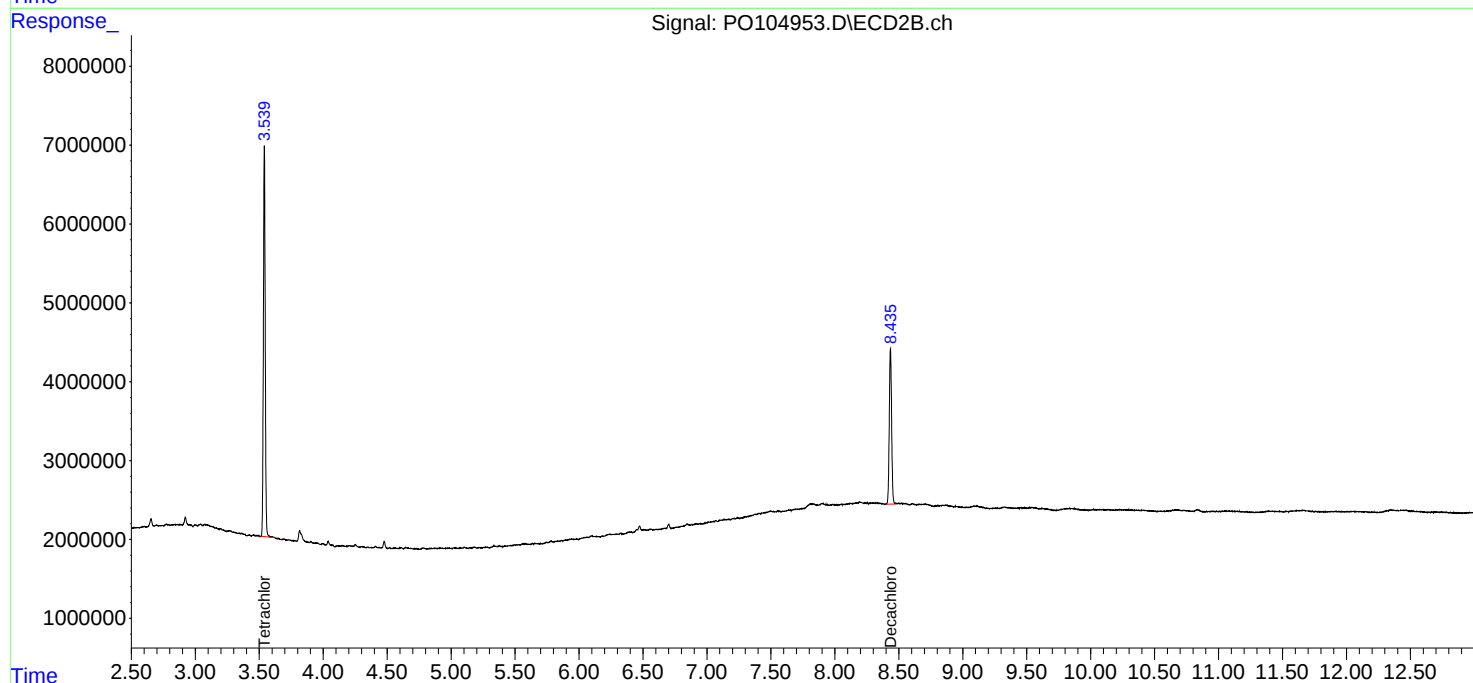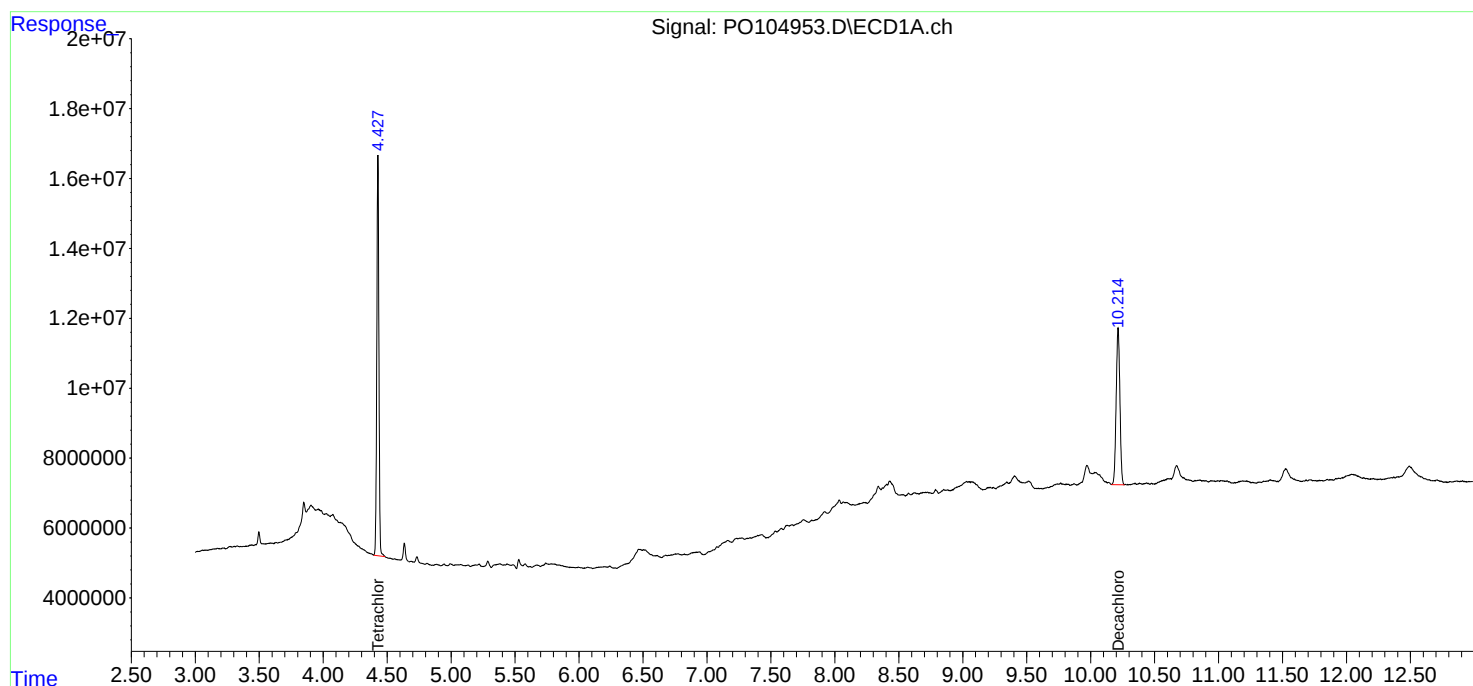

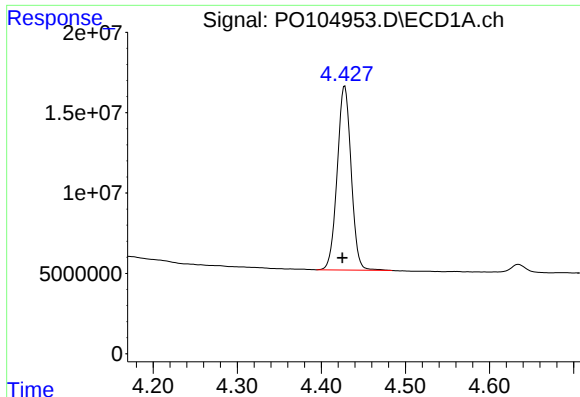

#1 Tetrachloro-m-xylene

R.T.: 4.428 min
Delta R.T.: 0.003 min
Response: 132043523
Conc: 14.75 ng/ml

Instrument :

ECD_O


ClientSampleId :

CLEAN-PADS

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 07/26/2024
Supervised By :Ankita Jodhani 07/26/2024

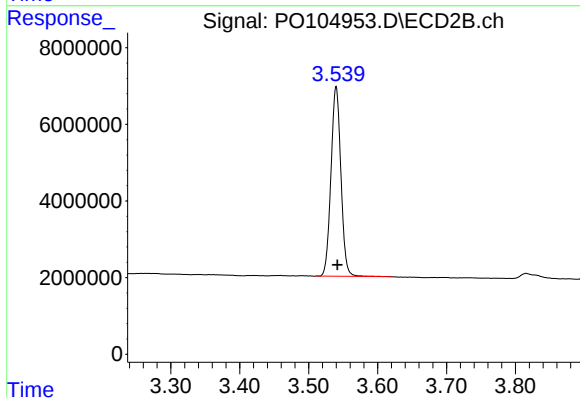


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.002 min
Response: 49597978
Conc: 15.20 ng/ml

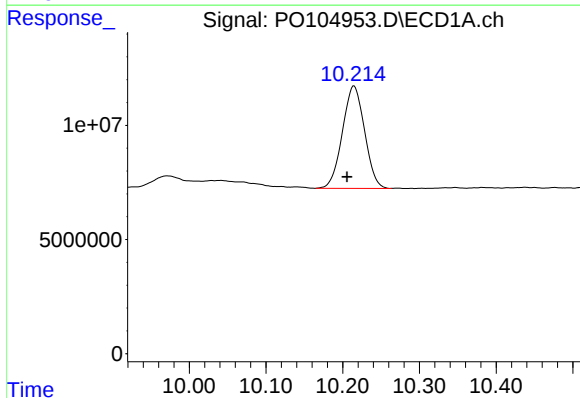

#2 Decachlorobiphenyl

R.T.: 10.214 min
Delta R.T.: 0.008 min
Response: 90529254
Conc: 14.76 ng/ml m

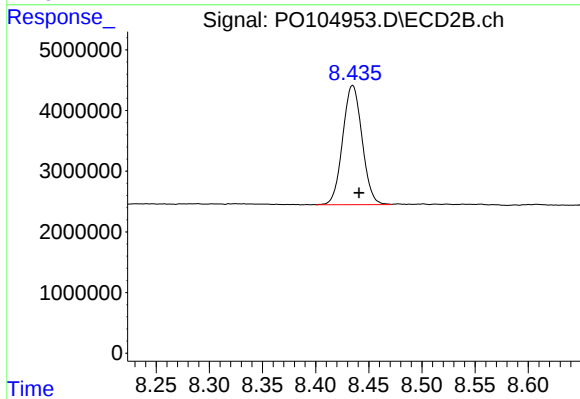

#2 Decachlorobiphenyl

R.T.: 8.435 min
Delta R.T.: -0.006 min
Response: 24988410
Conc: 11.92 ng/ml