

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072525\
 Data File : P0112528.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jul 2025 19:41
 Operator : YP/AJ
 Sample : Q2691-05 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 298

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/28/2025
 Supervised By :mohammad ahmed 07/29/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 00:49:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.673	3.665	55041169	19738454	6.769m	3.972 #
2) SA Decachlor...	8.690	8.637	17418872	3545228	2.382m	2.006m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072525\
Data File : P0112528.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jul 2025 19:41
Operator : YP/AJ
Sample : Q2691-05 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
298


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2025
Supervised By :mohammad ahmed 07/29/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 00:49:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

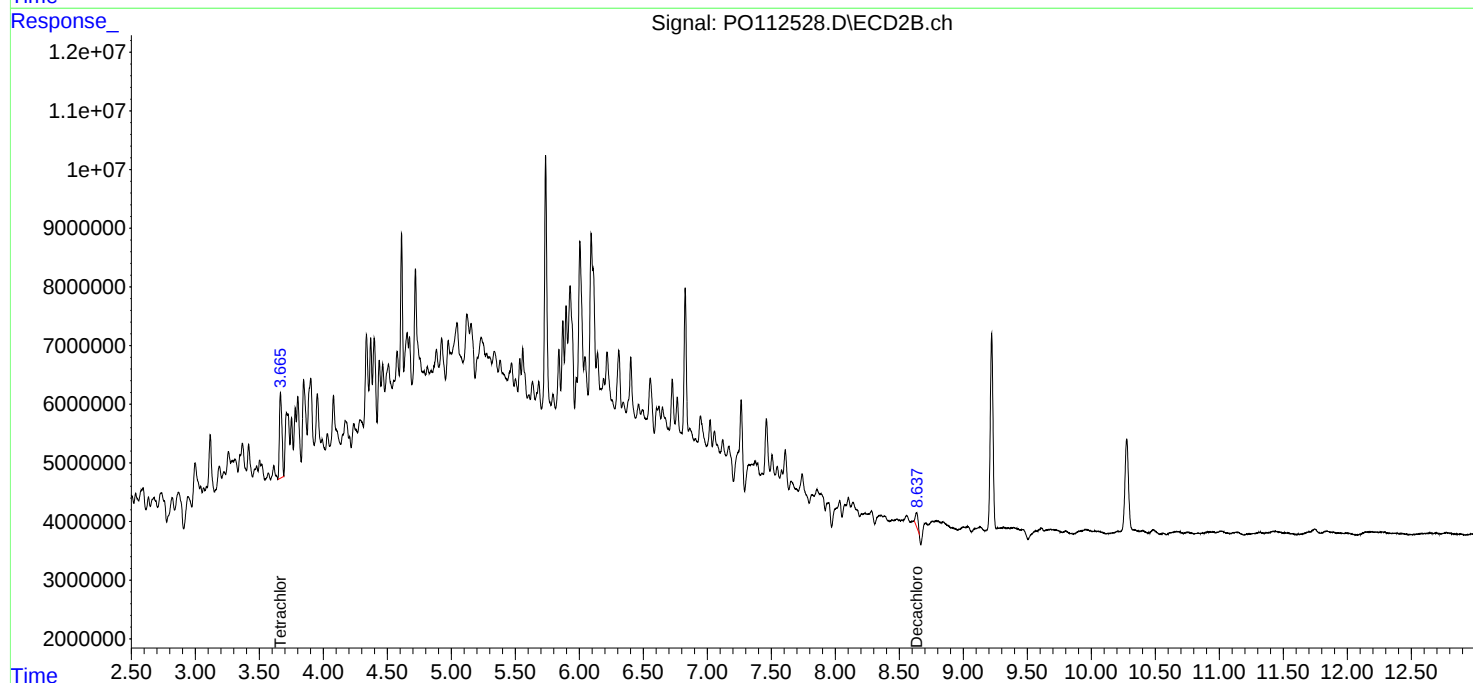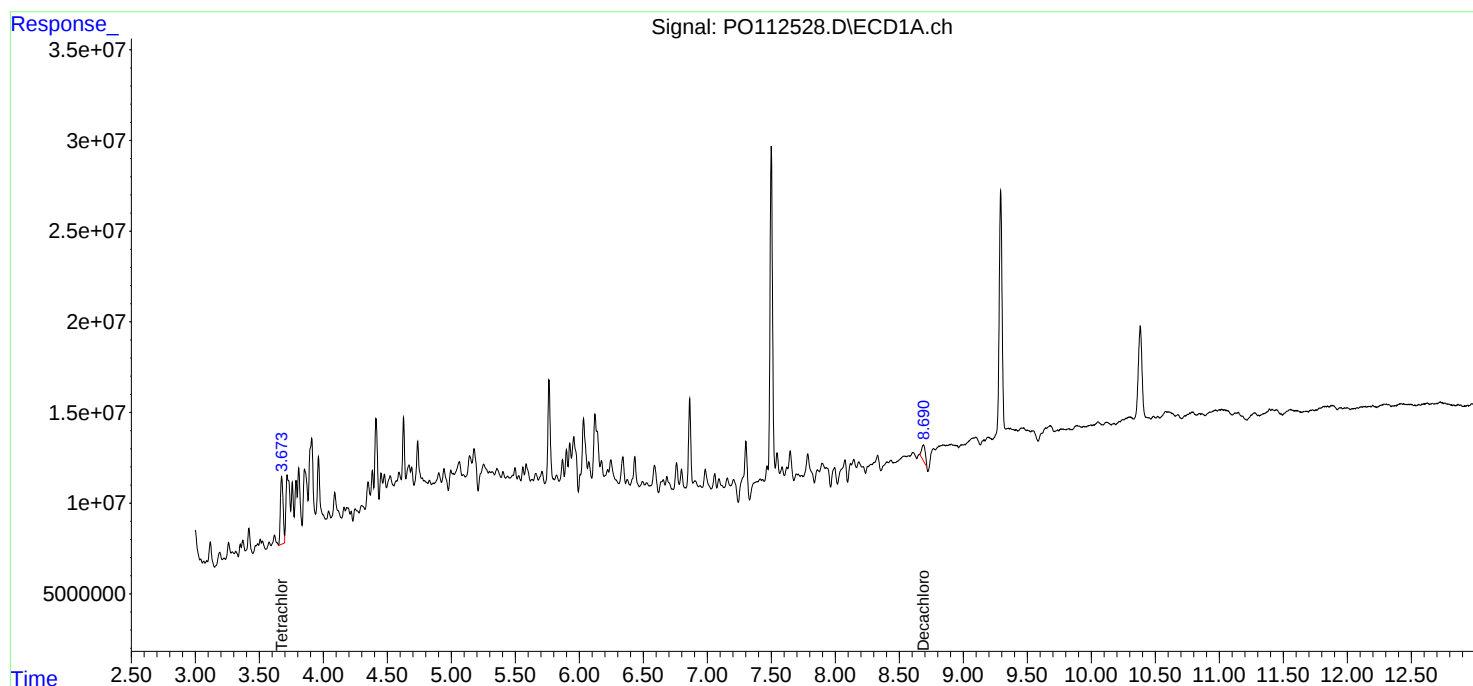

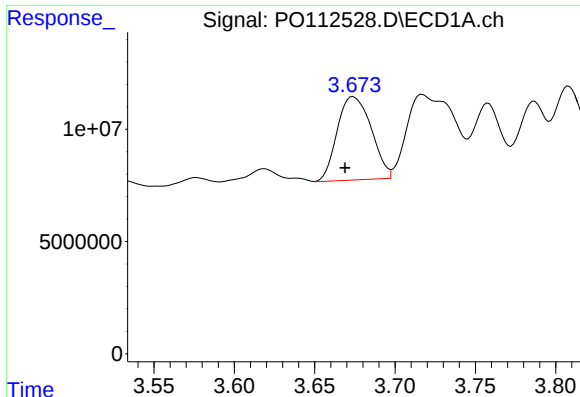


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: 0.004 min
Response: 55041169
Conc: 6.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
298


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2025
Supervised By :mohammad ahmed 07/29/2025

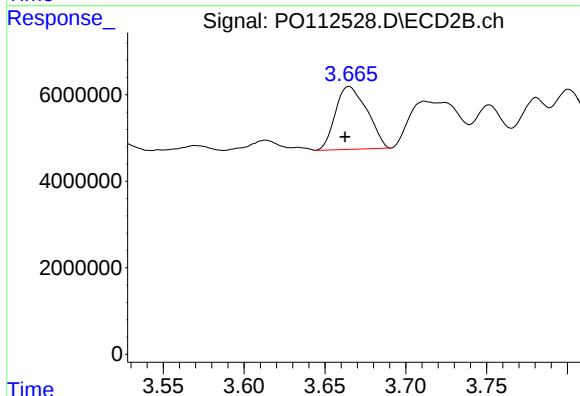


#1 Tetrachloro-m-xylene

R.T.: 3.665 min
Delta R.T.: 0.003 min
Response: 19738454
Conc: 3.97 ng/ml

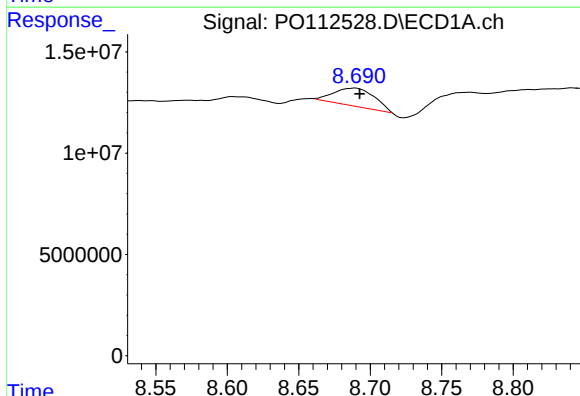

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.002 min
Response: 17418872
Conc: 2.38 ng/ml m

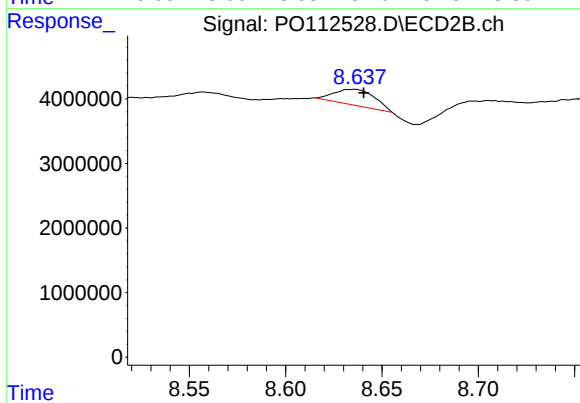

#2 Decachlorobiphenyl

R.T.: 8.637 min
Delta R.T.: -0.003 min
Response: 3545228
Conc: 2.01 ng/ml m