

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072621\
 Data File : P0079858.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jul 2021 19:44
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 05:11:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 23 05:30:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.003	4.123	1085125	467968	19.189	21.049
2) SA Decachlor...	11.115	9.535	925261	452608	23.413	26.389
Target Compounds						
8) L2 AR-1221-1	5.257	0.000	32846	0	55.012	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072621\
Data File : P0079858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jul 2021 19:44
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 05:11:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 23 05:30:42 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

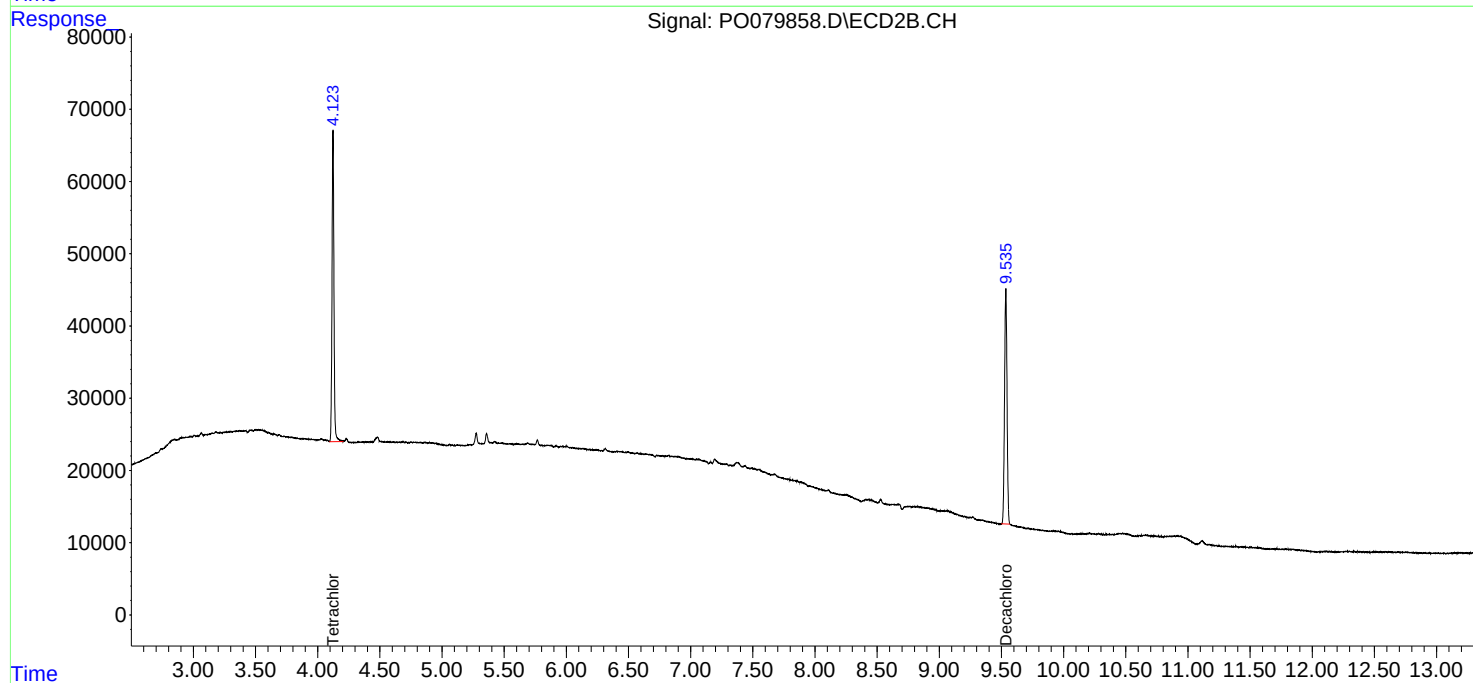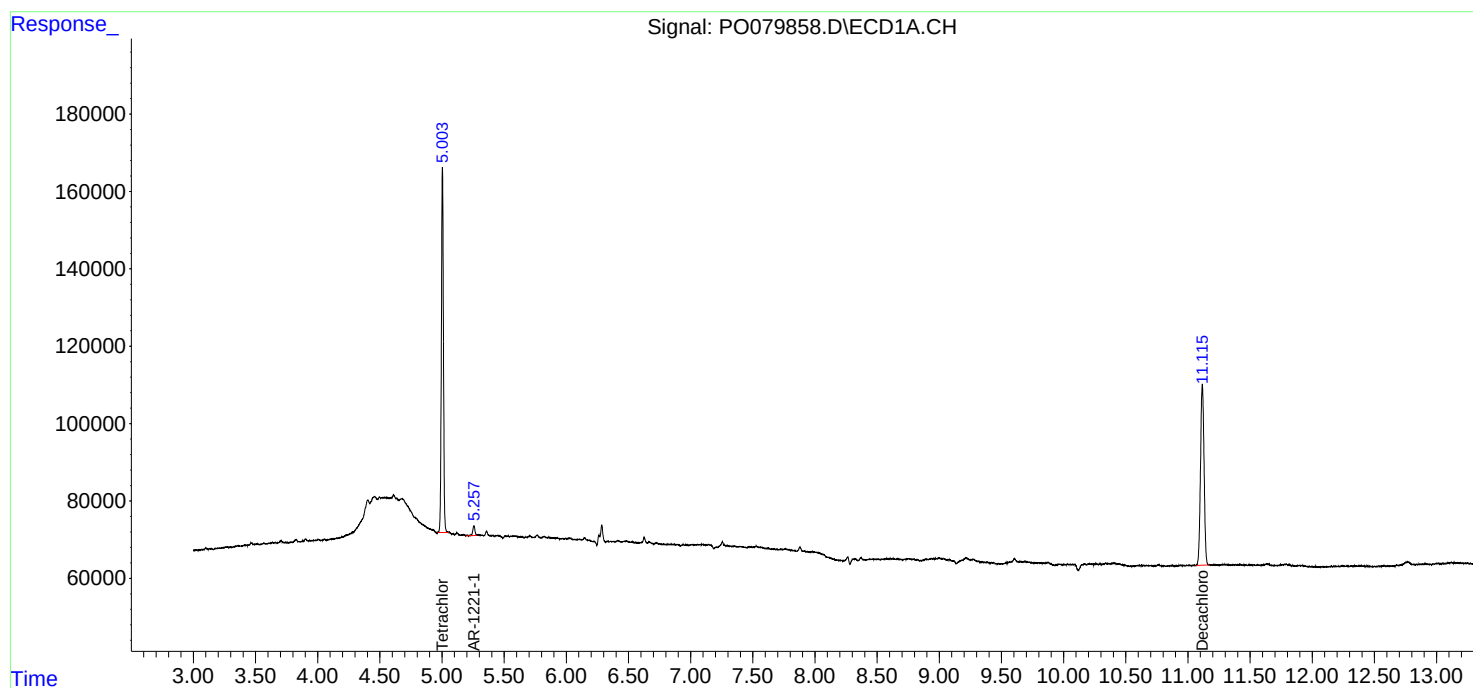


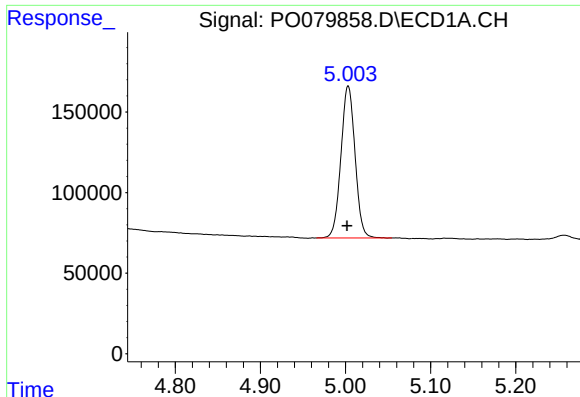

#1 Tetrachloro-m-xylene


R.T.: 5.003 min
Delta R.T.: 0.001 min
Response: 1085125
Conc: 19.19 ng/ml

Instrument :
ECD_O
ClientSampleId :

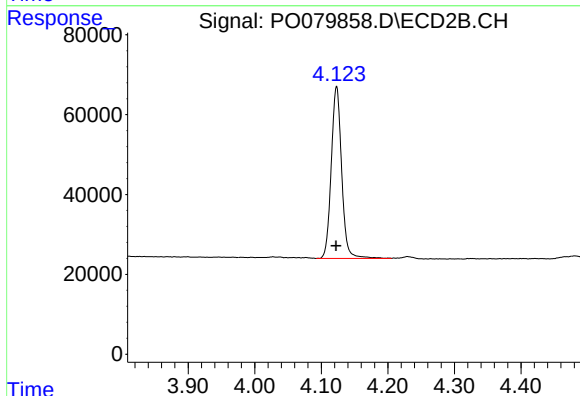


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.001 min
Response: 467968
Conc: 21.05 ng/ml

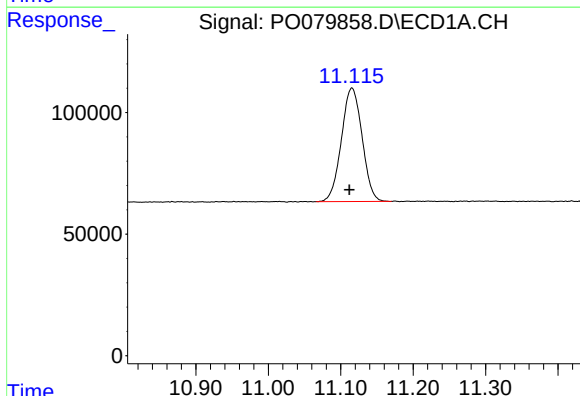


#2 Decachlorobiphenyl

R.T.: 11.115 min
Delta R.T.: 0.003 min
Response: 925261
Conc: 23.41 ng/ml

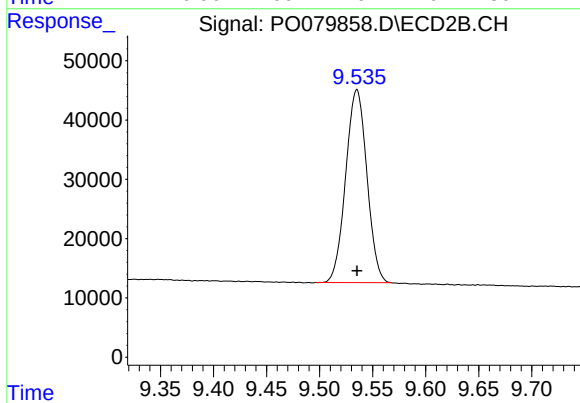

#2 Decachlorobiphenyl

R.T.: 9.535 min
Delta R.T.: 0.000 min
Response: 452608
Conc: 26.39 ng/ml

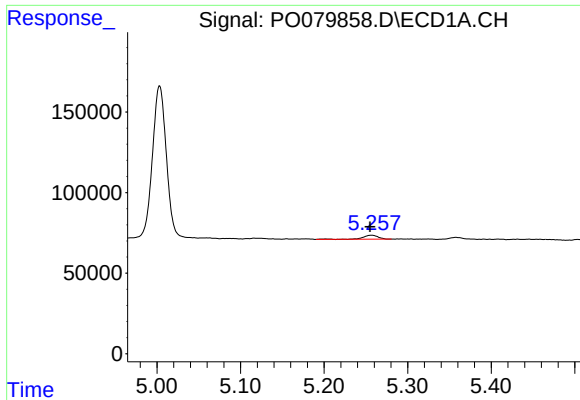

#8 AR-1221-1


R.T.: 5.257 min

Delta R.T.: 0.002 min

Response: 32846

Conc: 55.01 ng/ml

Instrument :
ECD_O
ClientSampleId :

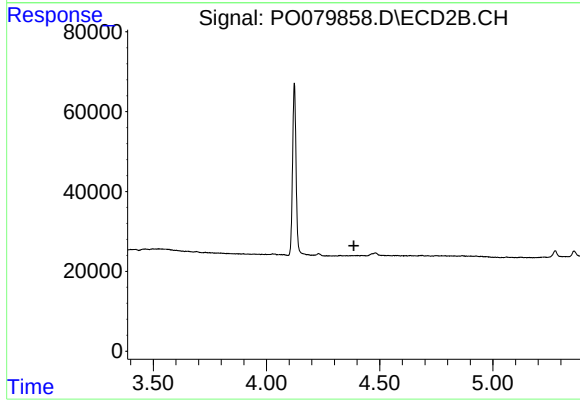

#8 AR-1221-1

R.T.: 0.000 min

Exp R.T. : 4.386 min

Response: 0

Conc: N.D.