

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072621\
 Data File : P0079879.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jul 2021 1:48
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 05:14:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 23 05:30:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.003	4.122	1114091	465766	19.701	20.950
2)	SA Decachlor...	11.115	9.535	1027495	471684	26.000	27.501
Target Compounds							
8)	L2 AR-1221-1	5.256	0.000	32978	0	55.232	N.D. #
9)	L2 AR-1221-2	0.000	4.480	0	10925	N.D.	57.508 #
24)	L5 AR-1248-4	7.254f	0.000	80838	0	38.526	N.D. #
26)	L6 AR-1254-1	7.254	0.000	80838	0	40.460	N.D. #
28)	L6 AR-1254-3	7.878f	0.000	18169	0	5.659	N.D. #
32)	L7 AR-1260-2	0.000	7.193f	0	10451	N.D.	7.378 #
43)	L9 AR-1268-3	0.000	8.683	0	22039	N.D.	8.948 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072621\
Data File : P0079879.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2021 1:48
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 05:14:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 23 05:30:42 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

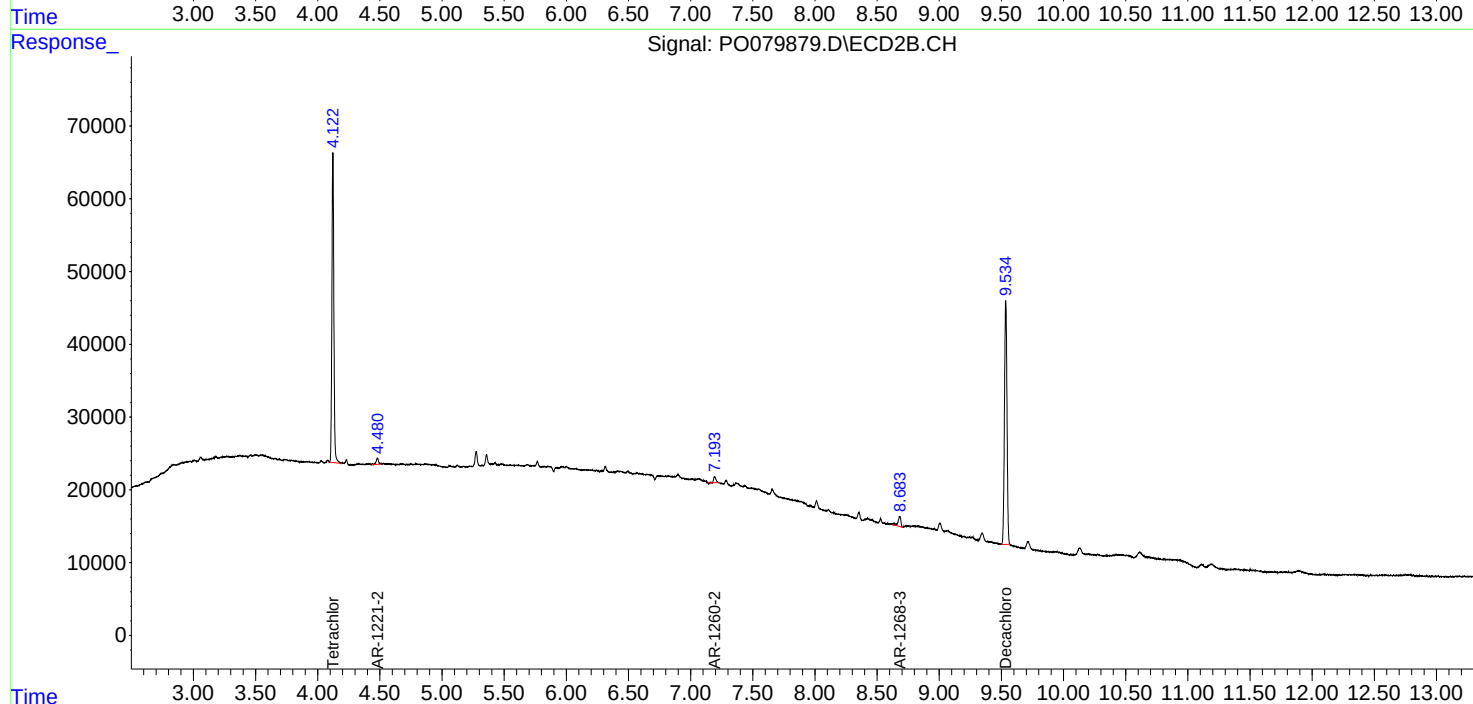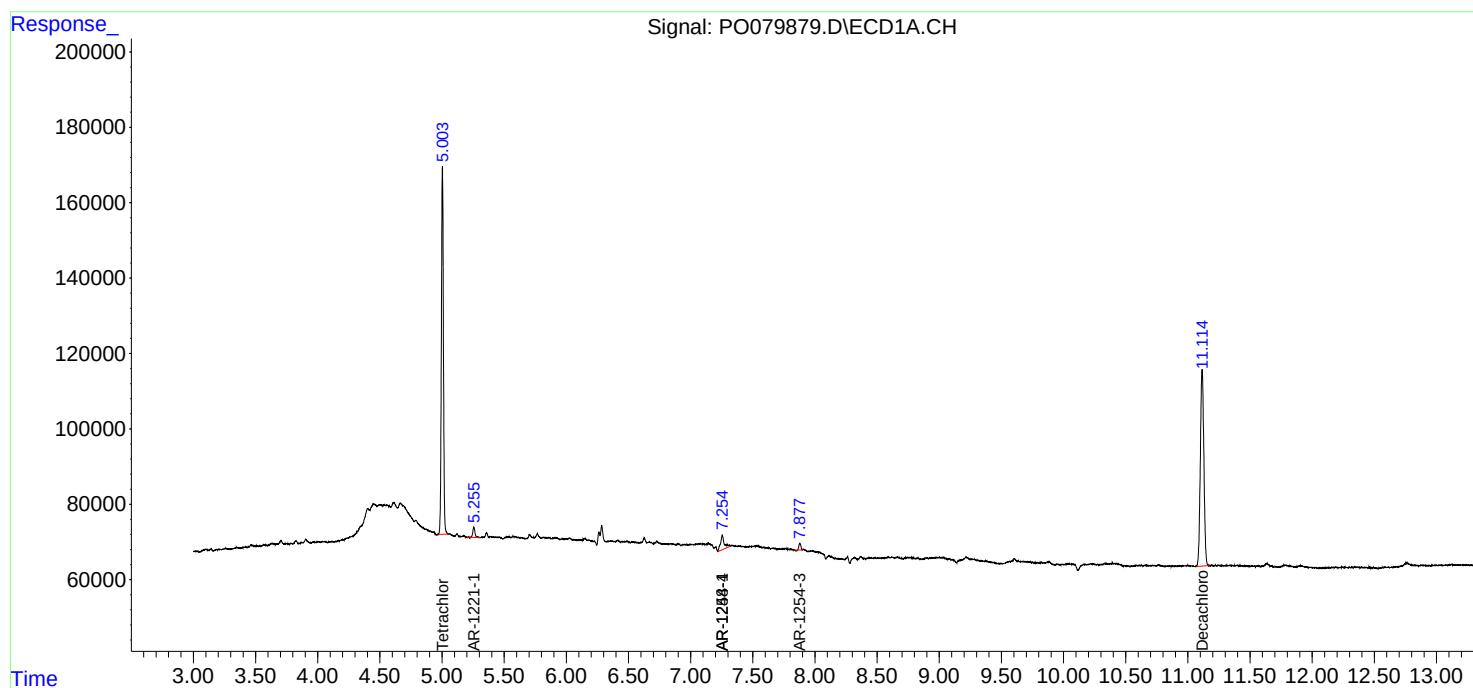


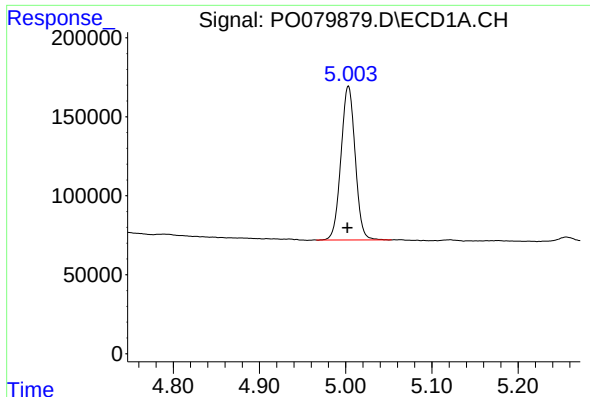

#1 Tetrachloro-m-xylene


R.T.: 5.003 min
Delta R.T.: 0.001 min
Response: 1114091
Conc: 19.70 ng/ml

Instrument :
ECD_O
ClientSampleId :

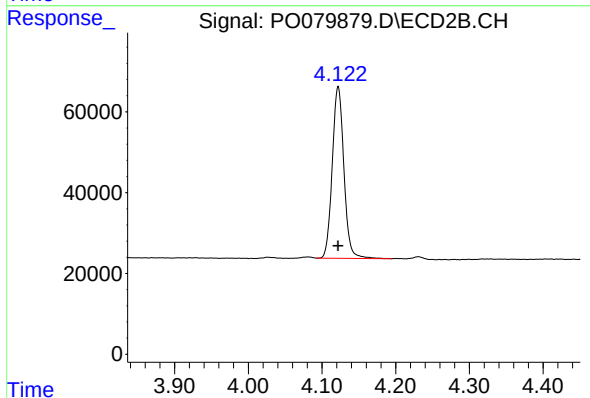


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.000 min
Response: 465766
Conc: 20.95 ng/ml

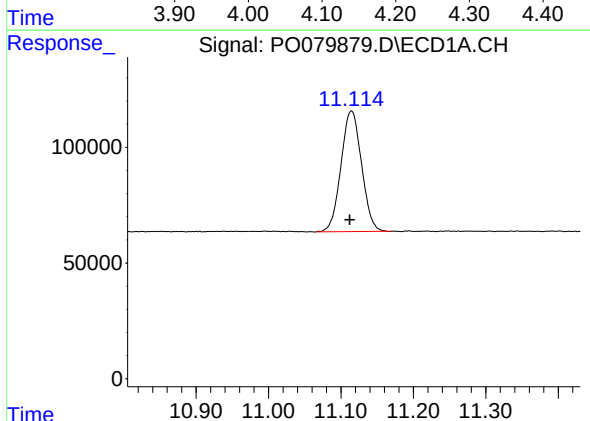


#2 Decachlorobiphenyl

R.T.: 11.115 min
Delta R.T.: 0.002 min
Response: 1027495
Conc: 26.00 ng/ml

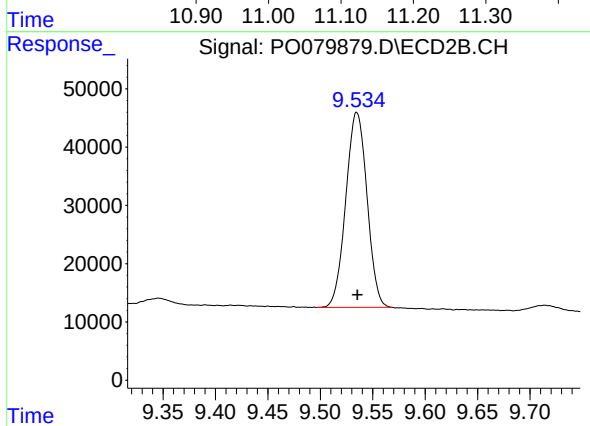

#2 Decachlorobiphenyl


R.T.: 9.535 min
Delta R.T.: 0.000 min
Response: 471684
Conc: 27.50 ng/ml

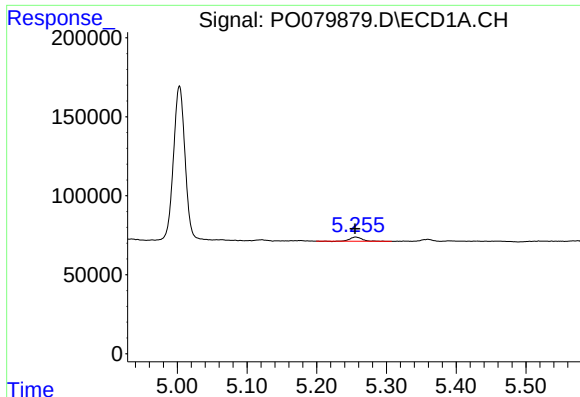

#8 AR-1221-1


R.T.: 5.256 min
Delta R.T.: 0.000 min
Response: 32978
Conc: 55.23 ng/ml

Instrument :
ECD_O
ClientSampleId :

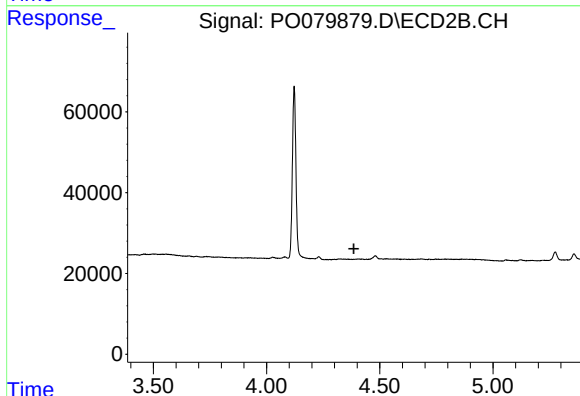


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.386 min
Response: 0
Conc: N.D.

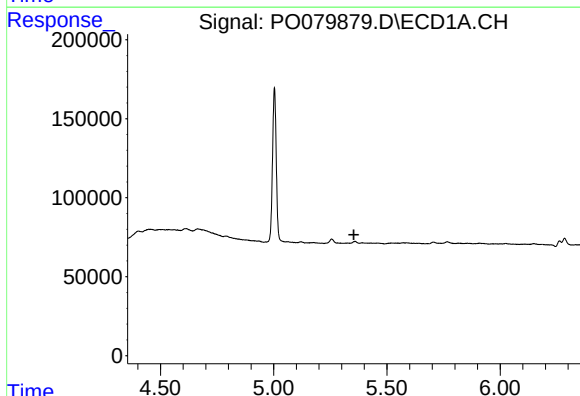


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.354 min
Response: 0
Conc: N.D.

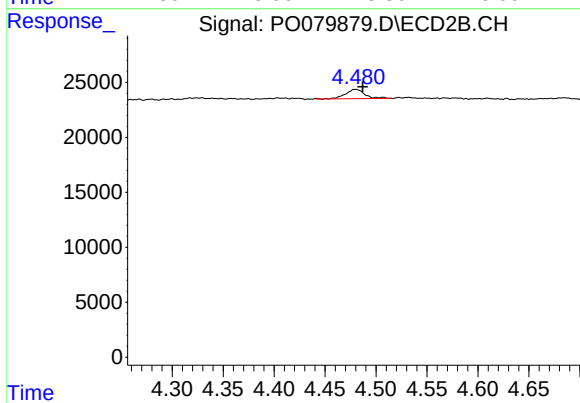

#9 AR-1221-2


R.T.: 4.480 min
Delta R.T.: -0.007 min
Response: 10925
Conc: 57.51 ng/ml

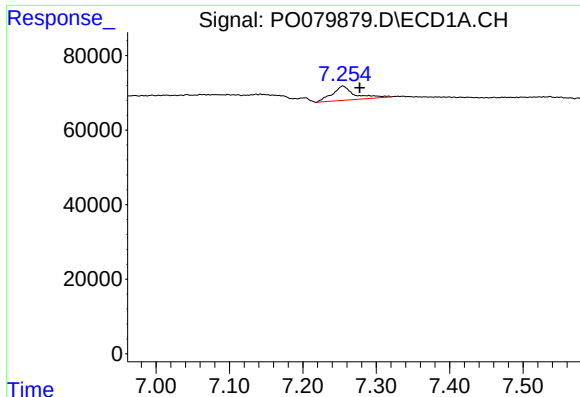

#24 AR-1248-4


R.T.: 7.254 min
Delta R.T.: -0.023 min
Response: 80838
Conc: 38.53 ng/ml

Instrument :
ECD_O
ClientSampleId :

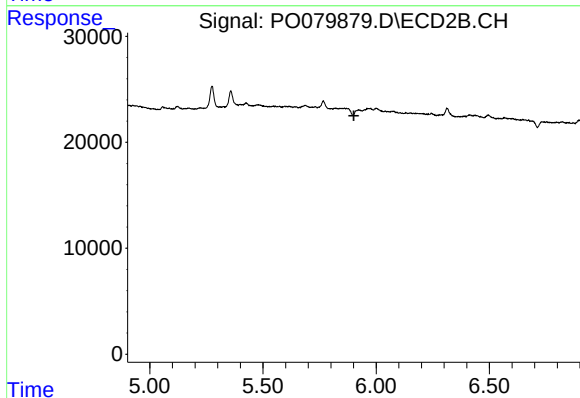


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.902 min
Response: 0
Conc: N.D.

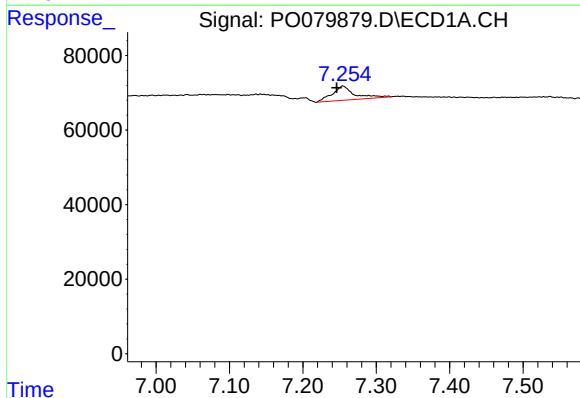


#26 AR-1254-1

R.T.: 7.254 min
Delta R.T.: 0.008 min
Response: 80838
Conc: 40.46 ng/ml

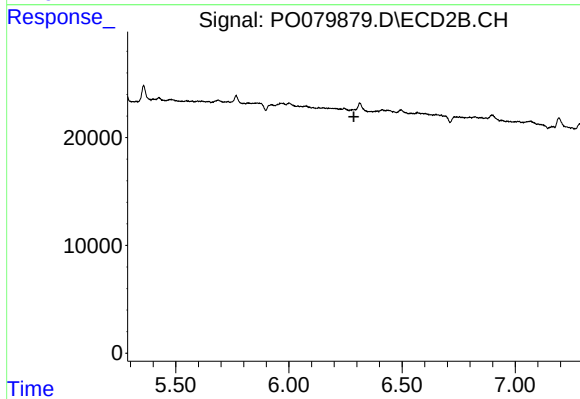

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

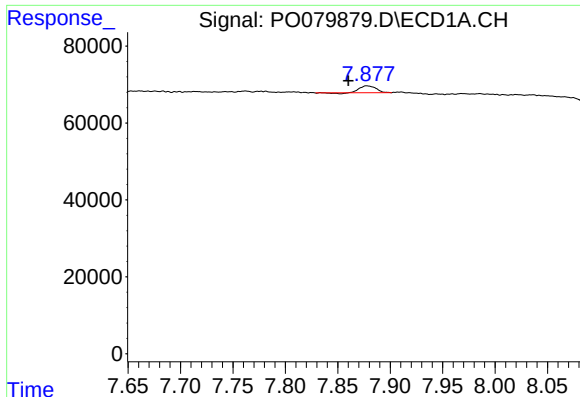

#28 AR-1254-3


R.T.: 7.878 min
Delta R.T.: 0.018 min
Response: 18169
Conc: 5.66 ng/ml

Instrument :
ECD_O
ClientSampleId :

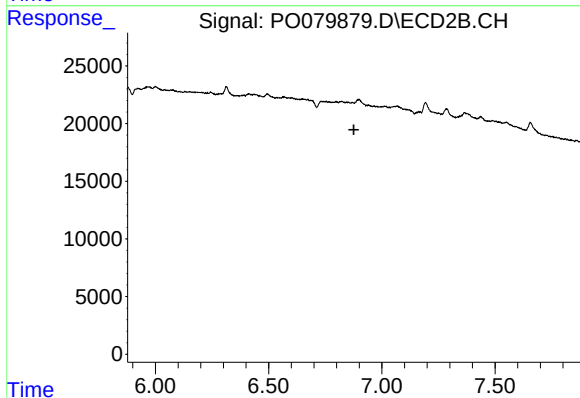


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.876 min
Response: 0
Conc: N.D.

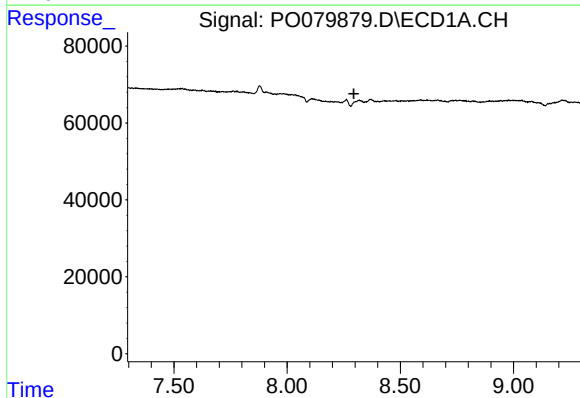


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.295 min
Response: 0
Conc: N.D.

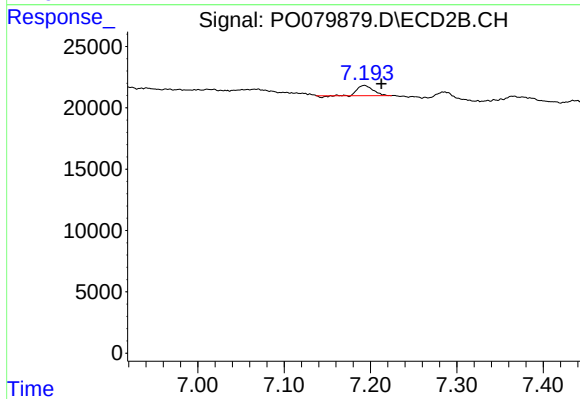

#32 AR-1260-2


R.T.: 7.193 min
Delta R.T.: -0.020 min
Response: 10451
Conc: 7.38 ng/ml

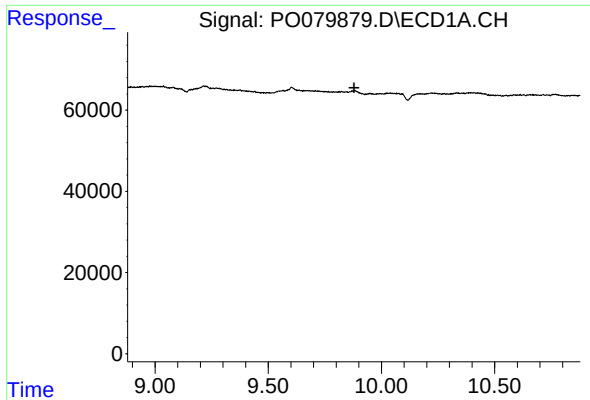

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.879 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

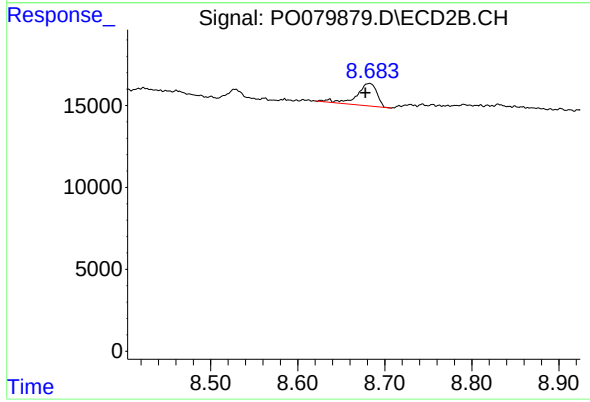

#43 AR-1268-3

R.T.: 8.683 min
Delta R.T.: 0.005 min
Response: 22039
Conc: 8.95 ng/ml