

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072623\
 Data File : P0096366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2023 10:18
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/27/2023
 Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 13:04:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 12:20:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.625	66635801	24865344	21.165	18.945
2) SA Decachlor...	10.228	8.651	47954174	24688292	24.370m	22.661

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072623\
Data File : P0096366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2023 10:18
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 13:04:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 12:20:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

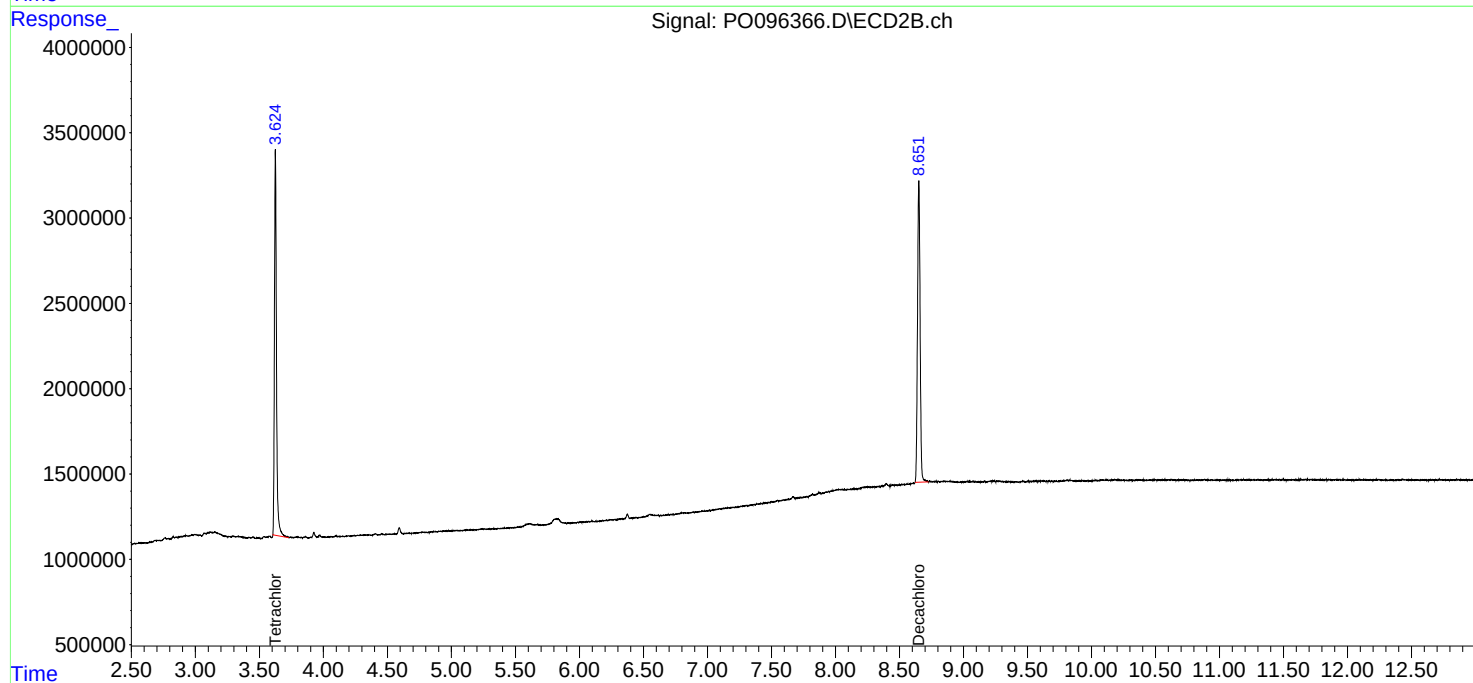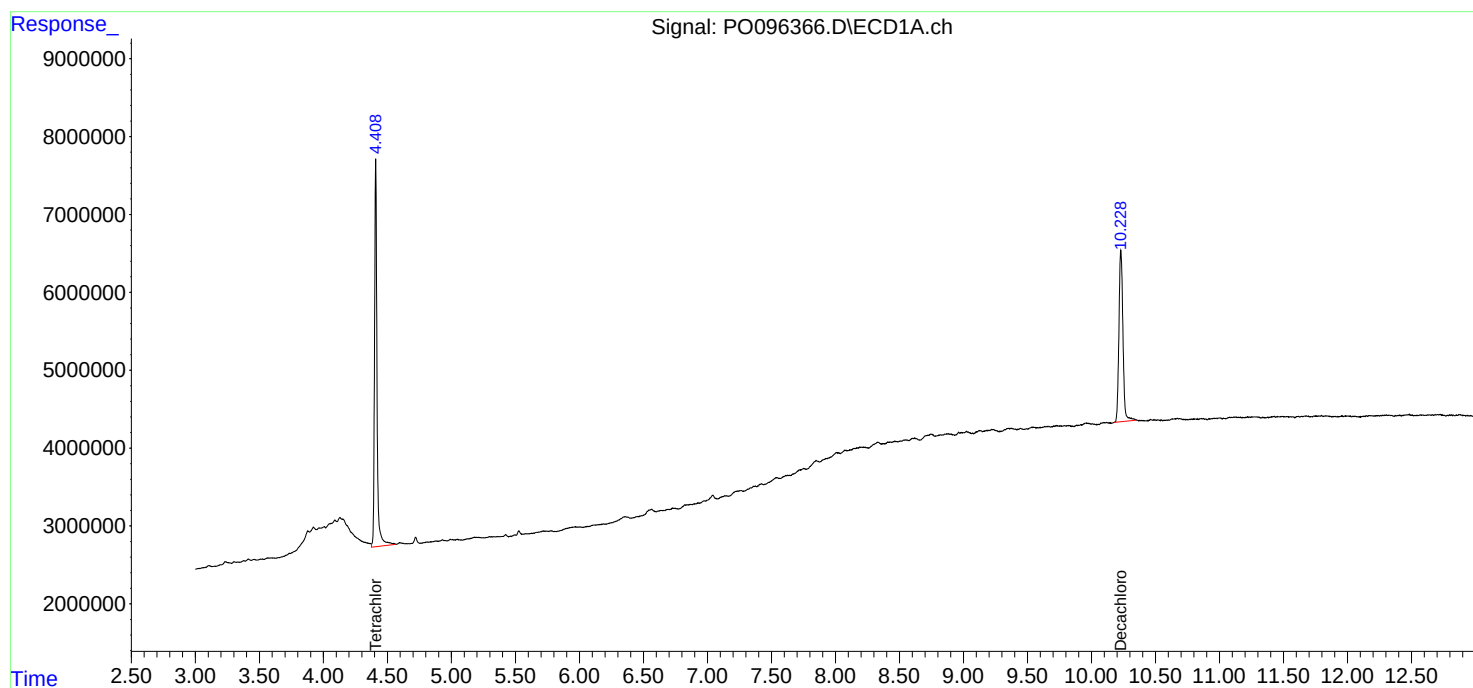

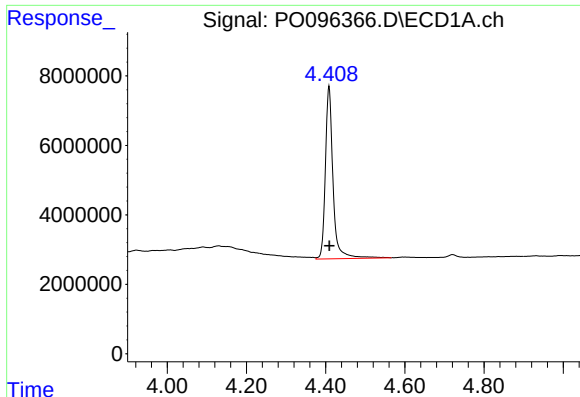


#1 Tetrachloro-m-xylene

R.T.: 4.409 min
Delta R.T.: -0.001 min
Response: 66635801
Conc: 21.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/27/2023
Supervised By :Ankita Jodhani 07/27/2023

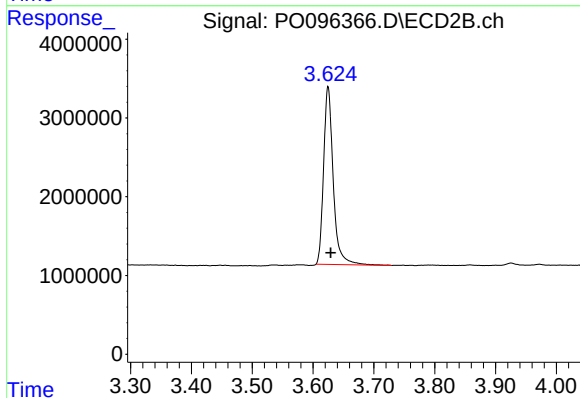


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: -0.004 min
Response: 24865344
Conc: 18.95 ng/ml

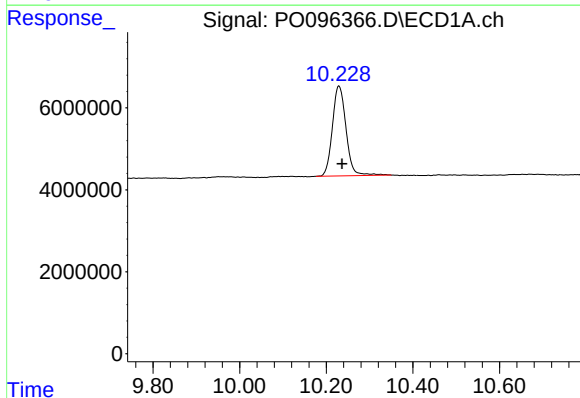

#2 Decachlorobiphenyl

R.T.: 10.228 min
Delta R.T.: -0.009 min
Response: 47954174
Conc: 24.37 ng/ml m

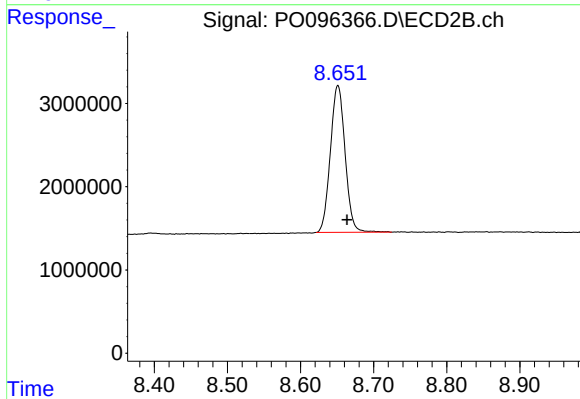

#2 Decachlorobiphenyl

R.T.: 8.651 min
Delta R.T.: -0.013 min
Response: 24688292
Conc: 22.66 ng/ml