

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072623\
 Data File : P0096399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2023 23:12
 Operator : YP/AJ
 Sample : 03775-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BUILDING-A-10-(0-5)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 03:07:11 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 22 12:20:47 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.626	59259645	19949881	18.822	15.200
2) SA Decachlor...	10.246	8.654	44443698	20427005	22.586	18.750

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072623\
Data File : P0096399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2023 23:12
Operator : YP/AJ
Sample : 03775-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BUILDING-A-10-(0-5)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 03:07:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072123.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 22 12:20:47 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

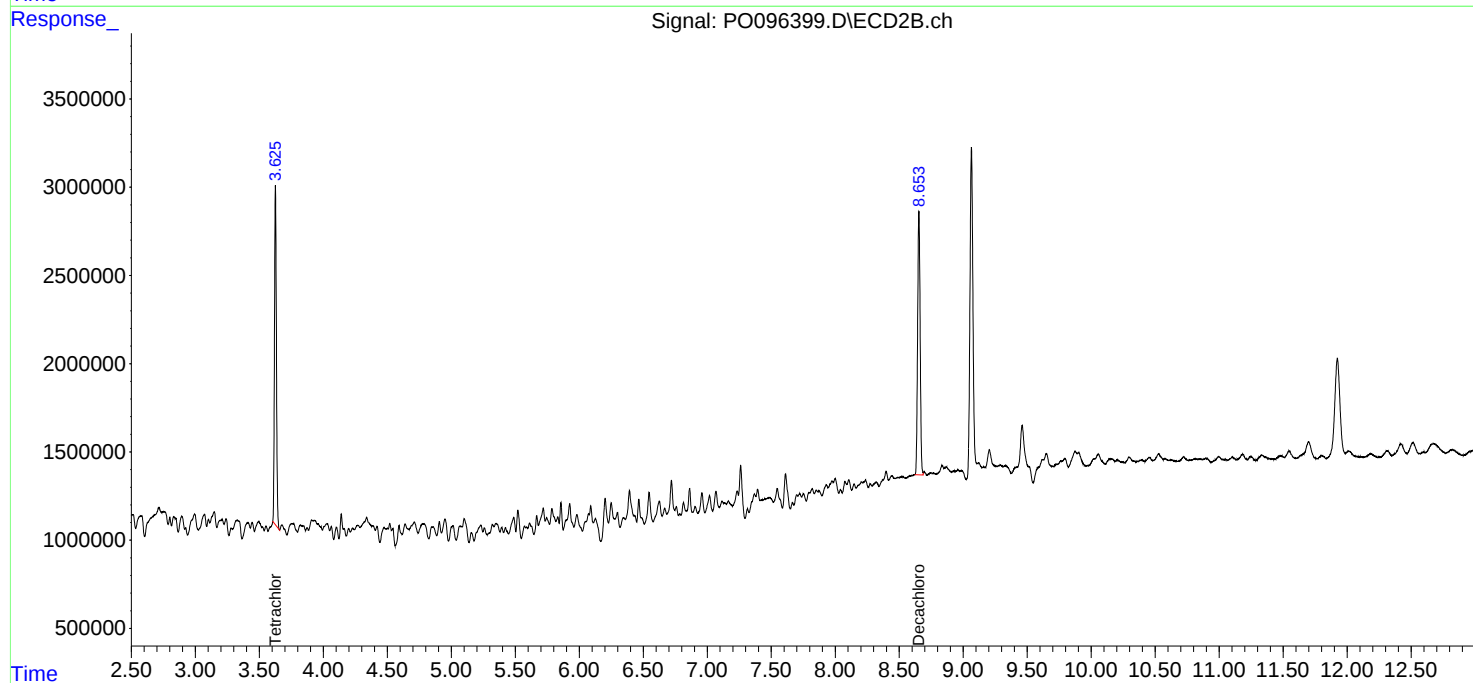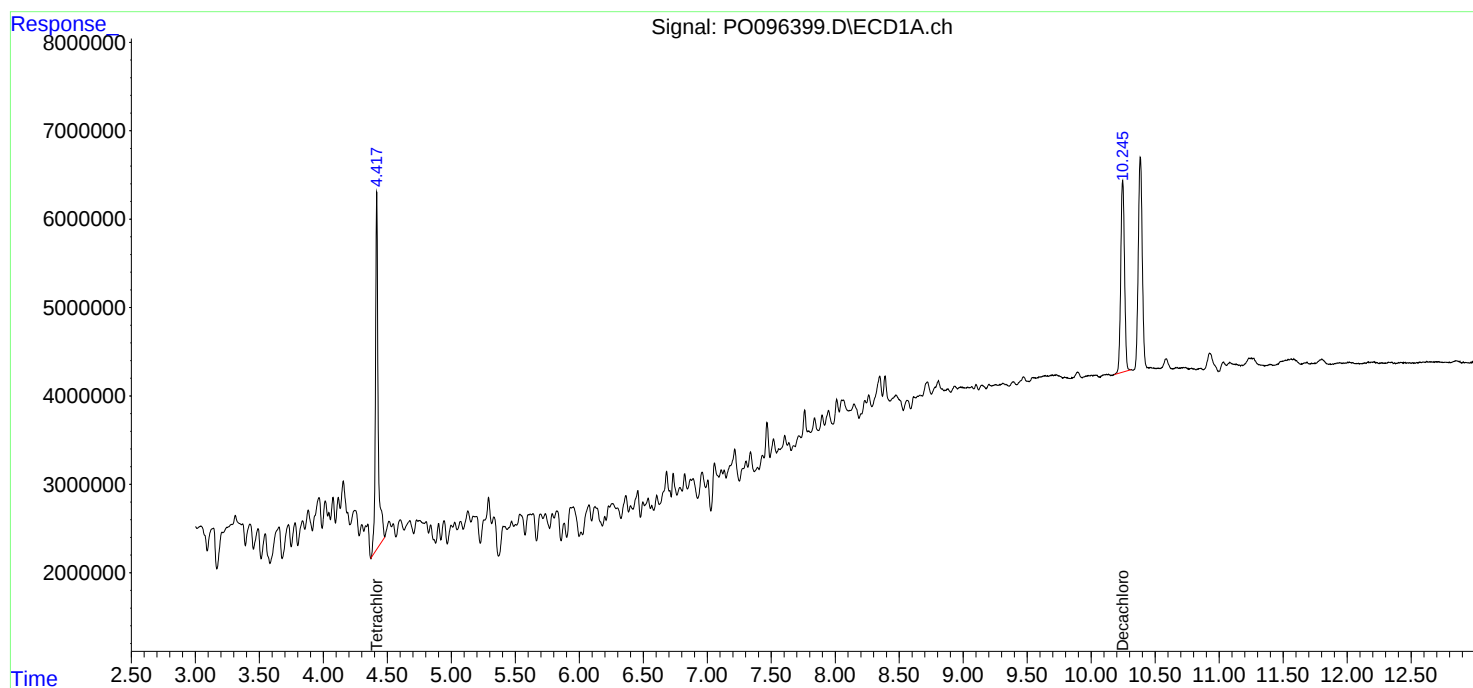


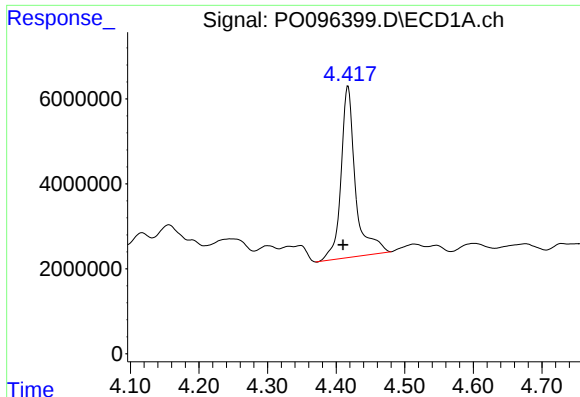

#1 Tetrachloro-m-xylene


R.T.: 4.417 min
Delta R.T.: 0.007 min
Response: 59259645
Conc: 18.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
BUILDING-A-10-(0-5)

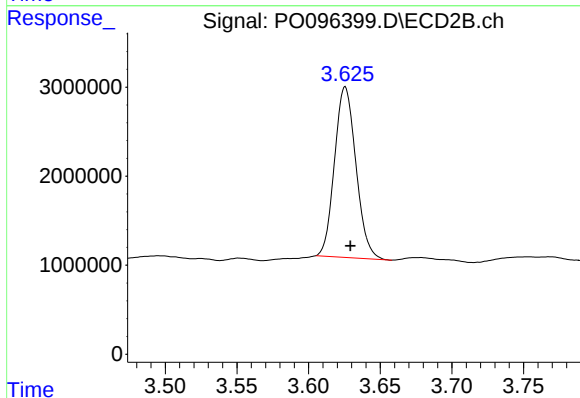


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: -0.004 min
Response: 19949881
Conc: 15.20 ng/ml

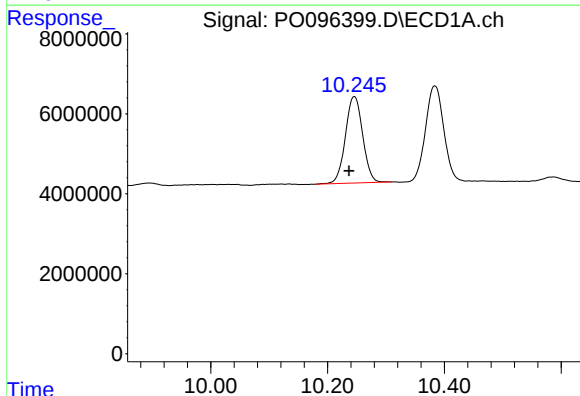

#2 Decachlorobiphenyl

R.T.: 10.246 min
Delta R.T.: 0.009 min
Response: 44443698
Conc: 22.59 ng/ml

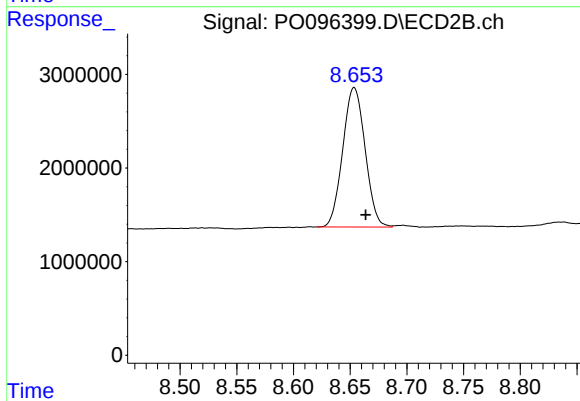

#2 Decachlorobiphenyl

R.T.: 8.654 min
Delta R.T.: -0.010 min
Response: 20427005
Conc: 18.75 ng/ml