

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072718\
Data File : P0047245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2018 3:36
Operator : SM/SJ
Sample : J4185-06
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OILY-WATER-3

Manual Integrations
APPROVED

Sohil
7/27/2018 8:03:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 06:54:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.646	861904	720882	4.269m	2.934m#
2) SA Decachlor...	10.092	8.642	477209	1371072	2.926m	8.722 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072718\
Data File : P0047245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2018 3:36
Operator : SM/SJ
Sample : J4185-06
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER-3


Manual Integrations
APPROVED

Sohil
7/27/2018 8:03:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 06:54:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

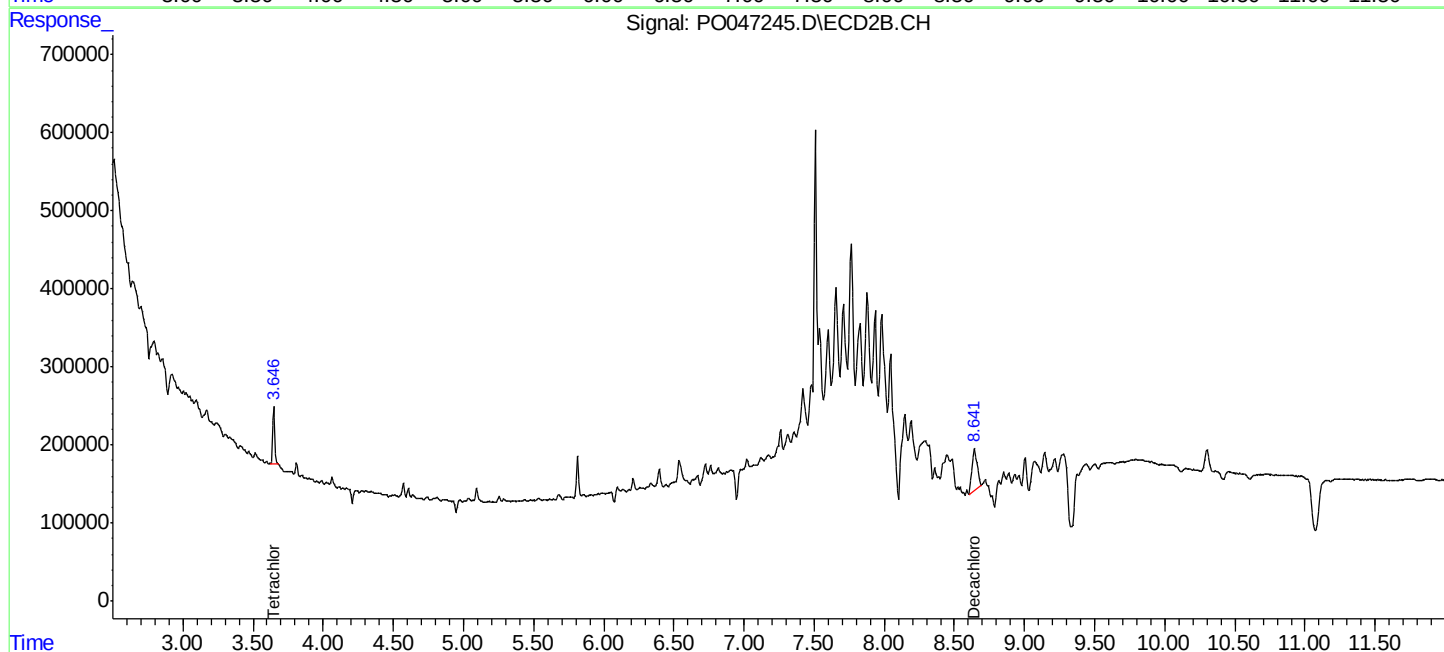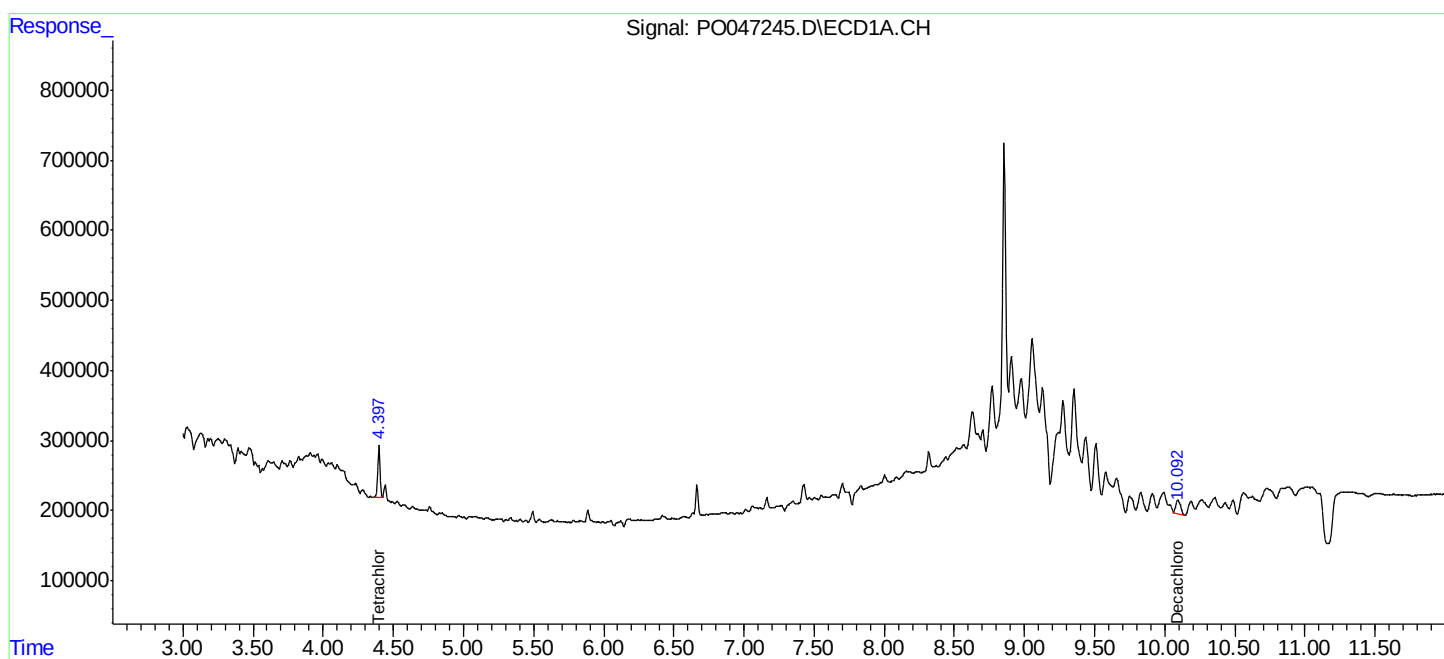

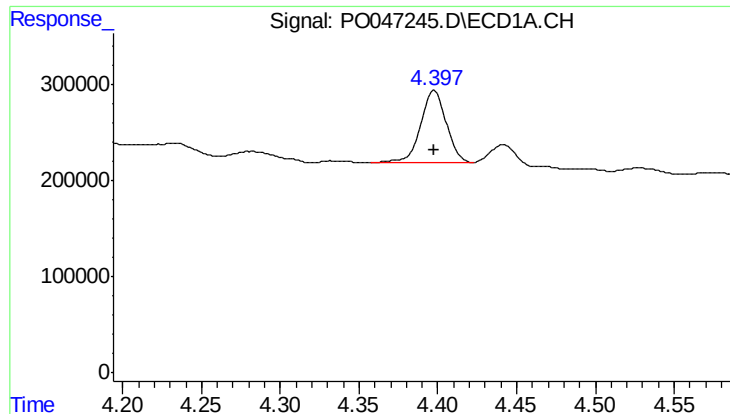


#1 Tetrachloro-m-xylene

R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 861904
Conc: 4.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
OILY-WATER-3


Manual Integrations
APPROVED

Sohil
7/27/2018 8:03:34 PM

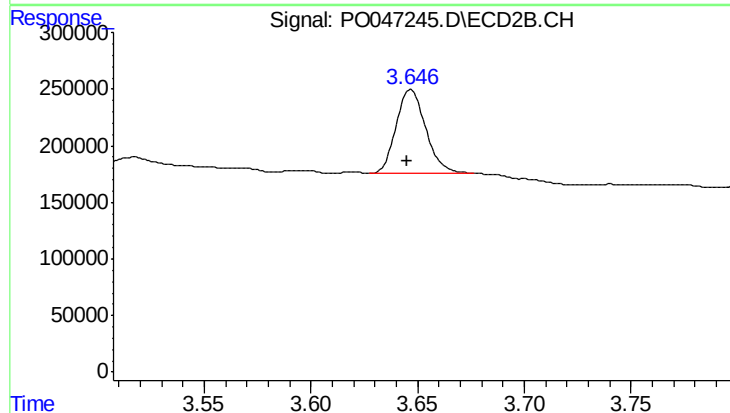


#1 Tetrachloro-m-xylene

R.T.: 3.646 min
Delta R.T.: 0.001 min
Response: 720882
Conc: 2.93 ng/ml m

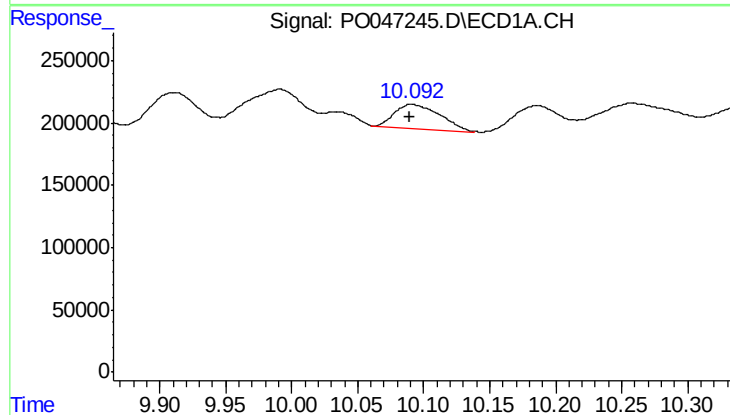

#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: 0.002 min
Response: 477209
Conc: 2.93 ng/ml m

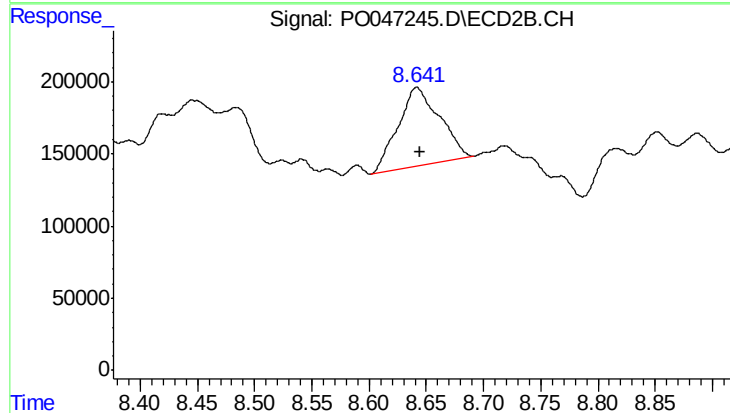

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.003 min
Response: 1371072
Conc: 8.72 ng/ml