

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072720\
 Data File : P0070081.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 1:44
 Operator : DD\AJ
 Sample : L3453-01 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-067

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 04:08:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.401	3.579	252461	310137	6.895	8.178
2)	SA Decachlor...	10.041	8.777	356747	294179	5.961	5.628
Target Compounds							
10)	L2 AR-1221-3	4.850	4.017	20368	24307	20.211	23.317
11)	L3 AR-1232-1	4.850	4.017	20368	24307	24.792	27.735
24)	L5 AR-1248-4	6.622	0.000	11408	0	5.634	N.D. #
26)	L6 AR-1254-1	6.609	0.000	13959	0	7.061	N.D. #
27)	L6 AR-1254-2	6.832	0.000	25022	0	8.028	N.D. #
30)	L6 AR-1254-5	7.921	6.929f	11771	52735	3.941	14.767 #
34)	L7 AR-1260-4	8.240f	0.000	24747	0	8.571	N.D. #
35)	L7 AR-1260-5	8.532	0.000	5486	0	0.804	N.D. #
36)	L8 AR-1262-1	0.000	6.929f	0	52735	N.D.	27.053 #
37)	L8 AR-1262-2	8.532	0.000	5486	0	0.733	N.D. #
39)	L8 AR-1262-4	8.885	0.000	7564	0	2.113	N.D. #
40)	L8 AR-1262-5	9.426	0.000	5541	0	2.084	N.D. #
42)	L9 AR-1268-2	8.885	0.000	7564	0	0.952	N.D. #
43)	L9 AR-1268-3	0.000	7.975f	0	80830	N.D.	12.972 #
44)	L9 AR-1268-4	9.426	0.000	5541	0	1.877	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072720\
Data File : P0070081.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 1:44
Operator : DD\AJ
Sample : L3453-01 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 04:08:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

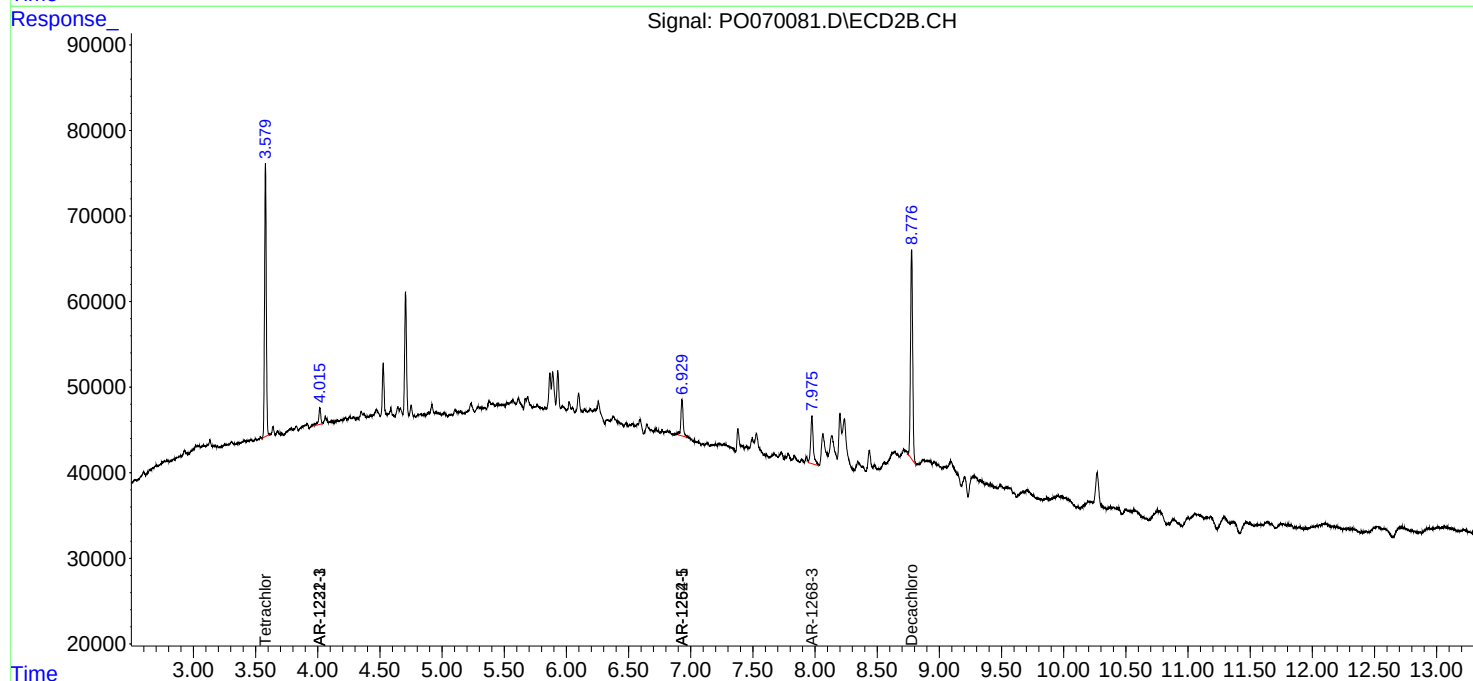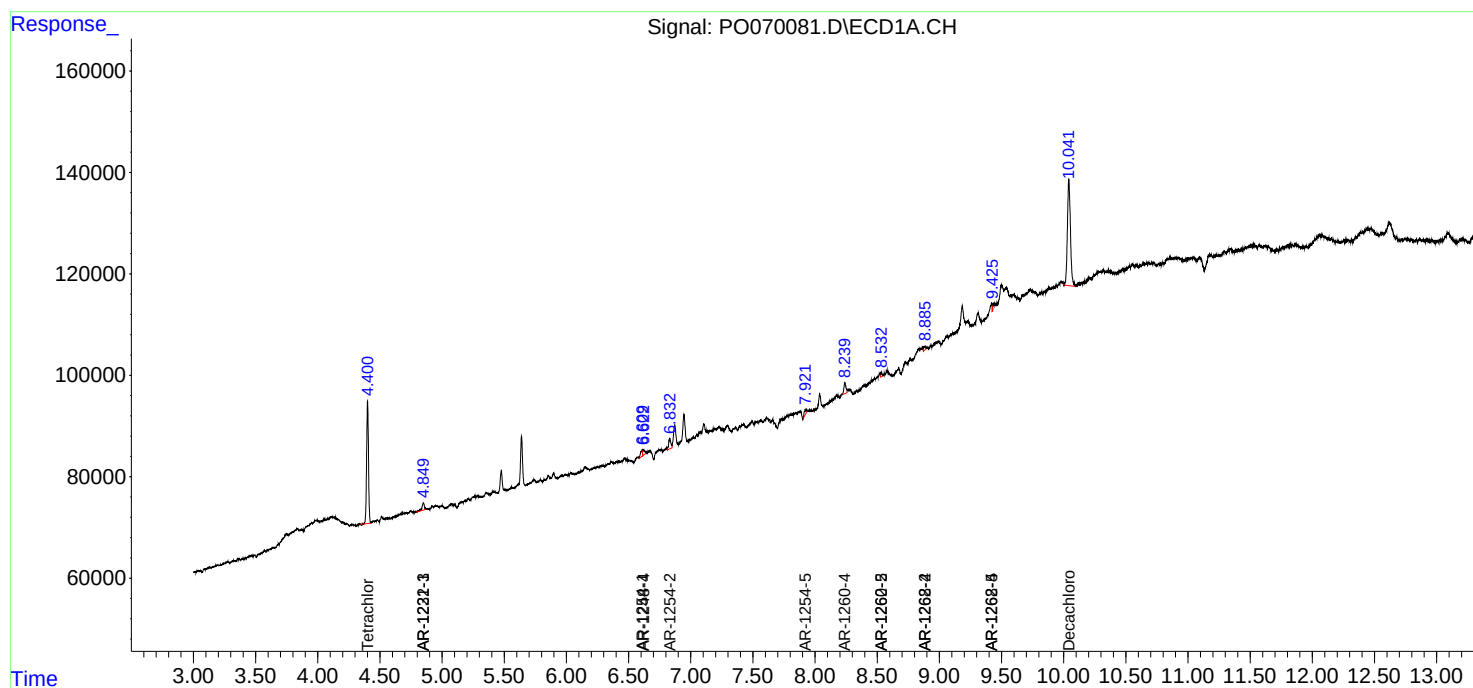


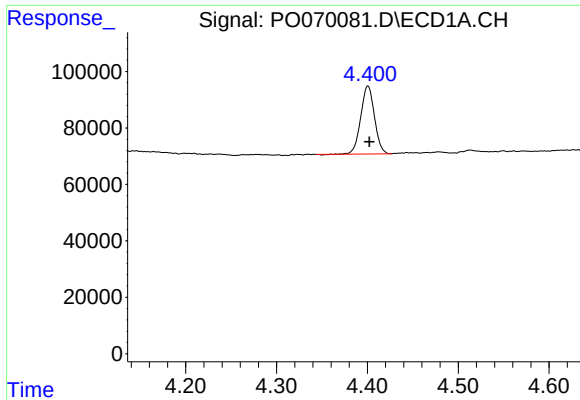

#1 Tetrachloro-m-xylene


R.T.: 4.401 min
Delta R.T.: -0.001 min
Response: 252461
Conc: 6.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

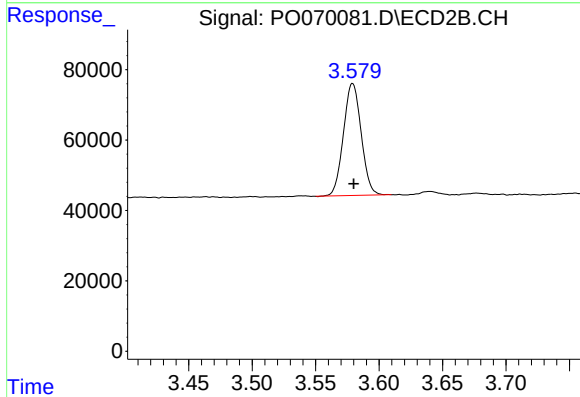


#1 Tetrachloro-m-xylene

R.T.: 3.579 min
Delta R.T.: 0.000 min
Response: 310137
Conc: 8.18 ng/ml

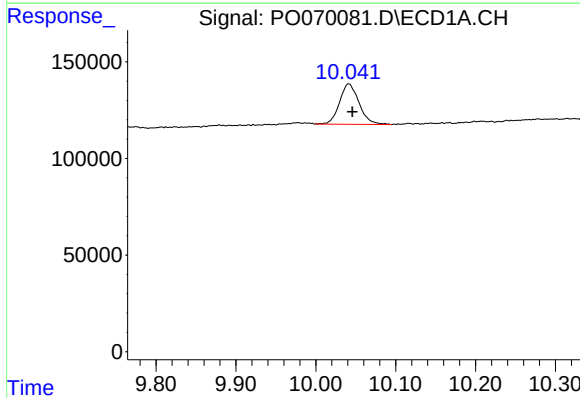


#2 Decachlorobiphenyl

R.T.: 10.041 min
Delta R.T.: -0.004 min
Response: 356747
Conc: 5.96 ng/ml

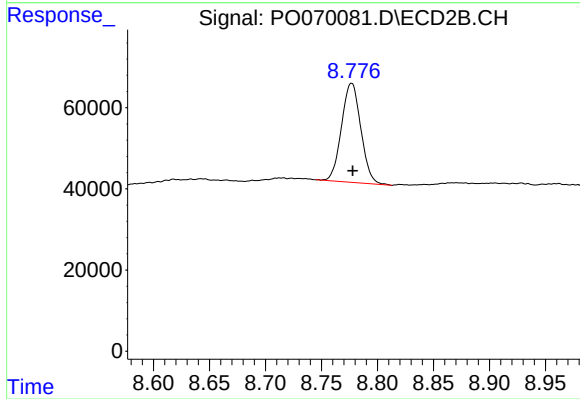

#2 Decachlorobiphenyl


R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 294179
Conc: 5.63 ng/ml

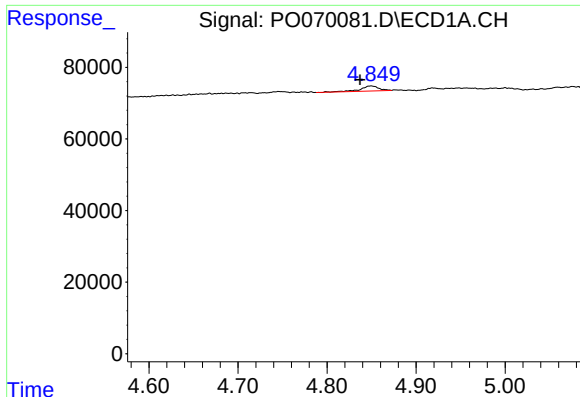

#10 AR-1221-3


R.T.: 4.850 min
Delta R.T.: 0.013 min
Response: 20368
Conc: 20.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

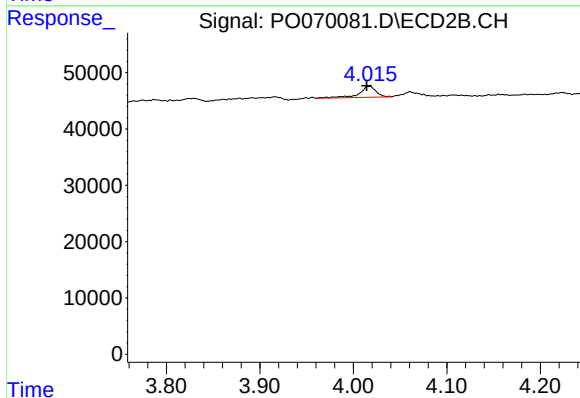


#10 AR-1221-3

R.T.: 4.017 min
Delta R.T.: 0.002 min
Response: 24307
Conc: 23.32 ng/ml

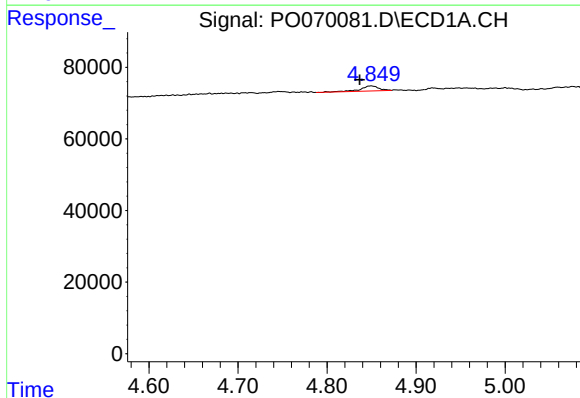


#11 AR-1232-1

R.T.: 4.850 min
Delta R.T.: 0.013 min
Response: 20368
Conc: 24.79 ng/ml

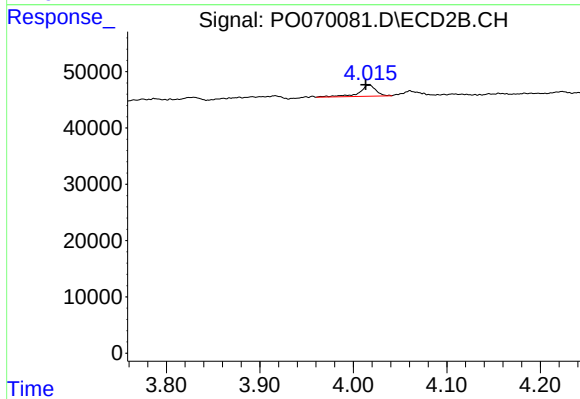

#11 AR-1232-1


R.T.: 4.017 min
Delta R.T.: 0.004 min
Response: 24307
Conc: 27.73 ng/ml

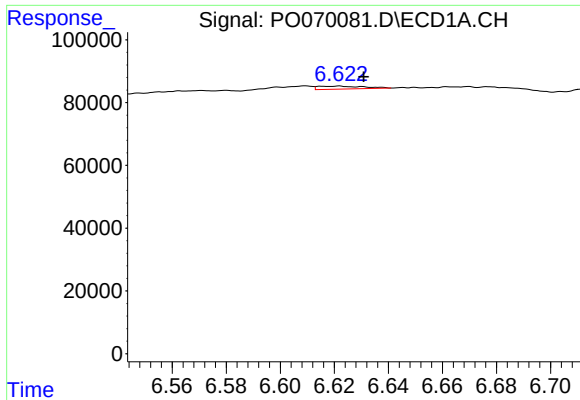

#24 AR-1248-4


R.T.: 6.622 min
Delta R.T.: -0.009 min
Response: 11408
Conc: 5.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

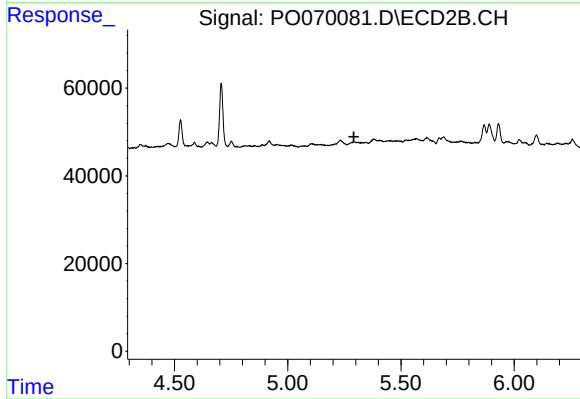


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.292 min
Response: 0
Conc: N.D.

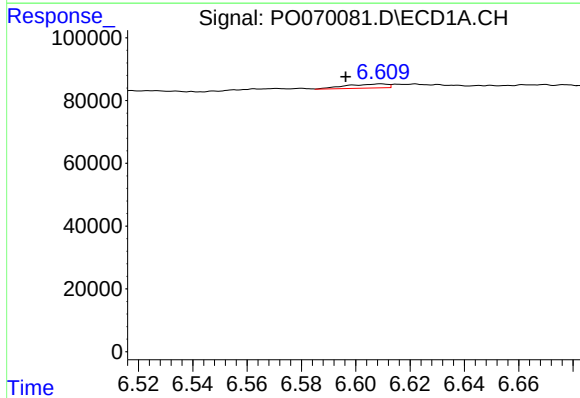


#26 AR-1254-1

R.T.: 6.609 min
Delta R.T.: 0.013 min
Response: 13959
Conc: 7.06 ng/ml

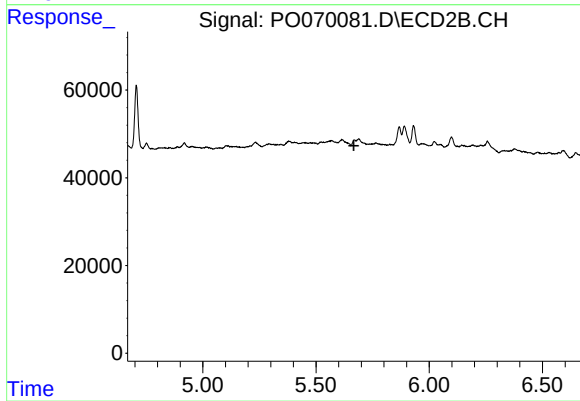

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.667 min
Response: 0
Conc: N.D.

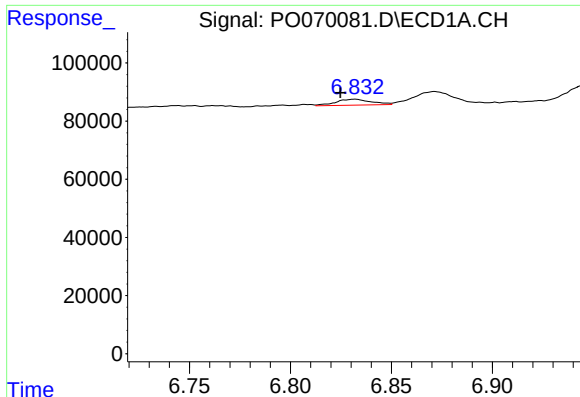

#27 AR-1254-2


R.T.: 6.832 min
Delta R.T.: 0.007 min
Response: 25022
Conc: 8.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

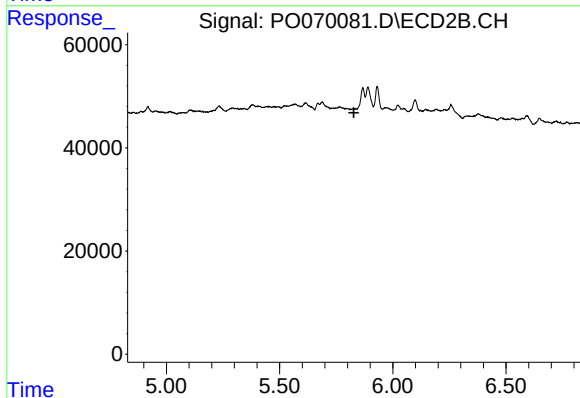


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.828 min
Response: 0
Conc: N.D.

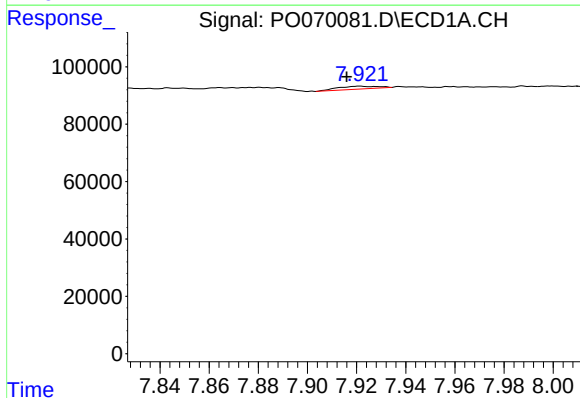


#30 AR-1254-5

R.T.: 7.921 min
Delta R.T.: 0.005 min
Response: 11771
Conc: 3.94 ng/ml

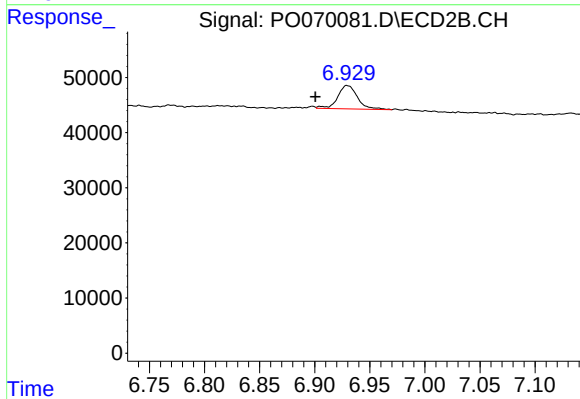

#30 AR-1254-5


R.T.: 6.929 min
Delta R.T.: 0.028 min
Response: 52735
Conc: 14.77 ng/ml

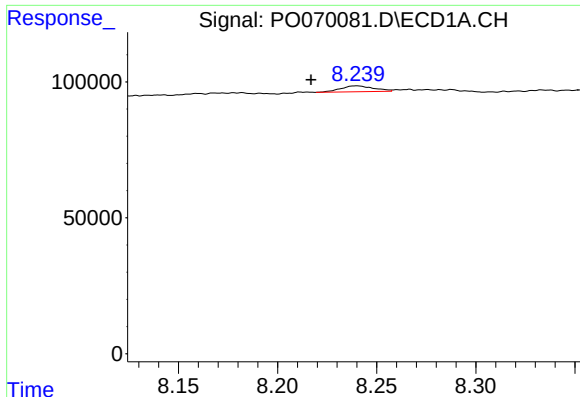

#34 AR-1260-4


R.T.: 8.240 min
Delta R.T.: 0.023 min
Response: 24747
Conc: 8.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

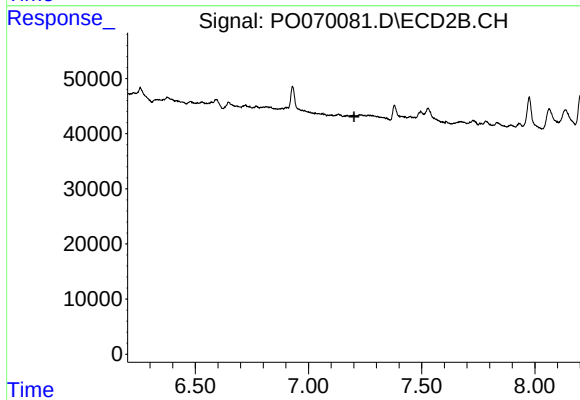


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.201 min
Response: 0
Conc: N.D.

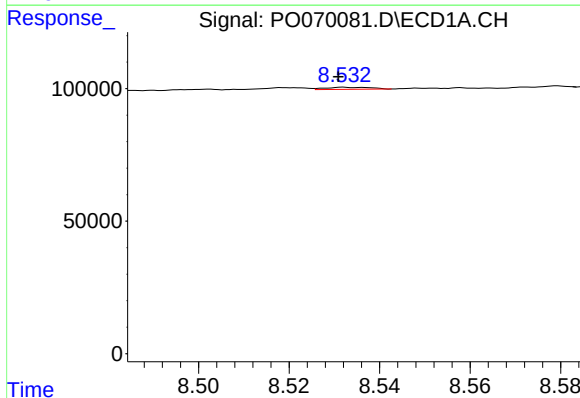


#35 AR-1260-5

R.T.: 8.532 min
Delta R.T.: 0.001 min
Response: 5486
Conc: 0.80 ng/ml

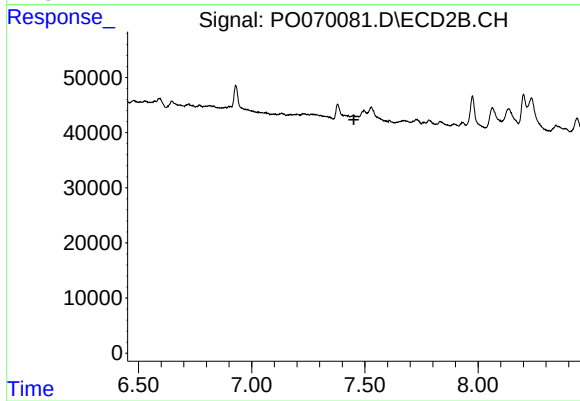

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.451 min
Response: 0
Conc: N.D.

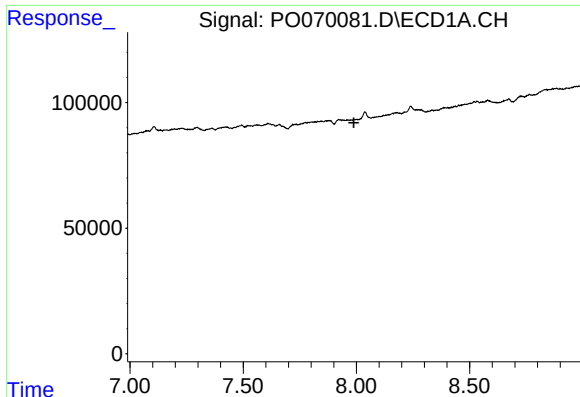

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

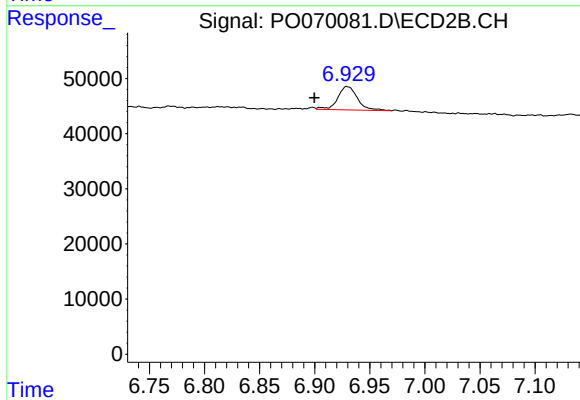


#36 AR-1262-1

R.T.: 6.929 min
Delta R.T.: 0.029 min
Response: 52735
Conc: 27.05 ng/ml

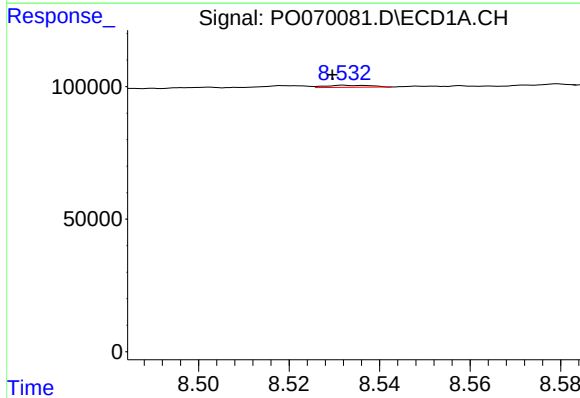


#37 AR-1262-2

R.T.: 8.532 min
Delta R.T.: 0.002 min
Response: 5486
Conc: 0.73 ng/ml

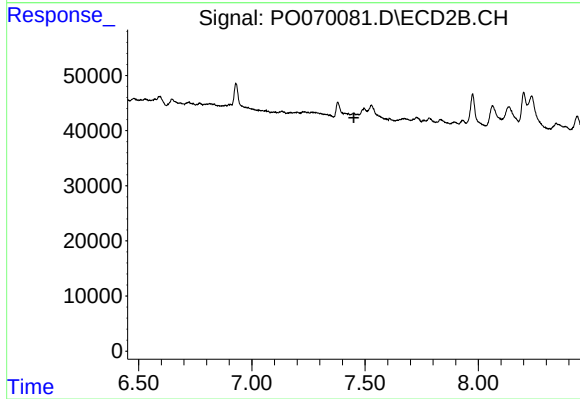

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.451 min
Response: 0
Conc: N.D.

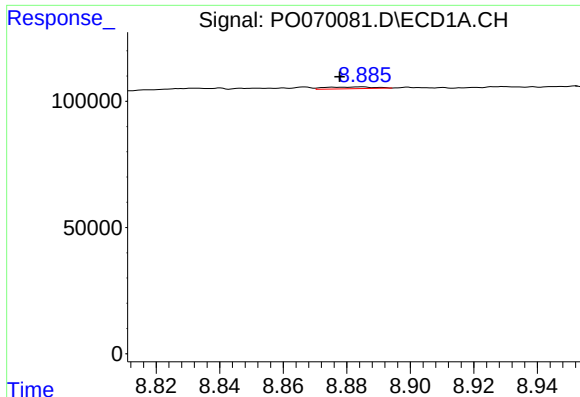

#39 AR-1262-4


R.T.: 8.885 min
Delta R.T.: 0.007 min
Response: 7564
Conc: 2.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

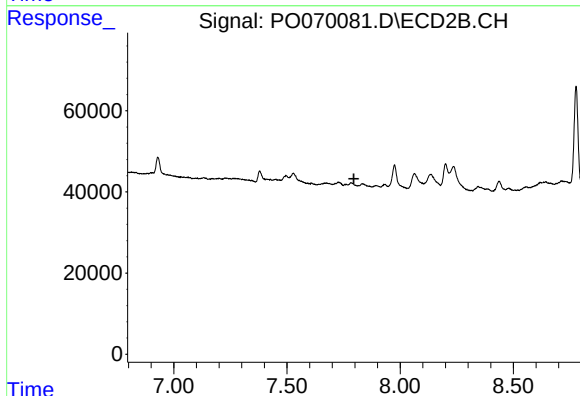


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 7.795 min
Response: 0
Conc: N.D.

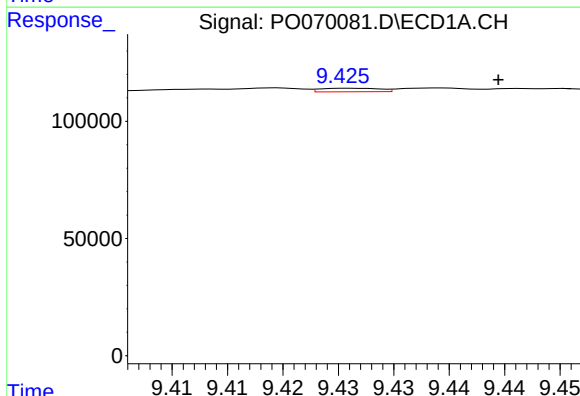


#40 AR-1262-5

R.T.: 9.426 min
Delta R.T.: -0.013 min
Response: 5541
Conc: 2.08 ng/ml

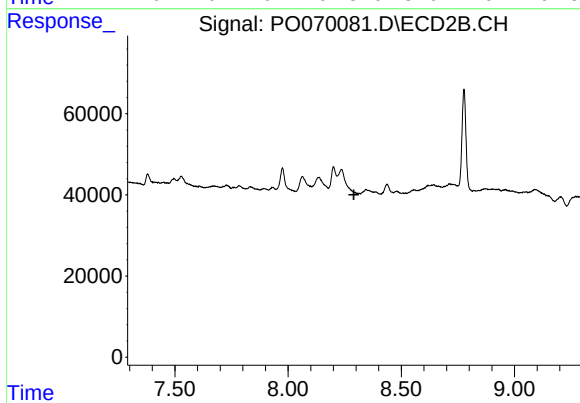

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.290 min
Response: 0
Conc: N.D.

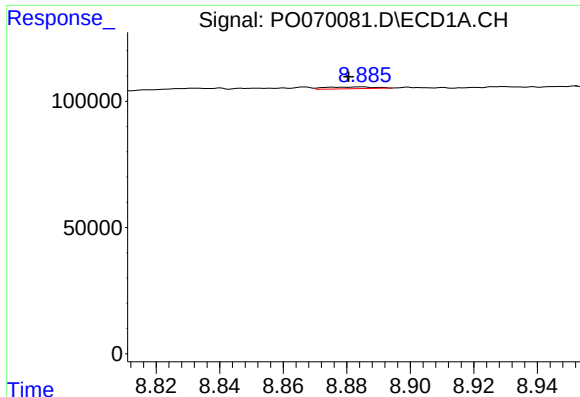

#42 AR-1268-2


R.T.: 8.885 min
Delta R.T.: 0.004 min
Response: 7564
Conc: 0.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

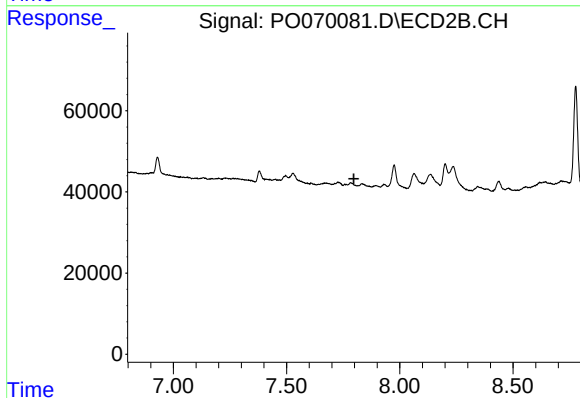


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.797 min
Response: 0
Conc: N.D.

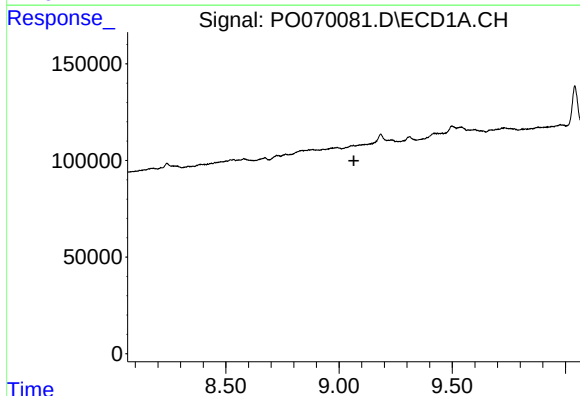


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.065 min
Response: 0
Conc: N.D.

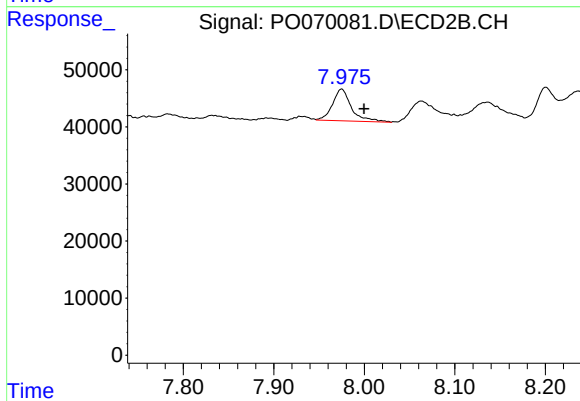

#43 AR-1268-3


R.T.: 7.975 min
Delta R.T.: -0.025 min
Response: 80830
Conc: 12.97 ng/ml

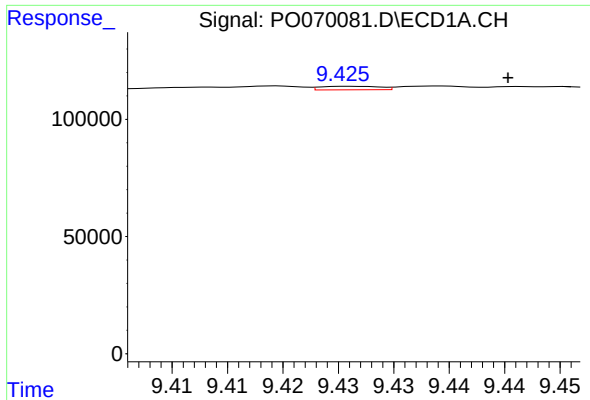

#44 AR-1268-4

R.T.: 9.426 min
Delta R.T.: -0.014 min
Response: 5541
Conc: 1.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

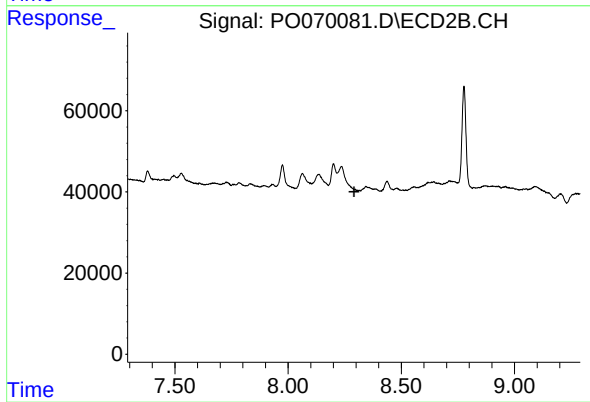

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 8.291 min
Response: 0
Conc: N.D.