

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072720\
 Data File : P0070045.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jul 2020 15:28
 Operator : DD\AJ
 Sample : L3450-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-016-IDWGW-20200723

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 17:55:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.580	652724	740551	17.827	19.528
2) SA Decachlor...	10.044	8.777	253393	267241	4.234	5.113

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072720\
Data File : P0070045.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2020 15:28
Operator : DD\AJ
Sample : L3450-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TT-016-IDWGW-20200723

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 17:55:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

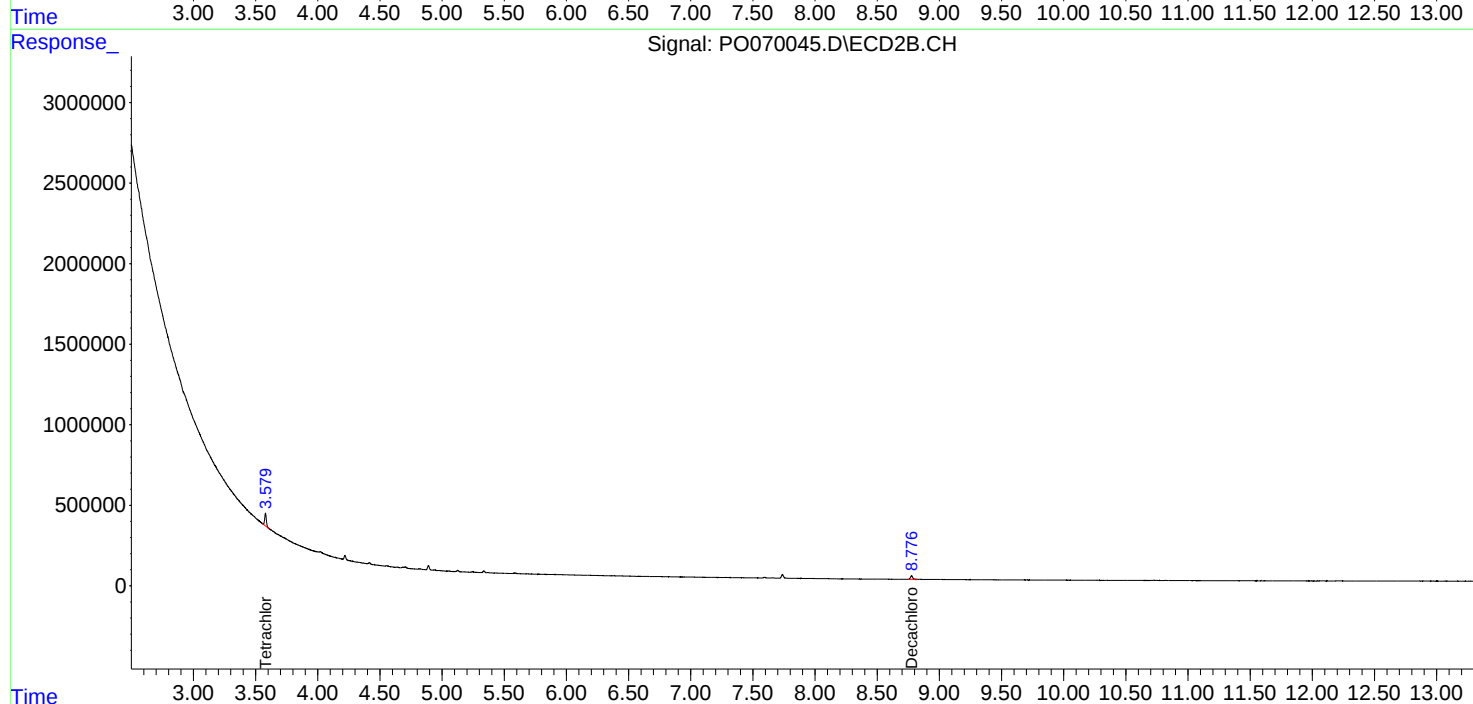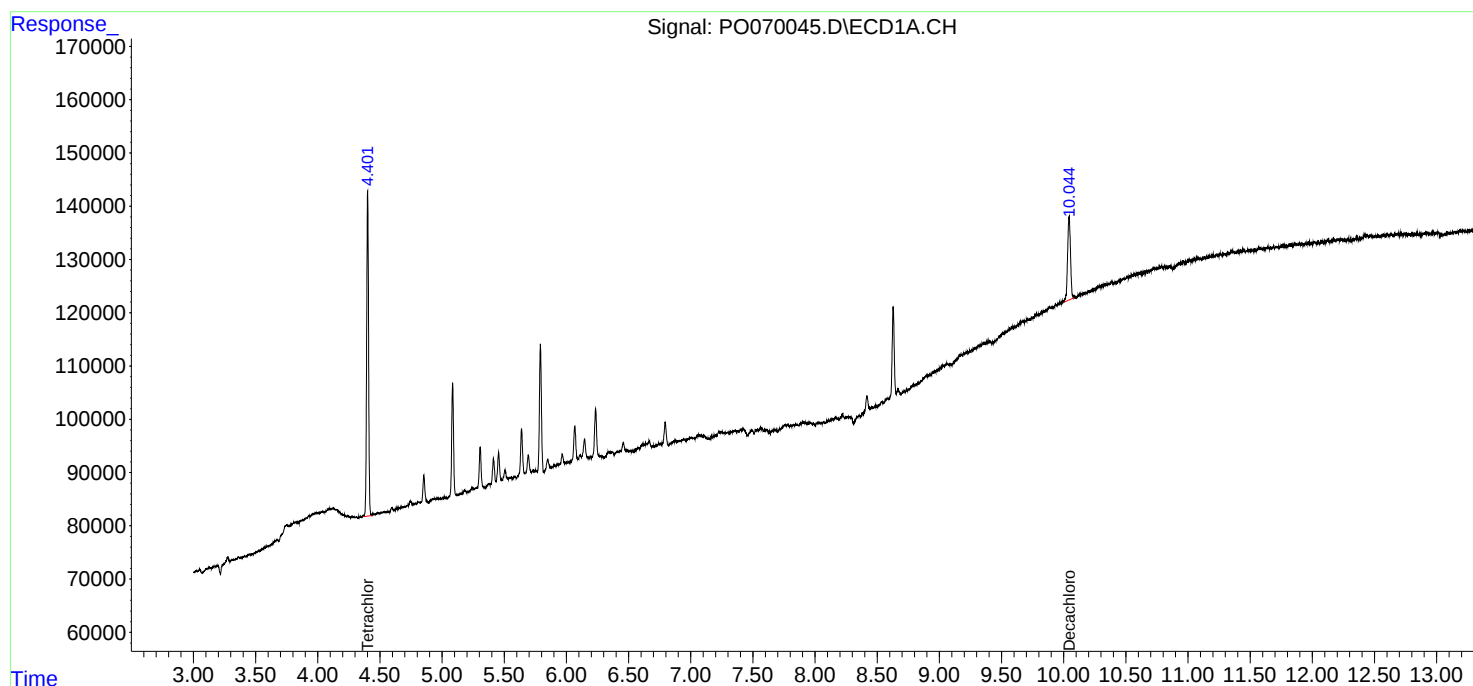


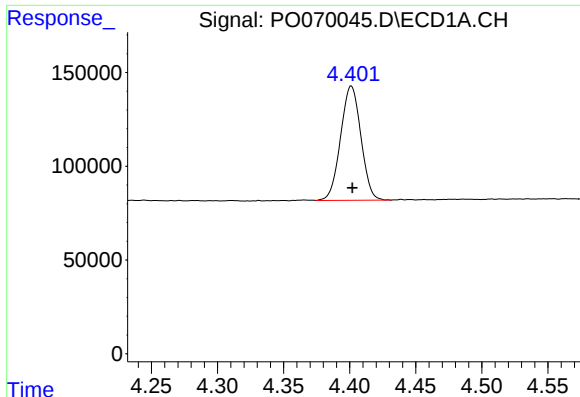

#1 Tetrachloro-m-xylene


R.T.: 4.401 min
Delta R.T.: 0.000 min
Response: 652724
Conc: 17.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-016-IDWGW-20200723

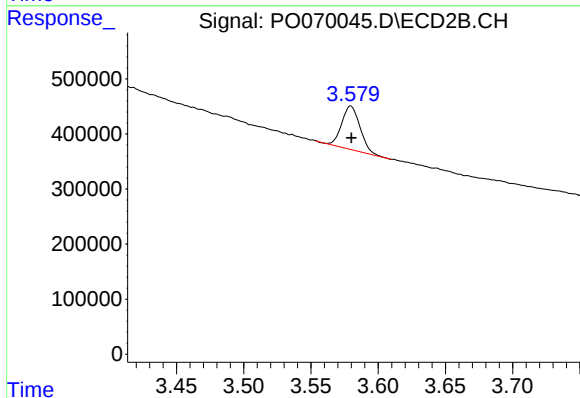


#1 Tetrachloro-m-xylene

R.T.: 3.580 min
Delta R.T.: 0.000 min
Response: 740551
Conc: 19.53 ng/ml

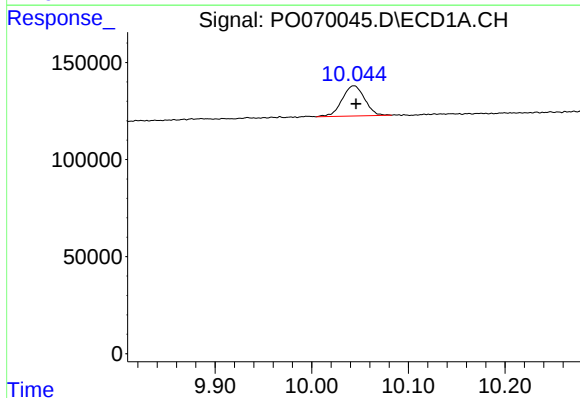

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.002 min
Response: 253393
Conc: 4.23 ng/ml

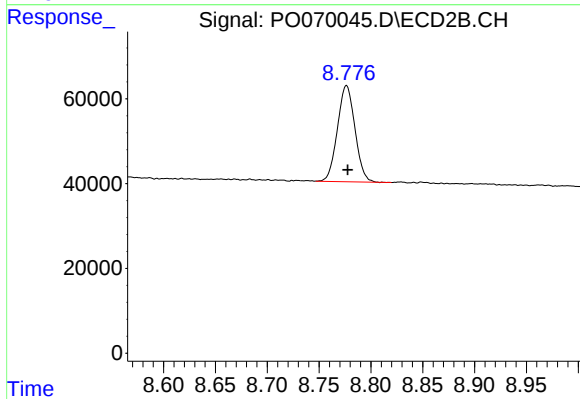

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: -0.001 min
Response: 267241
Conc: 5.11 ng/ml