

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072720\
 Data File : P0070048.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jul 2020 16:19
 Operator : DD\AJ
 Sample : L3450-02RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-016-IDWGW-20200723RE

Manual Integrations
 APPROVED

Ankita
 7/28/2020 12:14:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 27 17:56:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.579	657537	760908	17.958	20.065
2) SA Decachlor...	10.043	8.776	257986	273005	4.311	5.223m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072720\
Data File : P0070048.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2020 16:19
Operator : DD\AJ
Sample : L3450-02RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TT-016-IDWGW-20200723RE


Manual Integrations
APPROVED

Ankita
7/28/2020 12:14:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 27 17:56:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

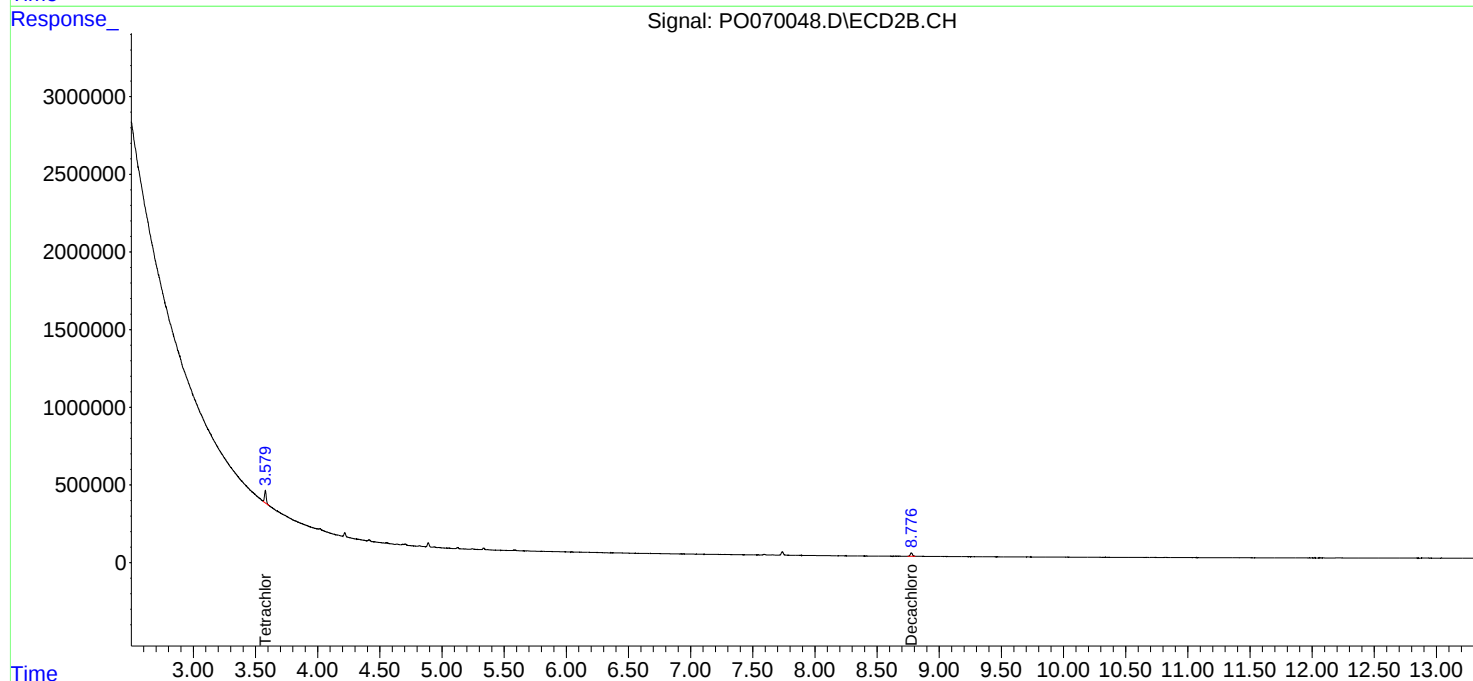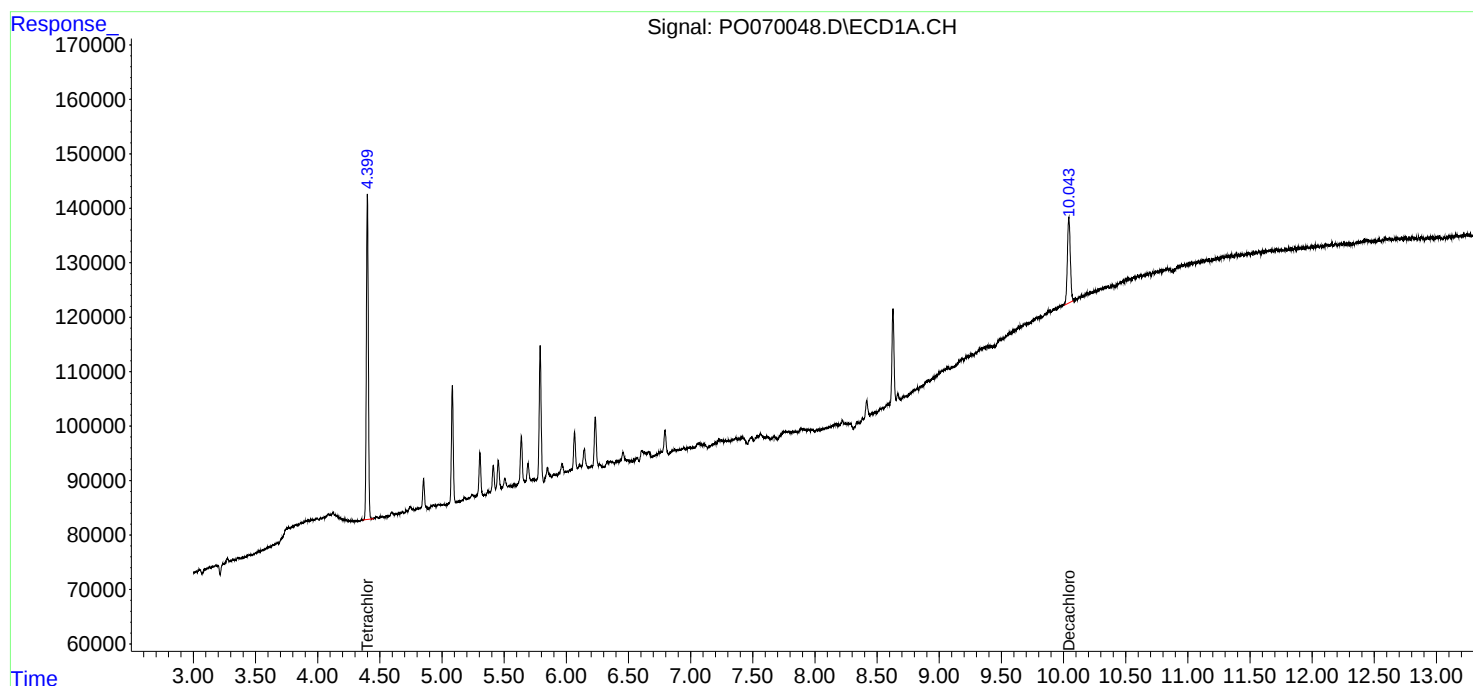

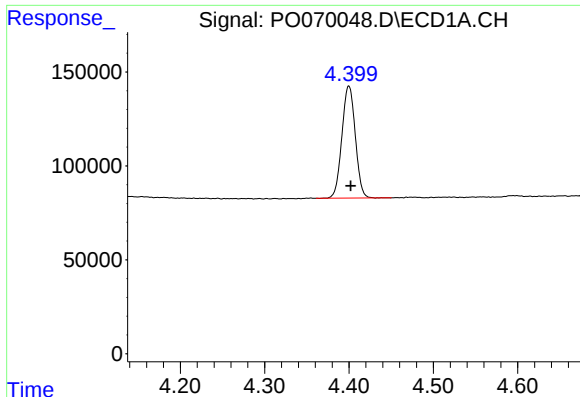


#1 Tetrachloro-m-xylene

R.T.: 4.400 min
Delta R.T.: -0.002 min
Response: 657537
Conc: 17.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-016-IDWGW-20200723RE


Manual Integrations
APPROVED

Ankita
7/28/2020 12:14:55 PM

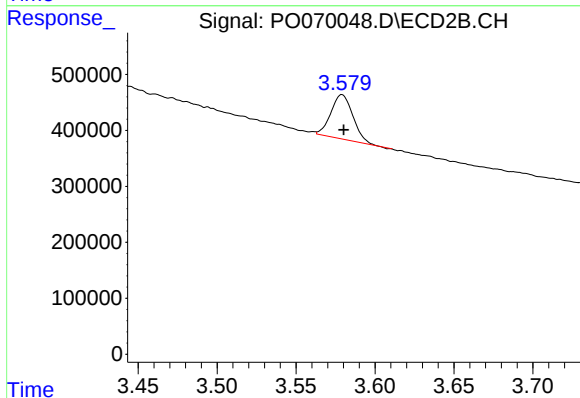


#1 Tetrachloro-m-xylene

R.T.: 3.579 min
Delta R.T.: 0.000 min
Response: 760908
Conc: 20.06 ng/ml

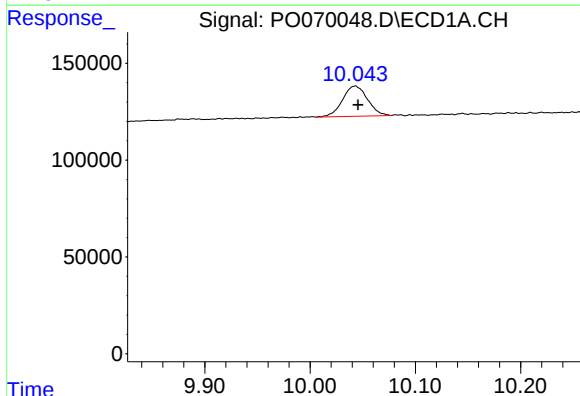

#2 Decachlorobiphenyl

R.T.: 10.043 min
Delta R.T.: -0.003 min
Response: 257986
Conc: 4.31 ng/ml

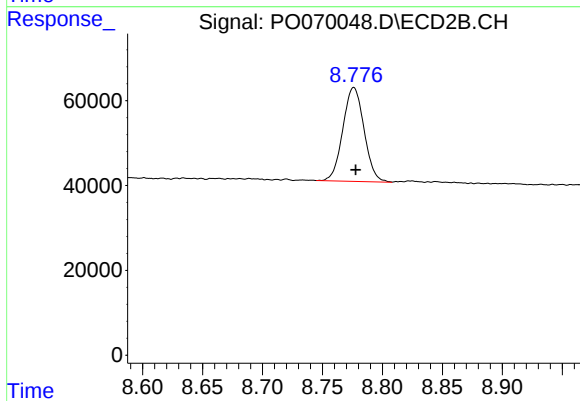

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: -0.002 min
Response: 273005
Conc: 5.22 ng/ml m