

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072720\
 Data File : P0070081.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 1:44
 Operator : DD\AJ
 Sample : L3453-01 2X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-067

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 04:08:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.579	252461	310137	6.895	8.178
2) SA Decachlor...	10.041	8.777	356747	294179	5.961	5.628

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072720\
Data File : P0070081.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 1:44
Operator : DD\AJ
Sample : L3453-01 2X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 04:08:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

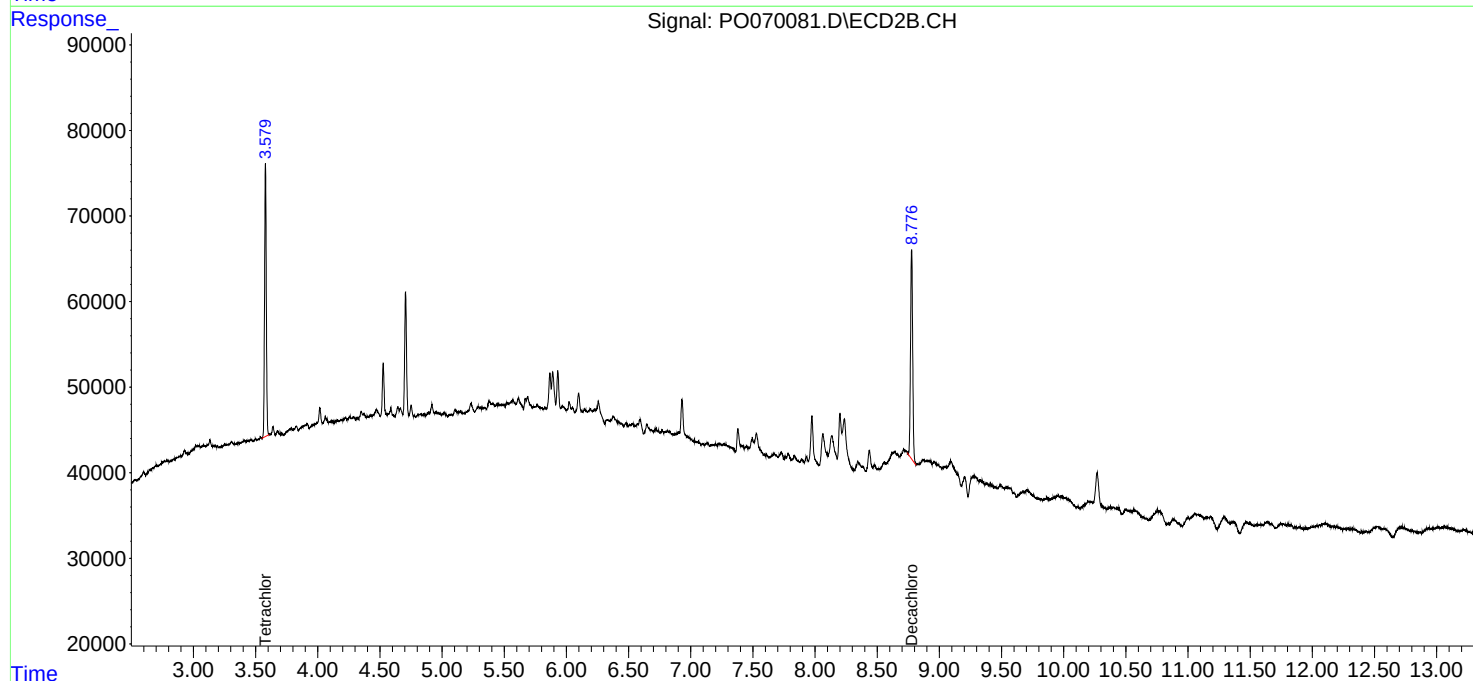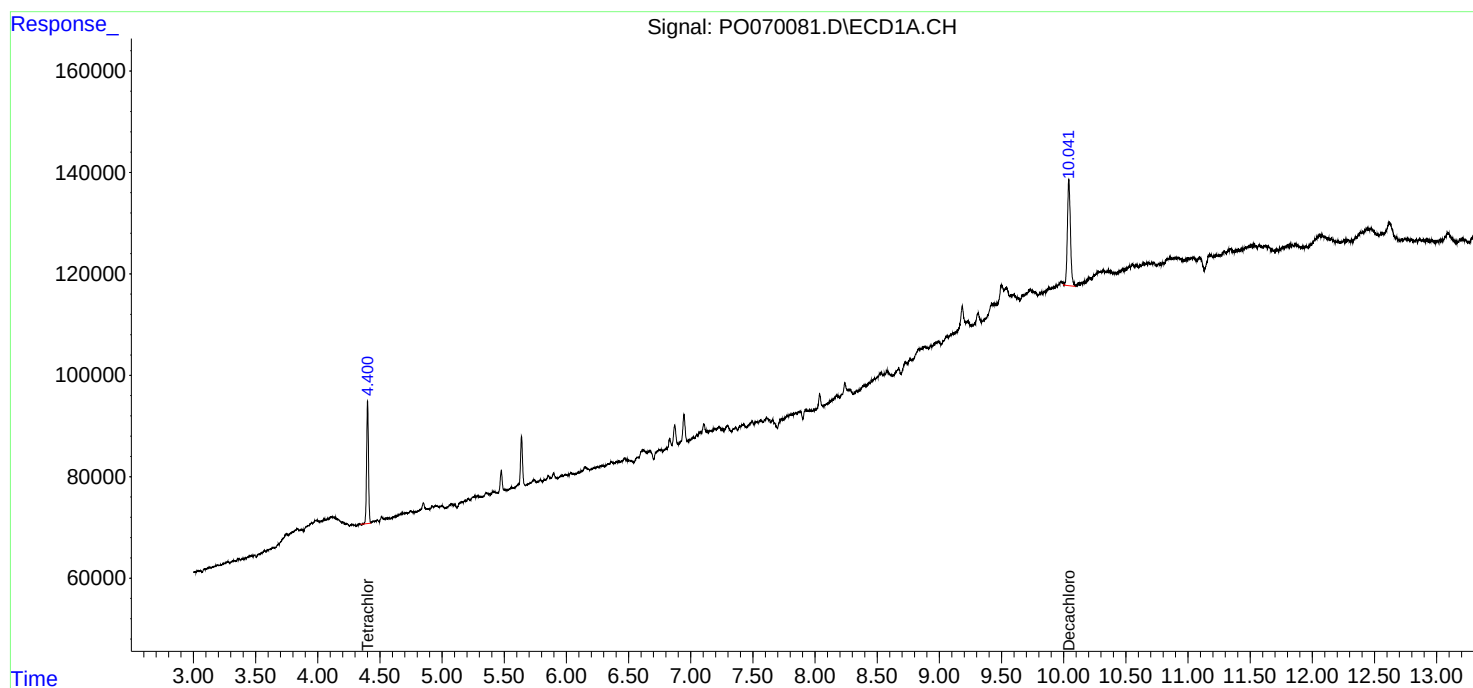


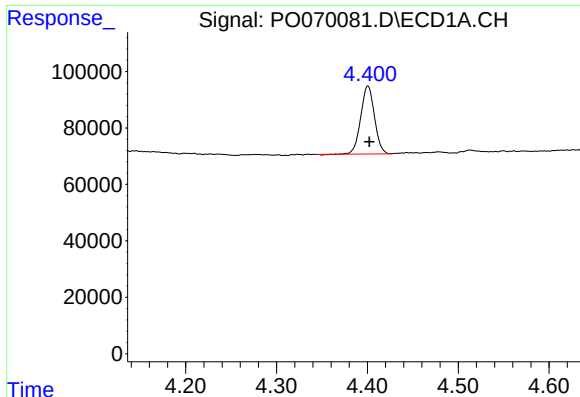

#1 Tetrachloro-m-xylene


R.T.: 4.401 min
Delta R.T.: -0.001 min
Response: 252461
Conc: 6.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067

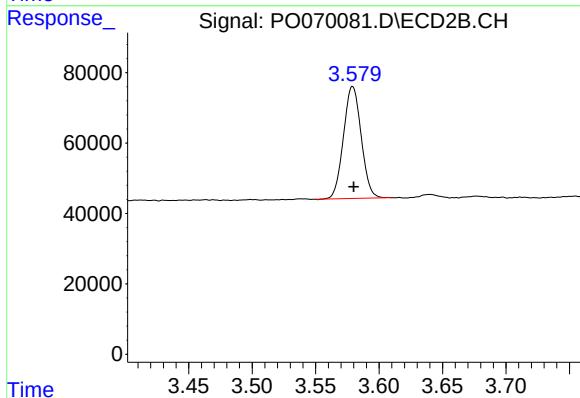


#1 Tetrachloro-m-xylene

R.T.: 3.579 min
Delta R.T.: 0.000 min
Response: 310137
Conc: 8.18 ng/ml

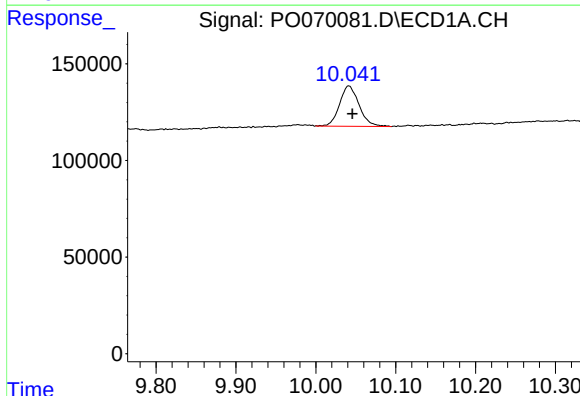

#2 Decachlorobiphenyl

R.T.: 10.041 min
Delta R.T.: -0.004 min
Response: 356747
Conc: 5.96 ng/ml

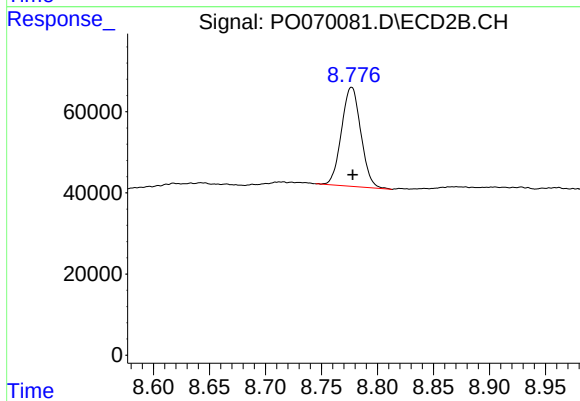

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 294179
Conc: 5.63 ng/ml