

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072722\
 Data File : P0088380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jul 2022 18:00
 Operator : YP/AJ
 Sample : N3898-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 61422-D

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/28/2022
 Supervised By :Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 07:27:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 26 11:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.445	3.607	50982282	23030659	19.984m	24.410
2) SA Decachlor...	10.304	8.598	20312922	26193579	9.565	25.065 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072722\
Data File : P0088380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jul 2022 18:00
Operator : YP/AJ
Sample : N3898-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
61422-D


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 07:27:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 26 11:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

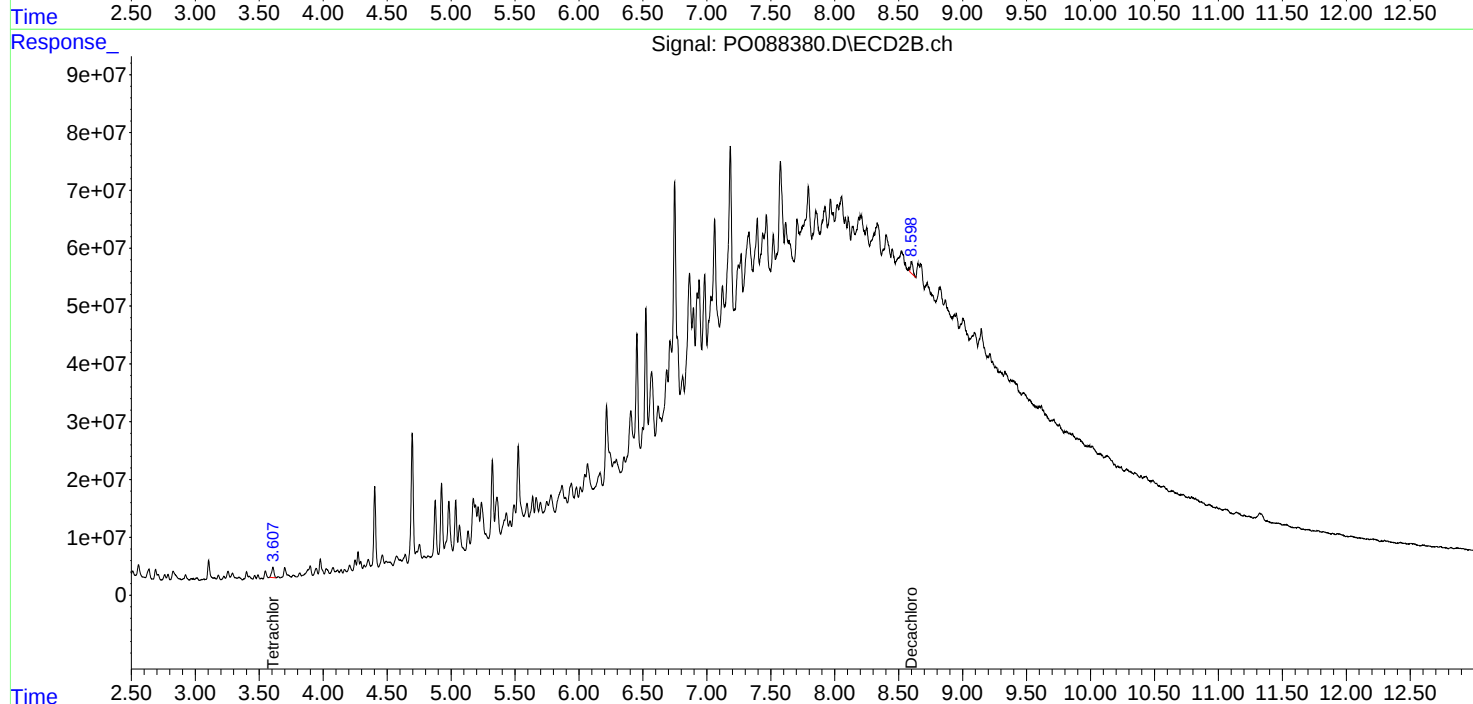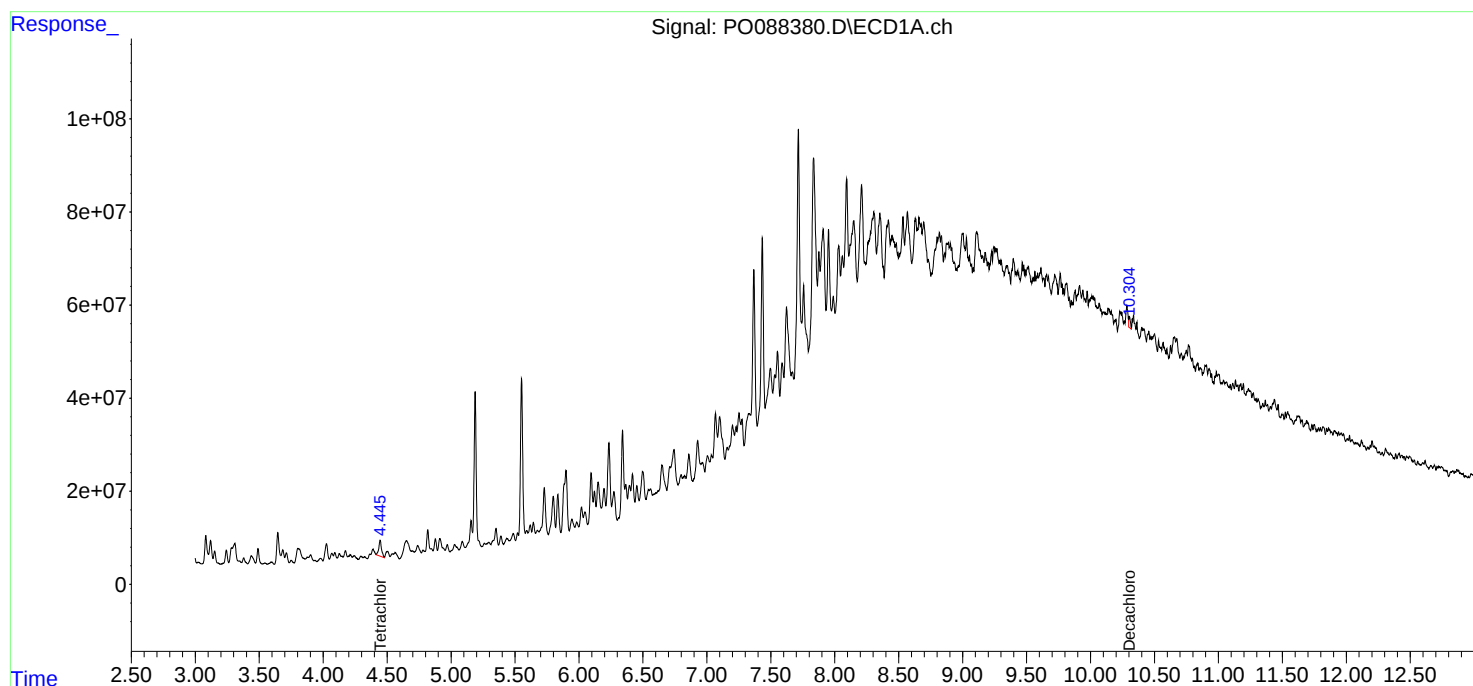

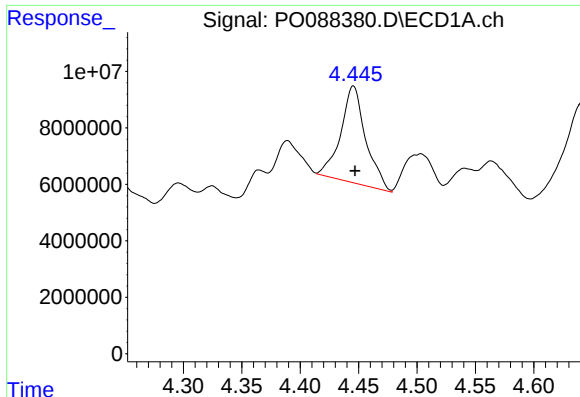


#1 Tetrachloro-m-xylene

R.T.: 4.445 min
Delta R.T.: -0.002 min
Response: 50982282
Conc: 19.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
61422-D


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

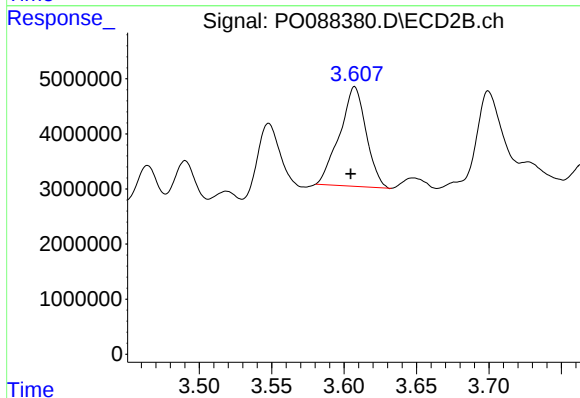


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: 0.003 min
Response: 23030659
Conc: 24.41 ng/ml

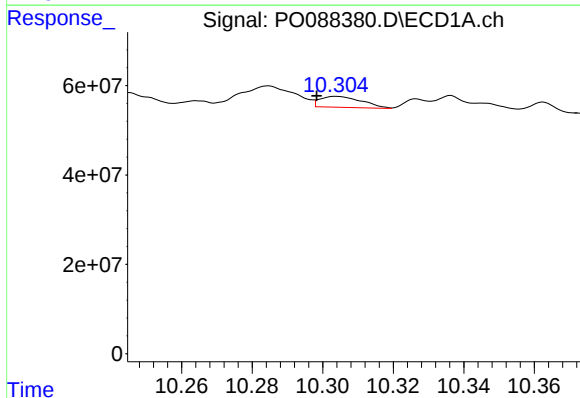

#2 Decachlorobiphenyl

R.T.: 10.304 min
Delta R.T.: 0.006 min
Response: 20312922
Conc: 9.56 ng/ml

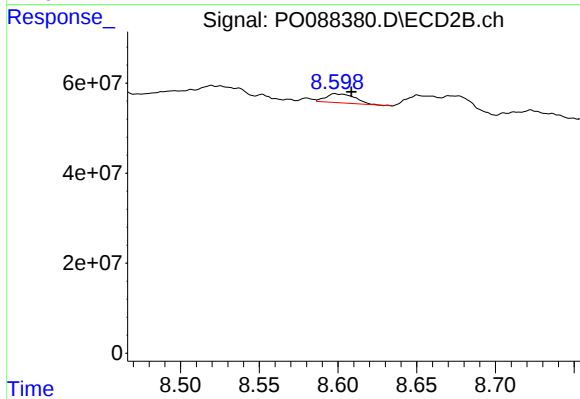

#2 Decachlorobiphenyl

R.T.: 8.598 min
Delta R.T.: -0.010 min
Response: 26193579
Conc: 25.06 ng/ml