

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072724\
 Data File : P0104986.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2024 15:22
 Operator : YP/AJ
 Sample : P3362-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-220

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/29/2024
 Supervised By :Ankita Jodhani 07/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 16:21:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.540	150.1E6	63331856	16.764m	19.412
2) SA Decachlor...	10.214	8.434	108.9E6	34788929	17.762m	16.589

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072724\
Data File : PO104986.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2024 15:22
Operator : YP/AJ
Sample : P3362-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-220


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :Ankita Jodhani 07/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 16:21:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

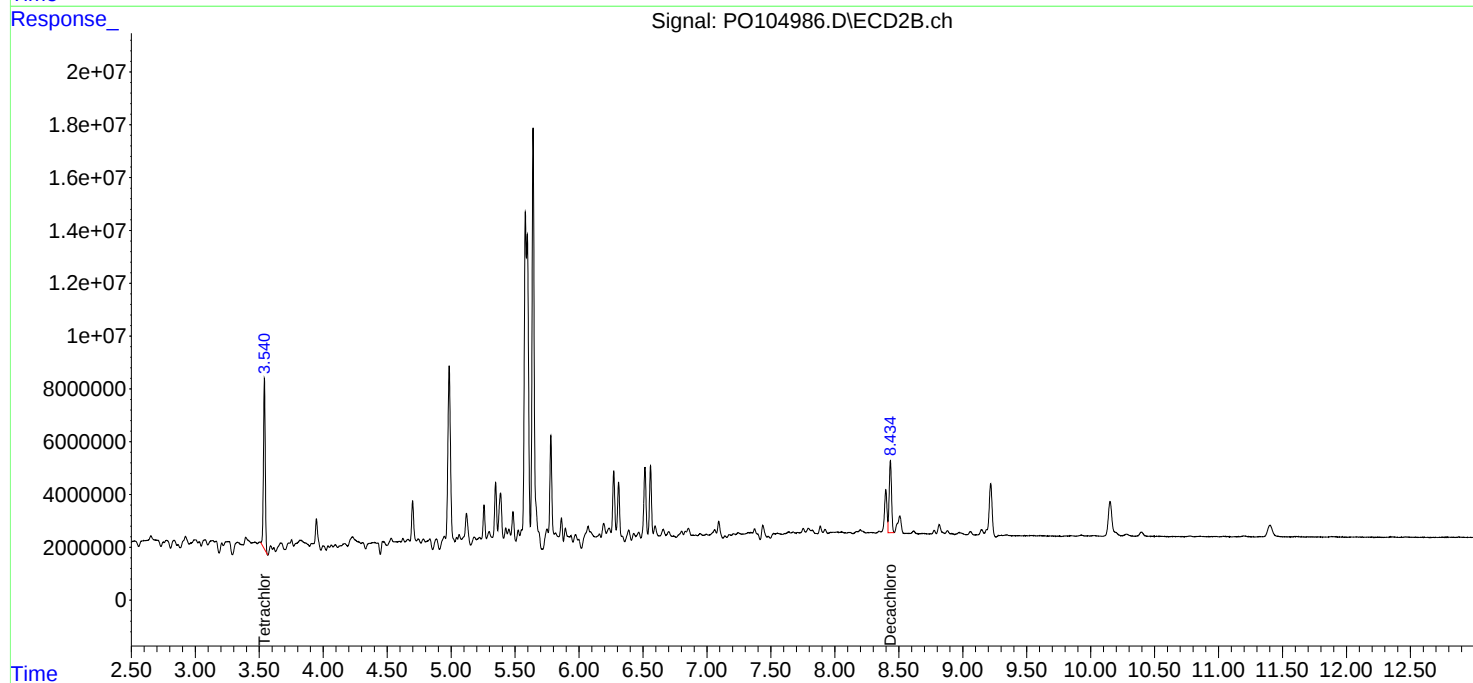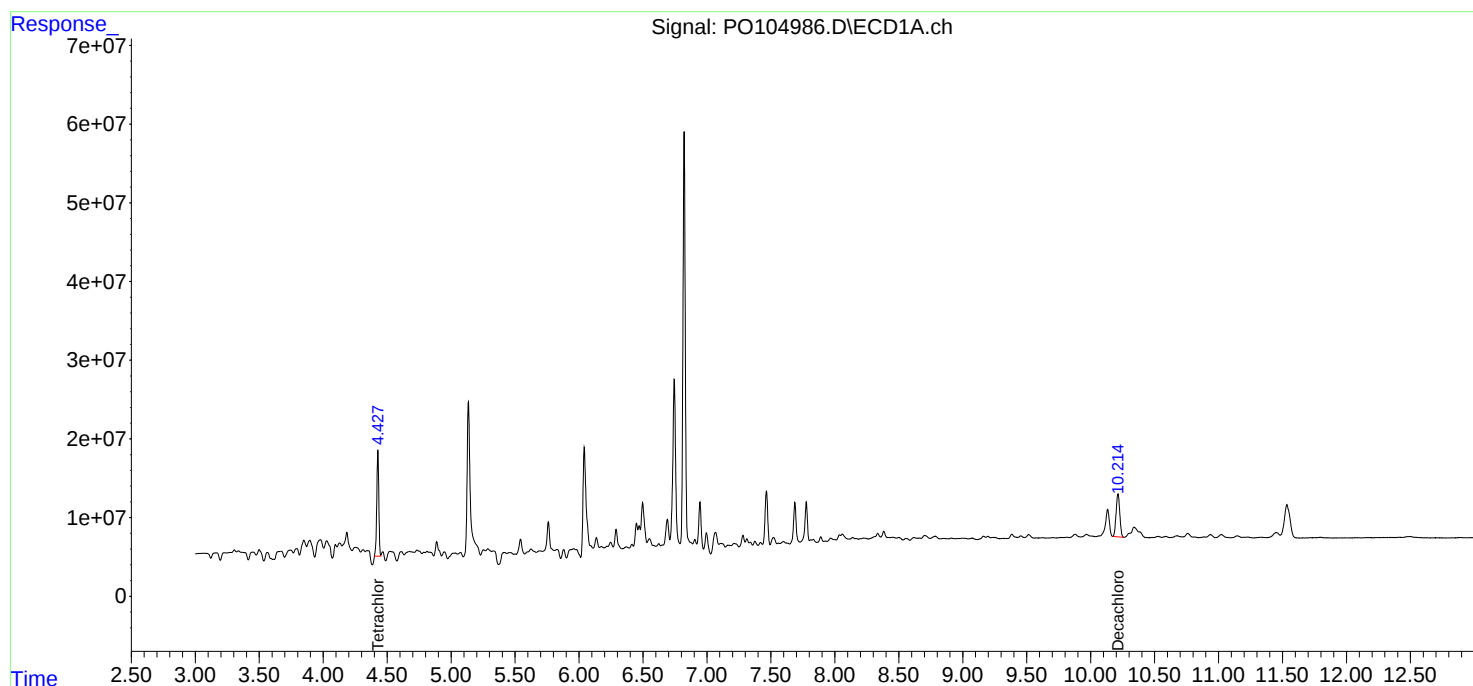

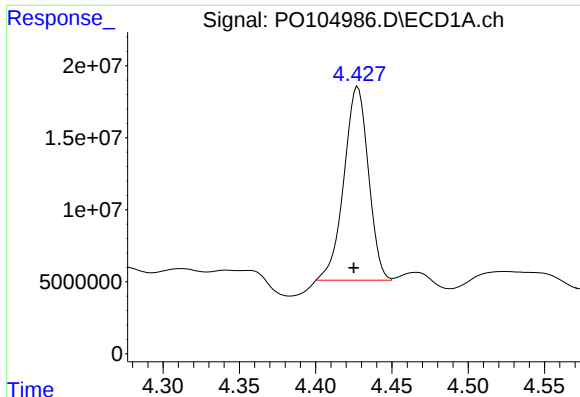


#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: 0.002 min
Response: 150098776
Conc: 16.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-220


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :Ankita Jodhani 07/29/2024

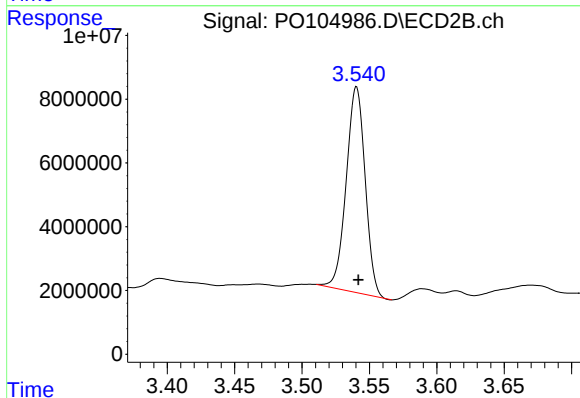


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.002 min
Response: 63331856
Conc: 19.41 ng/ml

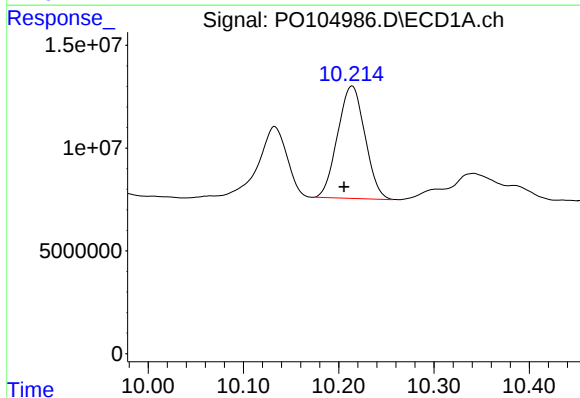

#2 Decachlorobiphenyl

R.T.: 10.214 min
Delta R.T.: 0.008 min
Response: 108925483
Conc: 17.76 ng/ml m

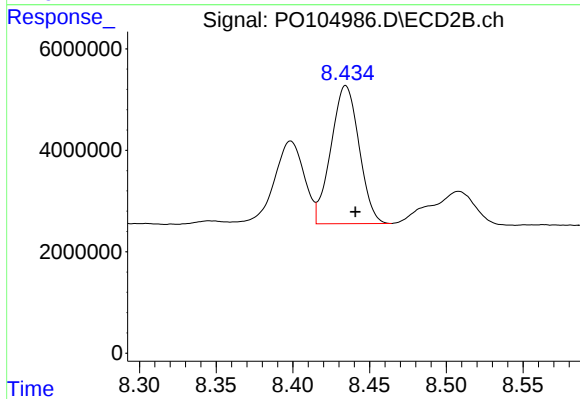

#2 Decachlorobiphenyl

R.T.: 8.434 min
Delta R.T.: -0.006 min
Response: 34788929
Conc: 16.59 ng/ml