

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072724\
 Data File : P0104992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jul 2024 17:06
 Operator : YP/AJ
 Sample : P3376-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-6-Full Waste Class

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/29/2024
 Supervised By :Ankita Jodhani 07/29/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 26 17:32:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.427	3.539	159.1E6	55371406	17.766	16.972
2) SA Decachlor...	10.215	8.434	93836790	26216944	15.301m	12.502

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072724\
Data File : PO104992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jul 2024 17:06
Operator : YP/AJ
Sample : P3376-04
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-6-Full Waste Class


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :Ankita Jodhani 07/29/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 26 17:32:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

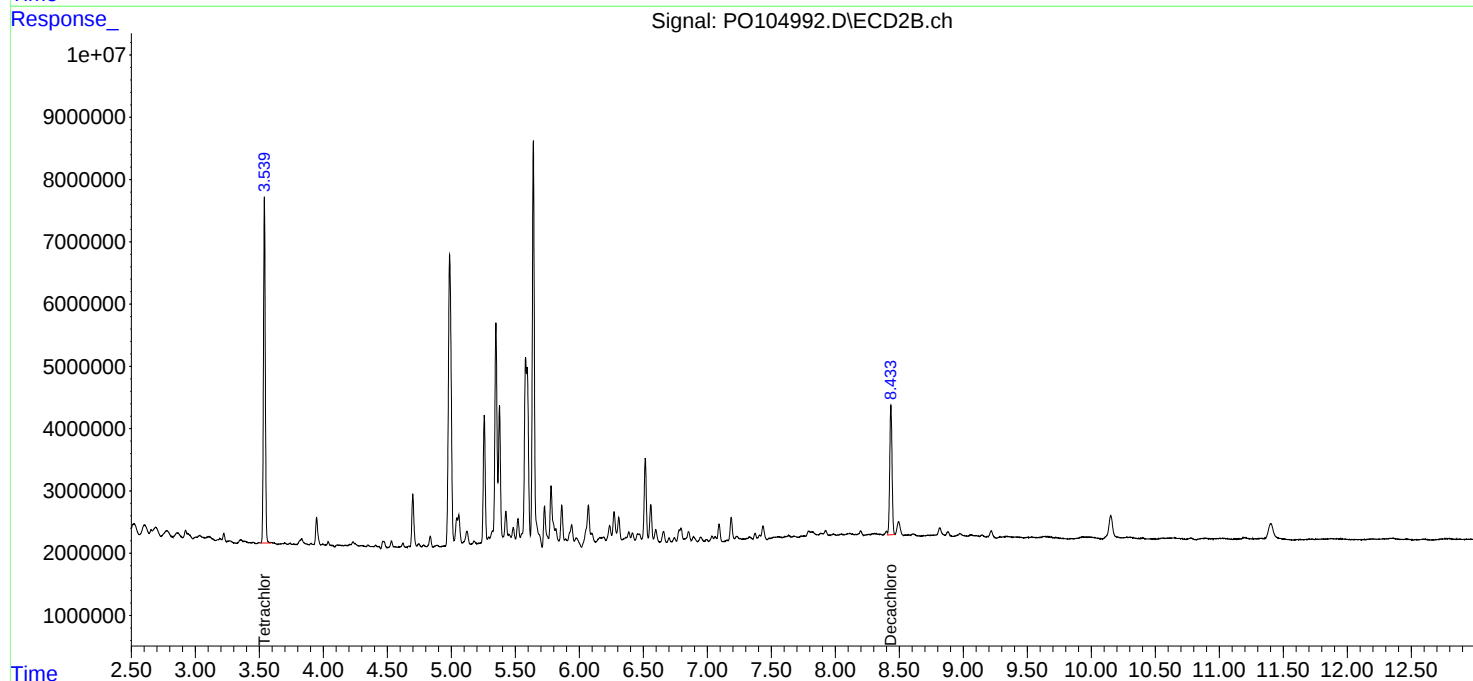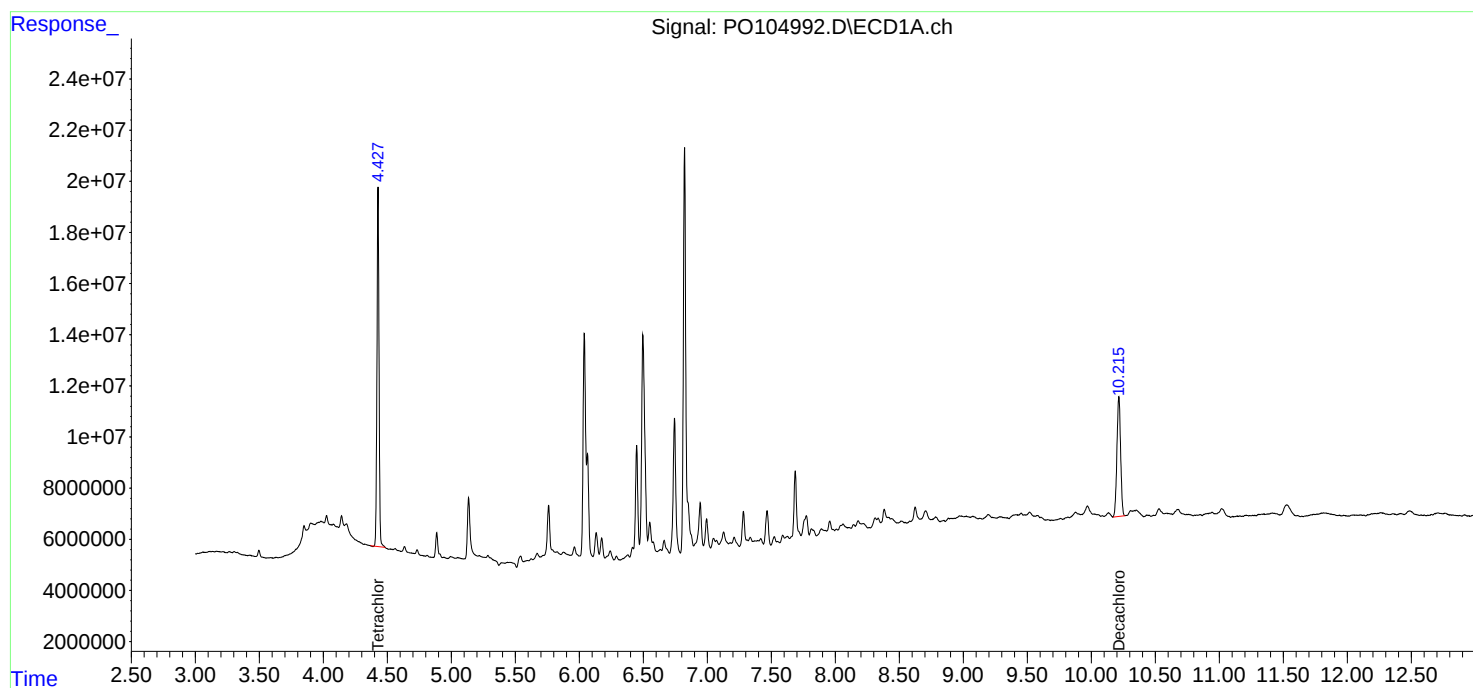

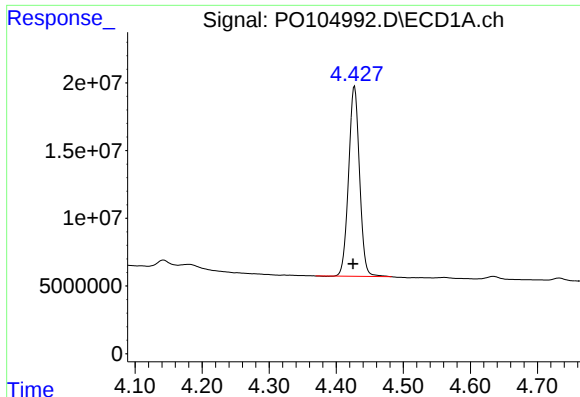


#1 Tetrachloro-m-xylene

R.T.: 4.427 min
Delta R.T.: 0.002 min
Response: 159069062
Conc: 17.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-6-Full Waste Class


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2024
Supervised By :Ankita Jodhani 07/29/2024

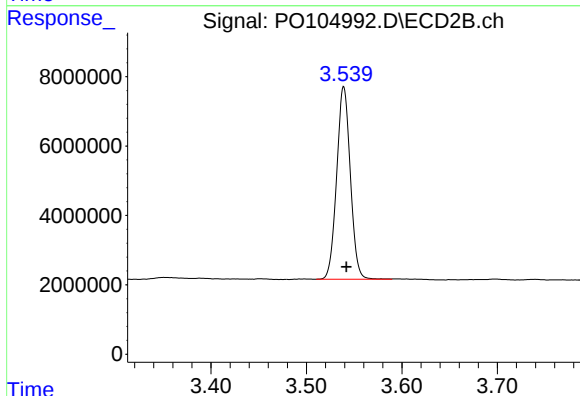


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.003 min
Response: 55371406
Conc: 16.97 ng/ml

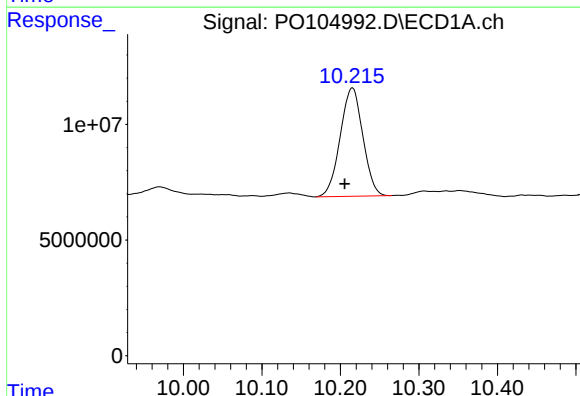

#2 Decachlorobiphenyl

R.T.: 10.215 min
Delta R.T.: 0.009 min
Response: 93836790
Conc: 15.30 ng/ml m

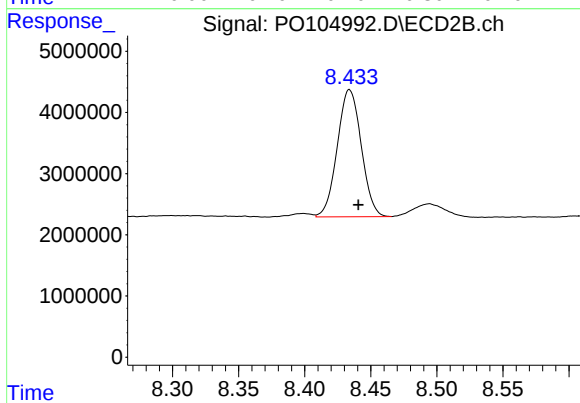

#2 Decachlorobiphenyl

R.T.: 8.434 min
Delta R.T.: -0.007 min
Response: 26216944
Conc: 12.50 ng/ml