

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072818\
Data File : P0047313.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2018 23:41
Operator : SM/SJ
Sample : J4193-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-035

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 06:31:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

	System Monitoring Compounds						
1)	SA Tetrachlo...	4.397	3.644	4051967	4470630	20.069	18.194
2)	SA Decachlor...	10.089	8.639	2054286	2041537	12.595	12.988

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072818\
Data File : P0047313.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2018 23:41
Operator : SM/SJ
Sample : J4193-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-035

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 06:31:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

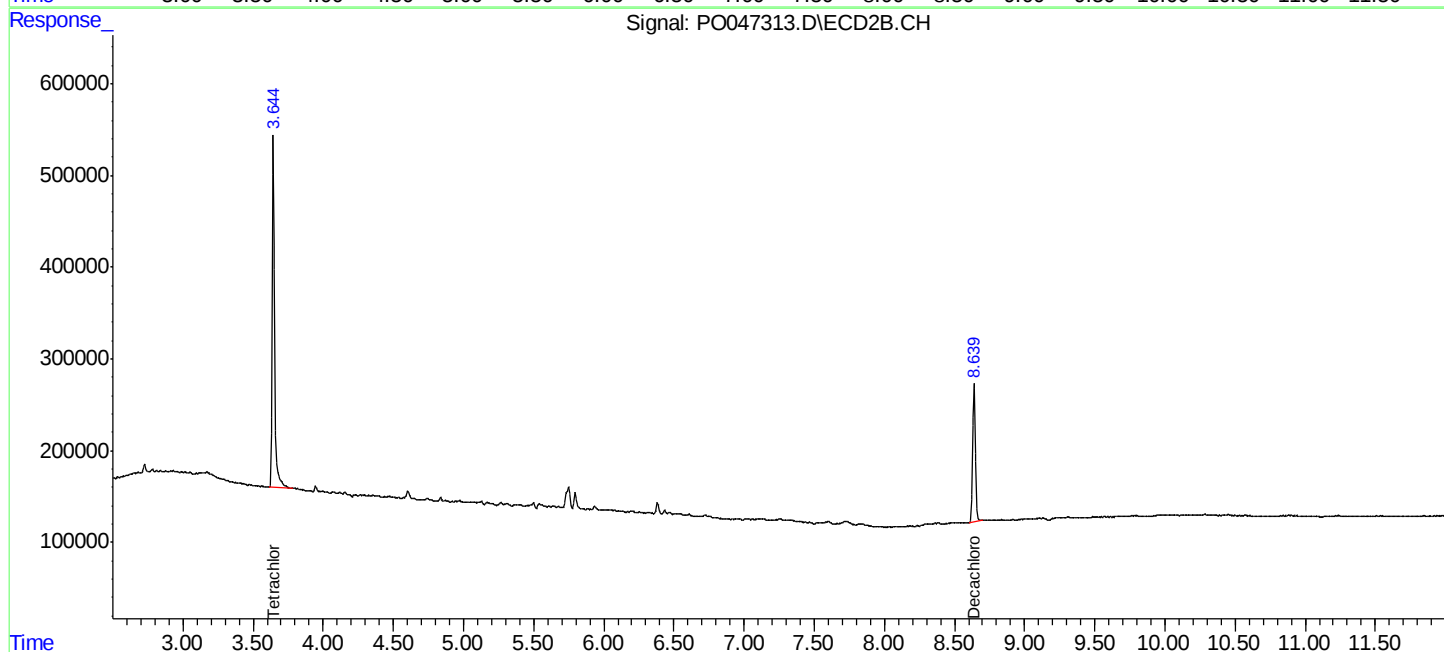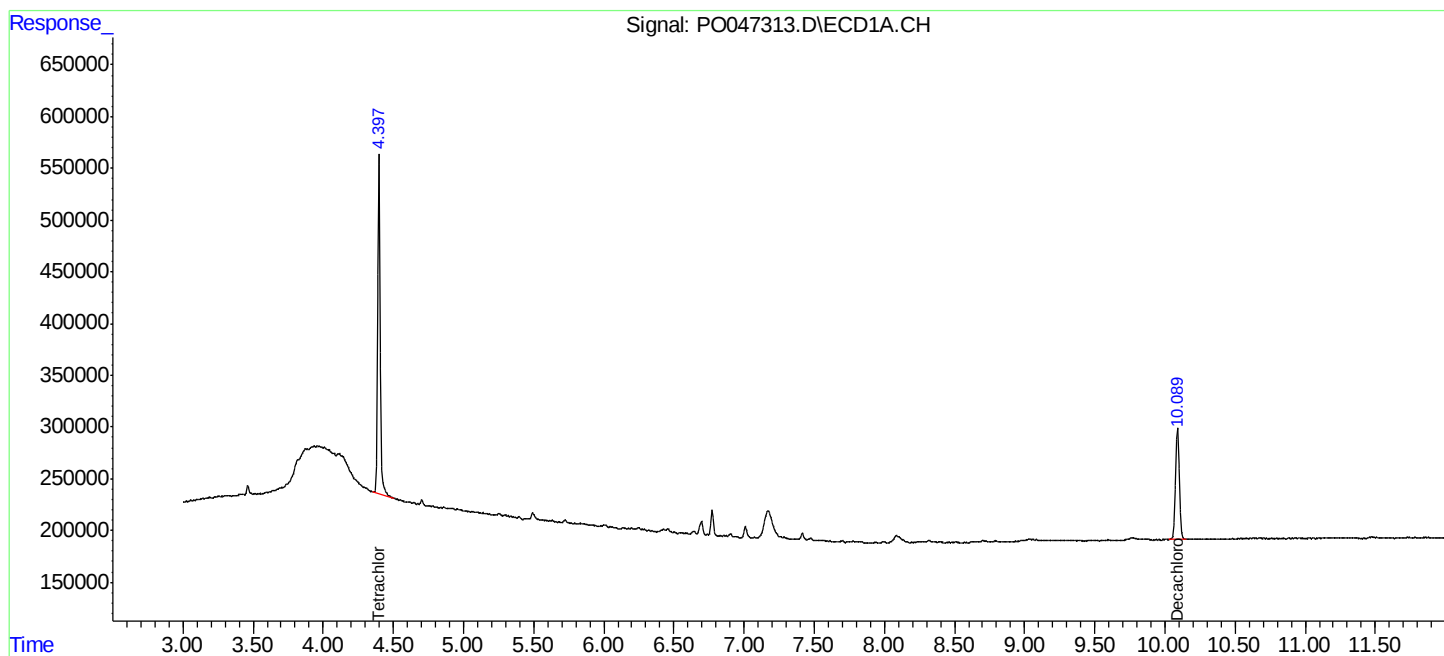


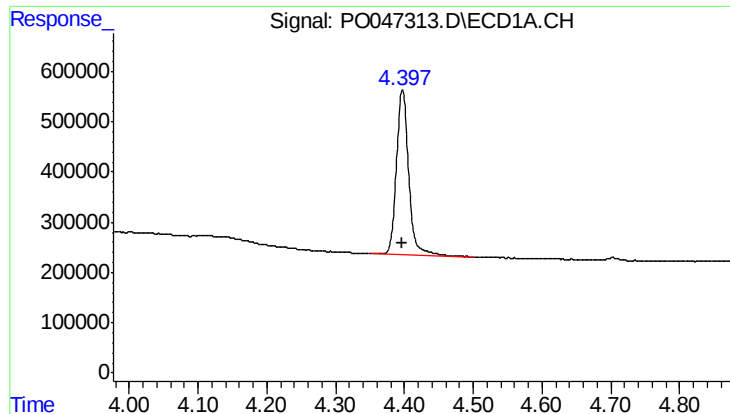

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 4051967
Conc: 20.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-035

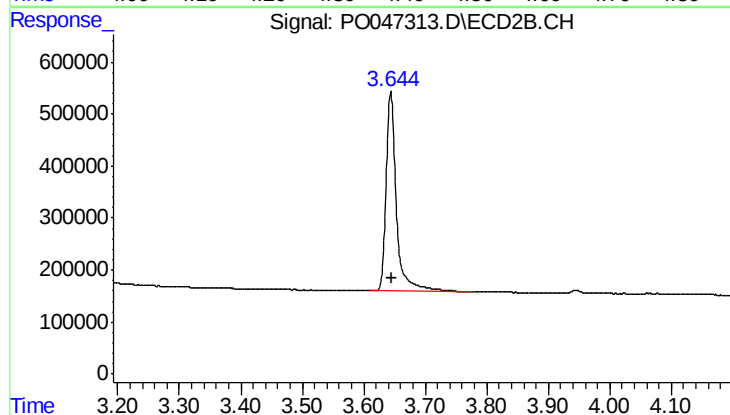


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: -0.001 min
Response: 4470630
Conc: 18.19 ng/ml

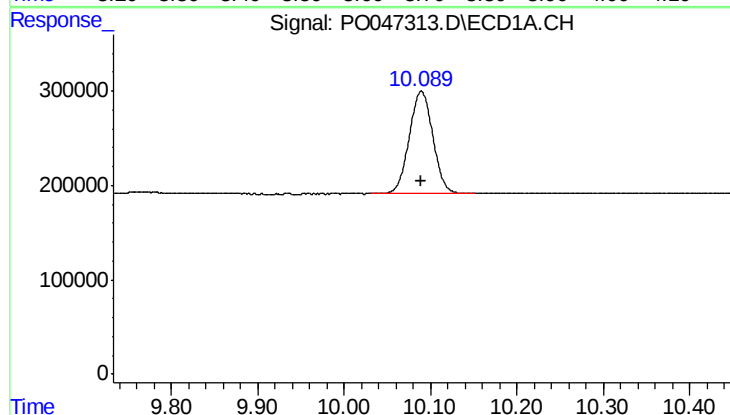

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: 0.000 min
Response: 2054286
Conc: 12.60 ng/ml

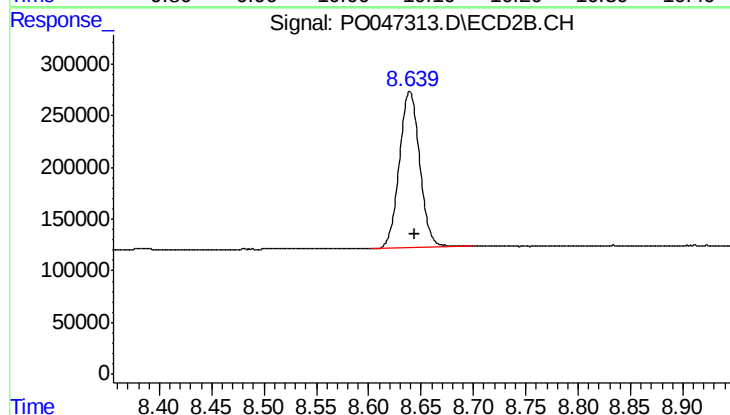

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: -0.005 min
Response: 2041537
Conc: 12.99 ng/ml