

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072818\
Data File : P0047322.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2018 2:04
Operator : SM/SJ
Sample : J4192-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 06:13:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

	System Monitoring Compounds						
1)	SA Tetrachlo...	4.396	3.643	4873373	5447135	24.138	22.168
2)	SA Decachlor...	10.089	8.638	3344666	3287636	20.507	20.915

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072818\
Data File : P0047322.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2018 2:04
Operator : SM/SJ
Sample : J4192-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 06:13:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072718.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 27 02:33:29 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

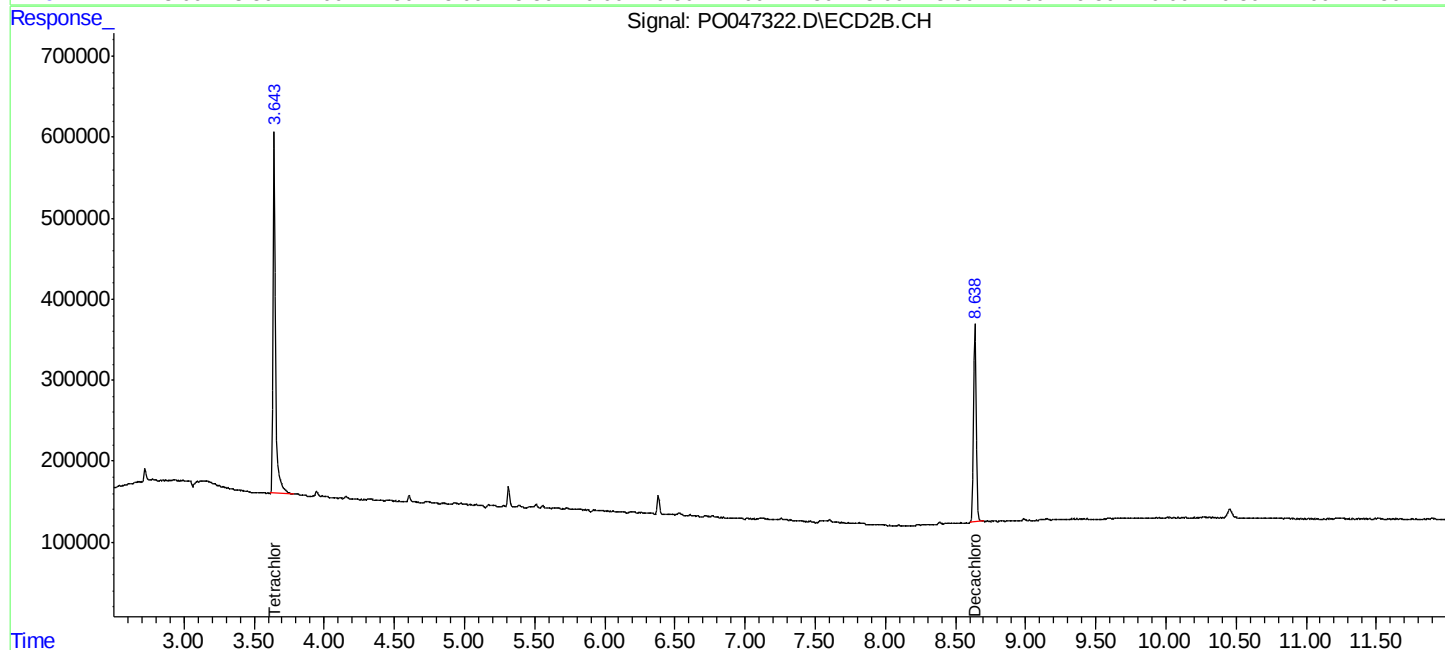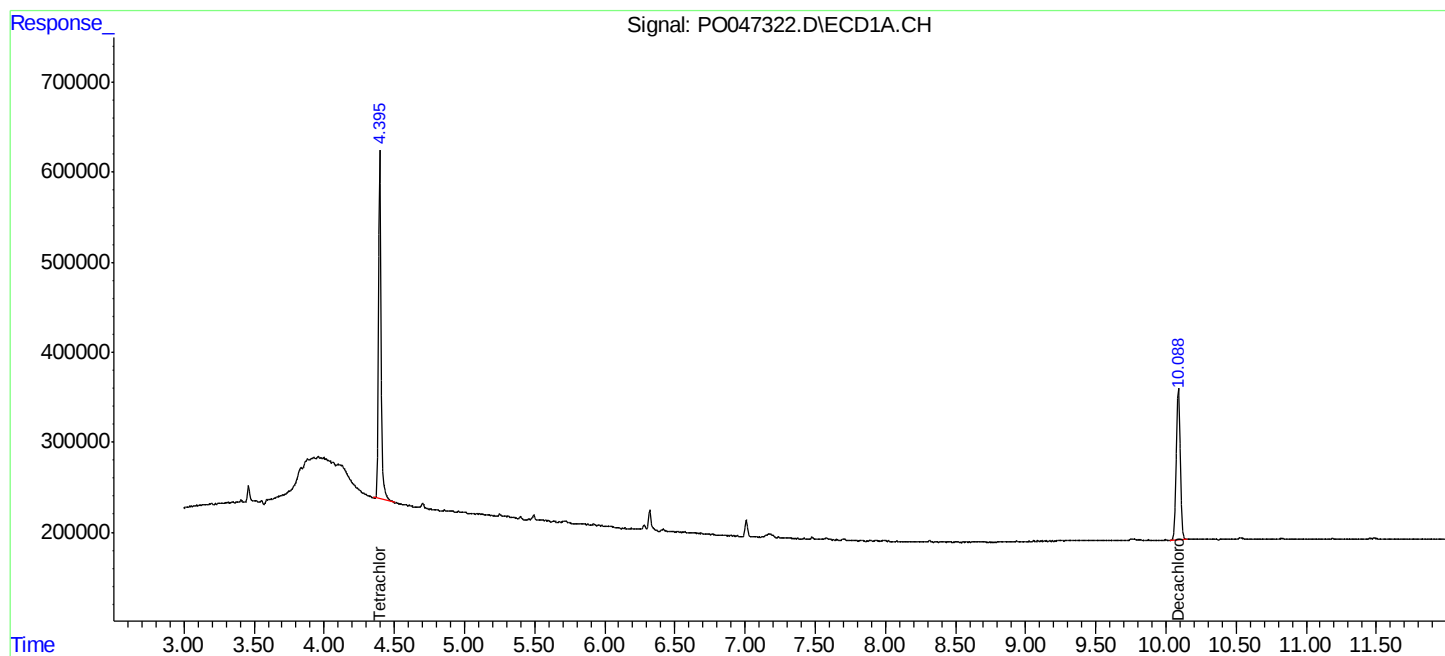


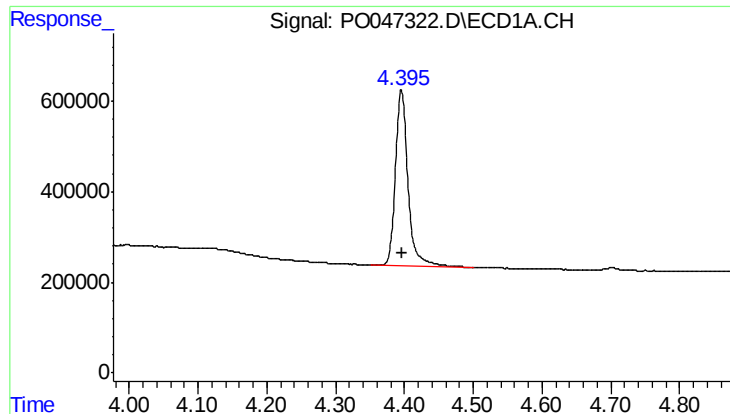

#1 Tetrachloro-m-xylene


R.T.: 4.396 min
Delta R.T.: -0.002 min
Response: 4873373
Conc: 24.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-001-B

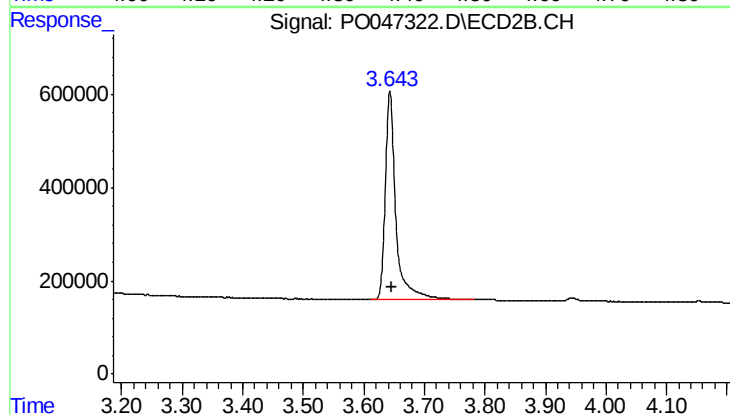


#1 Tetrachloro-m-xylene

R.T.: 3.643 min
Delta R.T.: -0.002 min
Response: 5447135
Conc: 22.17 ng/ml

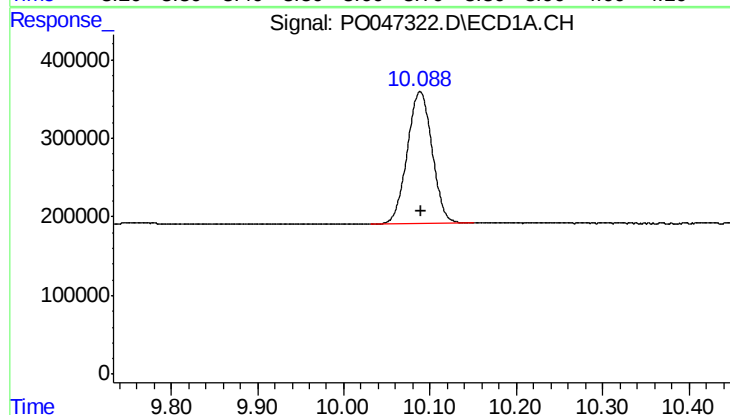

#2 Decachlorobiphenyl

R.T.: 10.089 min
Delta R.T.: -0.001 min
Response: 3344666
Conc: 20.51 ng/ml

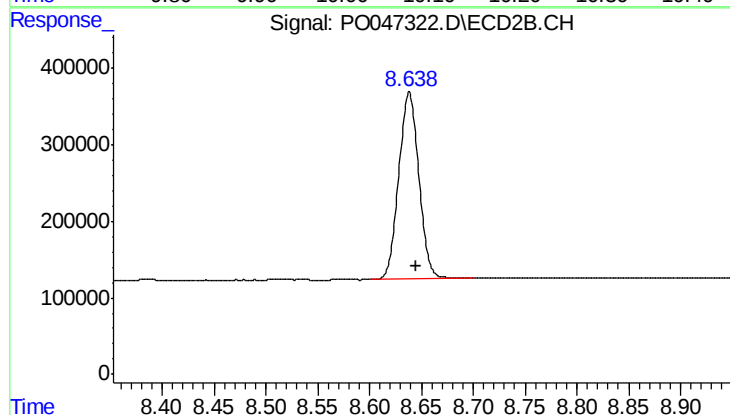

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: -0.006 min
Response: 3287636
Conc: 20.91 ng/ml