

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
 Data File : P0070096.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 9:17
 Operator : DD\AJ
 Sample : L3414-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 61820

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:41:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 13:54:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.582	1158462	1224795	31.639	32.297m
2) SA Decachlor...	10.048	8.779	1243835	994836	20.783	19.033

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
Data File : P0070096.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 9:17
Operator : DD\AJ
Sample : L3414-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
61820


Manual Integrations
APPROVED

Ankita
7/29/2020 4:41:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 13:54:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

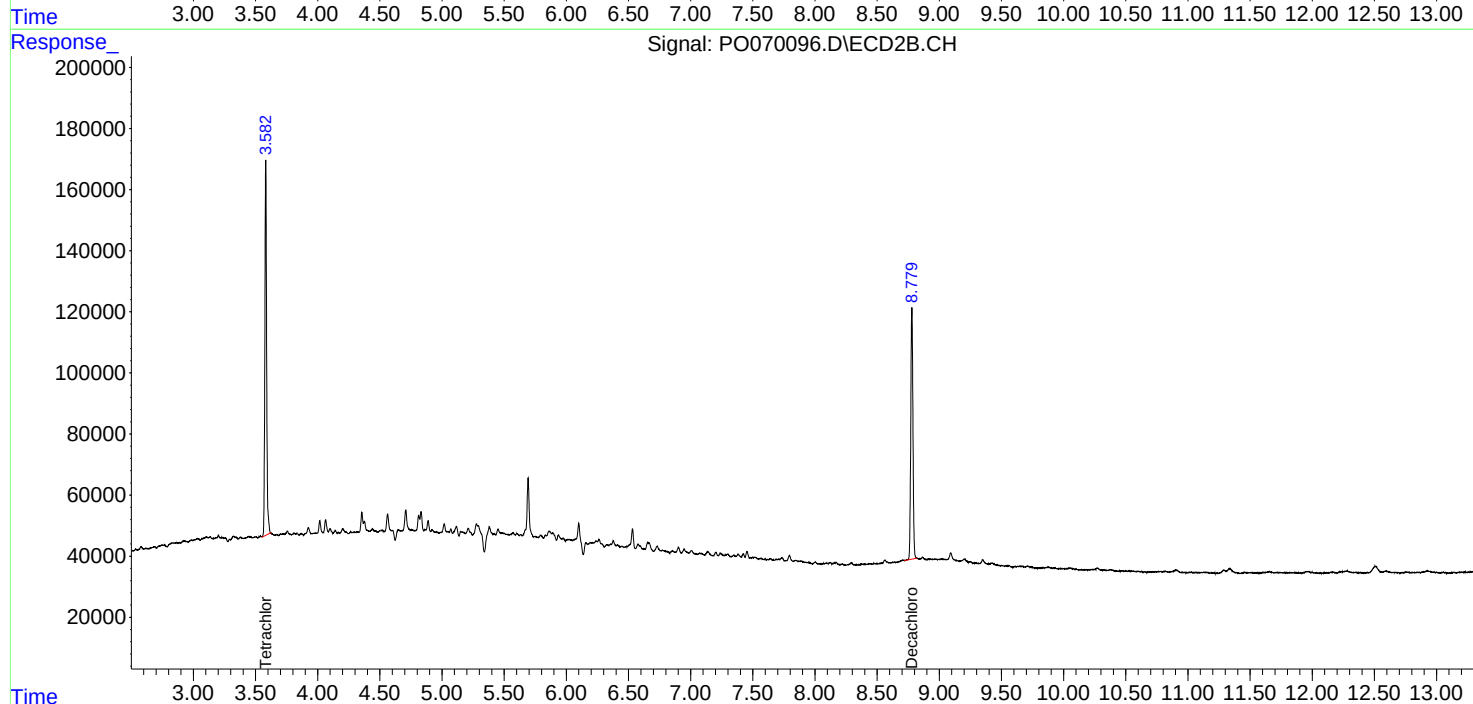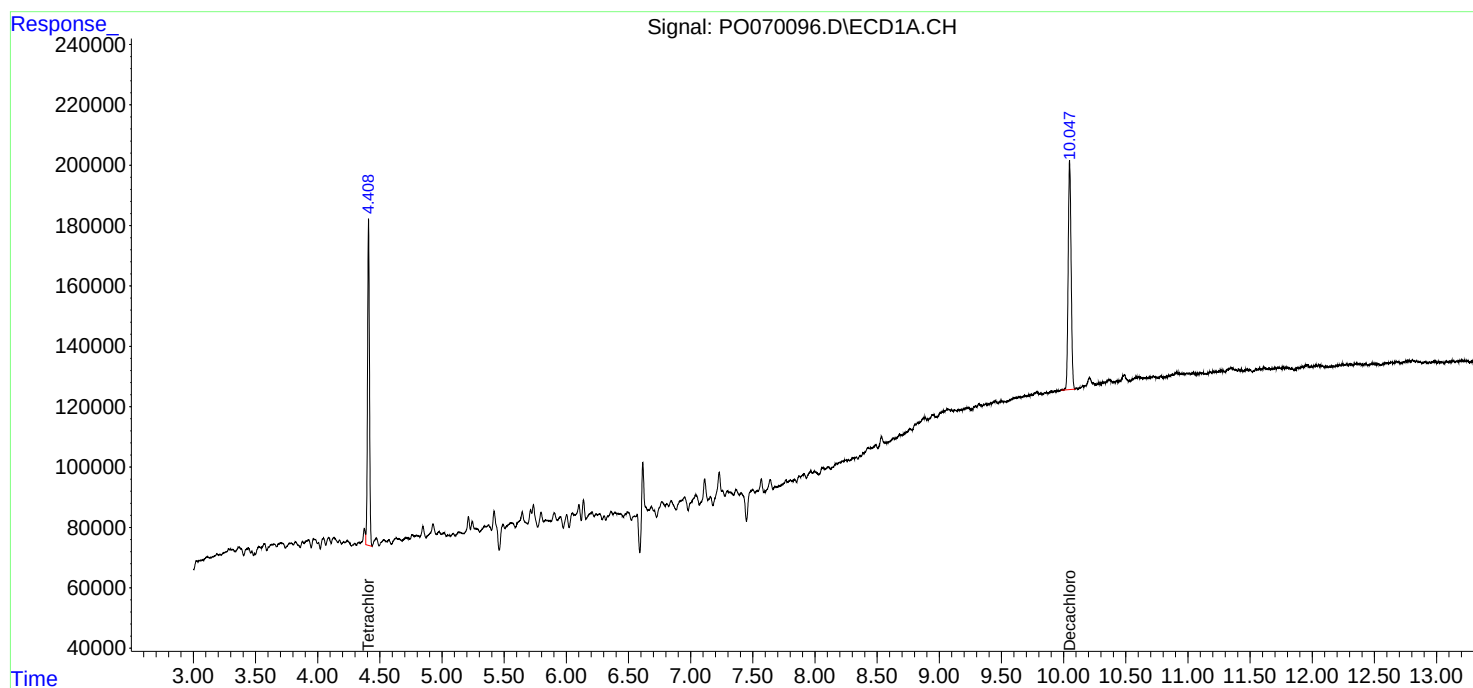

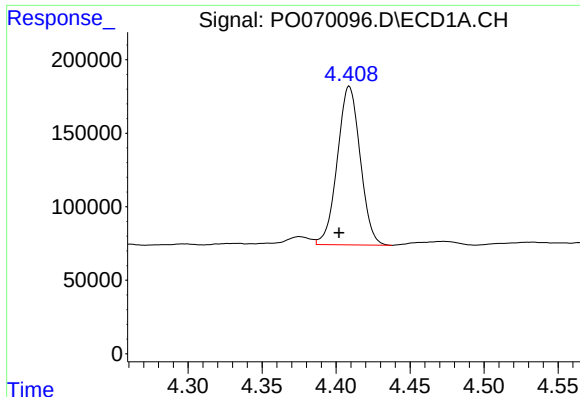


#1 Tetrachloro-m-xylene

R.T.: 4.409 min
Delta R.T.: 0.007 min
Response: 1158462
Conc: 31.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
61820


Manual Integrations
APPROVED

Ankita
7/29/2020 4:41:07 PM

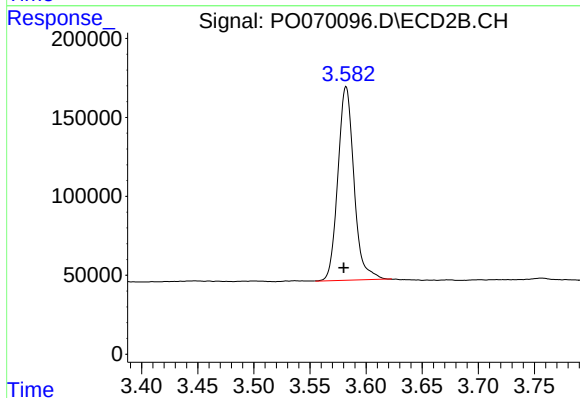


#1 Tetrachloro-m-xylene

R.T.: 3.582 min
Delta R.T.: 0.002 min
Response: 1224795
Conc: 32.30 ng/ml m

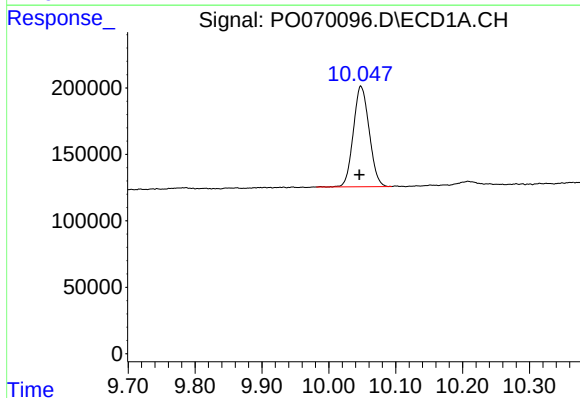

#2 Decachlorobiphenyl

R.T.: 10.048 min
Delta R.T.: 0.002 min
Response: 1243835
Conc: 20.78 ng/ml

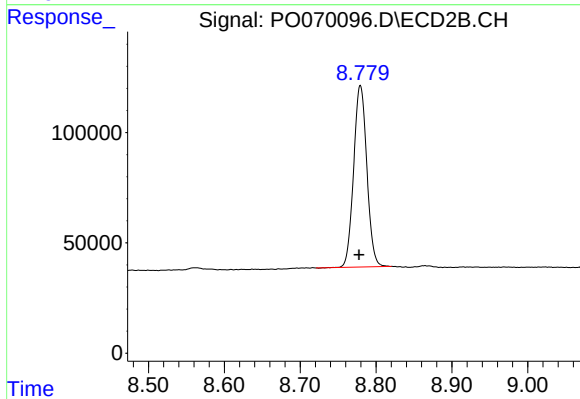

#2 Decachlorobiphenyl

R.T.: 8.779 min
Delta R.T.: 0.002 min
Response: 994836
Conc: 19.03 ng/ml