

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
 Data File : P0070097.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 9:34
 Operator : DD\AJ
 Sample : L3451-01RE 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-03-015-ARE

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:41:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 13:55:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.580	65011	79830	1.776	2.105m
2) SA Decachlor...	10.044	8.776	98685	85480	1.649	1.635m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
Data File : P0070097.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 9:34
Operator : DD\AJ
Sample : L3451-01RE 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-GF-03-015-ARE


Manual Integrations
APPROVED

Ankita
7/29/2020 4:41:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 13:55:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

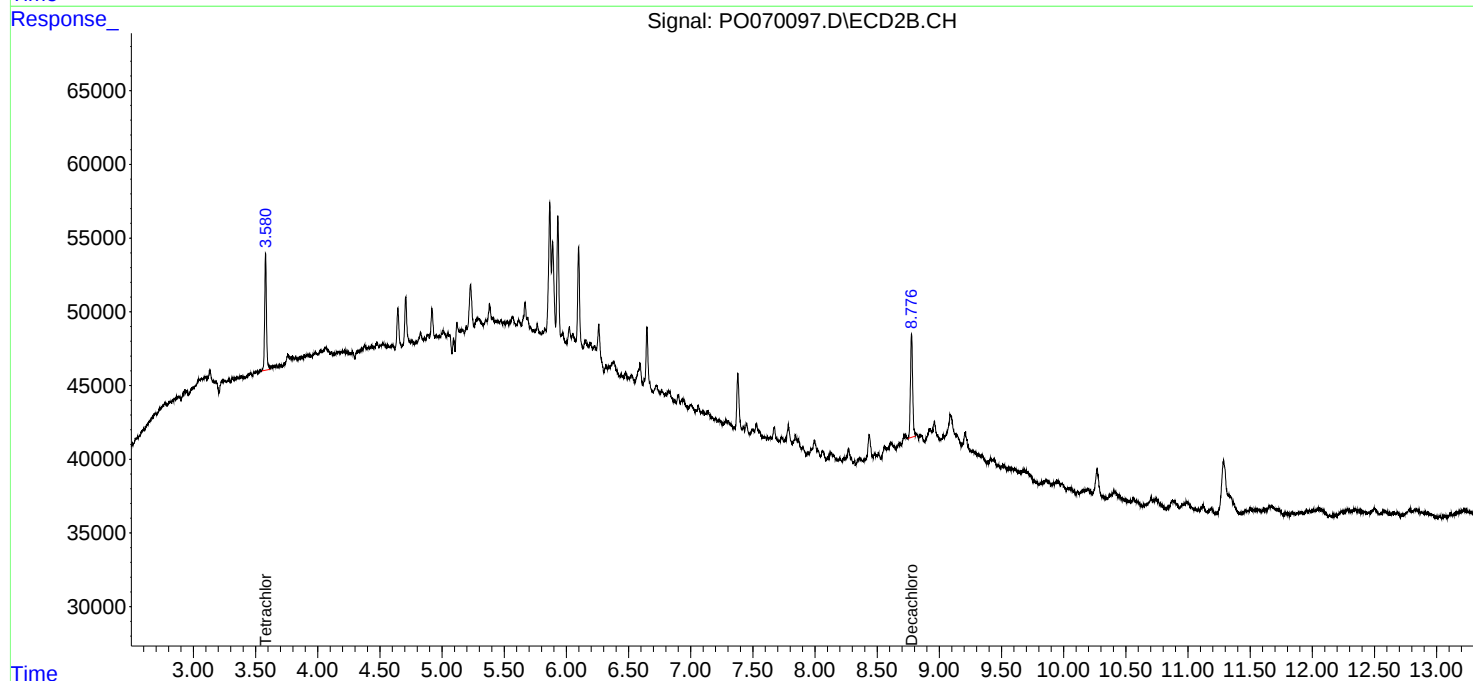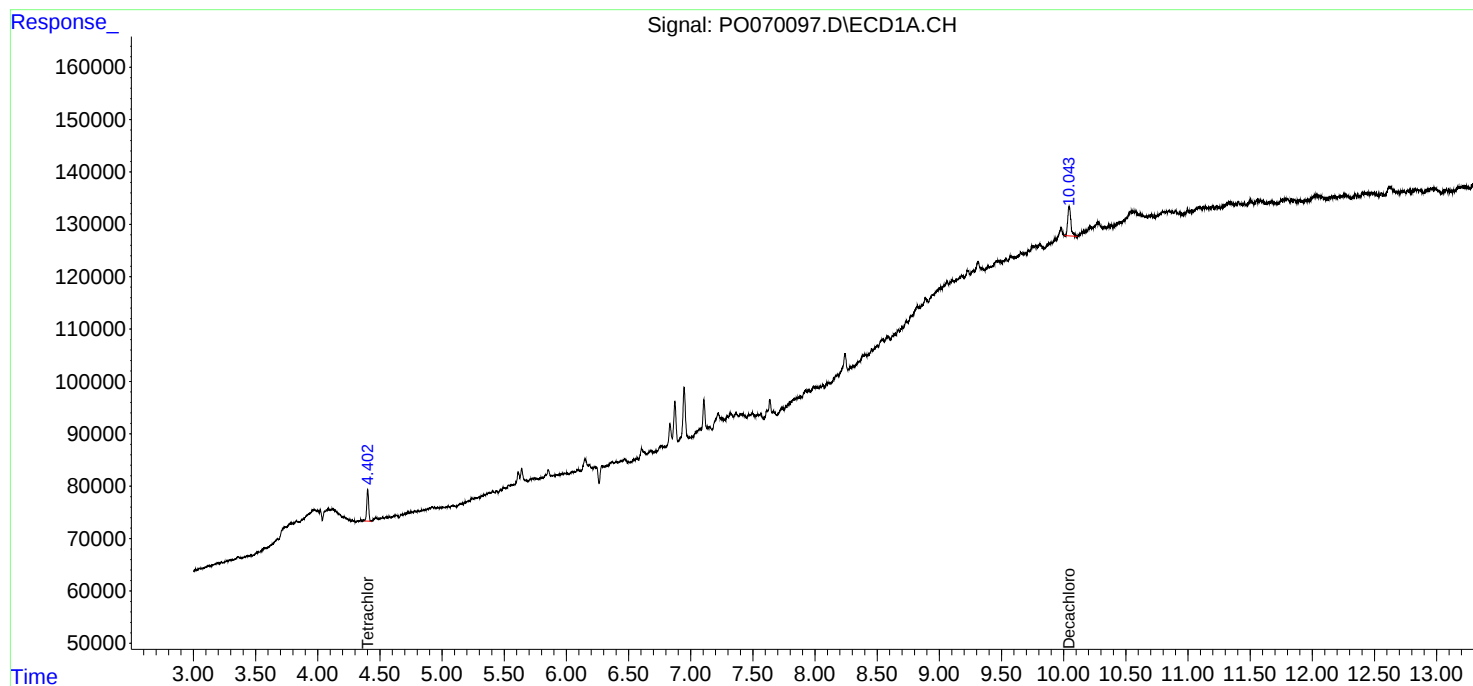

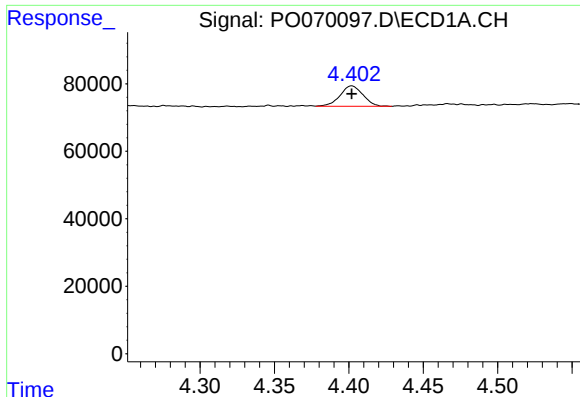


#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: 0.000 min
Response: 65011
Conc: 1.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-03-015-ARE


Manual Integrations
APPROVED

Ankita
7/29/2020 4:41:09 PM

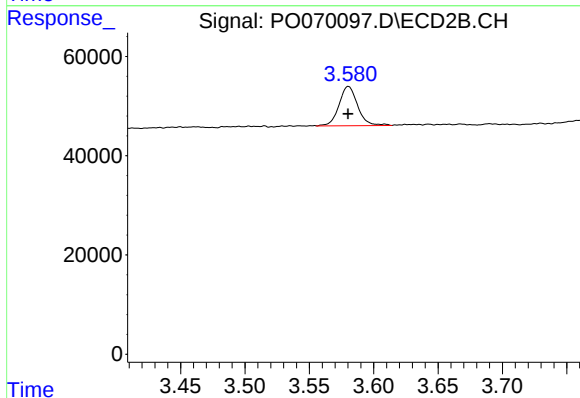


#1 Tetrachloro-m-xylene

R.T.: 3.580 min
Delta R.T.: 0.000 min
Response: 79830
Conc: 2.11 ng/ml m

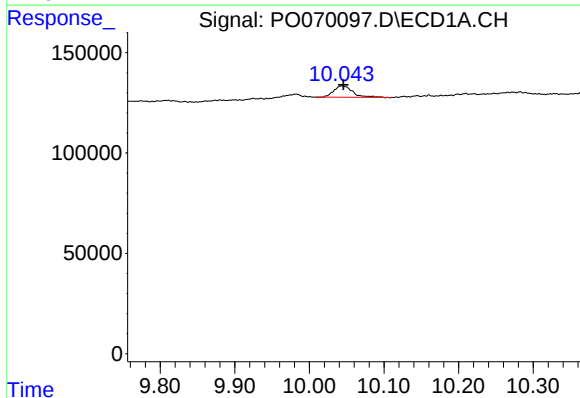

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.002 min
Response: 98685
Conc: 1.65 ng/ml

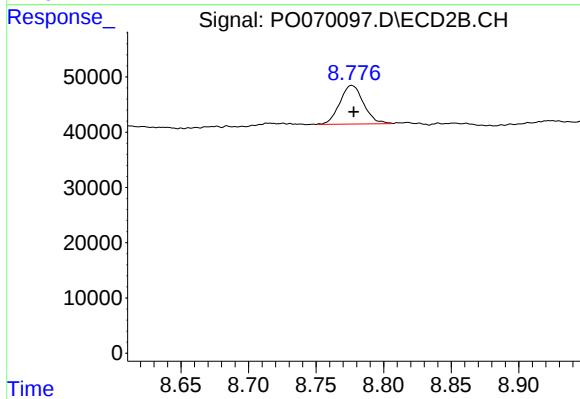

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: -0.002 min
Response: 85480
Conc: 1.64 ng/ml m