

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
 Data File : P0070098.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 9:52
 Operator : DD\AJ
 Sample : L3453-01RE 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-067RE

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:41:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 13:55:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.580	262463	289823	7.168	7.643
2) SA Decachlor...	10.042	8.777	331558	282817	5.540m	5.411

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
Data File : P0070098.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 9:52
Operator : DD\AJ
Sample : L3453-01RE 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067RE


Manual Integrations
APPROVED

Ankita
7/29/2020 4:41:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 13:55:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

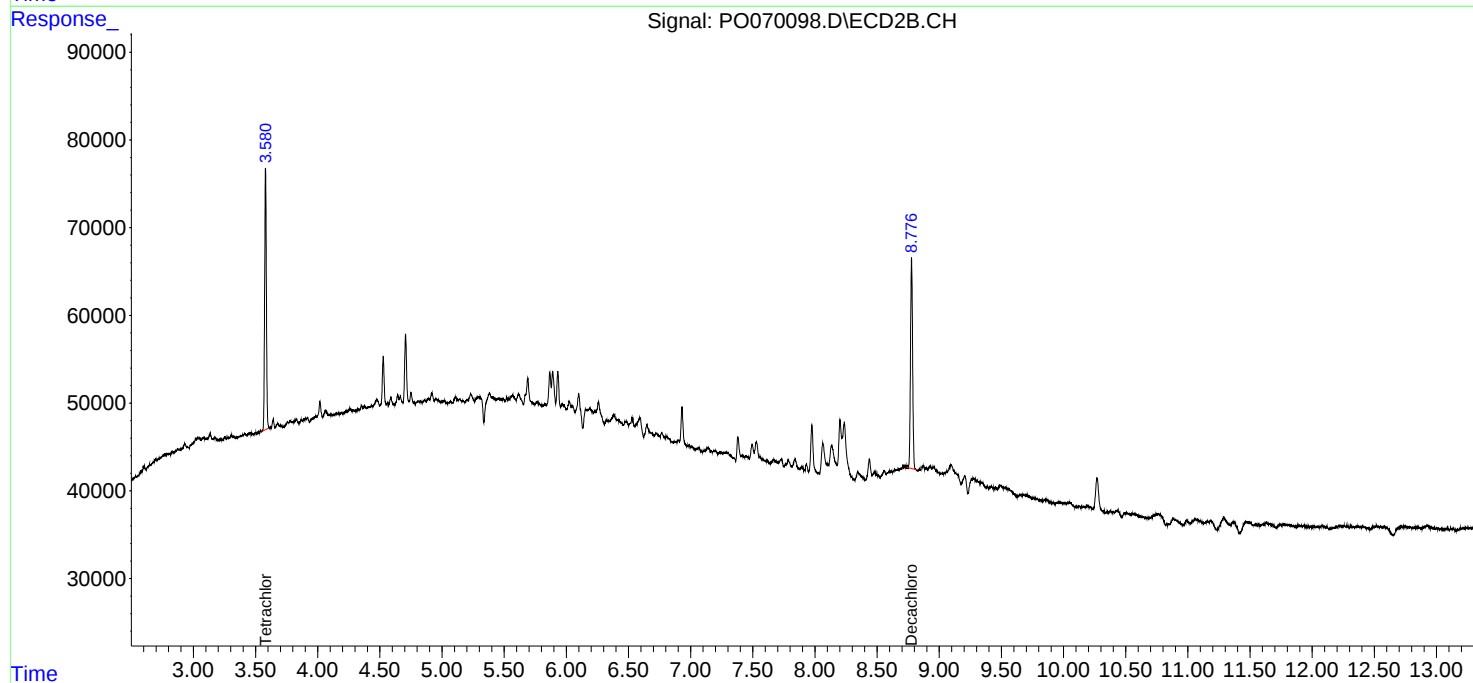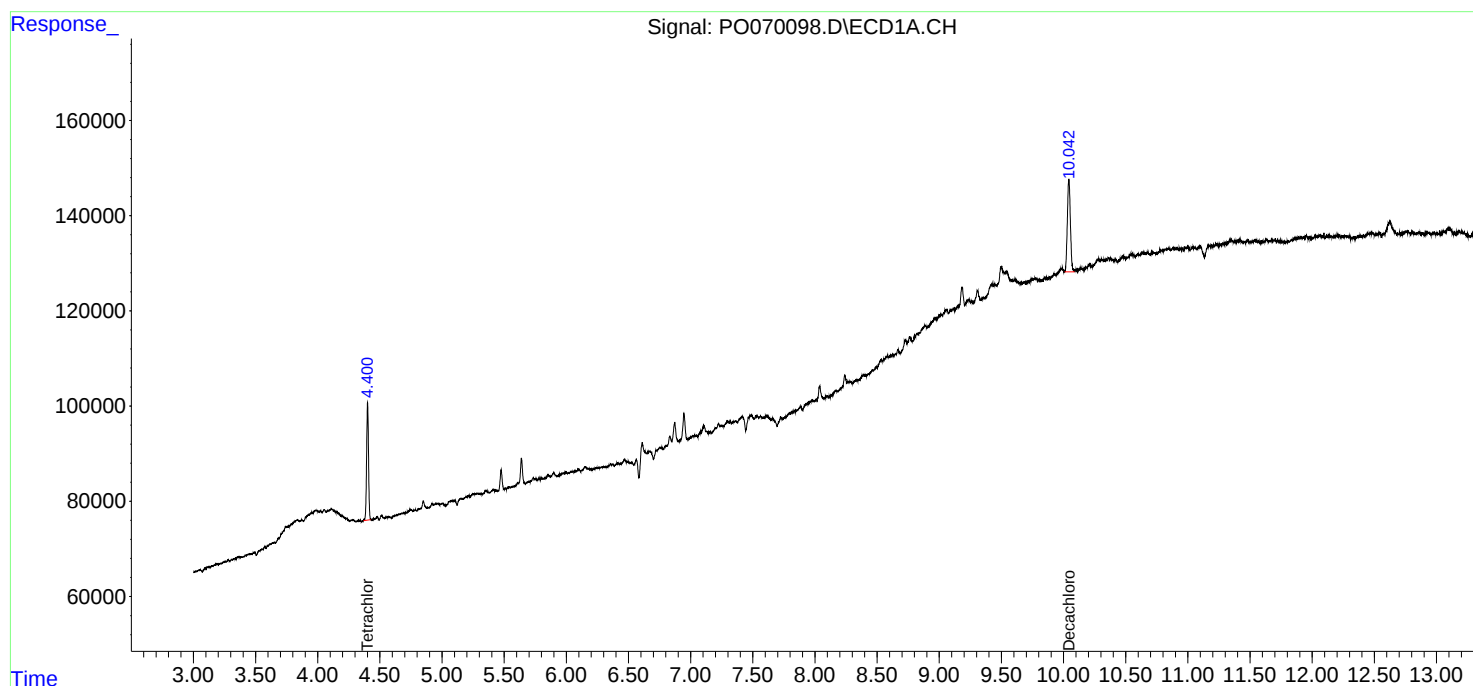

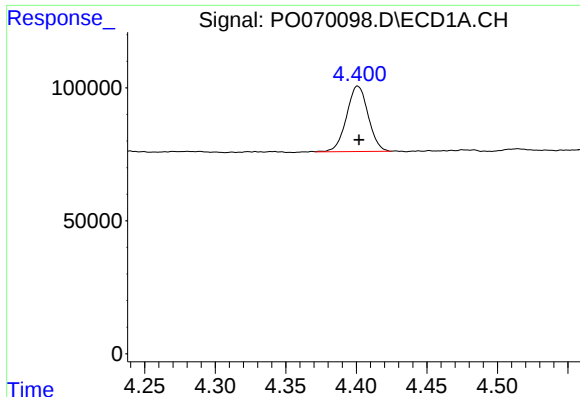


#1 Tetrachloro-m-xylene

R.T.: 4.401 min
Delta R.T.: -0.001 min
Response: 262463
Conc: 7.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-067RE


Manual Integrations
APPROVED

Ankita
7/29/2020 4:41:10 PM

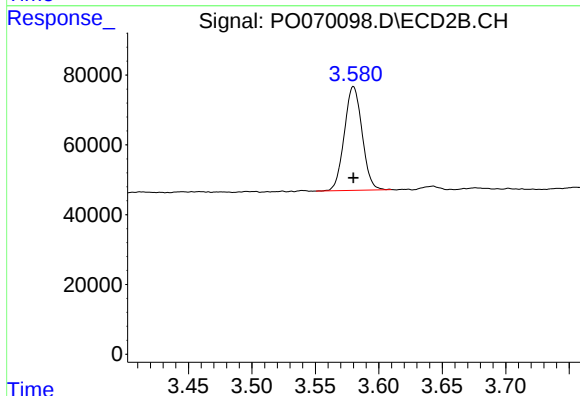


#1 Tetrachloro-m-xylene

R.T.: 3.580 min
Delta R.T.: 0.000 min
Response: 289823
Conc: 7.64 ng/ml

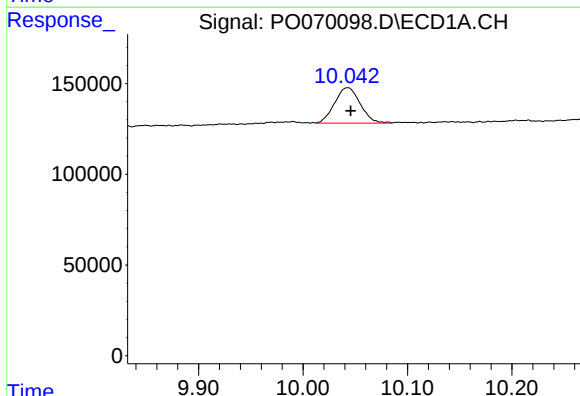

#2 Decachlorobiphenyl

R.T.: 10.042 min
Delta R.T.: -0.003 min
Response: 331558
Conc: 5.54 ng/ml m

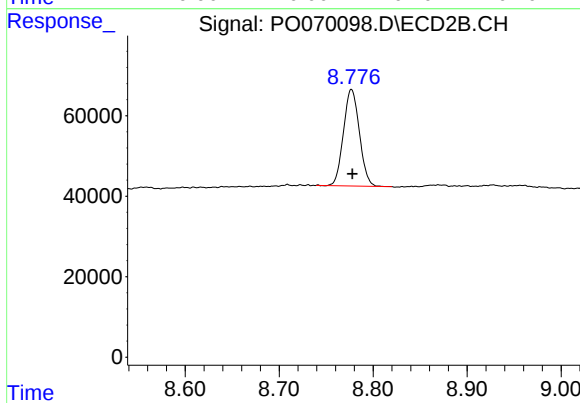

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.000 min
Response: 282817
Conc: 5.41 ng/ml