

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
 Data File : P0070128.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 19:40
 Operator : DD\AJ
 Sample : L3472-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 X068-S8

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:42:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 05:08:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.387	3.568	662101	751824	18.083	19.825
2) SA Decachlor...	10.025	8.762	913908	881968	15.271	16.874
Target Compounds						
31) L7 AR-1260-1	7.351	6.360	181342	247629	74.927m	92.886m
32) L7 AR-1260-2	7.617	6.560	382690	443499	107.713	131.702m
33) L7 AR-1260-3	7.974	6.709	433619	278806	143.364	93.151m#
34) L7 AR-1260-4	8.202	7.186	412491	344233	142.860	138.016
35) L7 AR-1260-5	8.516	7.437	758620	838796	111.188	130.591

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072820\
Data File : PO070128.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 19:40
Operator : DD\AJ
Sample : L3472-02
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
X068-S8


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 05:08:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

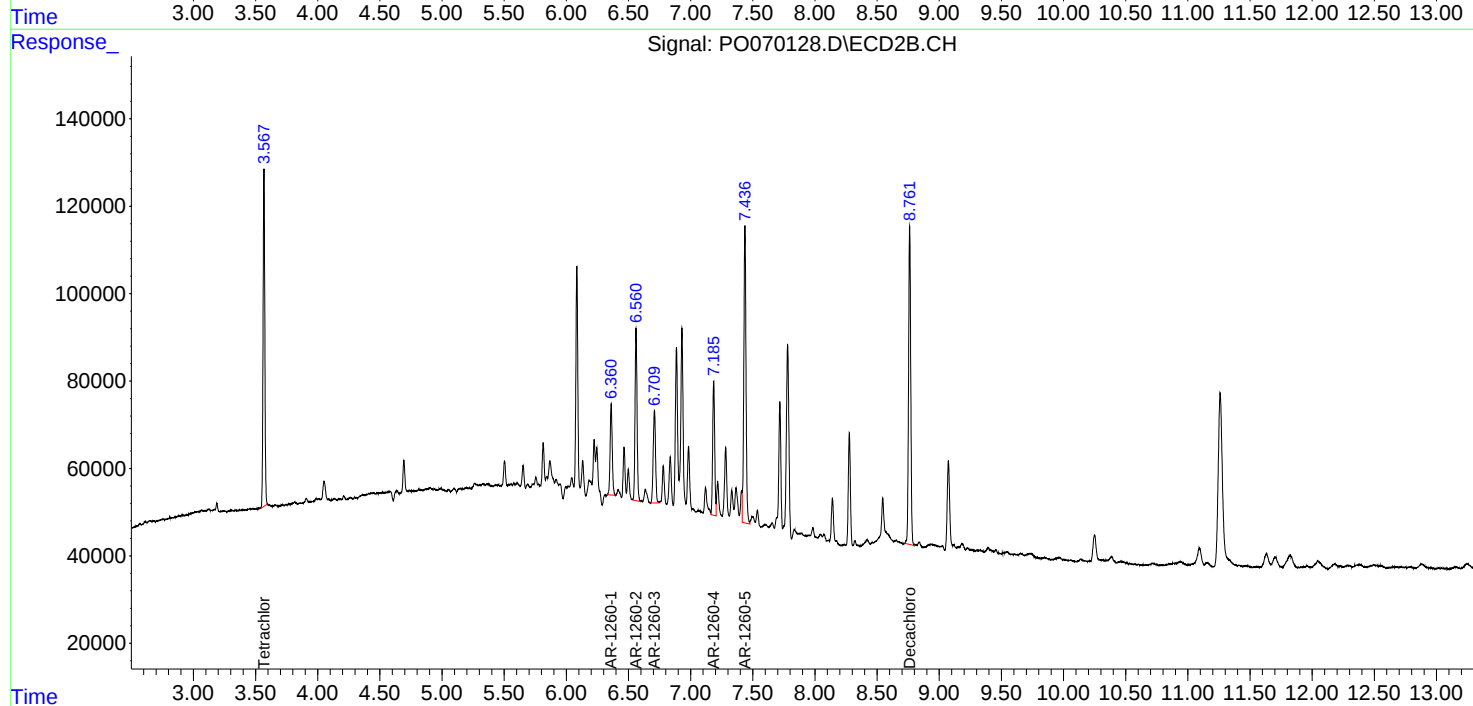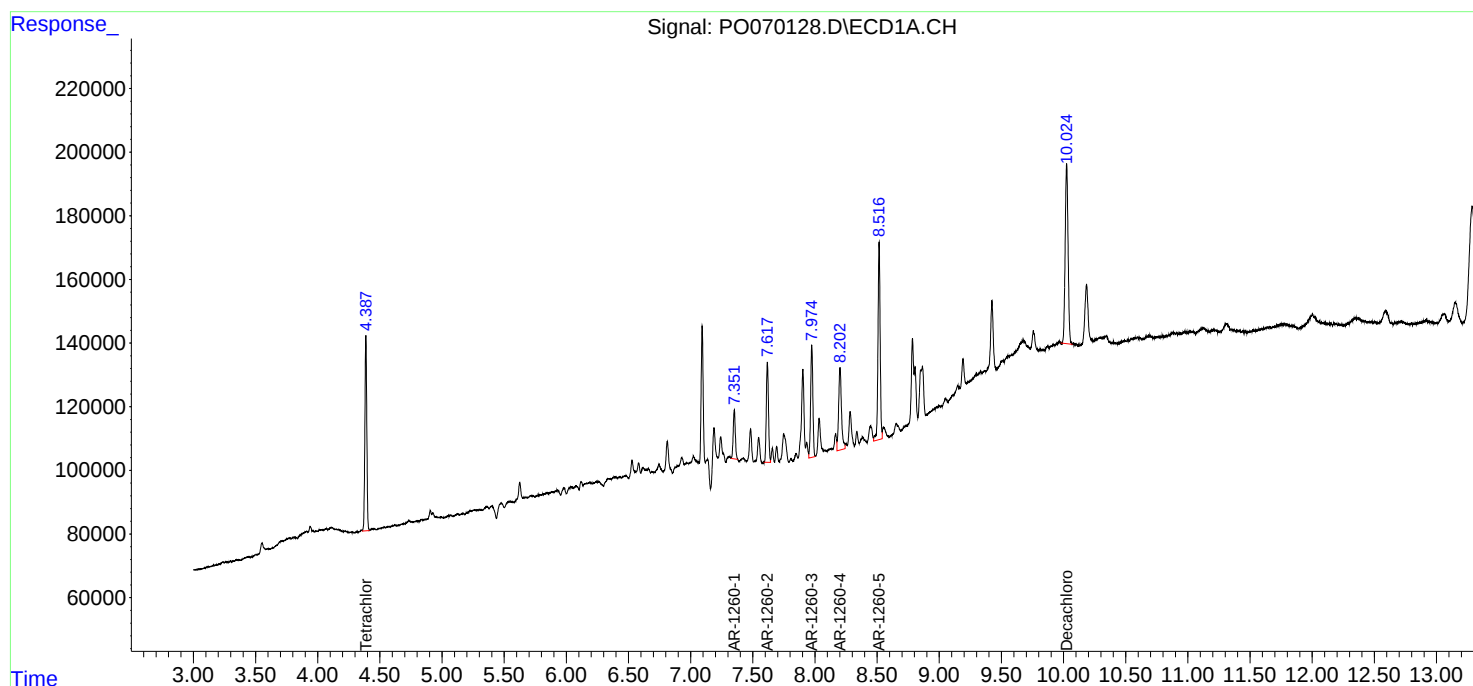

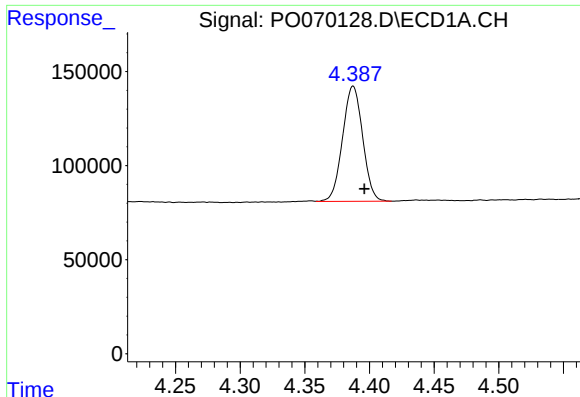


#1 Tetrachloro-m-xylene

R.T.: 4.387 min
Delta R.T.: -0.009 min
Response: 662101
Conc: 18.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-S8


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:13 PM

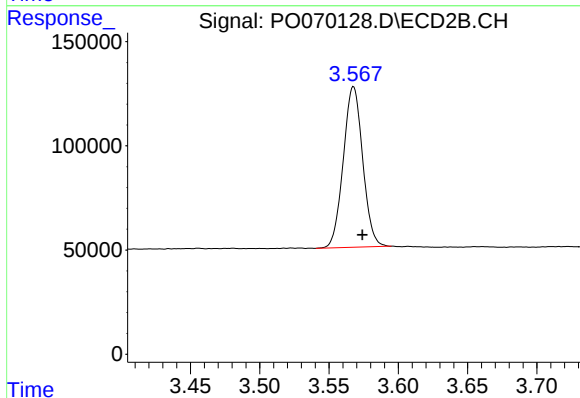


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: -0.006 min
Response: 751824
Conc: 19.83 ng/ml

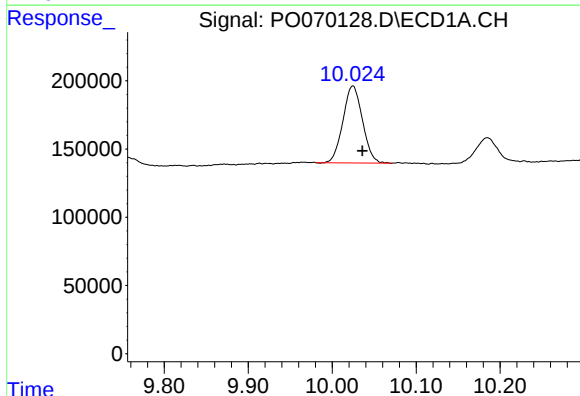


#2 Decachlorobiphenyl

R.T.: 10.025 min
Delta R.T.: -0.011 min
Response: 913908
Conc: 15.27 ng/ml

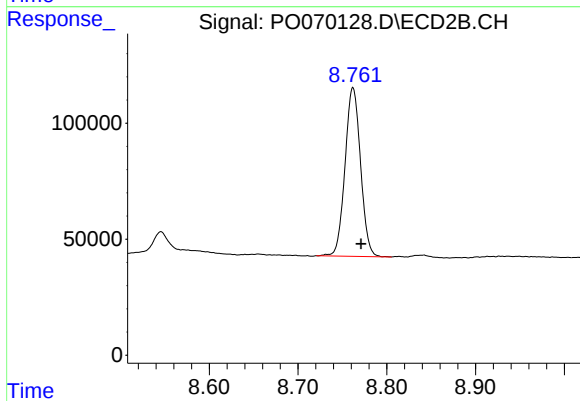

#2 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: -0.009 min
Response: 881968
Conc: 16.87 ng/ml

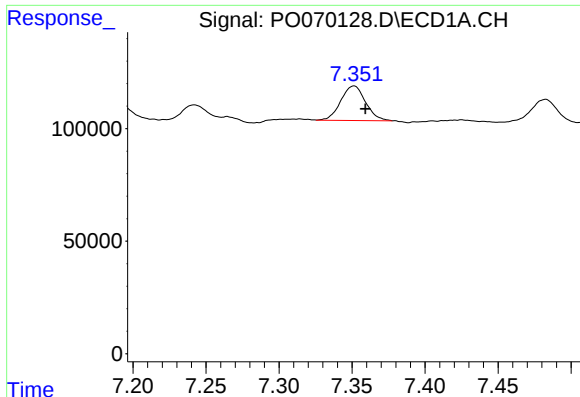


#31 AR-1260-1

R.T.: 7.351 min
Delta R.T.: -0.008 min
Response: 181342
Conc: 74.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
X068-S8


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:13 PM

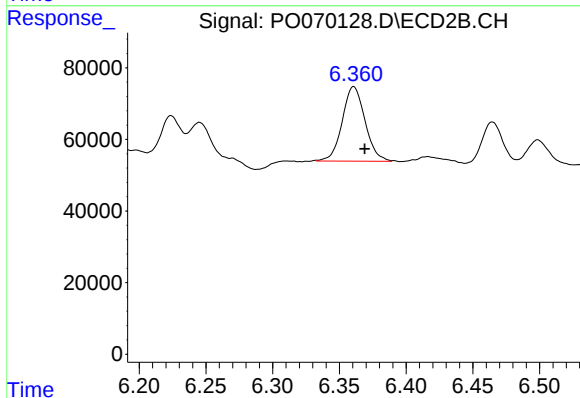


#31 AR-1260-1

R.T.: 6.360 min
Delta R.T.: -0.009 min
Response: 247629
Conc: 92.89 ng/ml m

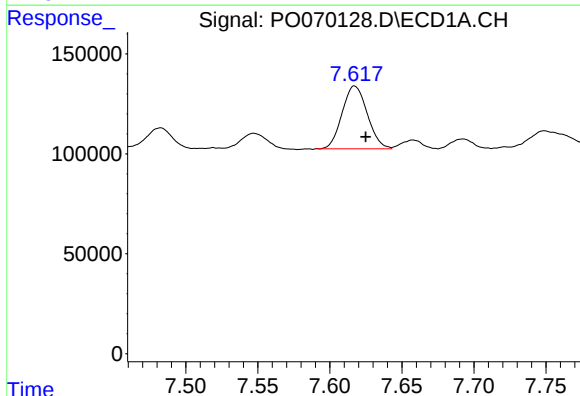


#32 AR-1260-2

R.T.: 7.617 min
Delta R.T.: -0.008 min
Response: 382690
Conc: 107.71 ng/ml

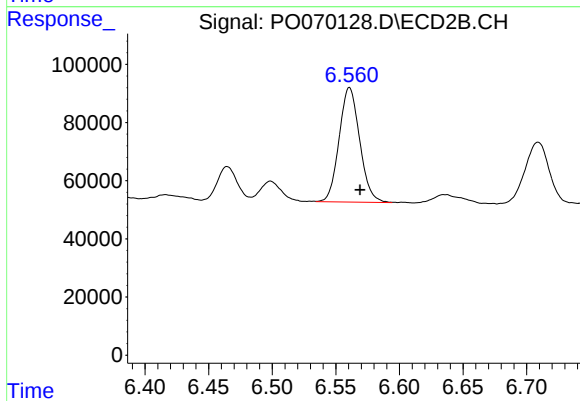

#32 AR-1260-2

R.T.: 6.560 min
Delta R.T.: -0.009 min
Response: 443499
Conc: 131.70 ng/ml m

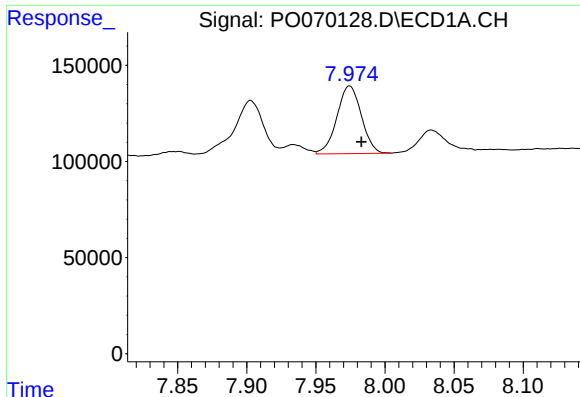


#33 AR-1260-3

R.T.: 7.974 min
Delta R.T.: -0.009 min
Response: 433619
Conc: 143.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-S8


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:13 PM

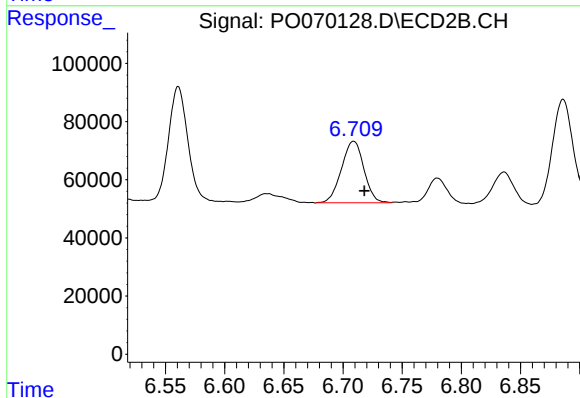


#33 AR-1260-3

R.T.: 6.709 min
Delta R.T.: -0.009 min
Response: 278806
Conc: 93.15 ng/ml m

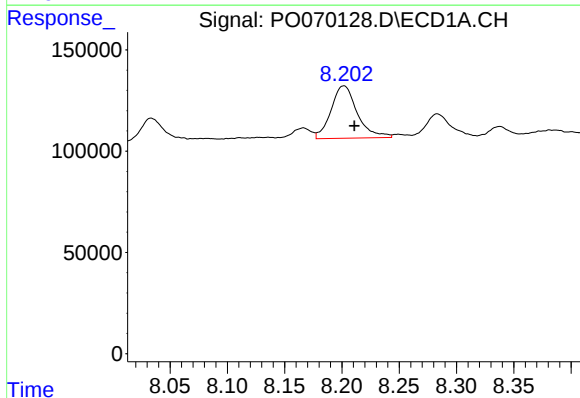


#34 AR-1260-4

R.T.: 8.202 min
Delta R.T.: -0.009 min
Response: 412491
Conc: 142.86 ng/ml

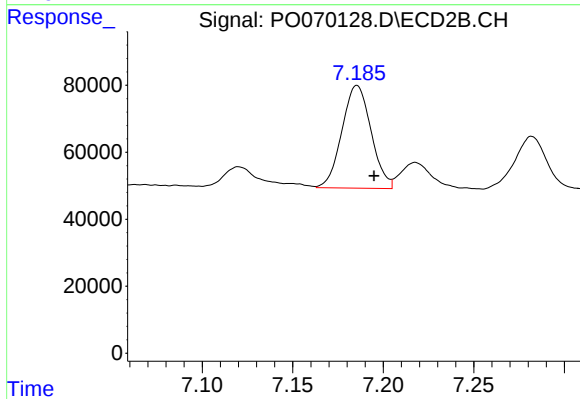

#34 AR-1260-4

R.T.: 7.186 min
Delta R.T.: -0.009 min
Response: 344233
Conc: 138.02 ng/ml

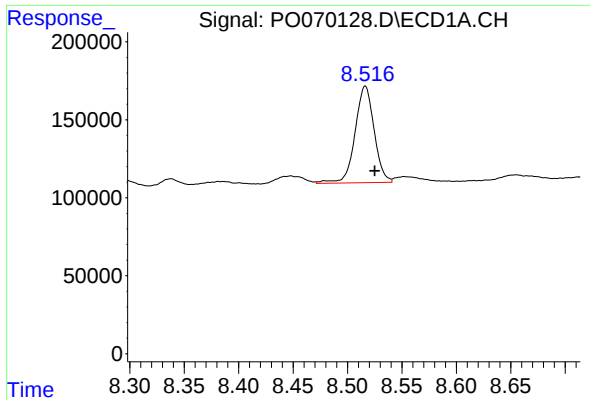


#35 AR-1260-5

R.T.: 8.516 min
Delta R.T.: -0.009 min
Response: 758620
Conc: 111.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-S8

Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:13 PM

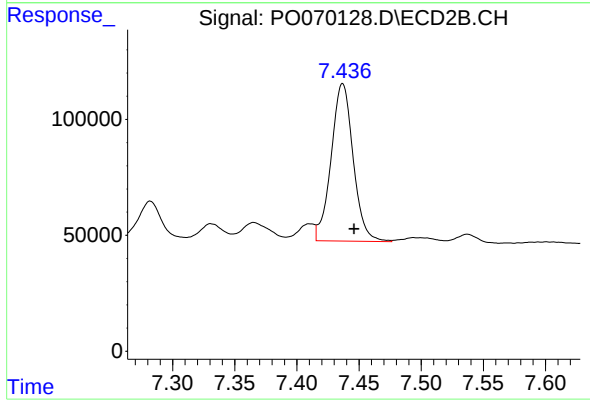

#35 AR-1260-5

R.T.: 7.437 min
Delta R.T.: -0.009 min
Response: 838796
Conc: 130.59 ng/ml