

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
 Data File : P0070132.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 20:49
 Operator : DD\AJ
 Sample : L3472-04 2X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 X068-S7

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:42:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 05:10:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.386	3.567	316958	428457	8.657m	11.298m#
2) SA Decachlor...	10.022	8.761	436814	397434	7.299	7.604
Target Compounds						
31) L7 AR-1260-1	7.348	6.360	473963	444824	195.832m	166.854
32) L7 AR-1260-2	7.616	6.560	1118428	786189	314.797	233.468 #
33) L7 AR-1260-3	7.972	6.709	694331	675053	229.561	225.540
34) L7 AR-1260-4	8.198	7.184	949187	448283	328.738	179.734 #
35) L7 AR-1260-5	8.514	7.436	1043802	940533	152.986	146.431

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
Data File : P0070132.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 20:49
Operator : DD\AJ
Sample : L3472-04 2X
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
X068-S7


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 05:10:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

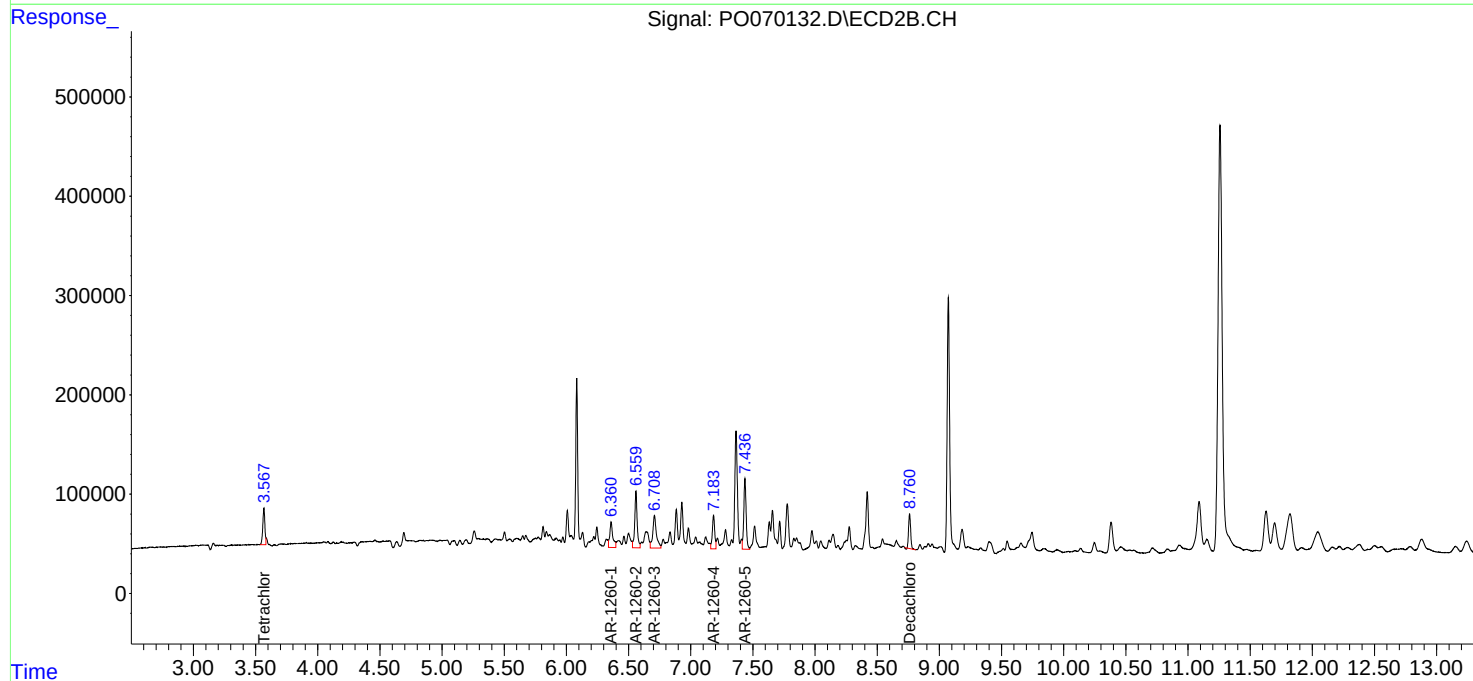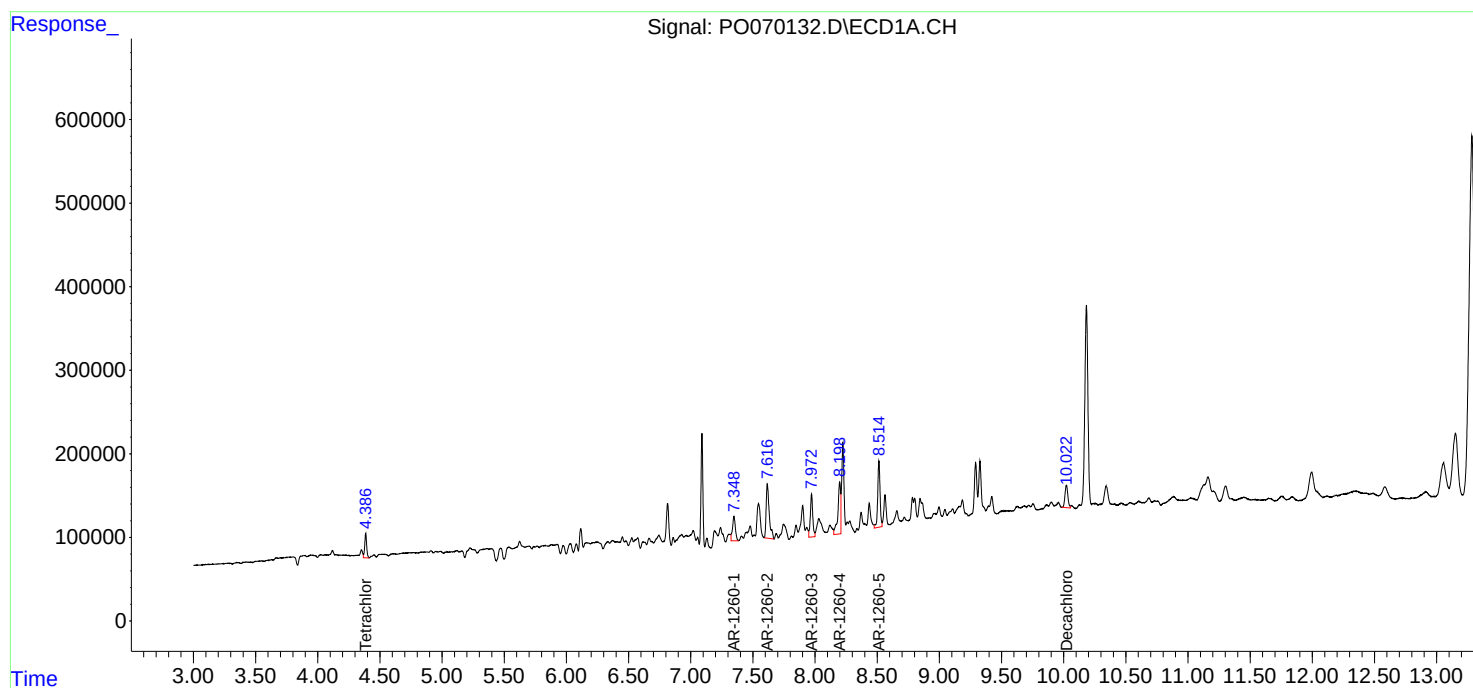

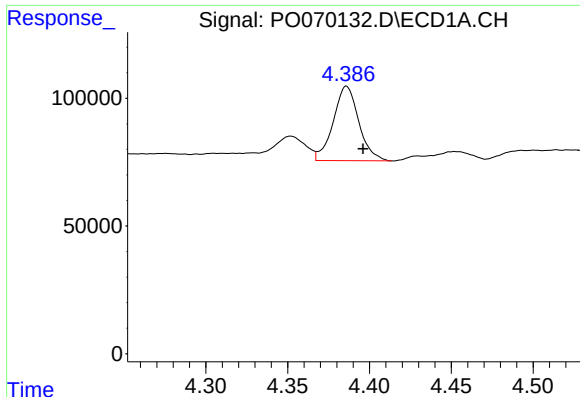


#1 Tetrachloro-m-xylene

R.T.: 4.386 min
Delta R.T.: -0.010 min
Response: 316958
Conc: 8.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
X068-S7


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:20 PM

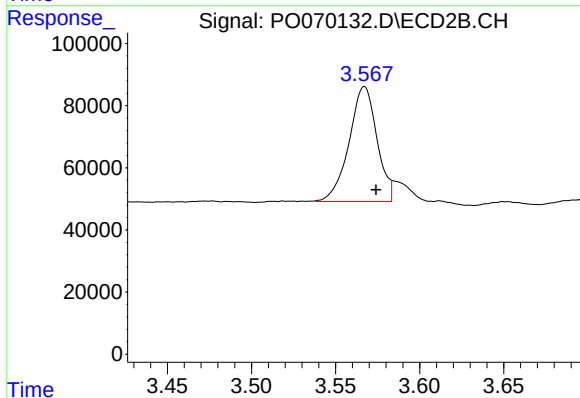


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.007 min
Response: 428457
Conc: 11.30 ng/ml m

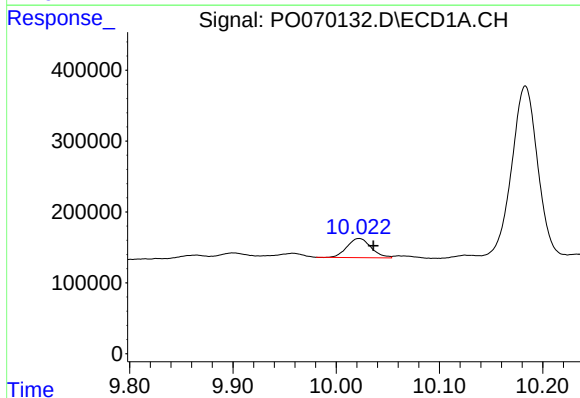


#2 Decachlorobiphenyl

R.T.: 10.022 min
Delta R.T.: -0.014 min
Response: 436814
Conc: 7.30 ng/ml

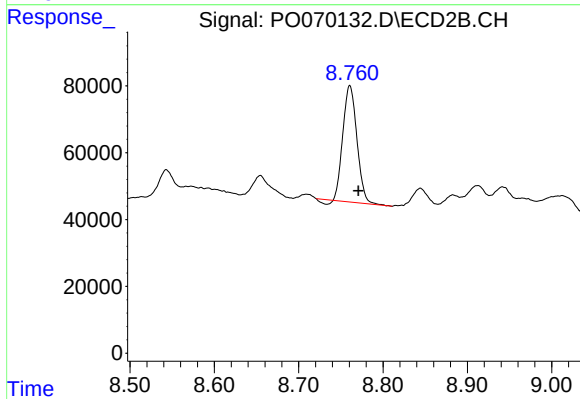

#2 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: -0.010 min
Response: 397434
Conc: 7.60 ng/ml

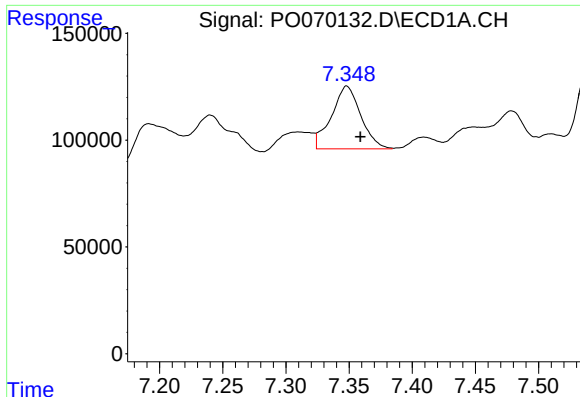


#31 AR-1260-1

R.T.: 7.348 min
Delta R.T.: -0.011 min
Response: 473963
Conc: 195.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
X068-S7


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:20 PM

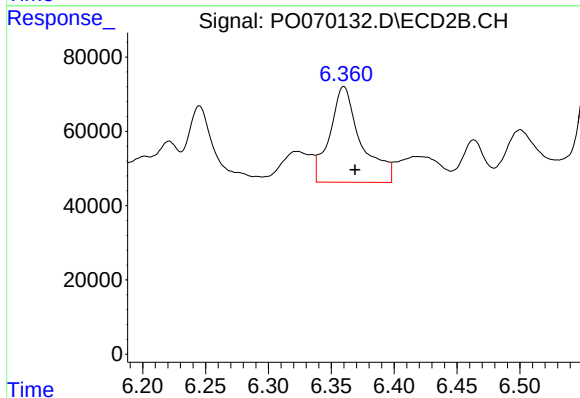


#31 AR-1260-1

R.T.: 6.360 min
Delta R.T.: -0.009 min
Response: 444824
Conc: 166.85 ng/ml

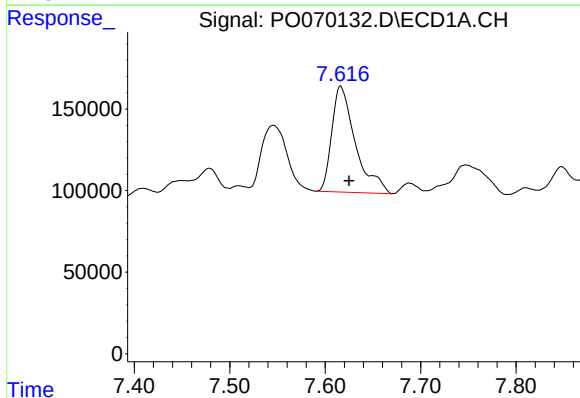


#32 AR-1260-2

R.T.: 7.616 min
Delta R.T.: -0.009 min
Response: 1118428
Conc: 314.80 ng/ml

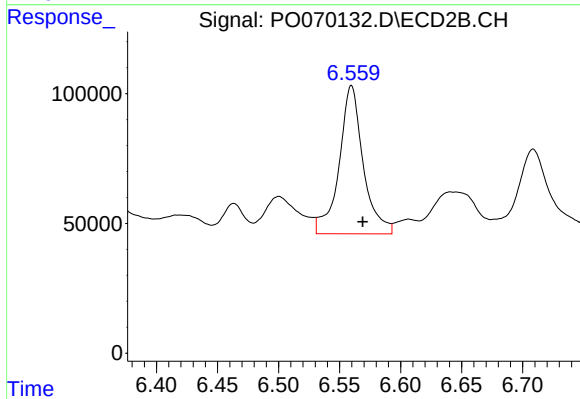

#32 AR-1260-2

R.T.: 6.560 min
Delta R.T.: -0.009 min
Response: 786189
Conc: 233.47 ng/ml

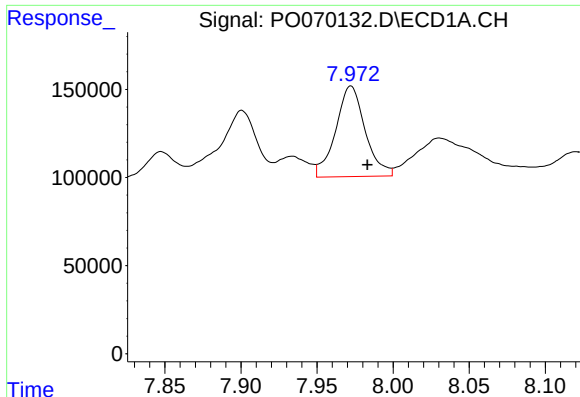


#33 AR-1260-3

R.T.: 7.972 min
Delta R.T.: -0.011 min
Response: 694331
Conc: 229.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-S7


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:20 PM

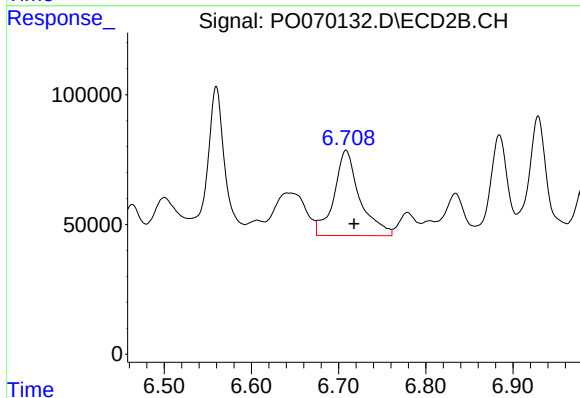


#33 AR-1260-3

R.T.: 6.709 min
Delta R.T.: -0.009 min
Response: 675053
Conc: 225.54 ng/ml

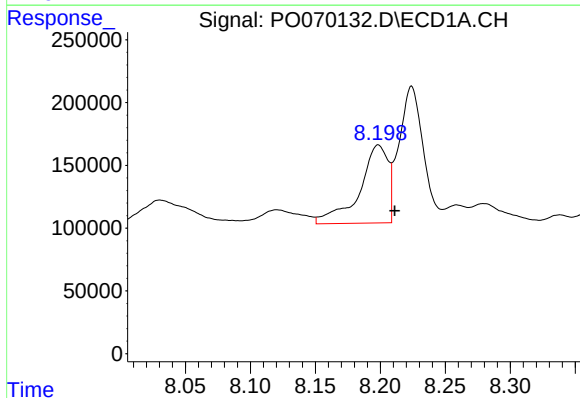


#34 AR-1260-4

R.T.: 8.198 min
Delta R.T.: -0.013 min
Response: 949187
Conc: 328.74 ng/ml

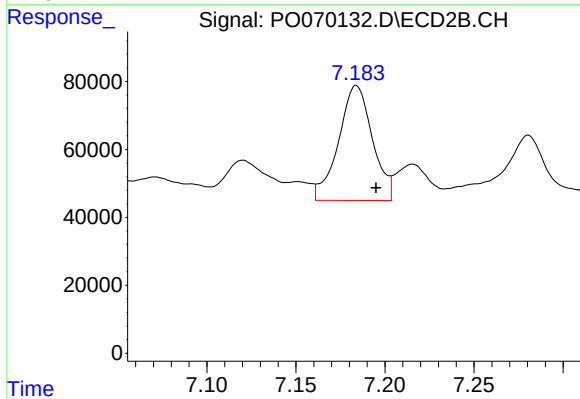

#34 AR-1260-4

R.T.: 7.184 min
Delta R.T.: -0.011 min
Response: 448283
Conc: 179.73 ng/ml

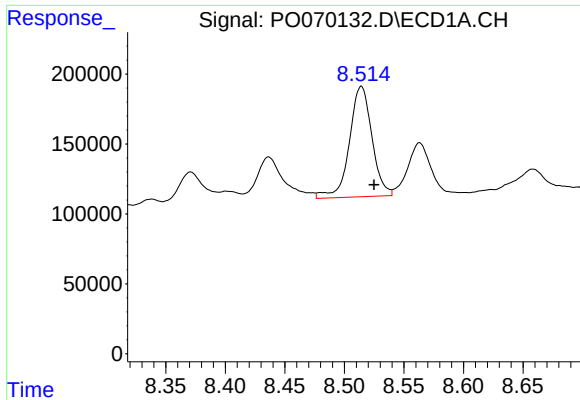


#35 AR-1260-5

R.T.: 8.514 min
Delta R.T.: -0.011 min
Response: 1043802
Conc: 152.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-S7

Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:20 PM

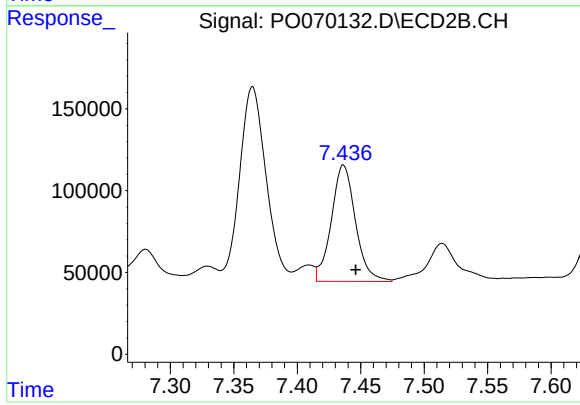

#35 AR-1260-5

R.T.: 7.436 min
Delta R.T.: -0.010 min
Response: 940533
Conc: 146.43 ng/ml