

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
 Data File : P0070137.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 22:15
 Operator : DD\AJ
 Sample : L3472-09 2X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 X068-DUP3

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:42:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 05:13:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.386	3.566	421938	623169	11.524	16.433m#
2) SA Decachlor...	10.021	8.763	594958	1135289	9.941m	21.720m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
Data File : P0070137.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 22:15
Operator : DD\AJ
Sample : L3472-09 2X
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
X068-DUP3


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 05:13:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

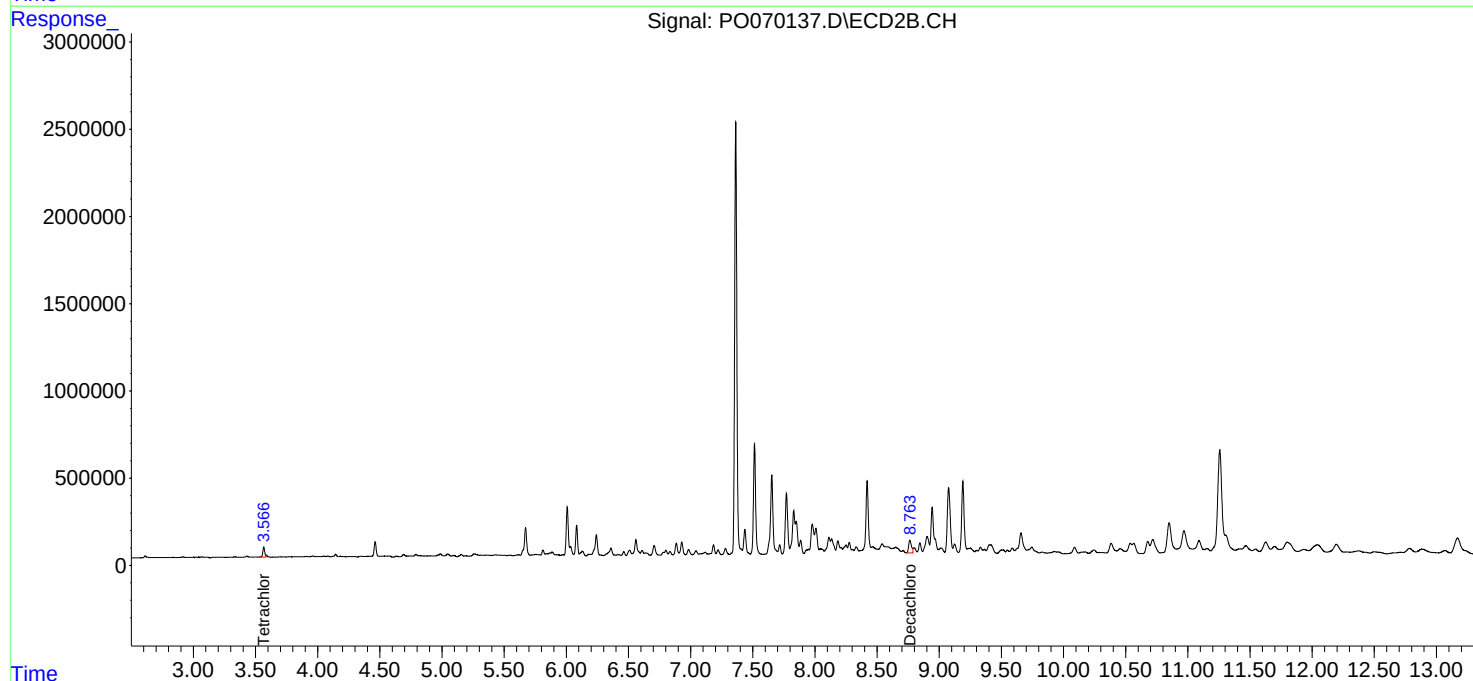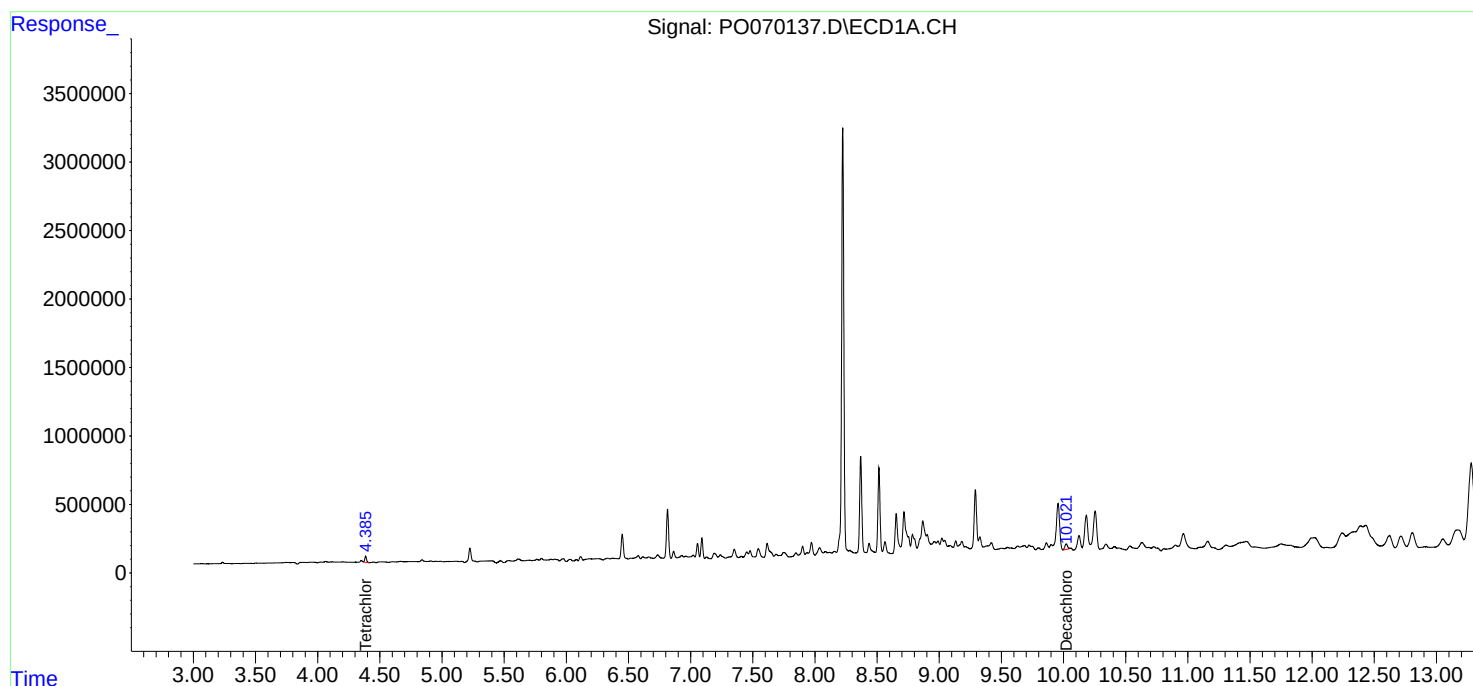

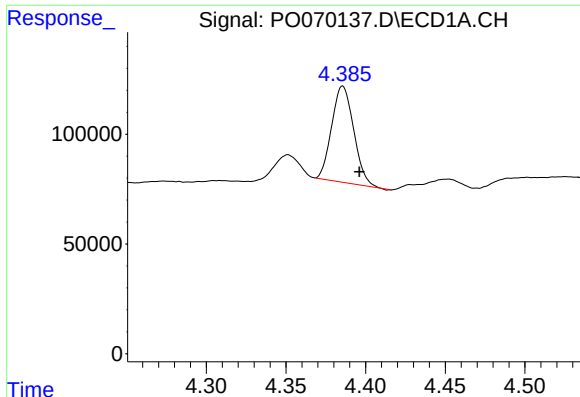


#1 Tetrachloro-m-xylene

R.T.: 4.386 min
Delta R.T.: -0.010 min
Response: 421938
Conc: 11.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-DUP3


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:35 PM

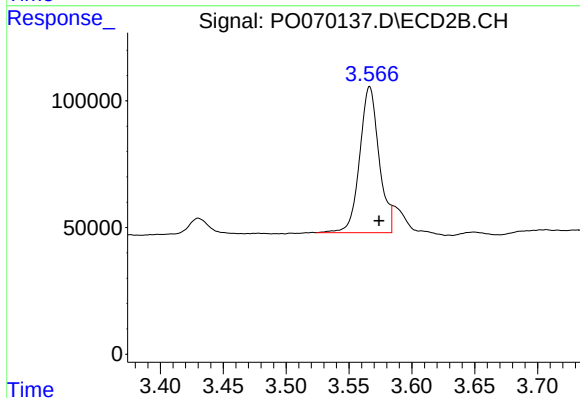


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.008 min
Response: 623169
Conc: 16.43 ng/ml m

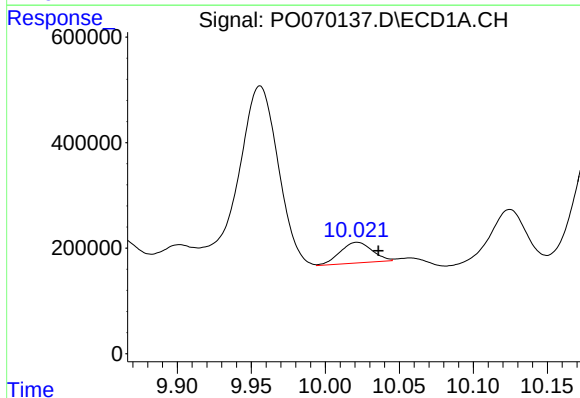

#2 Decachlorobiphenyl

R.T.: 10.021 min
Delta R.T.: -0.015 min
Response: 594958
Conc: 9.94 ng/ml m

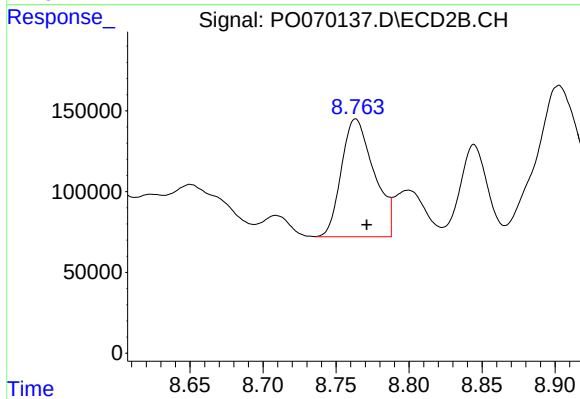

#2 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: -0.008 min
Response: 1135289
Conc: 21.72 ng/ml m