

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
 Data File : P0070140.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2020 23:06
 Operator : DD\AJ
 Sample : L3472-12 2X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 X068-B6

Manual Integrations
 APPROVED

Ankita
 7/29/2020 4:42:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 05:15:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 27 17:35:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.387	3.567	425487	448345	11.621	11.823
2) SA Decachlor...	10.022	8.762	522788	558825	8.735	10.691
Target Compounds						
31) L7 AR-1260-1	7.348	6.360	397812	632027	164.368m	237.073 #
32) L7 AR-1260-2	7.616	6.560	827878	969345	233.018	287.858
33) L7 AR-1260-3	7.973	6.709	1128721	623791	373.180	208.413 #
34) L7 AR-1260-4	8.200	7.185	925103	820213	320.397	328.855
35) L7 AR-1260-5	8.514	7.437	2437803	1882258	357.299	293.047

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072820\
Data File : P0070140.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2020 23:06
Operator : DD\AJ
Sample : L3472-12 2X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
X068-B6


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 05:15:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072720.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 27 17:35:07 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

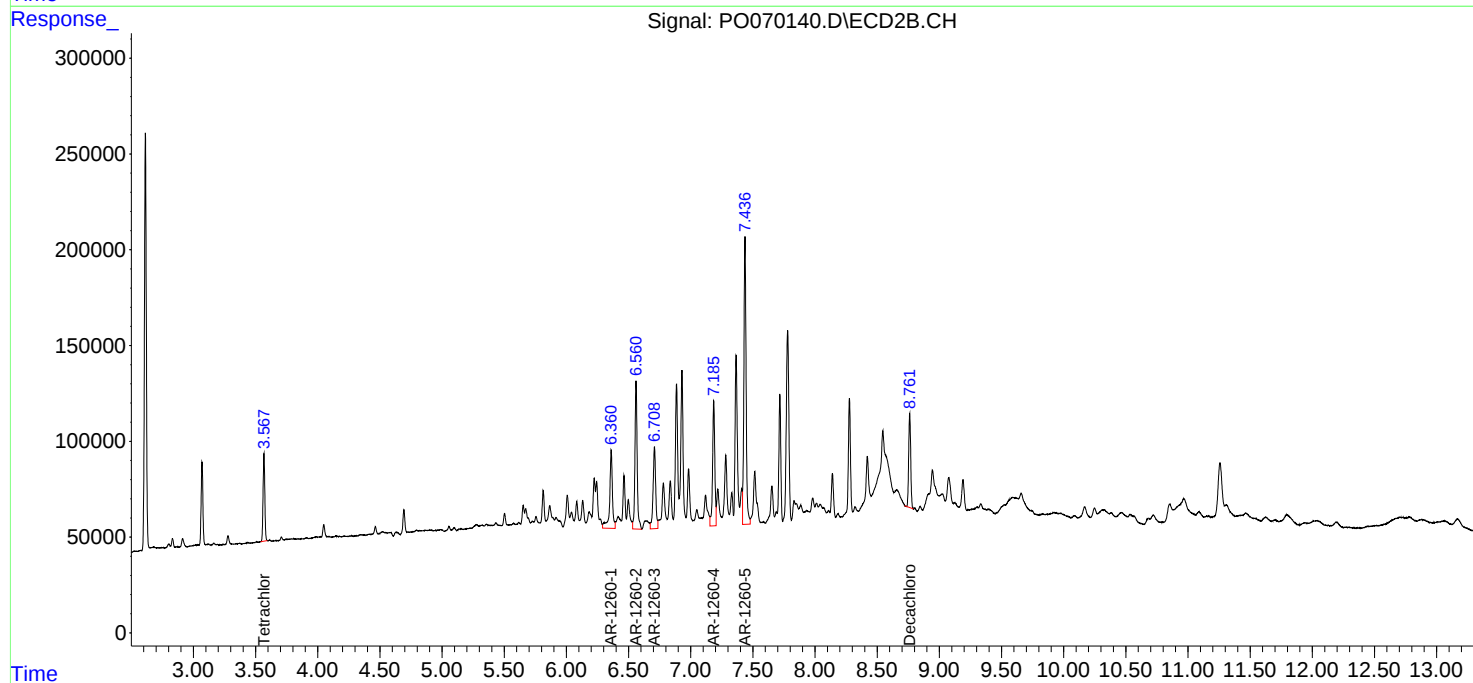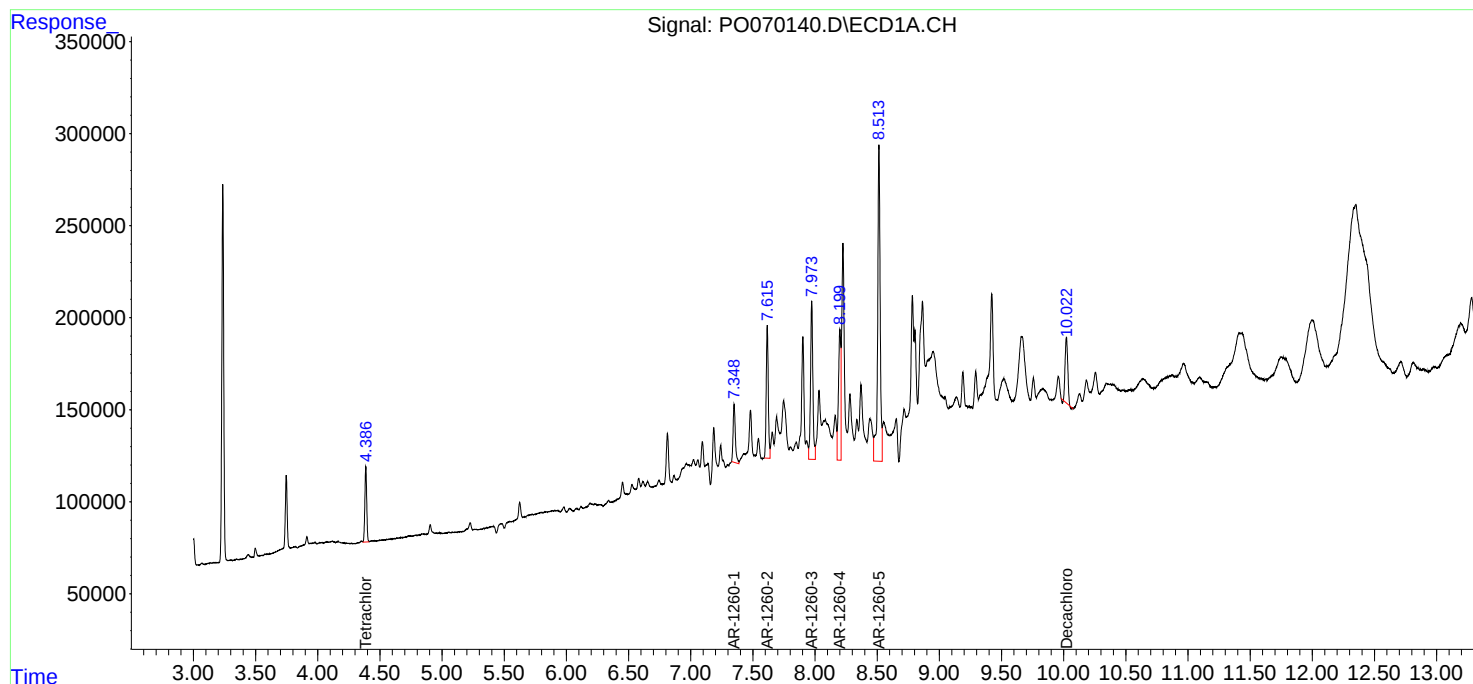

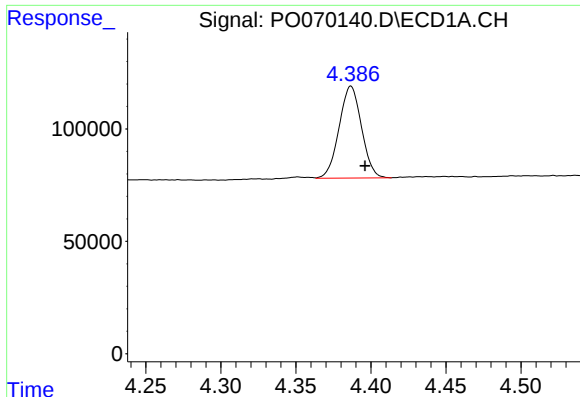


#1 Tetrachloro-m-xylene

R.T.: 4.387 min
Delta R.T.: -0.009 min
Response: 425487
Conc: 11.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-B6


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:38 PM

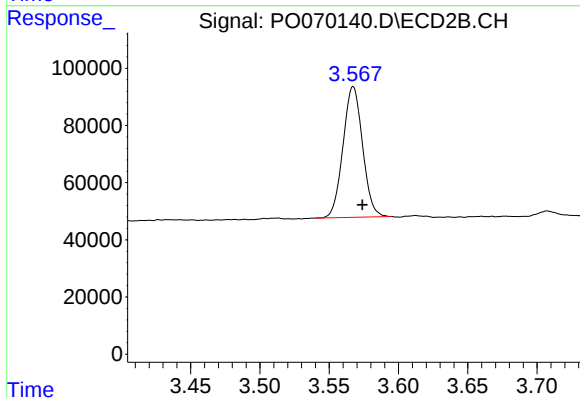


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.007 min
Response: 448345
Conc: 11.82 ng/ml

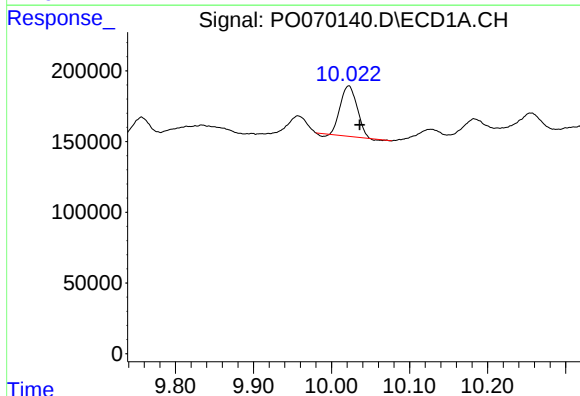


#2 Decachlorobiphenyl

R.T.: 10.022 min
Delta R.T.: -0.014 min
Response: 522788
Conc: 8.74 ng/ml

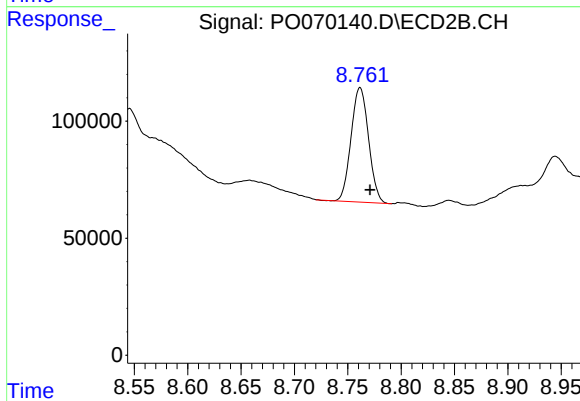

#2 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: -0.009 min
Response: 558825
Conc: 10.69 ng/ml

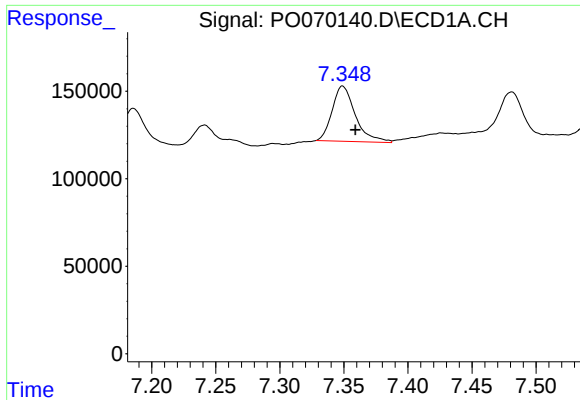


#31 AR-1260-1

R.T.: 7.348 min
Delta R.T.: -0.011 min
Response: 397812
Conc: 164.37 ng/ml m

Instrument :
ECD_O
ClientSampleId :
X068-B6


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:38 PM

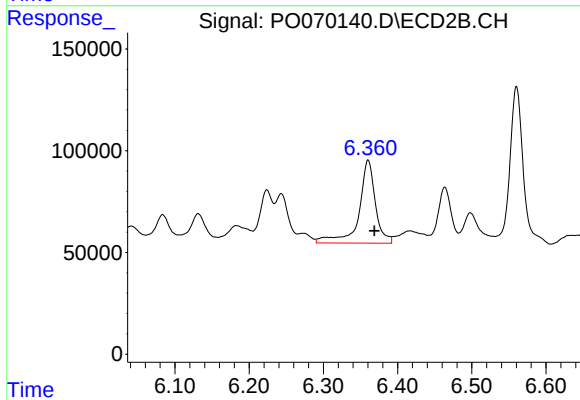


#31 AR-1260-1

R.T.: 6.360 min
Delta R.T.: -0.009 min
Response: 632027
Conc: 237.07 ng/ml

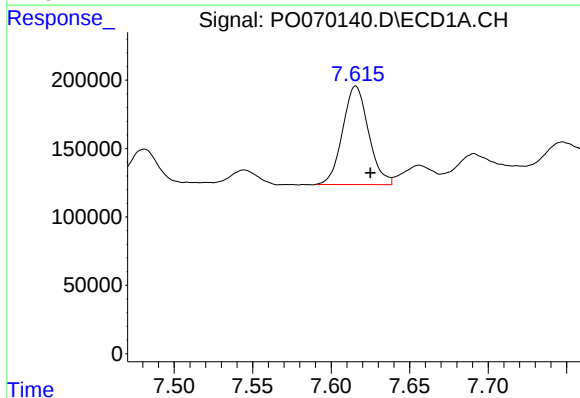


#32 AR-1260-2

R.T.: 7.616 min
Delta R.T.: -0.009 min
Response: 827878
Conc: 233.02 ng/ml

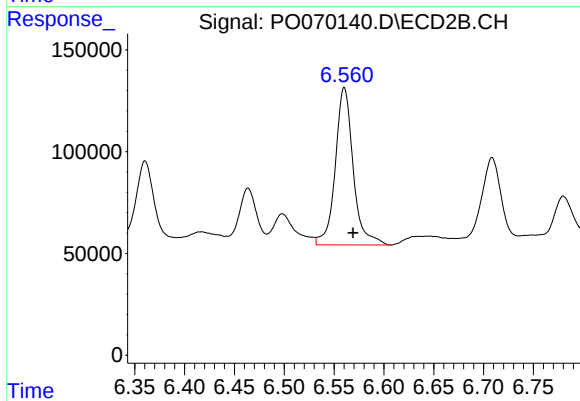

#32 AR-1260-2

R.T.: 6.560 min
Delta R.T.: -0.009 min
Response: 969345
Conc: 287.86 ng/ml

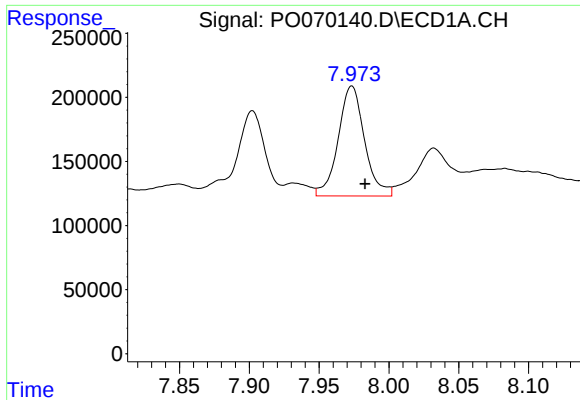


#33 AR-1260-3

R.T.: 7.973 min
Delta R.T.: -0.010 min
Response: 1128721
Conc: 373.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-B6


Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:38 PM

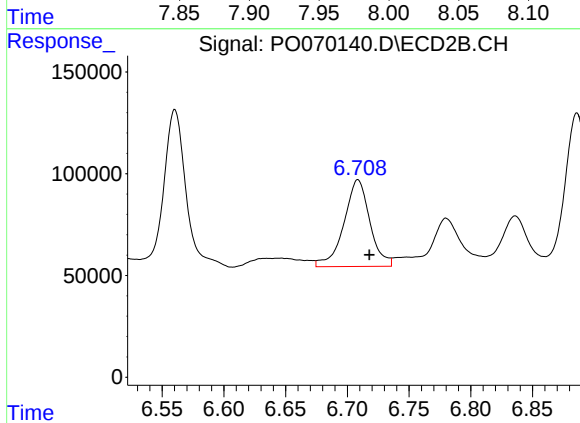


#33 AR-1260-3

R.T.: 6.709 min
Delta R.T.: -0.009 min
Response: 623791
Conc: 208.41 ng/ml

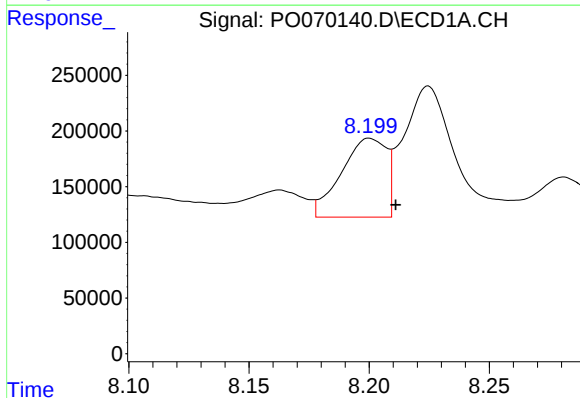


#34 AR-1260-4

R.T.: 8.200 min
Delta R.T.: -0.011 min
Response: 925103
Conc: 320.40 ng/ml

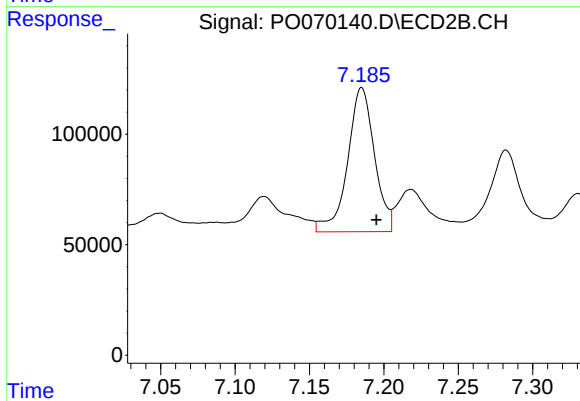

#34 AR-1260-4

R.T.: 7.185 min
Delta R.T.: -0.010 min
Response: 820213
Conc: 328.86 ng/ml

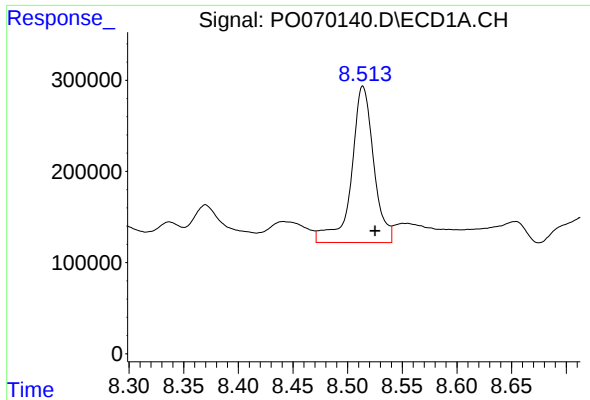


#35 AR-1260-5

R.T.: 8.514 min
Delta R.T.: -0.011 min
Response: 2437803
Conc: 357.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
X068-B6

Manual Integrations
APPROVED

Ankita
7/29/2020 4:42:38 PM

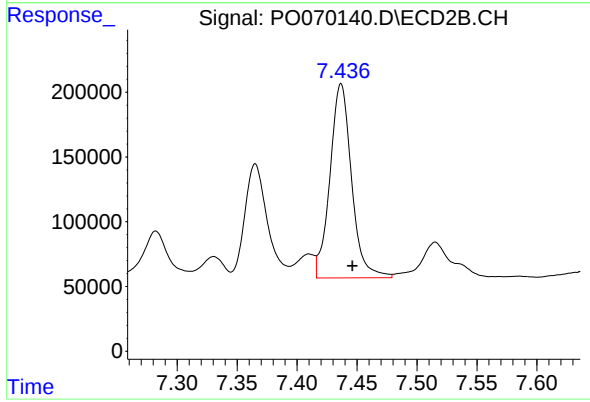

#35 AR-1260-5

R.T.: 7.437 min
Delta R.T.: -0.009 min
Response: 1882258
Conc: 293.05 ng/ml