

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072821\
 Data File : P0079892.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2021 23:14
 Operator : DD\AJ
 Sample : M2940-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 03:37:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.000	4.119	1294778	521383	21.487	22.767
2)	SA Decachlor...	11.110	9.526	1096991	504388	23.385	24.271
Target Compounds							
3)	L1 AR-1016-1	6.331	5.397	103493	49896	47.080	53.086
4)	L1 AR-1016-2	6.355	5.418	138650	70071	45.444	55.078
5)	L1 AR-1016-3	6.420	5.614	96392	34006	51.223	48.235
6)	L1 AR-1016-4	6.529	5.664	70590	29626	45.782	49.029
7)	L1 AR-1016-5	6.846	5.898	73192	38425	48.378	52.175
8)	L2 AR-1221-1	5.252	0.000	40291	0	62.527	N.D. #
9)	L2 AR-1221-2	5.354	4.481	20168	16037	43.923	74.775 #
10)	L2 AR-1221-3	5.441	4.574	65468	28274	42.427	43.551
11)	L3 AR-1232-1	5.441	4.574	65468	28274	45.940	46.889
12)	L3 AR-1232-2	6.034	5.418	74068	70071	106.031	124.606
13)	L3 AR-1232-3	6.355	5.614	138650	34006	104.031	112.955
14)	L3 AR-1232-4	6.529	5.710	70590	31688	108.392	111.315
15)	L3 AR-1232-5	6.626	5.898	72082	38425	161.417	127.949
16)	L4 AR-1242-1	6.331	5.397	103493	49896	62.095	70.061
17)	L4 AR-1242-2	6.355	5.418	138650	70071	60.287	72.360
18)	L4 AR-1242-3	6.420	5.614	96392	34006	67.901	63.379
19)	L4 AR-1242-4	6.529	5.710	70590	31688	62.207	56.433
20)	L4 AR-1242-5	0.000	6.282	0	25358	N.D.	38.970 #
21)	L5 AR-1248-1	6.331	5.397	103493	49896	81.640	90.360
22)	L5 AR-1248-2	6.626	5.664	72082	29626	41.347	35.959
23)	L5 AR-1248-3	6.846	5.710	73192	31688	35.712	38.183
24)	L5 AR-1248-4	0.000	5.898	0	38425	N.D.	40.664 #
26)	L6 AR-1254-1	7.245	6.282	36591	25358	16.751	18.699
27)	L6 AR-1254-2	7.475	6.443	50301	26883	15.318	22.420 #
28)	L6 AR-1254-3	7.875	6.887f	70352	51456	20.432	27.501 #
30)	L6 AR-1254-5	8.585	7.546	161193	87442	60.612	54.587
31)	L7 AR-1260-1	8.026	7.009	114318	72455	46.595	55.978
32)	L7 AR-1260-2	8.293	7.206	156383	102549	50.887	67.036 #
33)	L7 AR-1260-3	8.660	7.365	106371	86111	47.973	58.978
34)	L7 AR-1260-4	8.891	7.854	118909	60642	46.321	51.176
35)	L7 AR-1260-5	9.226	8.104	236721	139207	46.298	52.697
36)	L8 AR-1262-1	8.660	7.546	106371	87442	33.265	103.881 #
37)	L8 AR-1262-2	9.226	8.104	236721	139207	43.708	51.845
38)	L8 AR-1262-3	9.569f	8.394	154084	37994	40.740	34.208
39)	L8 AR-1262-4	9.622f	8.458	98113	107403	34.723	53.717 #
40)	L8 AR-1262-5	10.330	8.964	199865	39307	105.107	40.296 #
41)	L9 AR-1268-1	9.569f	8.394	154084	37994	23.800	12.504 #
42)	L9 AR-1268-2	9.622f	8.458	98113	107403	16.488	39.473 #
44)	L9 AR-1268-4	10.330	8.964	199865	39307	86.986	36.715 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072821\
 Data File : P0079892.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jul 2021 23:14
 Operator : DD\AJ
 Sample : M2940-07
 Misc : AR1660 LOD 40 PPB
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 03:37:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	0.000	9.263	0	15837	N.D.	2.280 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072821\
Data File : PO079892.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jul 2021 23:14
Operator : DD\AJ
Sample : M2940-07
Misc : AR1660 LOD 40 PPB
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 03:37:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

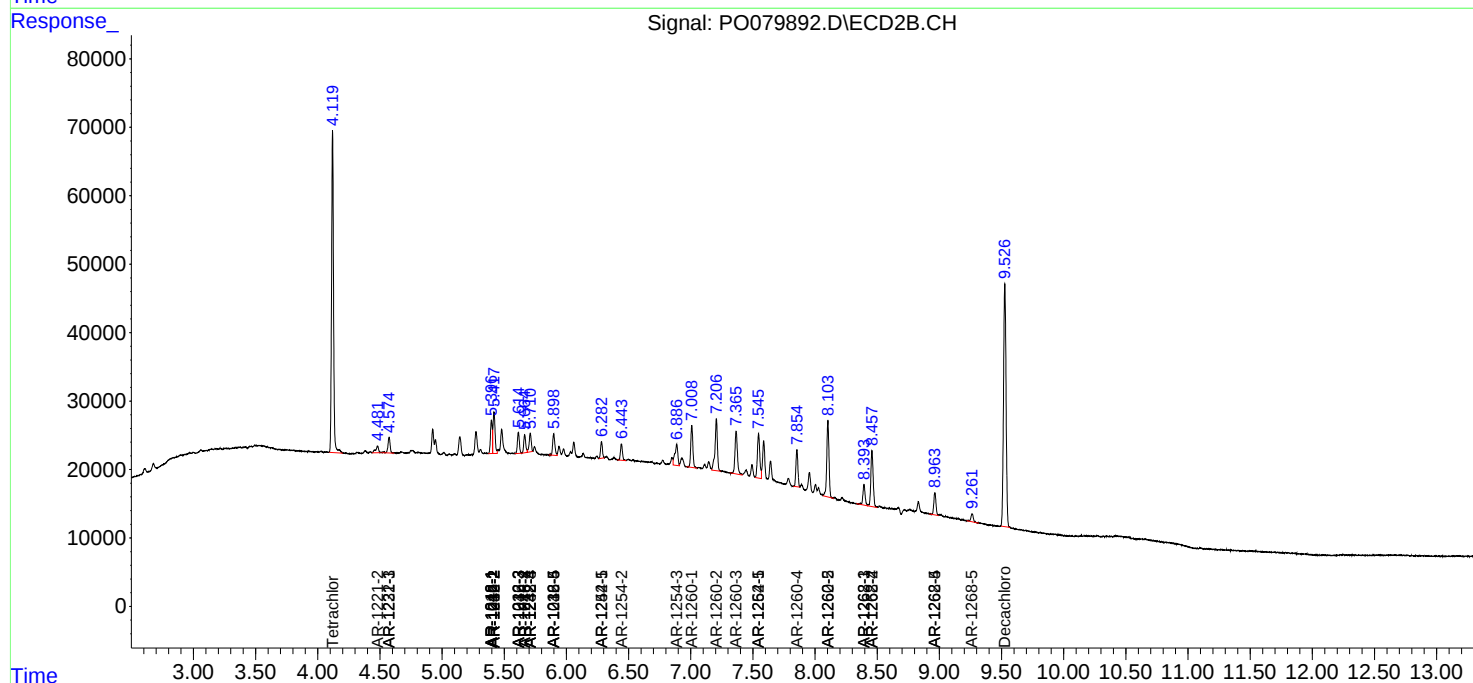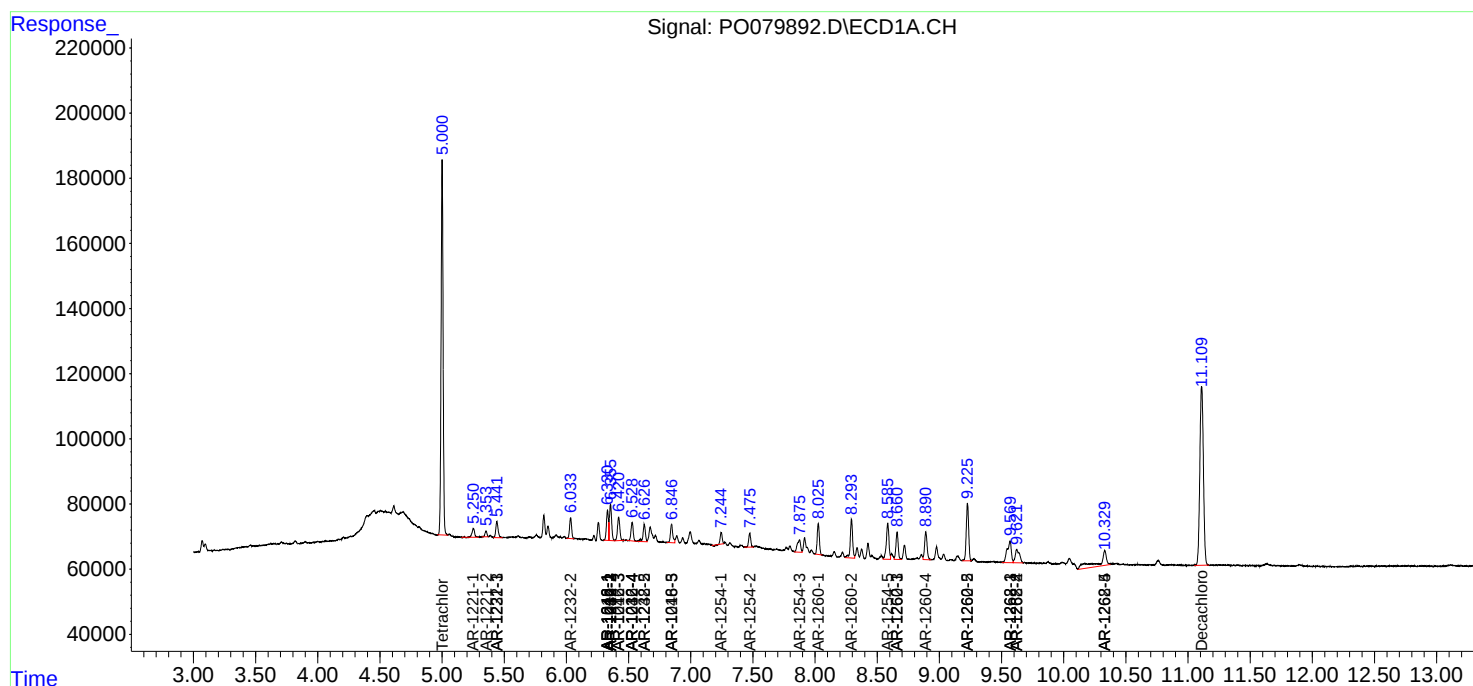


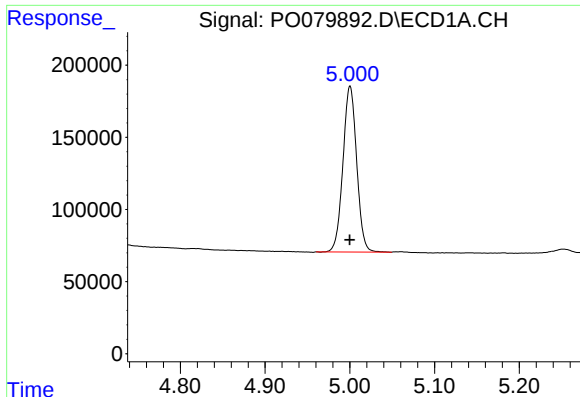

#1 Tetrachloro-m-xylene


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 1294778
Conc: 21.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

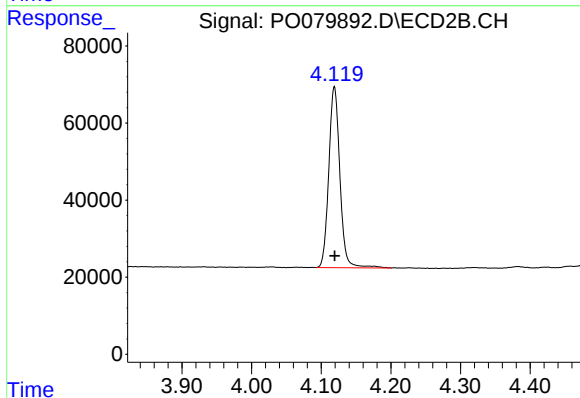


#1 Tetrachloro-m-xylene

R.T.: 4.119 min
Delta R.T.: 0.000 min
Response: 521383
Conc: 22.77 ng/ml

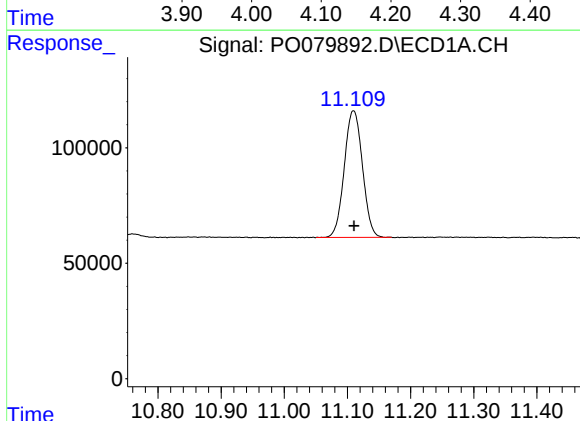


#2 Decachlorobiphenyl

R.T.: 11.110 min
Delta R.T.: 0.000 min
Response: 1096991
Conc: 23.38 ng/ml

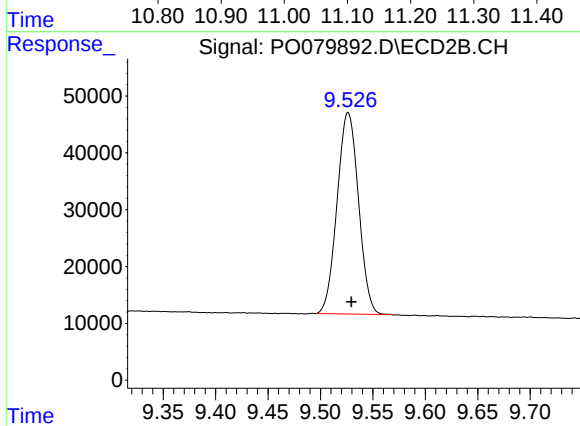

#2 Decachlorobiphenyl


R.T.: 9.526 min
Delta R.T.: -0.003 min
Response: 504388
Conc: 24.27 ng/ml

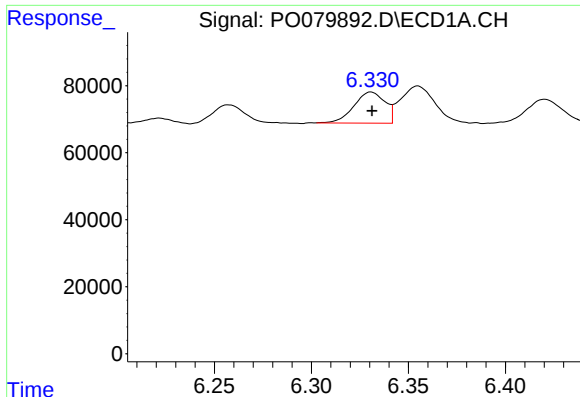

#3 AR-1016-1


R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 103493
Conc: 47.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

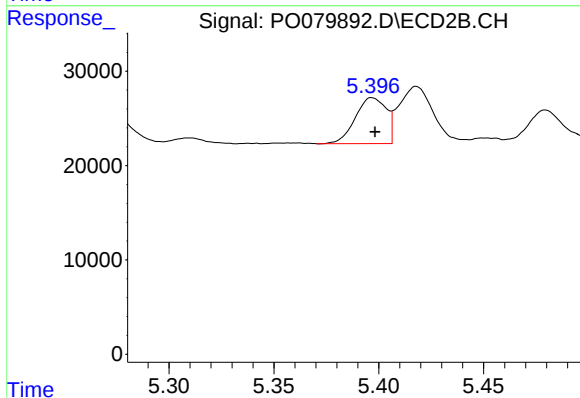


#3 AR-1016-1

R.T.: 5.397 min
Delta R.T.: -0.001 min
Response: 49896
Conc: 53.09 ng/ml

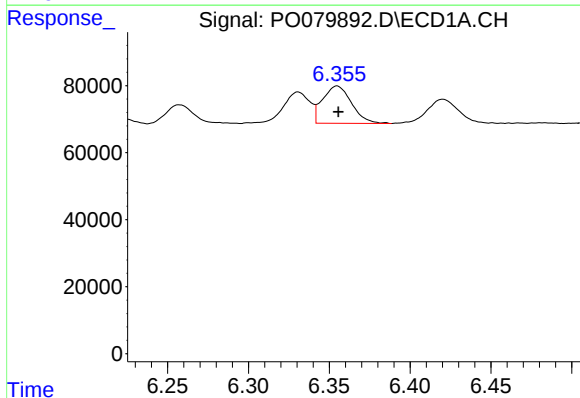


#4 AR-1016-2

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 138650
Conc: 45.44 ng/ml

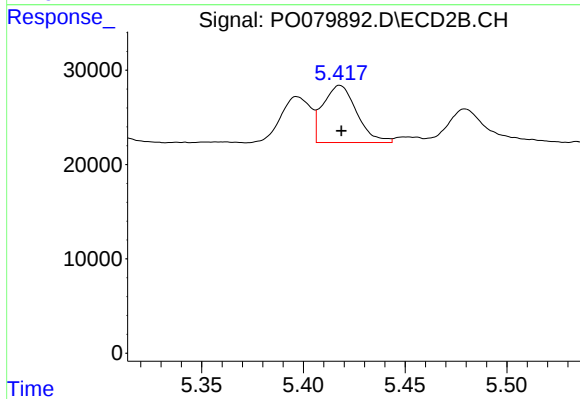

#4 AR-1016-2


R.T.: 5.418 min
Delta R.T.: 0.000 min
Response: 70071
Conc: 55.08 ng/ml

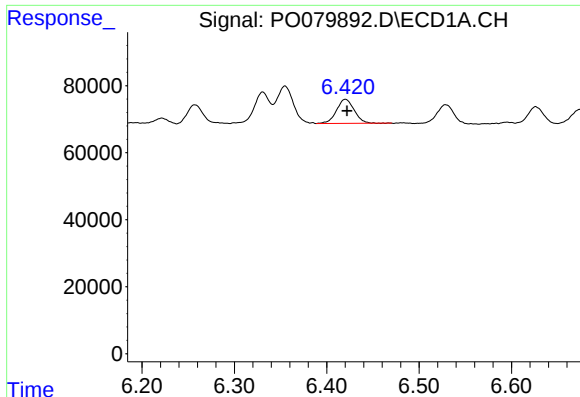

#5 AR-1016-3


R.T.: 6.420 min
Delta R.T.: -0.002 min
Response: 96392
Conc: 51.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

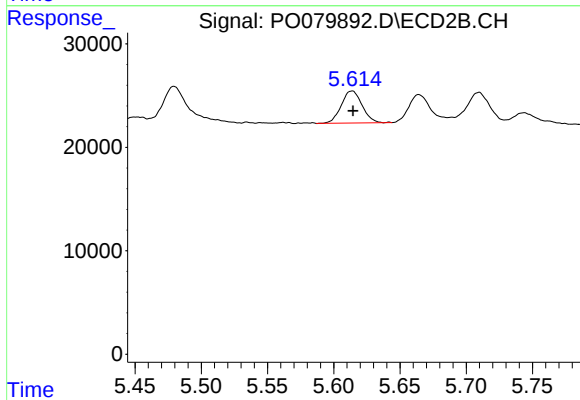


#5 AR-1016-3

R.T.: 5.614 min
Delta R.T.: 0.000 min
Response: 34006
Conc: 48.23 ng/ml

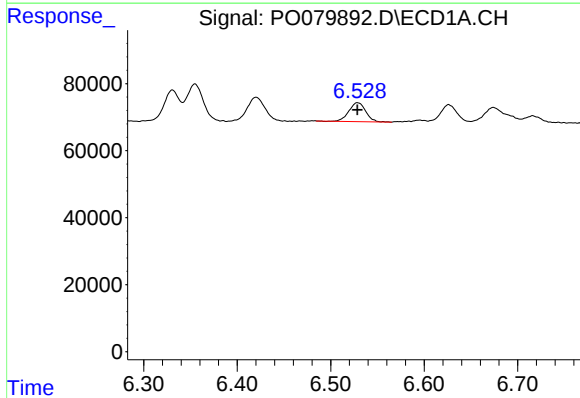


#6 AR-1016-4

R.T.: 6.529 min
Delta R.T.: 0.000 min
Response: 70590
Conc: 45.78 ng/ml

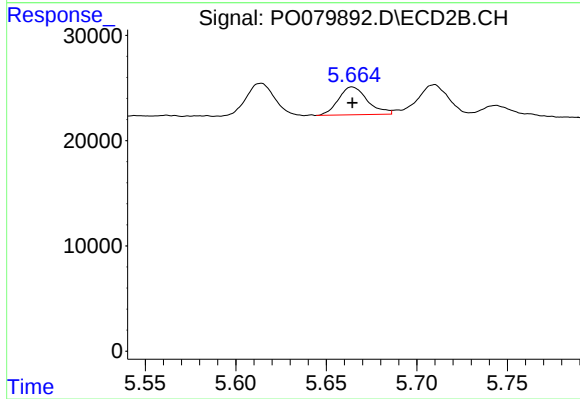

#6 AR-1016-4


R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 29626
Conc: 49.03 ng/ml

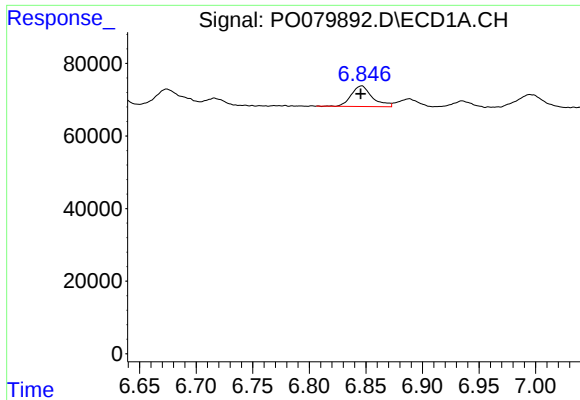

#7 AR-1016-5


R.T.: 6.846 min
Delta R.T.: 0.000 min
Response: 73192
Conc: 48.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

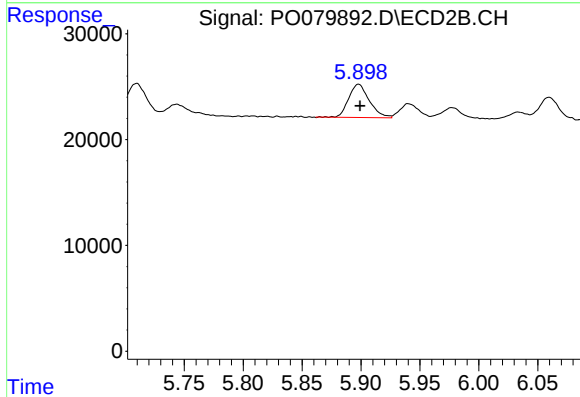


#7 AR-1016-5

R.T.: 5.898 min
Delta R.T.: -0.001 min
Response: 38425
Conc: 52.18 ng/ml

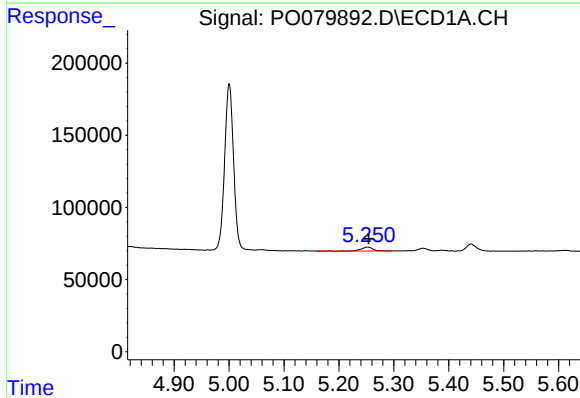


#8 AR-1221-1

R.T.: 5.252 min
Delta R.T.: -0.002 min
Response: 40291
Conc: 62.53 ng/ml

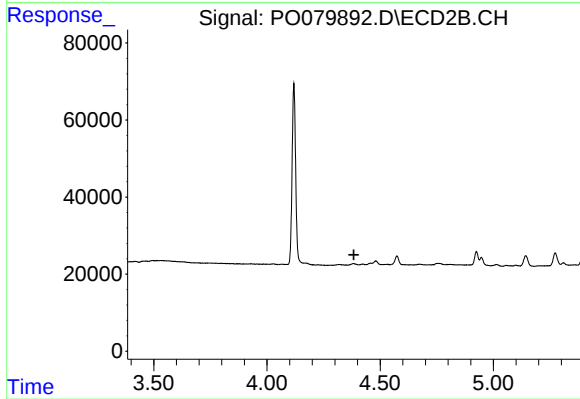

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 4.384 min
Response: 0
Conc: N.D.

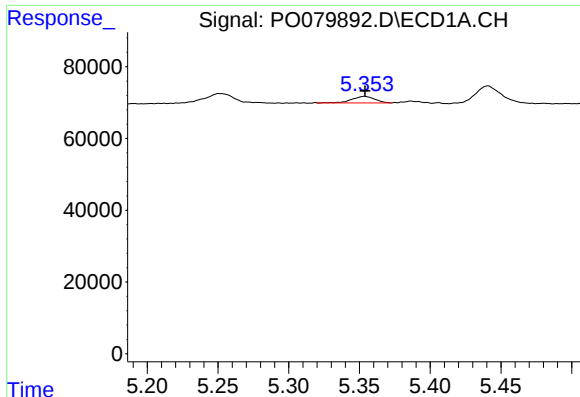

#9 AR-1221-2


R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 20168
Conc: 43.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

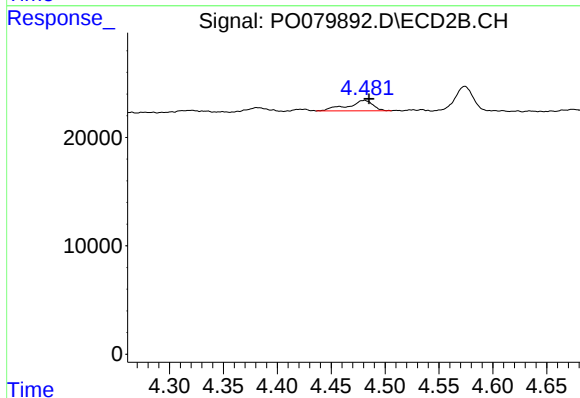


#9 AR-1221-2

R.T.: 4.481 min
Delta R.T.: -0.004 min
Response: 16037
Conc: 74.77 ng/ml

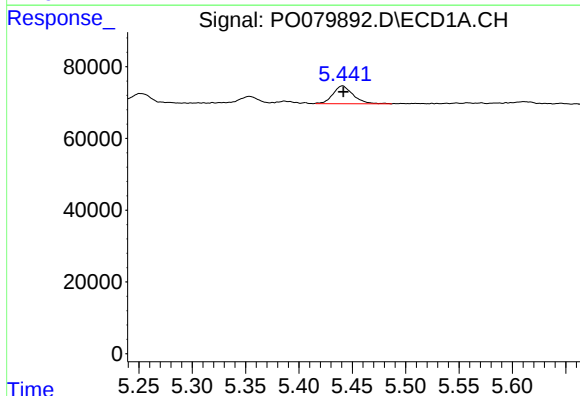


#10 AR-1221-3

R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 65468
Conc: 42.43 ng/ml

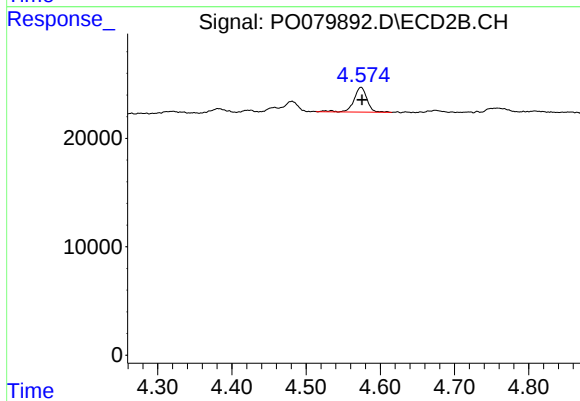

#10 AR-1221-3


R.T.: 4.574 min
Delta R.T.: -0.002 min
Response: 28274
Conc: 43.55 ng/ml

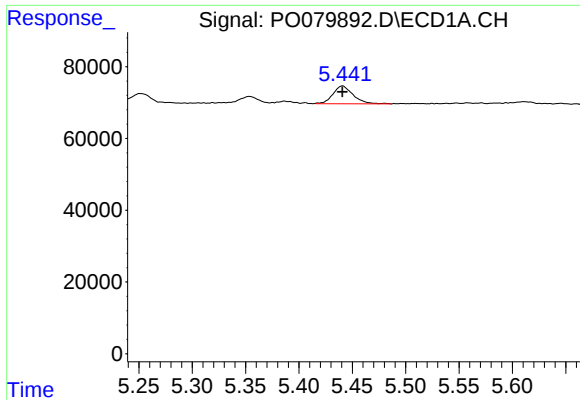

#11 AR-1232-1


R.T.: 5.441 min
Delta R.T.: 0.000 min
Response: 65468
Conc: 45.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

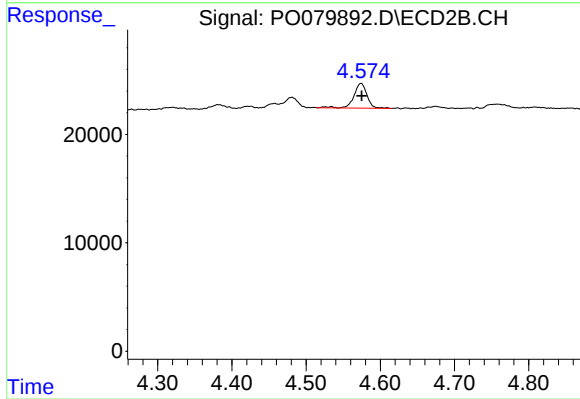


#11 AR-1232-1

R.T.: 4.574 min
Delta R.T.: -0.001 min
Response: 28274
Conc: 46.89 ng/ml

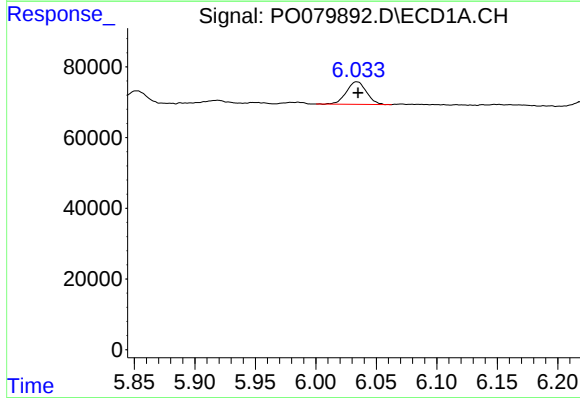


#12 AR-1232-2

R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 74068
Conc: 106.03 ng/ml

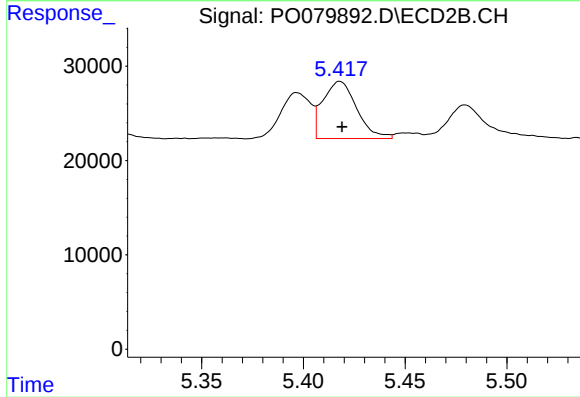

#12 AR-1232-2


R.T.: 5.418 min
Delta R.T.: 0.000 min
Response: 70071
Conc: 124.61 ng/ml

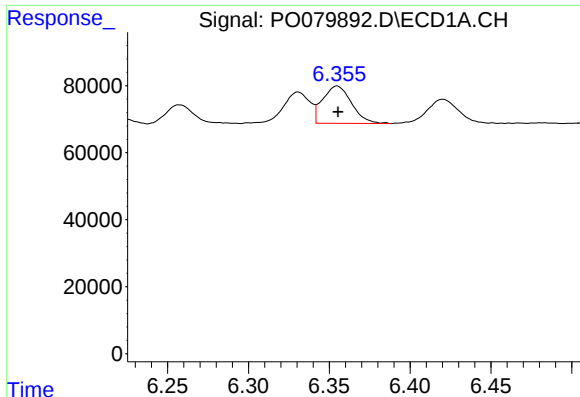

#13 AR-1232-3


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 138650
Conc: 104.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

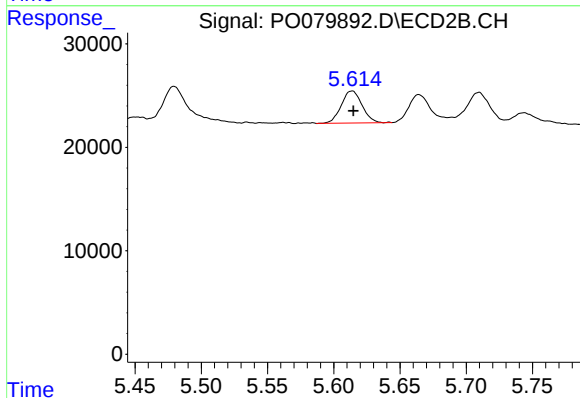


#13 AR-1232-3

R.T.: 5.614 min
Delta R.T.: -0.001 min
Response: 34006
Conc: 112.95 ng/ml

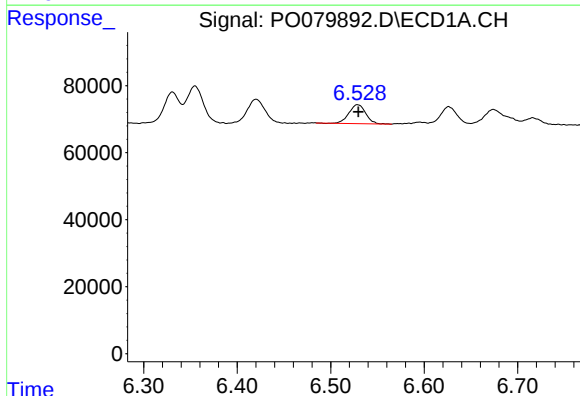


#14 AR-1232-4

R.T.: 6.529 min
Delta R.T.: 0.000 min
Response: 70590
Conc: 108.39 ng/ml

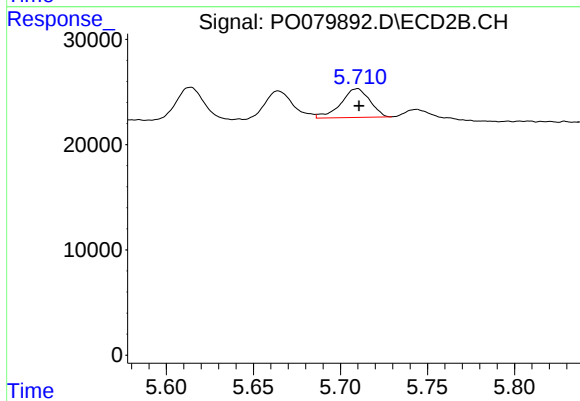

#14 AR-1232-4


R.T.: 5.710 min
Delta R.T.: -0.001 min
Response: 31688
Conc: 111.32 ng/ml

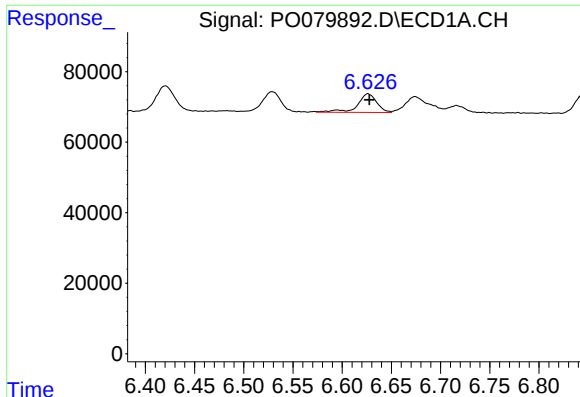

#15 AR-1232-5


R.T.: 6.626 min
Delta R.T.: -0.002 min
Response: 72082
Conc: 161.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

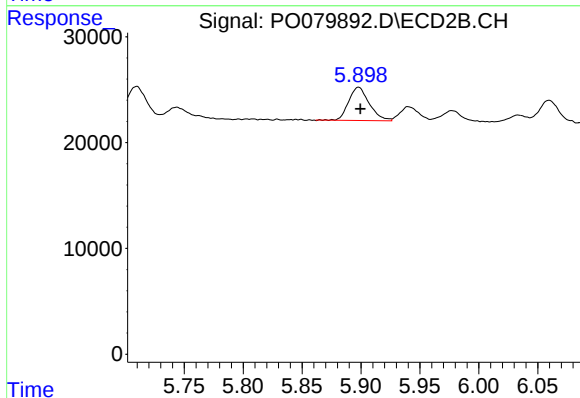


#15 AR-1232-5

R.T.: 5.898 min
Delta R.T.: -0.001 min
Response: 38425
Conc: 127.95 ng/ml

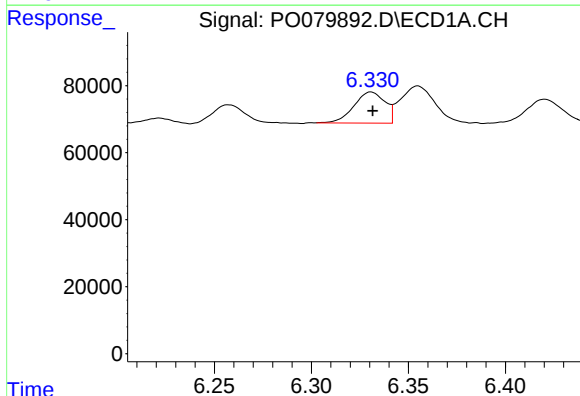


#16 AR-1242-1

R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 103493
Conc: 62.10 ng/ml

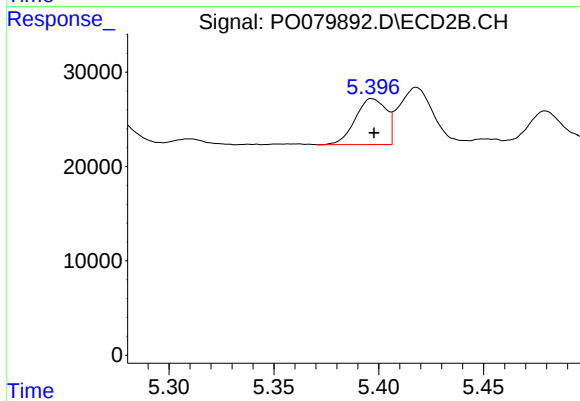

#16 AR-1242-1


R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 49896
Conc: 70.06 ng/ml

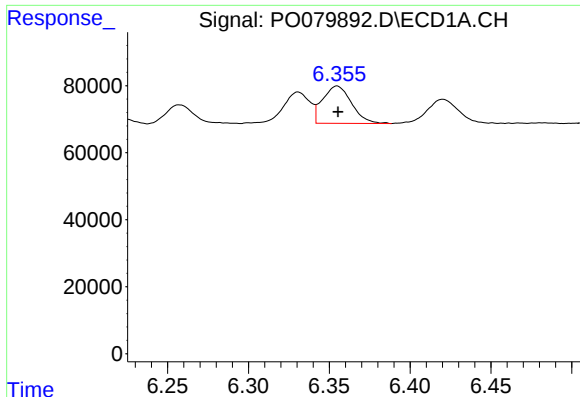

#17 AR-1242-2


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 138650
Conc: 60.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

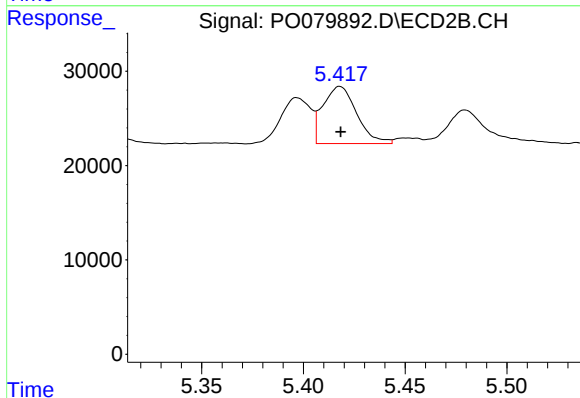


#17 AR-1242-2

R.T.: 5.418 min
Delta R.T.: 0.000 min
Response: 70071
Conc: 72.36 ng/ml

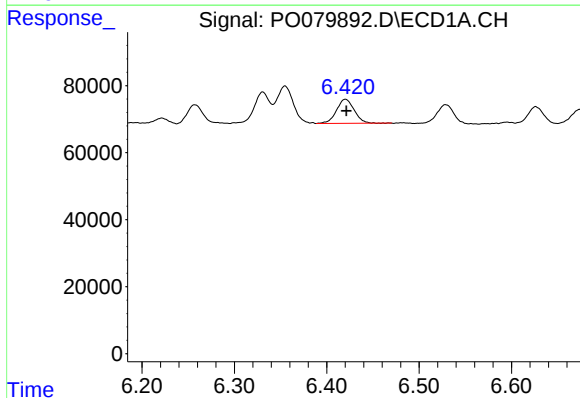


#18 AR-1242-3

R.T.: 6.420 min
Delta R.T.: -0.001 min
Response: 96392
Conc: 67.90 ng/ml

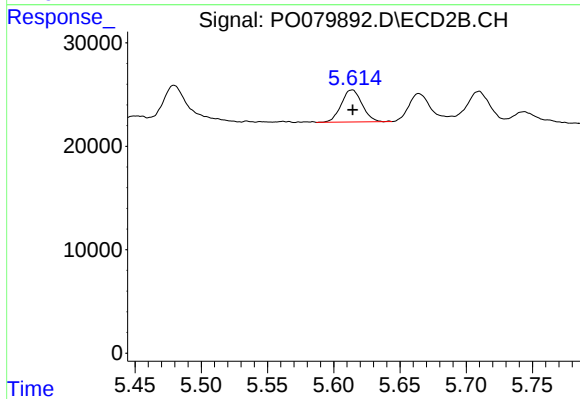

#18 AR-1242-3


R.T.: 5.614 min
Delta R.T.: 0.000 min
Response: 34006
Conc: 63.38 ng/ml

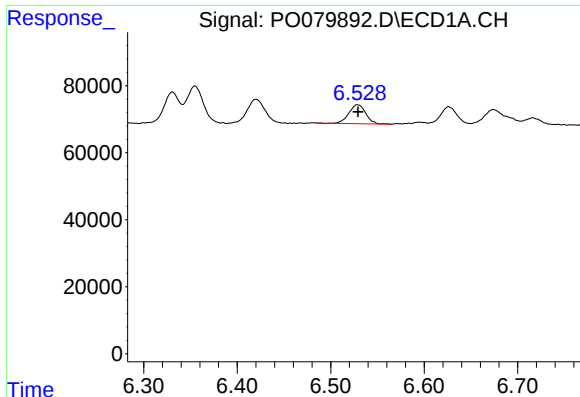

#19 AR-1242-4


R.T.: 6.529 min
Delta R.T.: 0.000 min
Response: 70590
Conc: 62.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

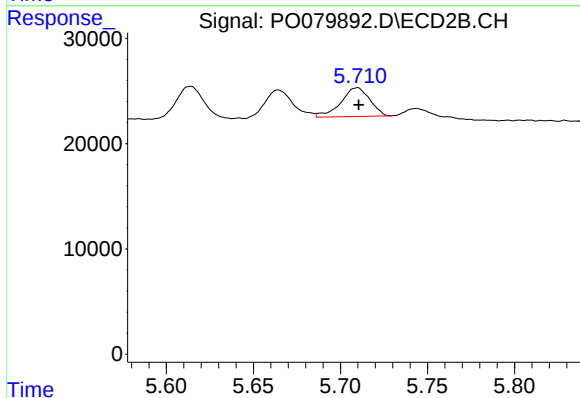


#19 AR-1242-4

R.T.: 5.710 min
Delta R.T.: -0.001 min
Response: 31688
Conc: 56.43 ng/ml

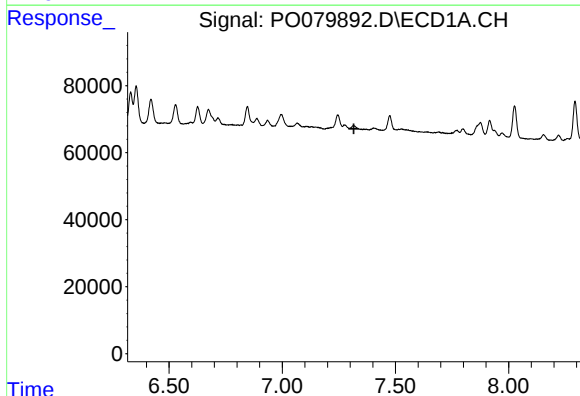


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.316 min
Response: 0
Conc: N.D.

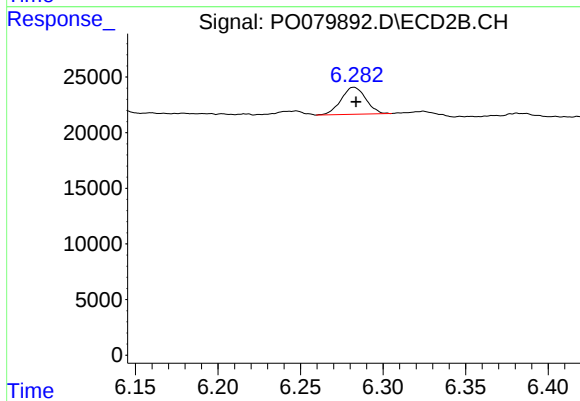

#20 AR-1242-5


R.T.: 6.282 min
Delta R.T.: -0.001 min
Response: 25358
Conc: 38.97 ng/ml

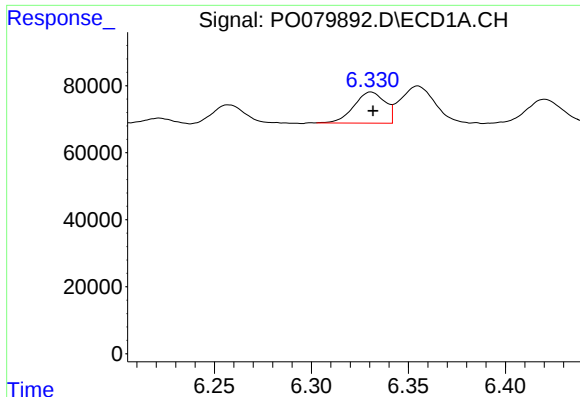

#21 AR-1248-1


R.T.: 6.331 min
Delta R.T.: 0.000 min
Response: 103493
Conc: 81.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

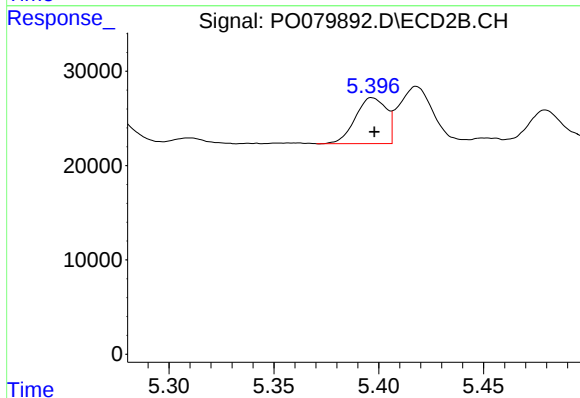


#21 AR-1248-1

R.T.: 5.397 min
Delta R.T.: -0.001 min
Response: 49896
Conc: 90.36 ng/ml

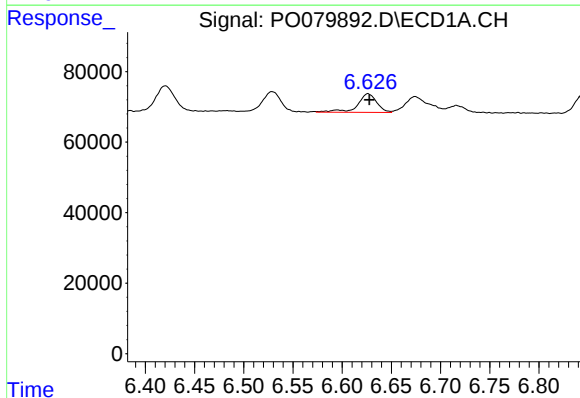


#22 AR-1248-2

R.T.: 6.626 min
Delta R.T.: -0.002 min
Response: 72082
Conc: 41.35 ng/ml

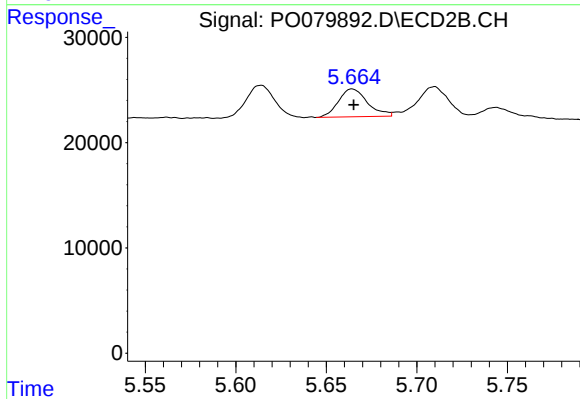

#22 AR-1248-2


R.T.: 5.664 min
Delta R.T.: 0.000 min
Response: 29626
Conc: 35.96 ng/ml

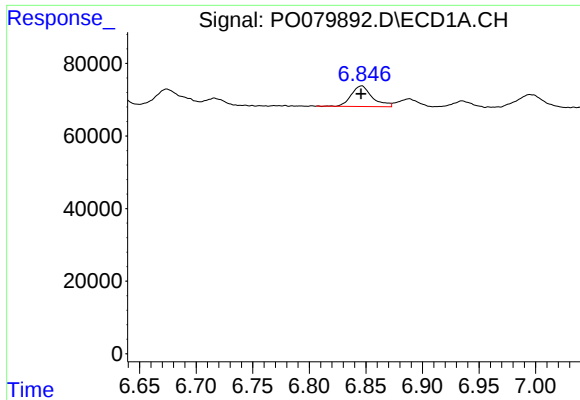

#23 AR-1248-3


R.T.: 6.846 min
Delta R.T.: 0.000 min
Response: 73192
Conc: 35.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

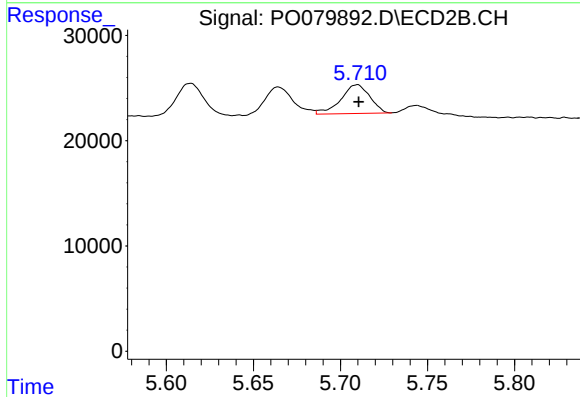


#23 AR-1248-3

R.T.: 5.710 min
Delta R.T.: -0.001 min
Response: 31688
Conc: 38.18 ng/ml

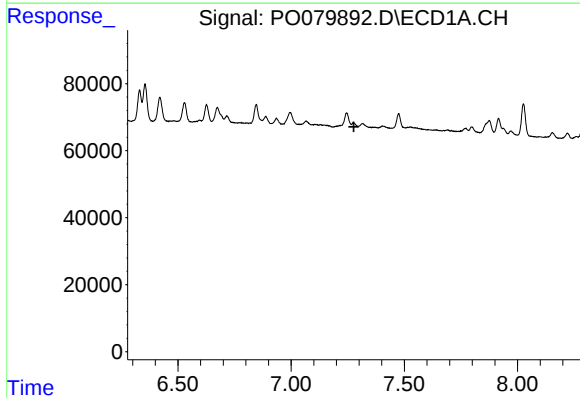


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 7.277 min
Response: 0
Conc: N.D.

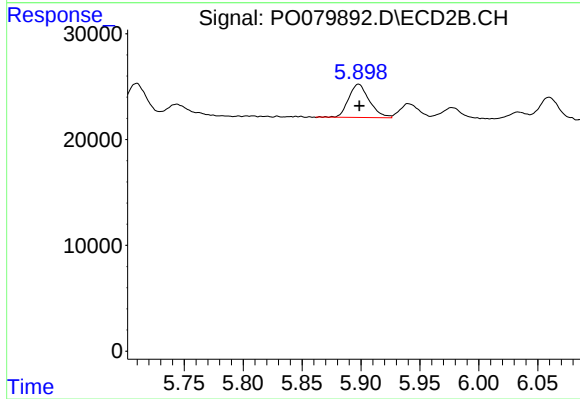

#24 AR-1248-4


R.T.: 5.898 min
Delta R.T.: 0.000 min
Response: 38425
Conc: 40.66 ng/ml

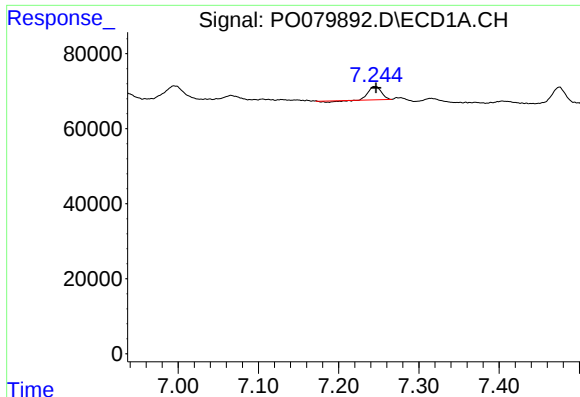

#26 AR-1254-1


R.T.: 7.245 min
Delta R.T.: -0.001 min
Response: 36591
Conc: 16.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

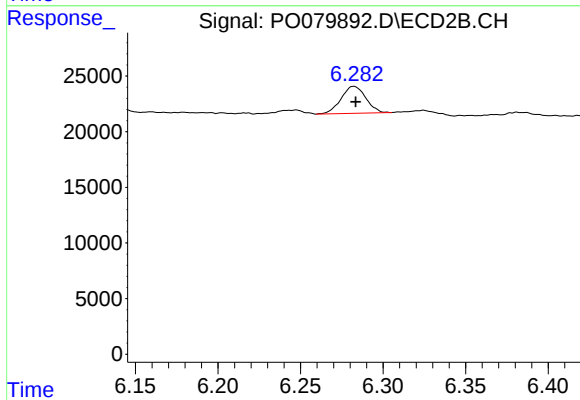


#26 AR-1254-1

R.T.: 6.282 min
Delta R.T.: -0.001 min
Response: 25358
Conc: 18.70 ng/ml

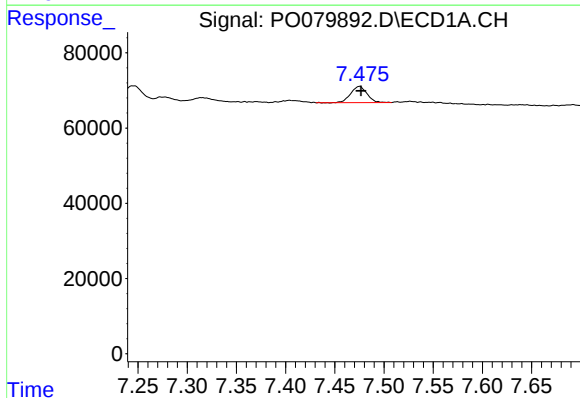


#27 AR-1254-2

R.T.: 7.475 min
Delta R.T.: -0.002 min
Response: 50301
Conc: 15.32 ng/ml

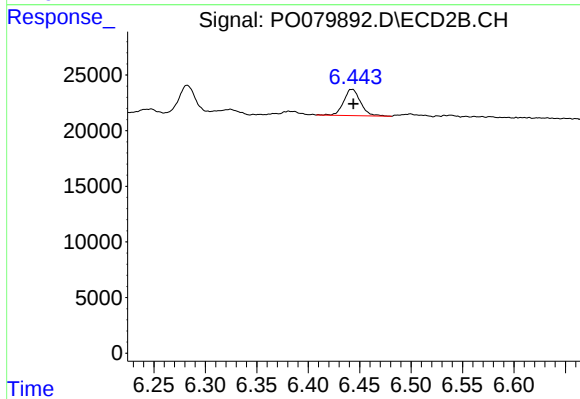

#27 AR-1254-2


R.T.: 6.443 min
Delta R.T.: -0.001 min
Response: 26883
Conc: 22.42 ng/ml

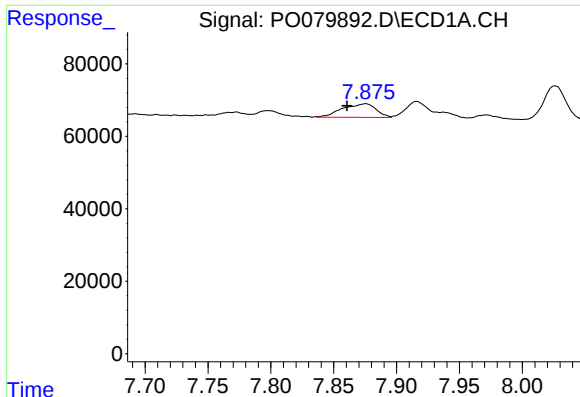

#28 AR-1254-3


R.T.: 7.875 min
Delta R.T.: 0.015 min
Response: 70352
Conc: 20.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

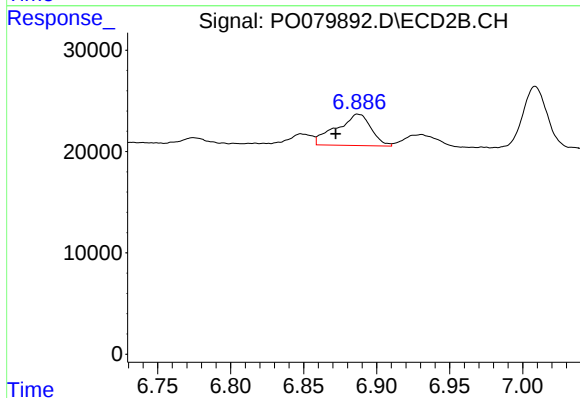


#28 AR-1254-3

R.T.: 6.887 min
Delta R.T.: 0.015 min
Response: 51456
Conc: 27.50 ng/ml

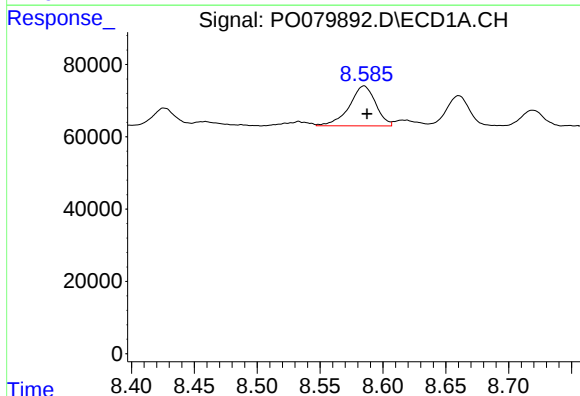


#30 AR-1254-5

R.T.: 8.585 min
Delta R.T.: -0.003 min
Response: 161193
Conc: 60.61 ng/ml

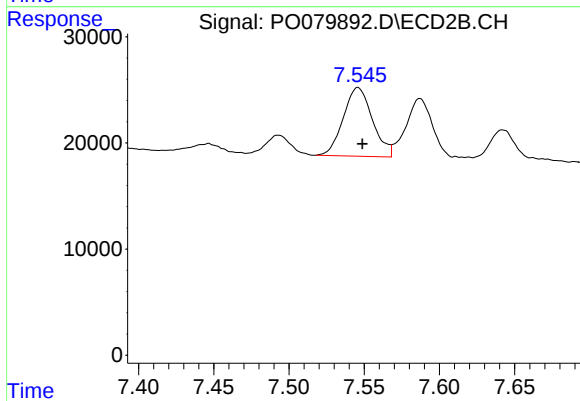

#30 AR-1254-5


R.T.: 7.546 min
Delta R.T.: -0.003 min
Response: 87442
Conc: 54.59 ng/ml

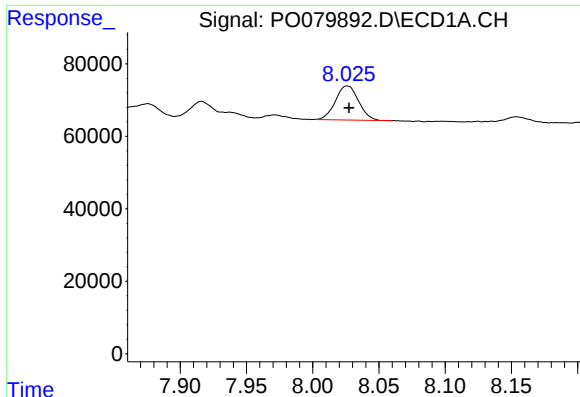

#31 AR-1260-1


R.T.: 8.026 min
Delta R.T.: -0.001 min
Response: 114318
Conc: 46.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

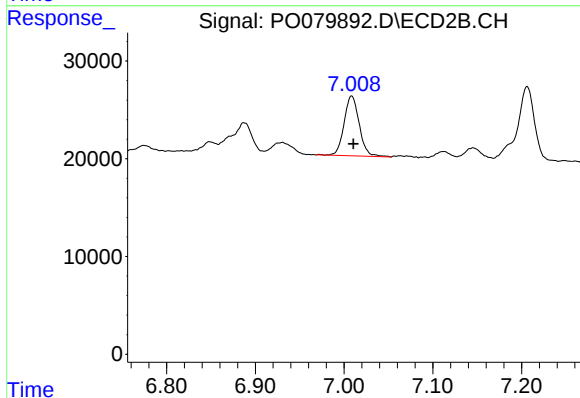


#31 AR-1260-1

R.T.: 7.009 min
Delta R.T.: -0.002 min
Response: 72455
Conc: 55.98 ng/ml

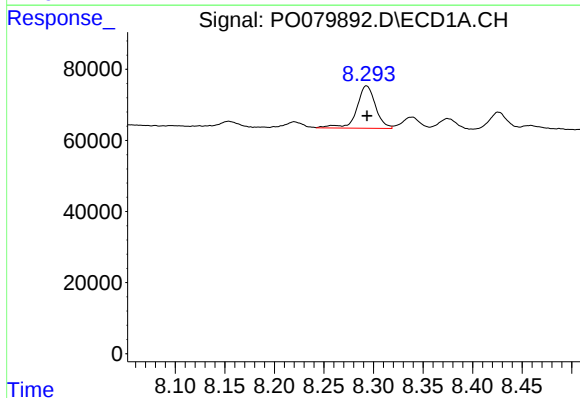


#32 AR-1260-2

R.T.: 8.293 min
Delta R.T.: 0.000 min
Response: 156383
Conc: 50.89 ng/ml

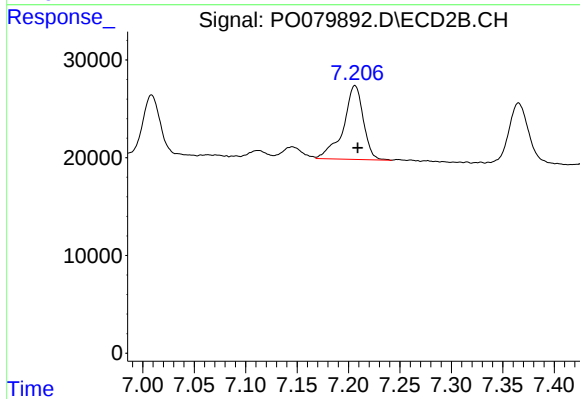

#32 AR-1260-2


R.T.: 7.206 min
Delta R.T.: -0.003 min
Response: 102549
Conc: 67.04 ng/ml

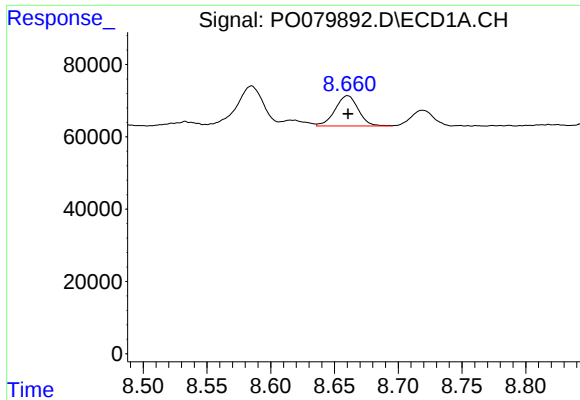

#33 AR-1260-3


R.T.: 8.660 min
Delta R.T.: 0.000 min
Response: 106371
Conc: 47.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

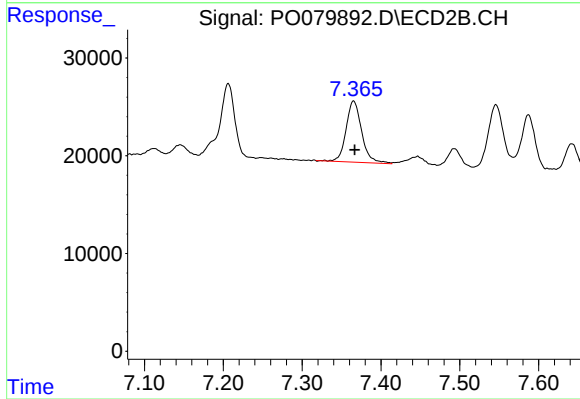


#33 AR-1260-3

R.T.: 7.365 min
Delta R.T.: -0.002 min
Response: 86111
Conc: 58.98 ng/ml

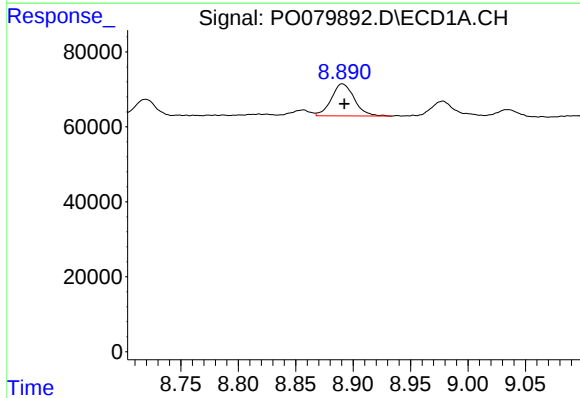


#34 AR-1260-4

R.T.: 8.891 min
Delta R.T.: -0.002 min
Response: 118909
Conc: 46.32 ng/ml

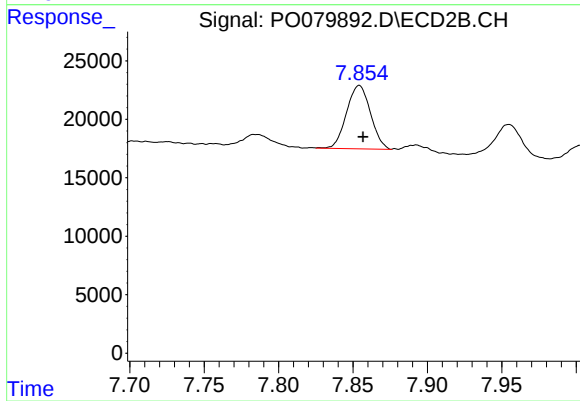

#34 AR-1260-4


R.T.: 7.854 min
Delta R.T.: -0.003 min
Response: 60642
Conc: 51.18 ng/ml

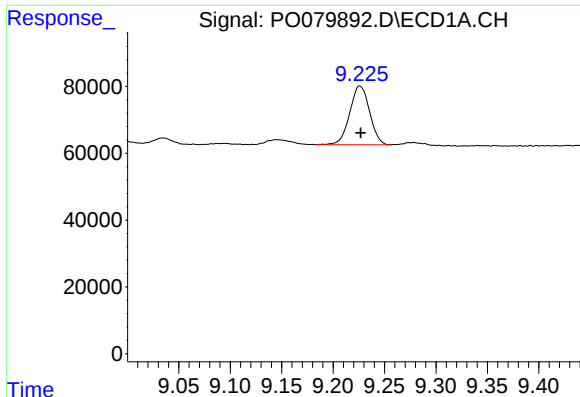

#35 AR-1260-5


R.T.: 9.226 min
Delta R.T.: 0.000 min
Response: 236721
Conc: 46.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

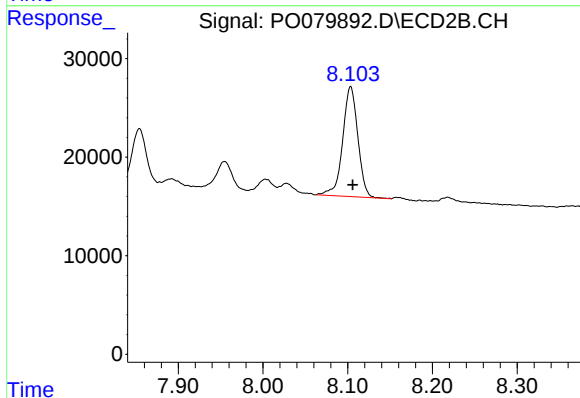


#35 AR-1260-5

R.T.: 8.104 min
Delta R.T.: -0.002 min
Response: 139207
Conc: 52.70 ng/ml

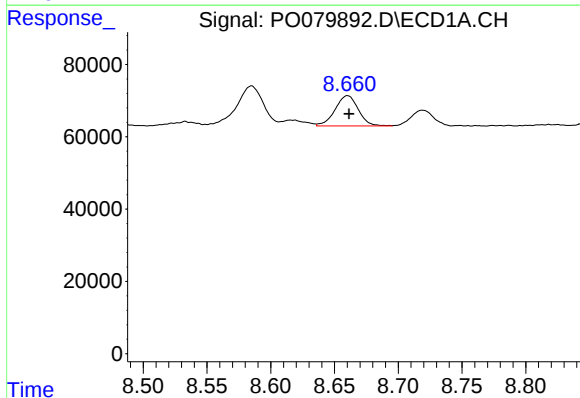


#36 AR-1262-1

R.T.: 8.660 min
Delta R.T.: -0.001 min
Response: 106371
Conc: 33.26 ng/ml

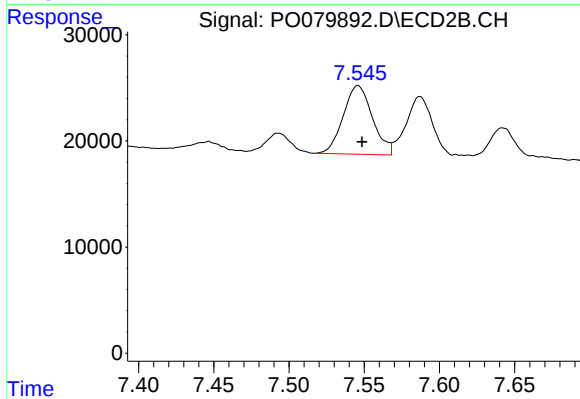

#36 AR-1262-1


R.T.: 7.546 min
Delta R.T.: -0.003 min
Response: 87442
Conc: 103.88 ng/ml

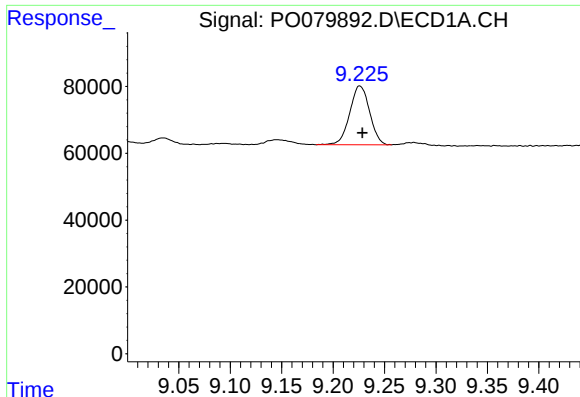

#37 AR-1262-2


R.T.: 9.226 min
Delta R.T.: -0.002 min
Response: 236721
Conc: 43.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

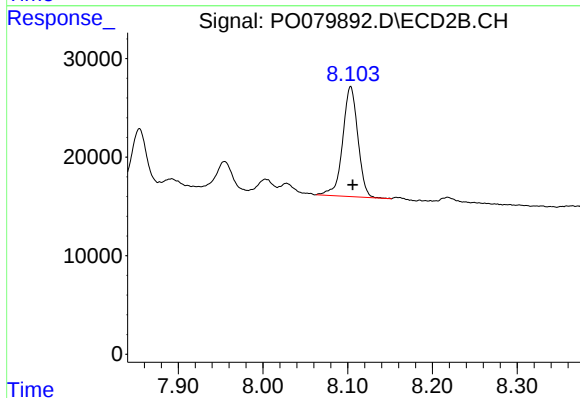


#37 AR-1262-2

R.T.: 8.104 min
Delta R.T.: -0.003 min
Response: 139207
Conc: 51.84 ng/ml

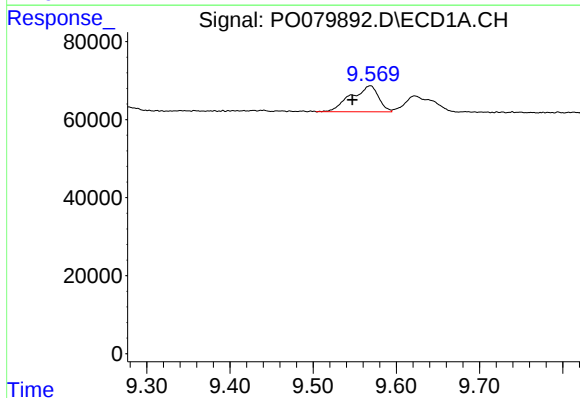


#38 AR-1262-3

R.T.: 9.569 min
Delta R.T.: 0.022 min
Response: 154084
Conc: 40.74 ng/ml

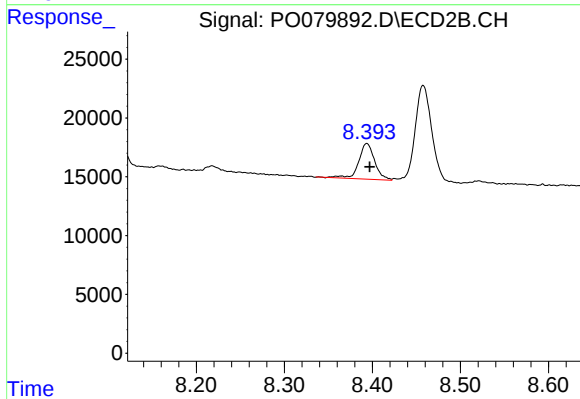

#38 AR-1262-3


R.T.: 8.394 min
Delta R.T.: -0.003 min
Response: 37994
Conc: 34.21 ng/ml

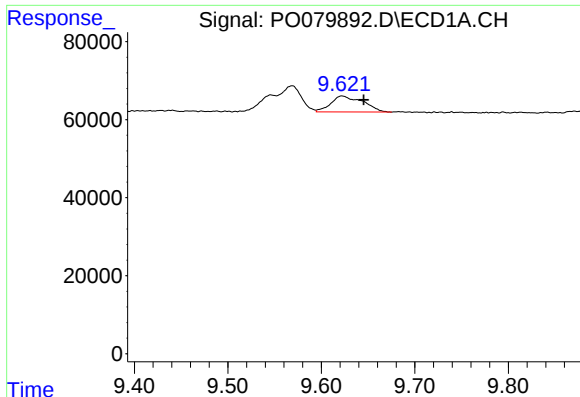

#39 AR-1262-4


R.T.: 9.622 min
Delta R.T.: -0.023 min
Response: 98113
Conc: 34.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

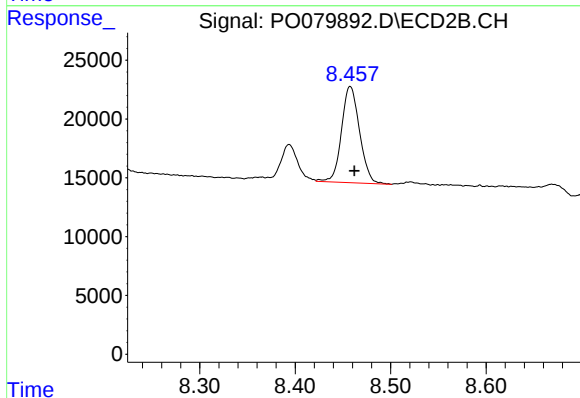


#39 AR-1262-4

R.T.: 8.458 min
Delta R.T.: -0.004 min
Response: 107403
Conc: 53.72 ng/ml

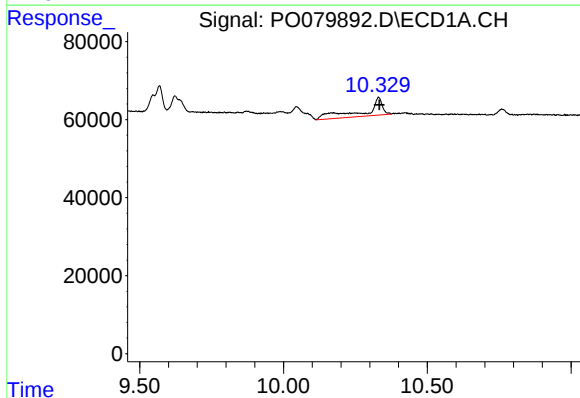


#40 AR-1262-5

R.T.: 10.330 min
Delta R.T.: -0.004 min
Response: 199865
Conc: 105.11 ng/ml

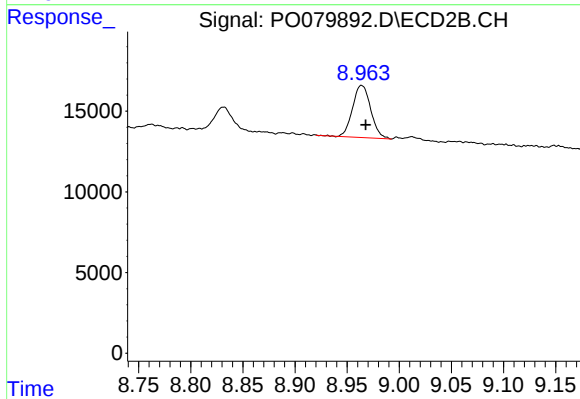

#40 AR-1262-5


R.T.: 8.964 min
Delta R.T.: -0.004 min
Response: 39307
Conc: 40.30 ng/ml

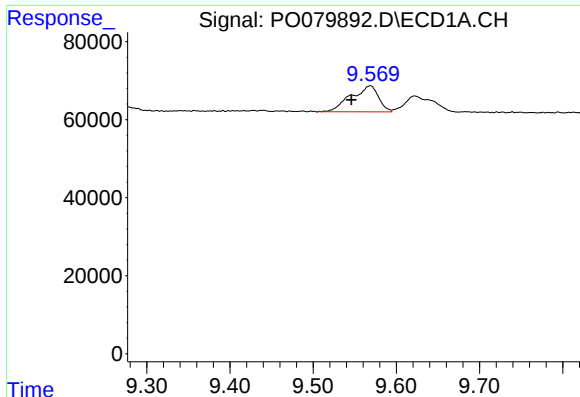

#41 AR-1268-1


R.T.: 9.569 min
Delta R.T.: 0.023 min
Response: 154084
Conc: 23.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

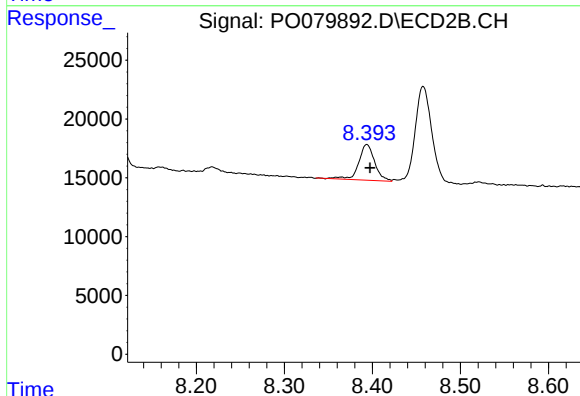


#41 AR-1268-1

R.T.: 8.394 min
Delta R.T.: -0.004 min
Response: 37994
Conc: 12.50 ng/ml

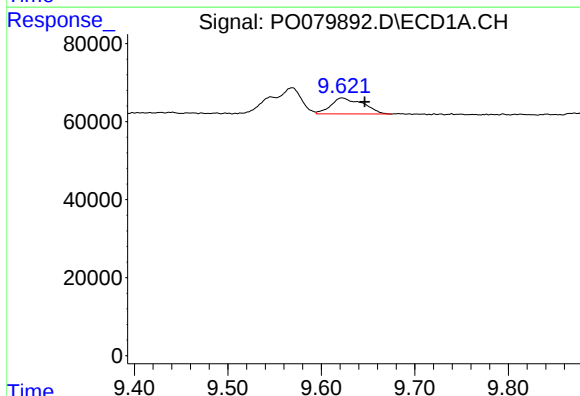


#42 AR-1268-2

R.T.: 9.622 min
Delta R.T.: -0.024 min
Response: 98113
Conc: 16.49 ng/ml

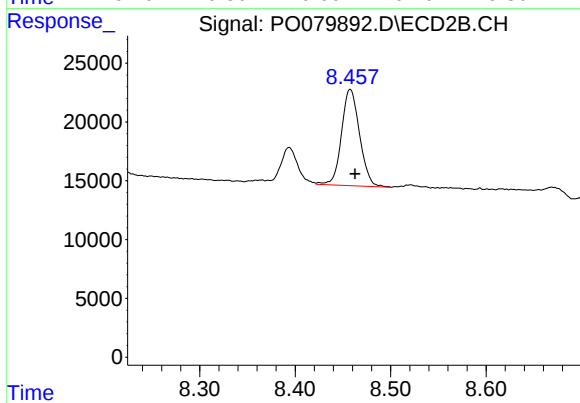

#42 AR-1268-2


R.T.: 8.458 min
Delta R.T.: -0.005 min
Response: 107403
Conc: 39.47 ng/ml

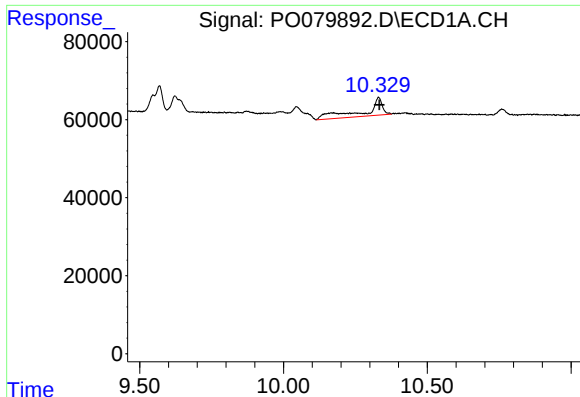

#44 AR-1268-4


R.T.: 10.330 min
Delta R.T.: -0.003 min
Response: 199865
Conc: 86.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2021

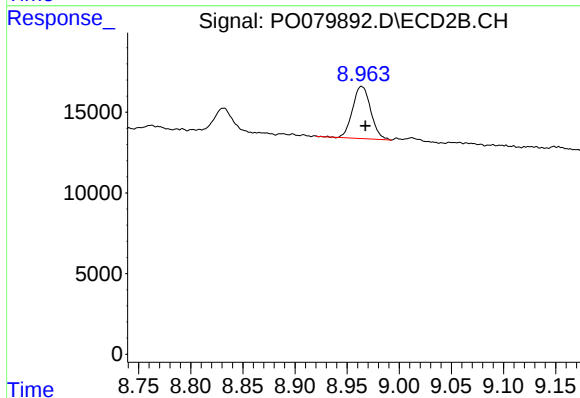


#44 AR-1268-4

R.T.: 8.964 min
Delta R.T.: -0.004 min
Response: 39307
Conc: 36.71 ng/ml

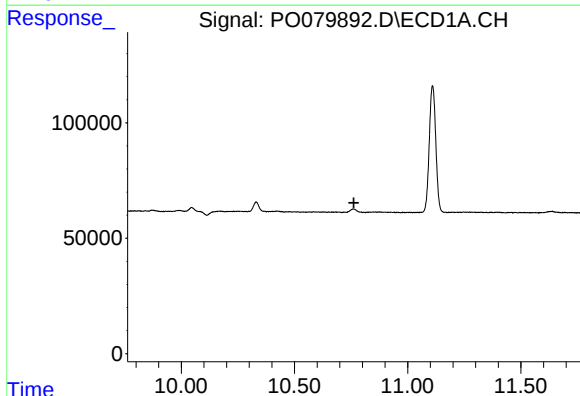

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.762 min
Response: 0
Conc: N.D.

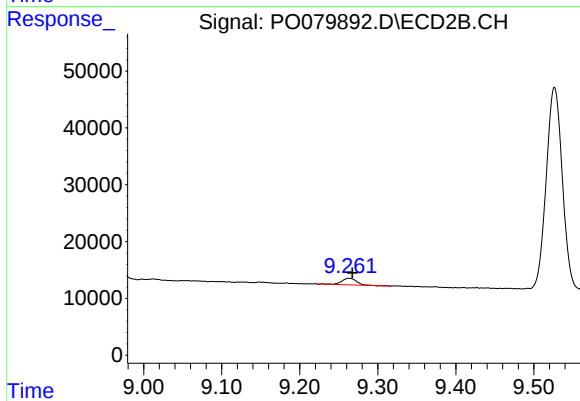

#45 AR-1268-5

R.T.: 9.263 min
Delta R.T.: -0.004 min
Response: 15837
Conc: 2.28 ng/ml