

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072821\
 Data File : P0079920.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2021 7:52
 Operator : DD\AJ
 Sample : M2940-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 08:19:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.000	4.118	1270583	501431	21.086	21.895
2) SA Decachlor...	11.110	9.525	1079645	481723	23.015	23.180
Target Compounds						
36) L8 AR-1262-1	8.659	7.545	80240	22865	25.093	27.164
37) L8 AR-1262-2	9.227	8.103	135307	74339	24.983	27.686
38) L8 AR-1262-3	9.544	8.394	93548	32147	24.734	28.943
39) L8 AR-1262-4	9.622f	8.458	77991	58500	27.602	29.259
40) L8 AR-1262-5	10.331	8.964	46028	30648	24.205	31.419 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072821\
Data File : P0079920.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2021 7:52
Operator : DD\AJ
Sample : M2940-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 08:19:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

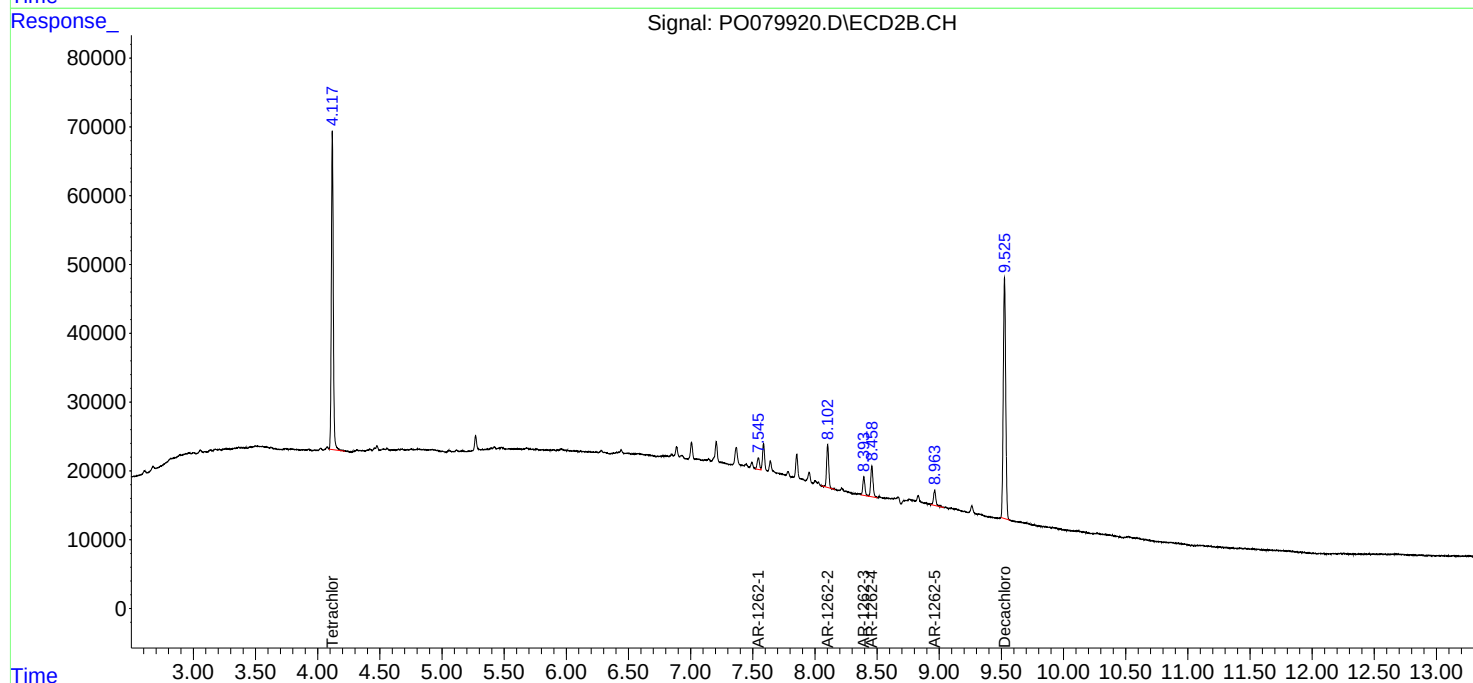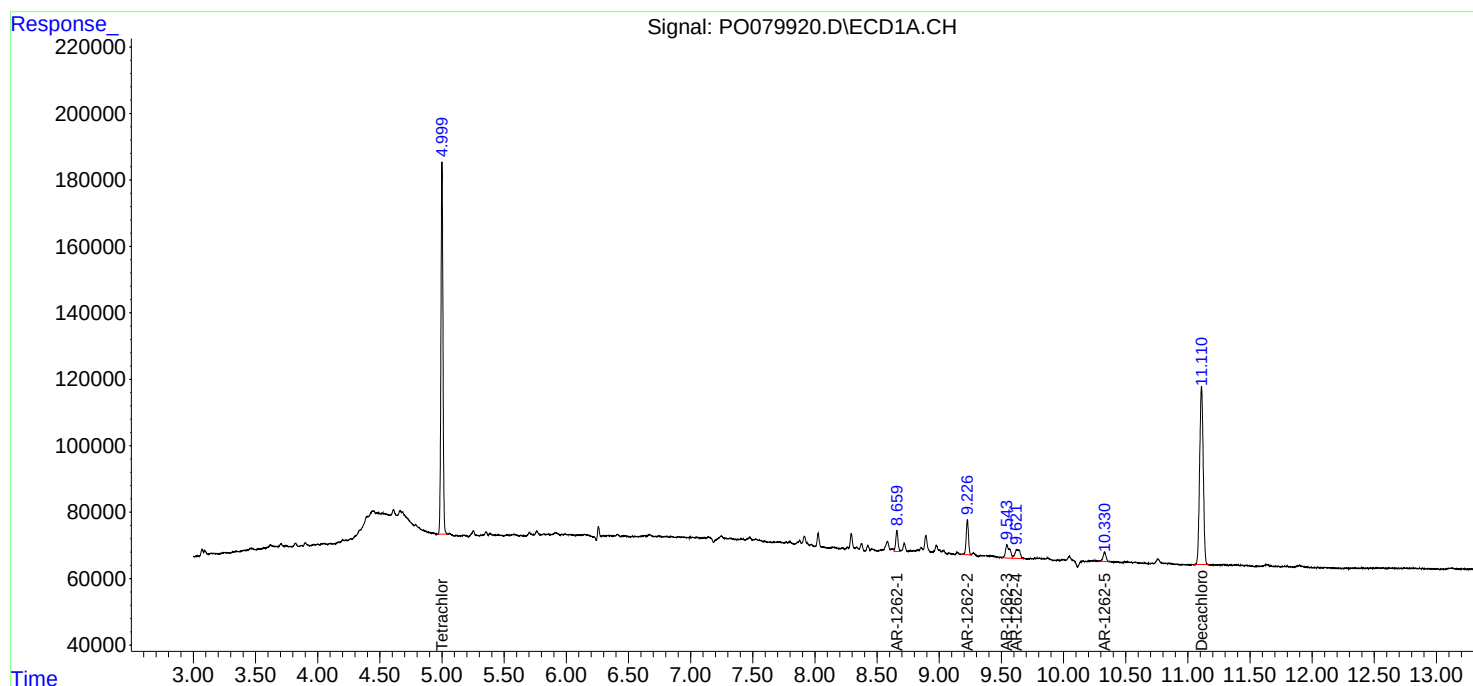


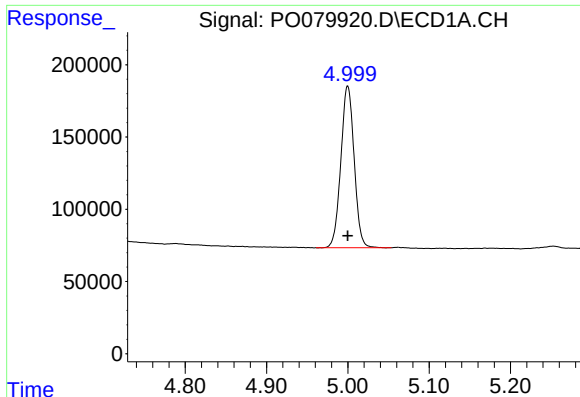

#1 Tetrachloro-m-xylene


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 1270583
Conc: 21.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

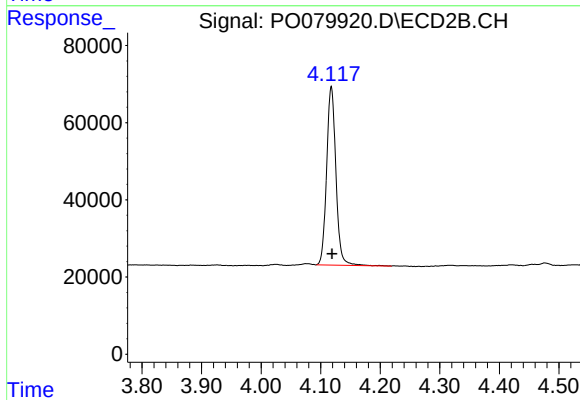


#1 Tetrachloro-m-xylene

R.T.: 4.118 min
Delta R.T.: -0.001 min
Response: 501431
Conc: 21.90 ng/ml

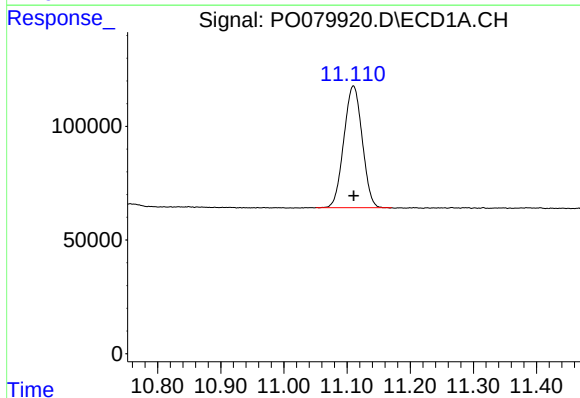


#2 Decachlorobiphenyl

R.T.: 11.110 min
Delta R.T.: 0.000 min
Response: 1079645
Conc: 23.02 ng/ml

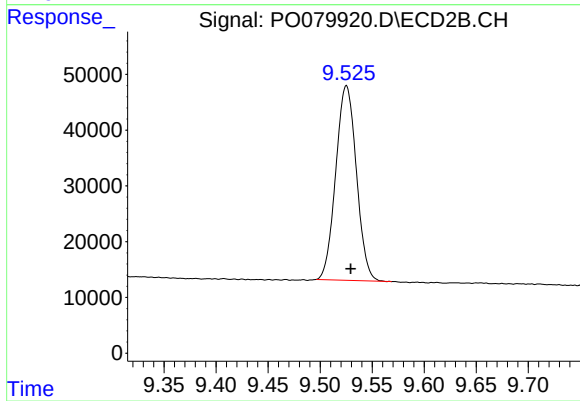

#2 Decachlorobiphenyl


R.T.: 9.525 min
Delta R.T.: -0.004 min
Response: 481723
Conc: 23.18 ng/ml

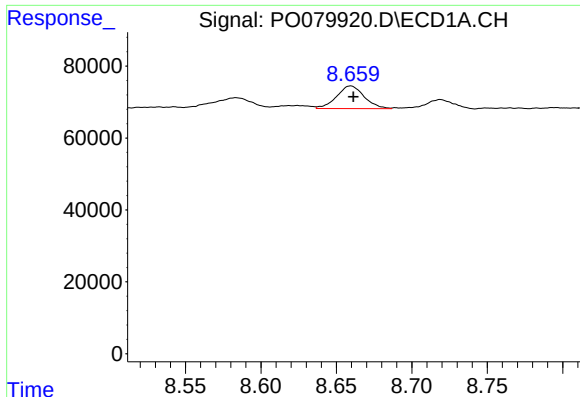

#36 AR-1262-1


R.T.: 8.659 min
Delta R.T.: -0.002 min
Response: 80240
Conc: 25.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

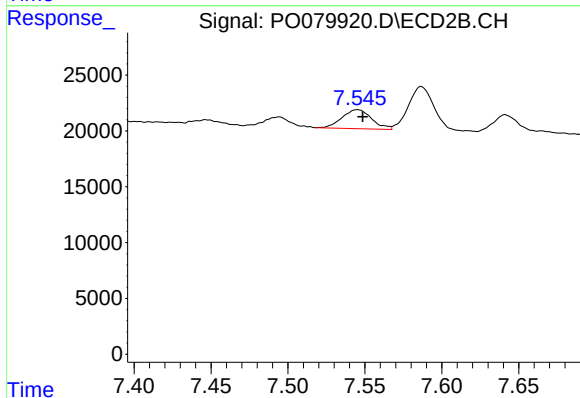


#36 AR-1262-1

R.T.: 7.545 min
Delta R.T.: -0.003 min
Response: 22865
Conc: 27.16 ng/ml

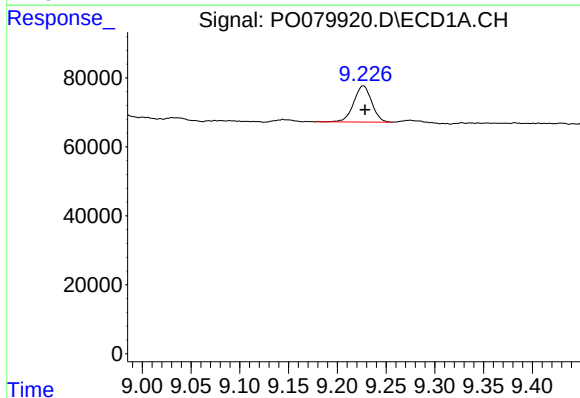


#37 AR-1262-2

R.T.: 9.227 min
Delta R.T.: -0.002 min
Response: 135307
Conc: 24.98 ng/ml

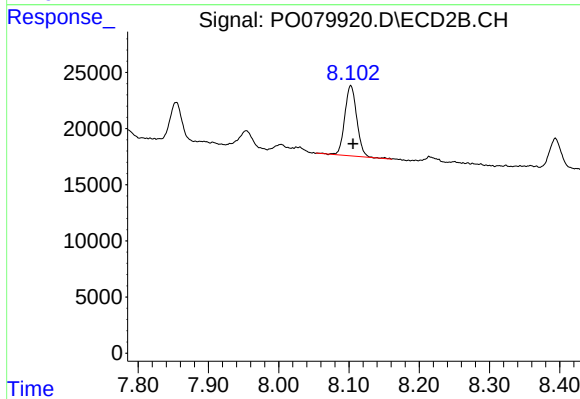

#37 AR-1262-2


R.T.: 8.103 min
Delta R.T.: -0.003 min
Response: 74339
Conc: 27.69 ng/ml

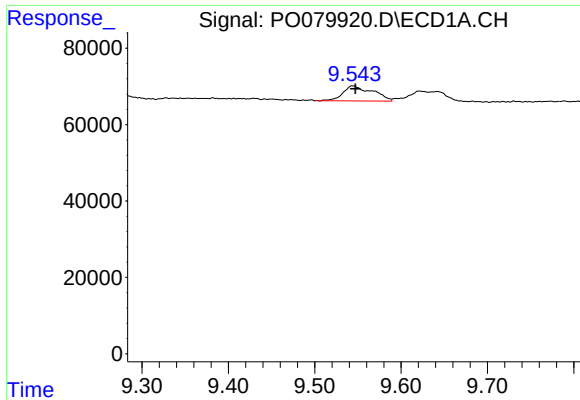

#38 AR-1262-3


R.T.: 9.544 min
Delta R.T.: -0.003 min
Response: 93548
Conc: 24.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

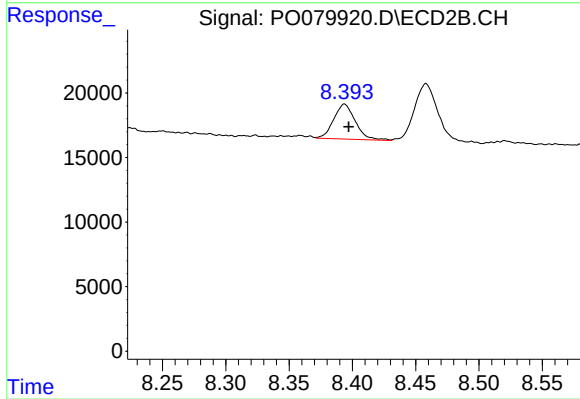


#38 AR-1262-3

R.T.: 8.394 min
Delta R.T.: -0.003 min
Response: 32147
Conc: 28.94 ng/ml

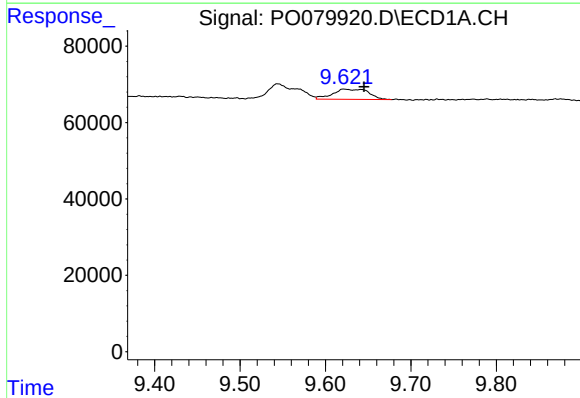


#39 AR-1262-4

R.T.: 9.622 min
Delta R.T.: -0.024 min
Response: 77991
Conc: 27.60 ng/ml

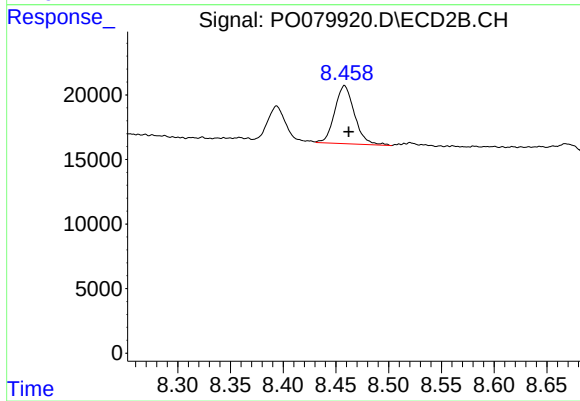

#39 AR-1262-4


R.T.: 8.458 min
Delta R.T.: -0.004 min
Response: 58500
Conc: 29.26 ng/ml

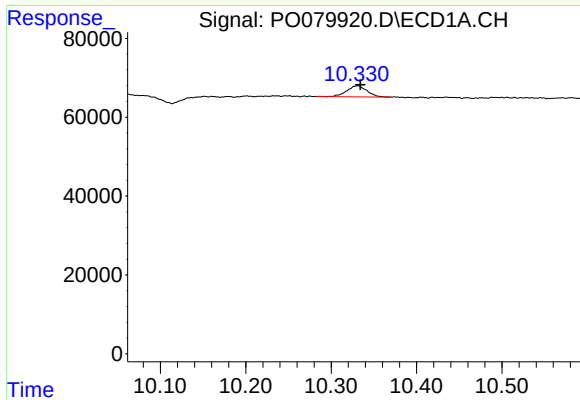

#40 AR-1262-5

R.T.: 10.331 min
Delta R.T.: -0.003 min
Response: 46028
Conc: 24.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

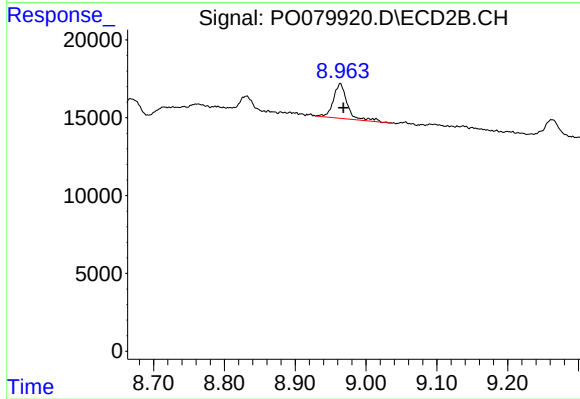

#40 AR-1262-5

R.T.: 8.964 min
Delta R.T.: -0.004 min
Response: 30648
Conc: 31.42 ng/ml