

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072821\
 Data File : P0079921.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jul 2021 8:09
 Operator : DD\AJ
 Sample : M2940-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 08:28:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 28 18:45:36 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.000	4.118	1314870	512969	21.821	22.399
2) SA Decachlor...	11.108	9.526	1202818	532838	25.641	25.640
Target Compounds						
41) L9 AR-1268-1	9.545	8.394	155769	89223	24.060	29.365
42) L9 AR-1268-2	9.643	8.459	147058	78948	24.713	29.015
43) L9 AR-1268-3	9.876	8.671	120944	71599	24.069	30.887 #
44) L9 AR-1268-4	10.330	8.964	66110	31136	28.773	29.082
45) L9 AR-1268-5	10.760	9.264	426054	202488	25.555	29.156



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072821\
Data File : P0079921.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jul 2021 8:09
Operator : DD\AJ
Sample : M2940-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 08:28:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 28 18:45:36 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

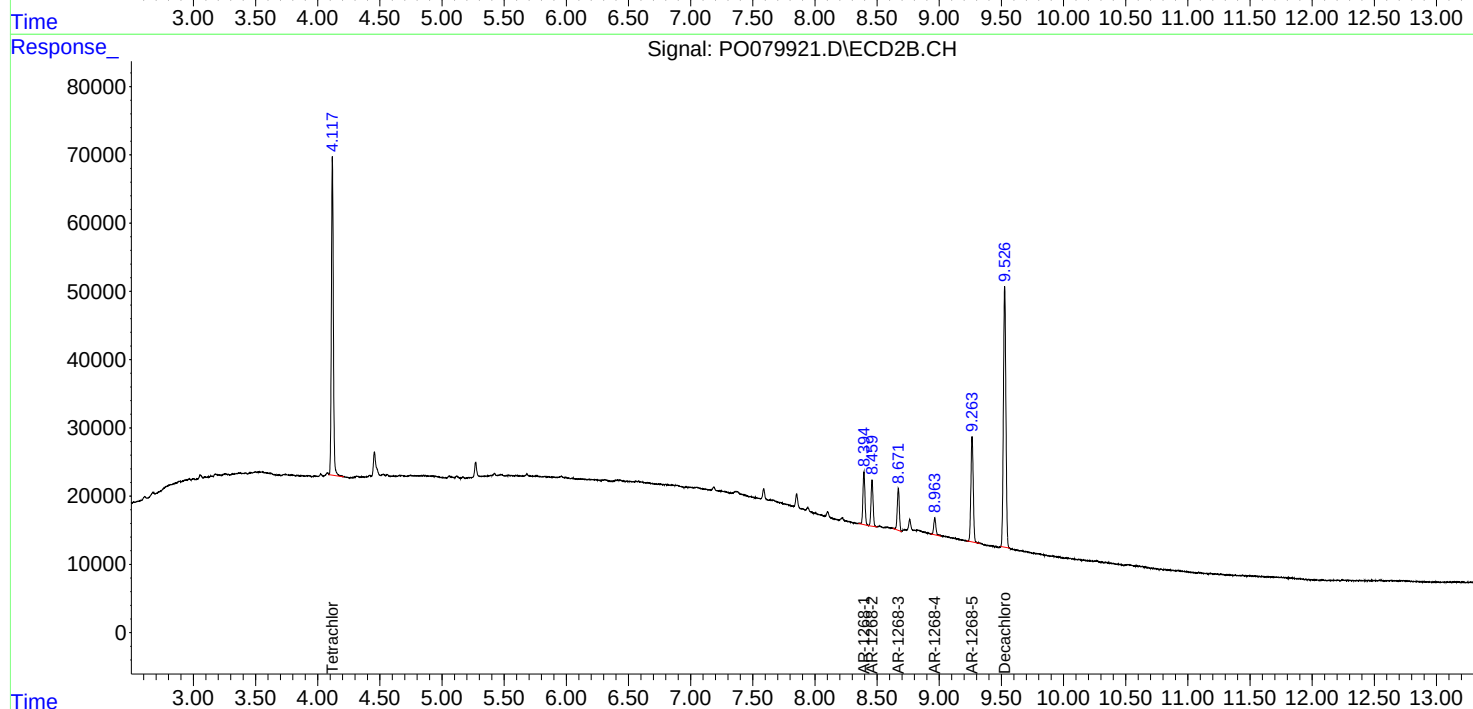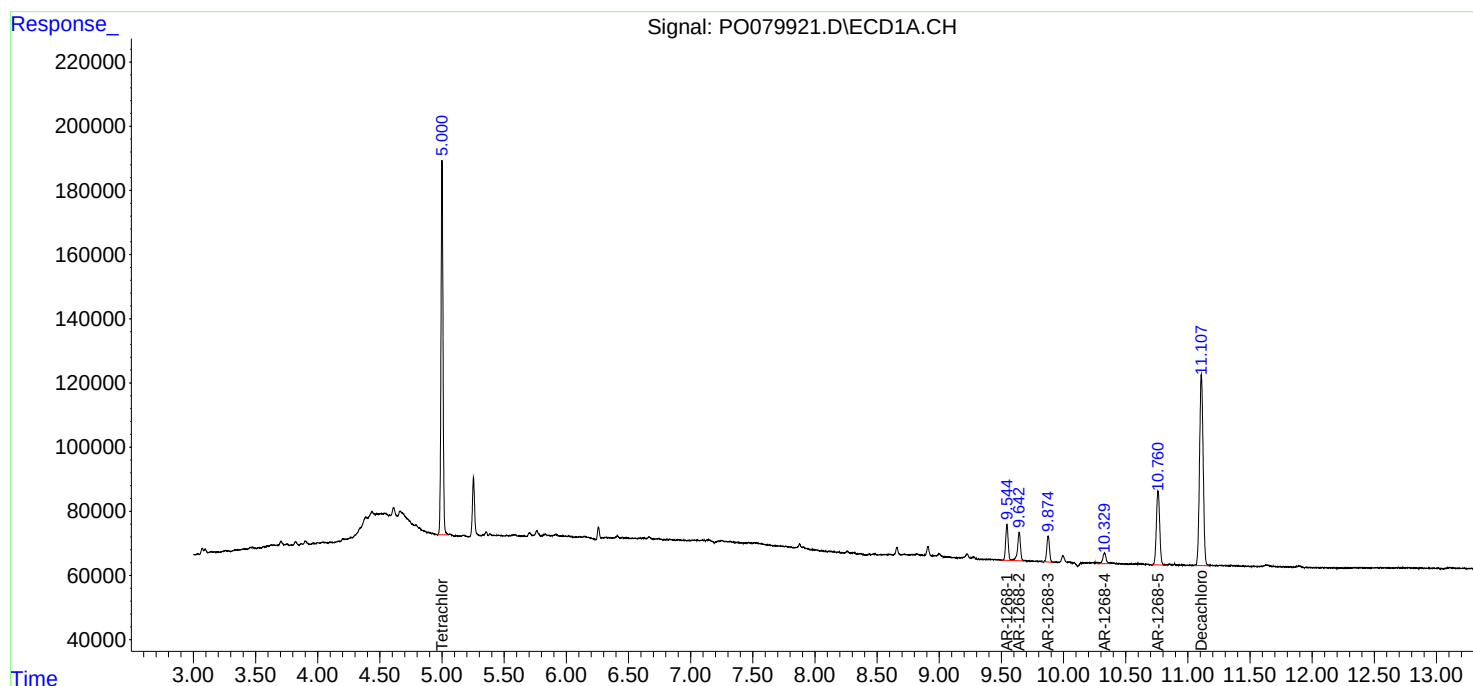


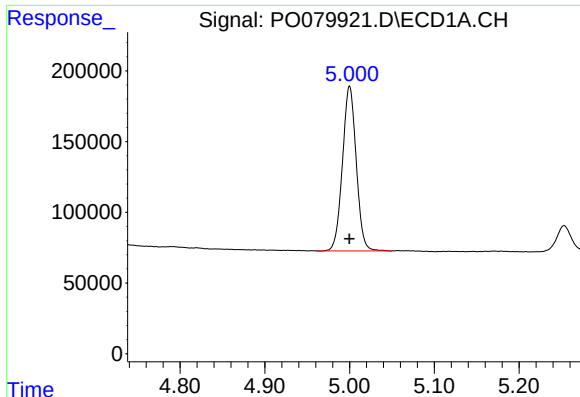

#1 Tetrachloro-m-xylene


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 1314870
Conc: 21.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

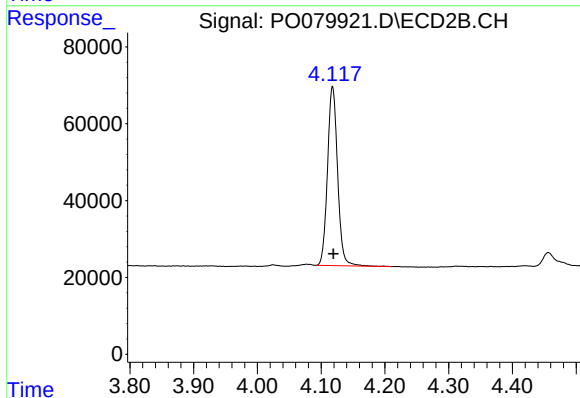


#1 Tetrachloro-m-xylene

R.T.: 4.118 min
Delta R.T.: -0.001 min
Response: 512969
Conc: 22.40 ng/ml

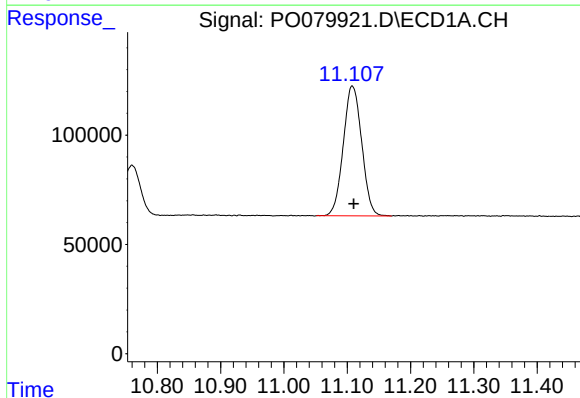


#2 Decachlorobiphenyl

R.T.: 11.108 min
Delta R.T.: -0.003 min
Response: 1202818
Conc: 25.64 ng/ml

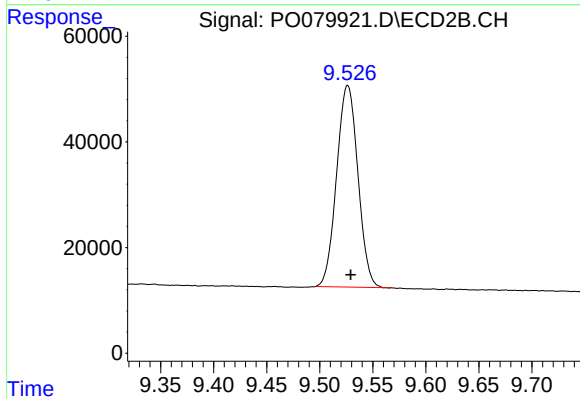

#2 Decachlorobiphenyl


R.T.: 9.526 min
Delta R.T.: -0.003 min
Response: 532838
Conc: 25.64 ng/ml

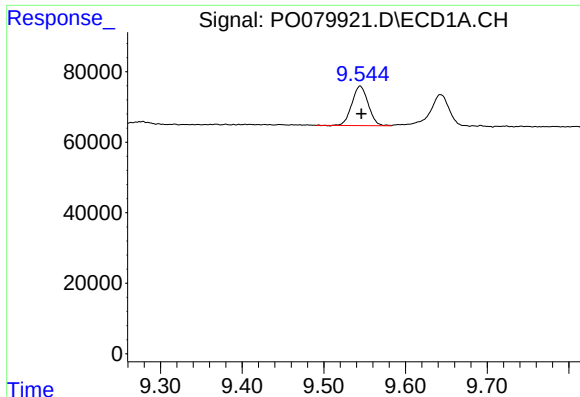

#41 AR-1268-1


R.T.: 9.545 min
Delta R.T.: -0.001 min
Response: 155769
Conc: 24.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

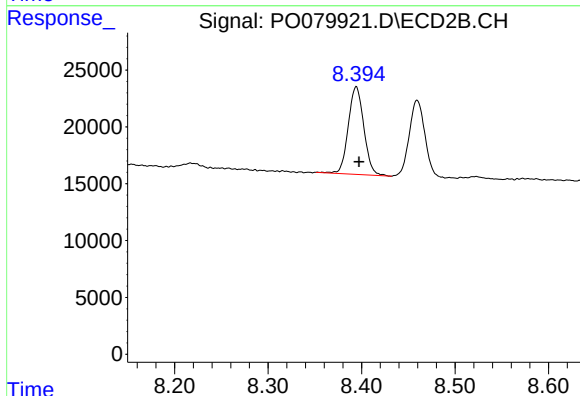


#41 AR-1268-1

R.T.: 8.394 min
Delta R.T.: -0.003 min
Response: 89223
Conc: 29.36 ng/ml

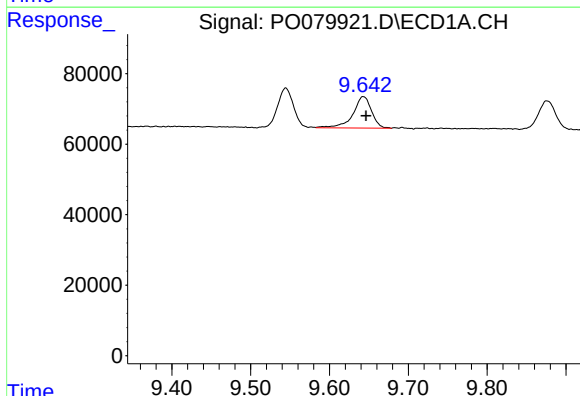


#42 AR-1268-2

R.T.: 9.643 min
Delta R.T.: -0.003 min
Response: 147058
Conc: 24.71 ng/ml

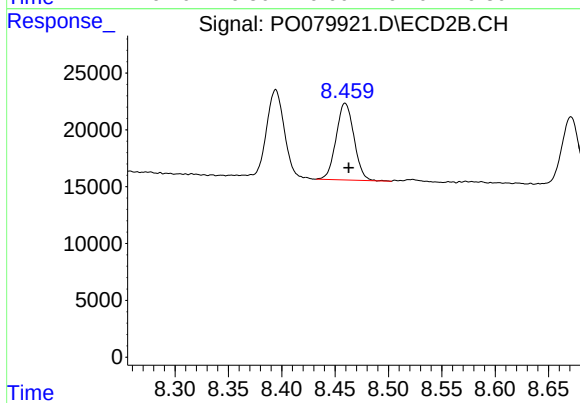

#42 AR-1268-2


R.T.: 8.459 min
Delta R.T.: -0.003 min
Response: 78948
Conc: 29.01 ng/ml

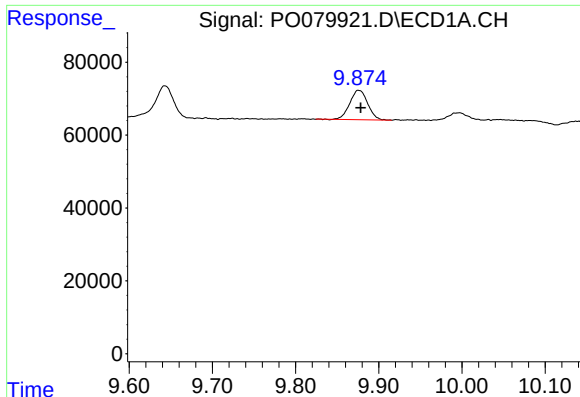

#43 AR-1268-3


R.T.: 9.876 min
Delta R.T.: -0.002 min
Response: 120944
Conc: 24.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

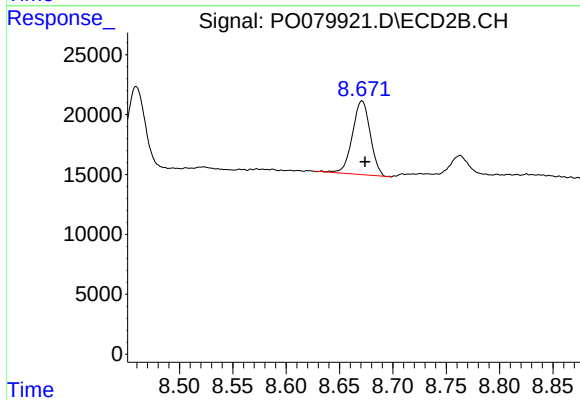


#43 AR-1268-3

R.T.: 8.671 min
Delta R.T.: -0.003 min
Response: 71599
Conc: 30.89 ng/ml

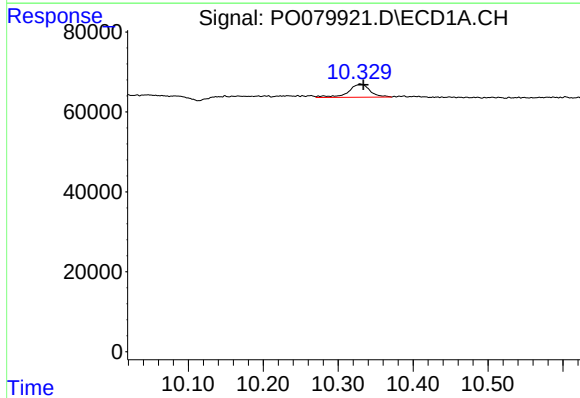


#44 AR-1268-4

R.T.: 10.330 min
Delta R.T.: -0.004 min
Response: 66110
Conc: 28.77 ng/ml

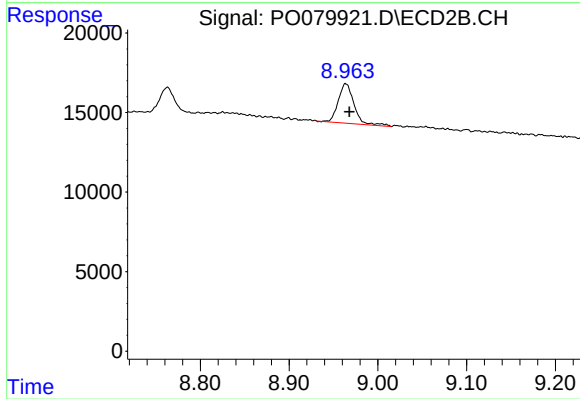

#44 AR-1268-4


R.T.: 8.964 min
Delta R.T.: -0.004 min
Response: 31136
Conc: 29.08 ng/ml

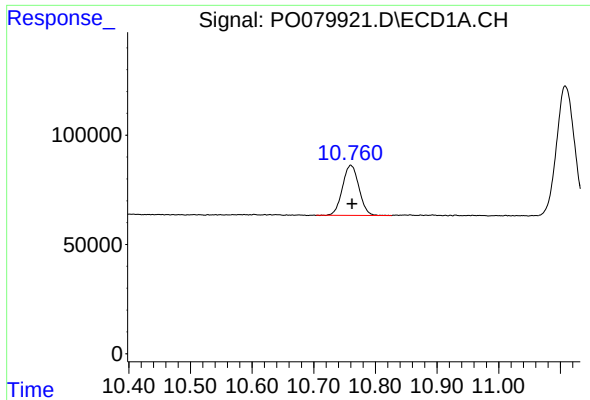

#45 AR-1268-5

R.T.: 10.760 min
Delta R.T.: -0.002 min
Response: 426054
Conc: 25.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2021

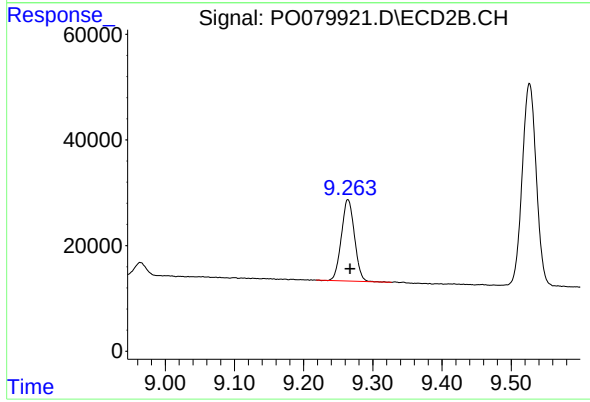

#45 AR-1268-5

R.T.: 9.264 min
Delta R.T.: -0.003 min
Response: 202488
Conc: 29.16 ng/ml