

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072825\
 Data File : P0112545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2025 14:24
 Operator : YP/AJ
 Sample : Q2707-01 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OILY-SPEEDY-DRY

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/29/2025
 Supervised By :mohammad ahmed 07/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 15:00:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.669	3.661	9622844	6028903	1.183m	1.213m
2) SA Decachlor...	8.694	8.641	8796964	1912796	1.203m	1.082

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072825\
Data File : PO112545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2025 14:24
Operator : YP/AJ
Sample : Q2707-01 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-SPEEDY-DRY


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2025
Supervised By :mohammad ahmed 07/30/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 15:00:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

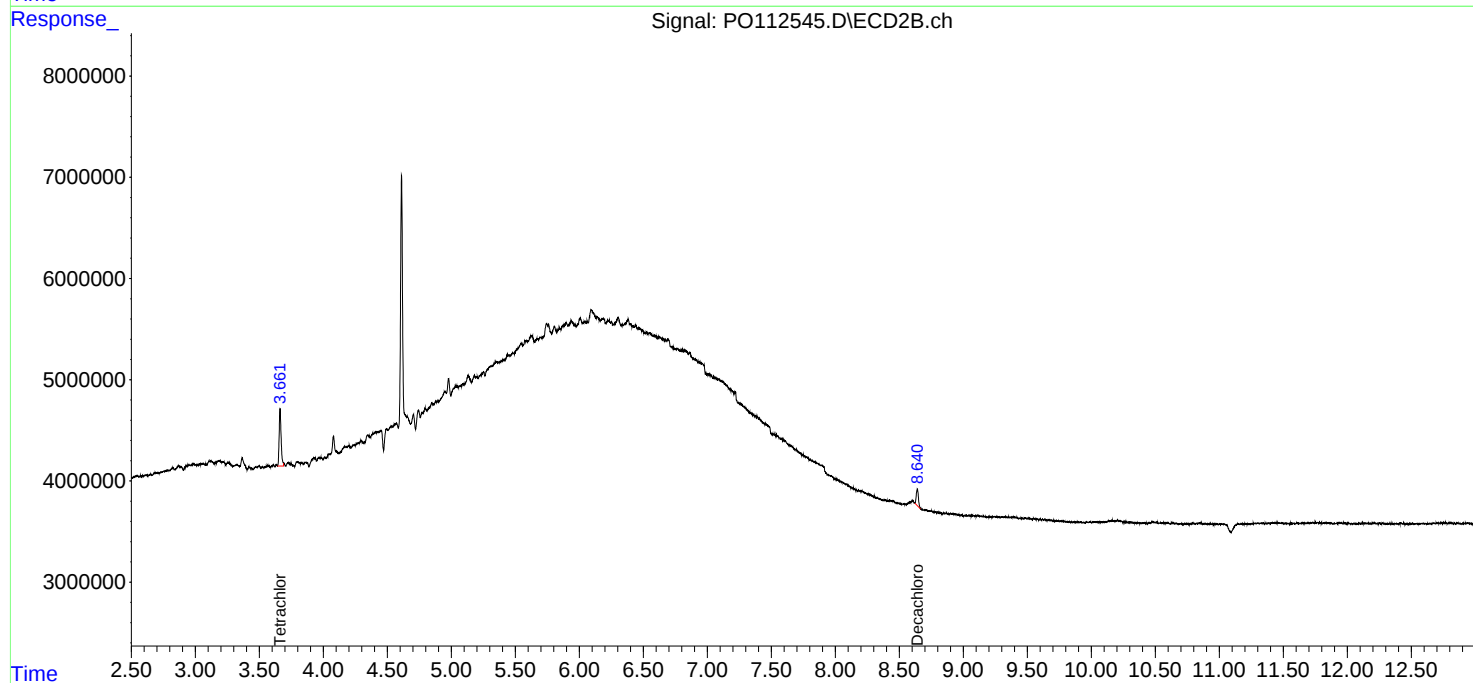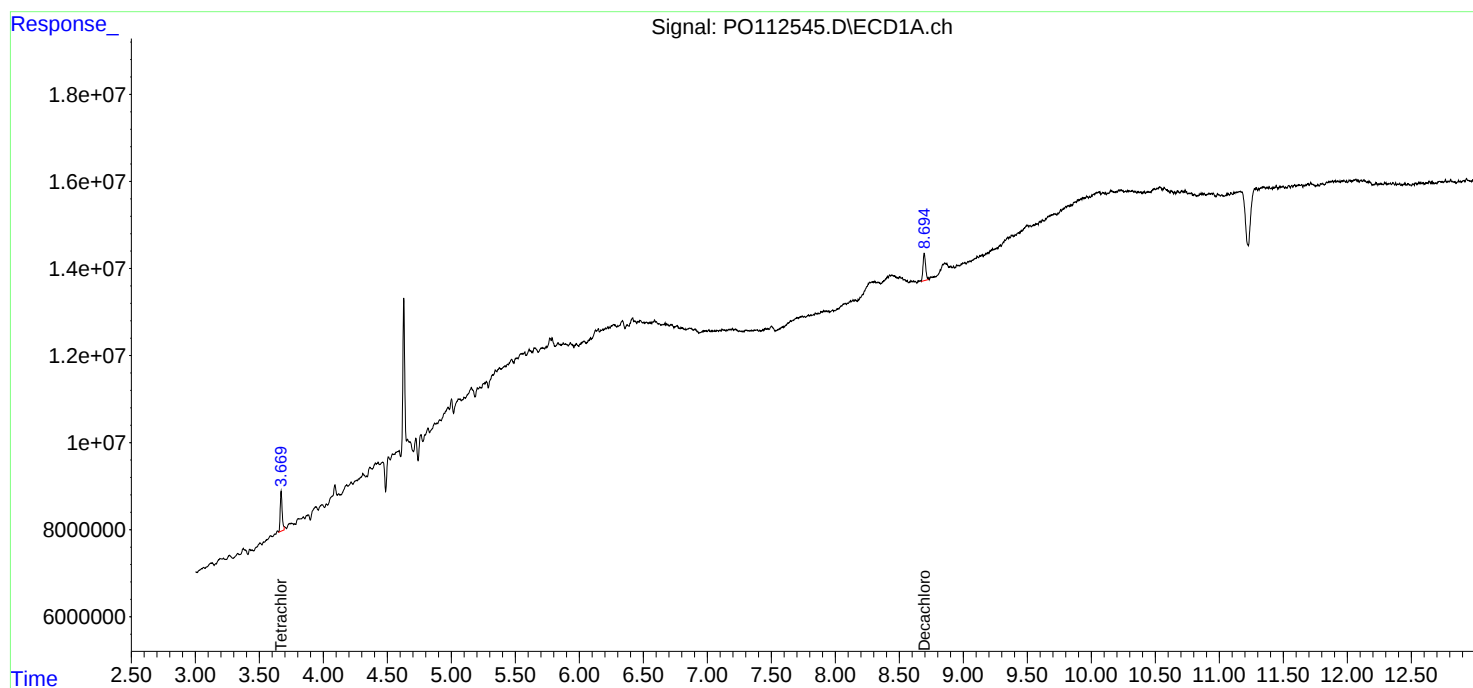

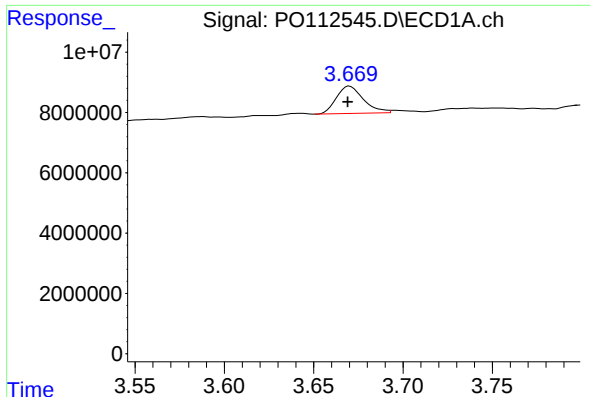


#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 9622844
Conc: 1.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
OILY-SPEEDY-DRY


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2025
Supervised By :mohammad ahmed 07/30/2025

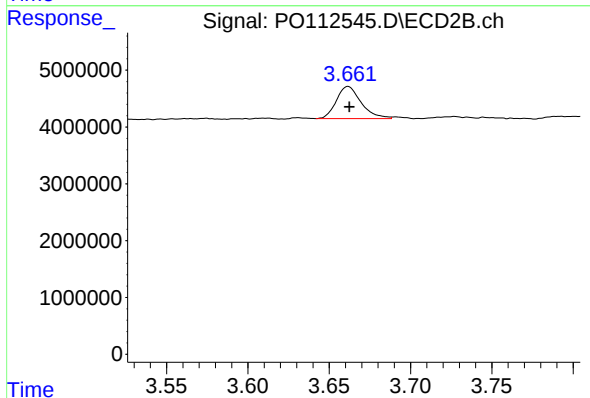


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.001 min
Response: 6028903
Conc: 1.21 ng/ml m

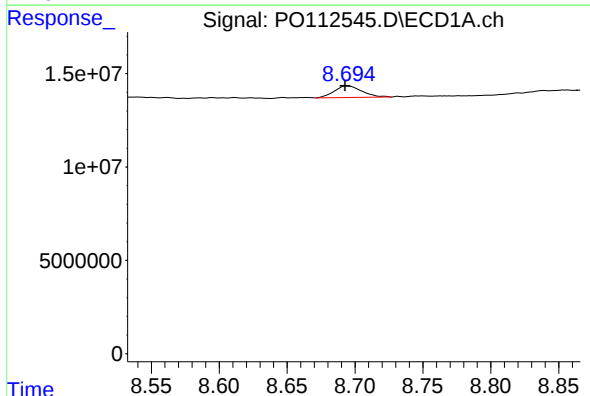

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 8796964
Conc: 1.20 ng/ml m

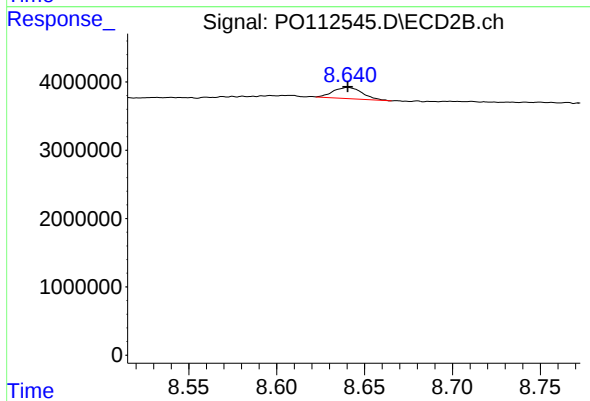

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 1912796
Conc: 1.08 ng/ml