

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072825\
 Data File : P0112562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2025 22:09
 Operator : YP/AJ
 Sample : Q2707-03 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 OILY-LIQUID

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/29/2025
 Supervised By :mohammad ahmed 07/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 05:01:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.674	3.664	5249663	2137337	0.646m	0.430m#
2) SA Decachlor...	8.690	8.638	8732538	1328751	1.194m	0.752m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072825\
Data File : P0112562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2025 22:09
Operator : YP/AJ
Sample : Q2707-03 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-LIQUID


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2025
Supervised By :mohammad ahmed 07/30/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 05:01:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

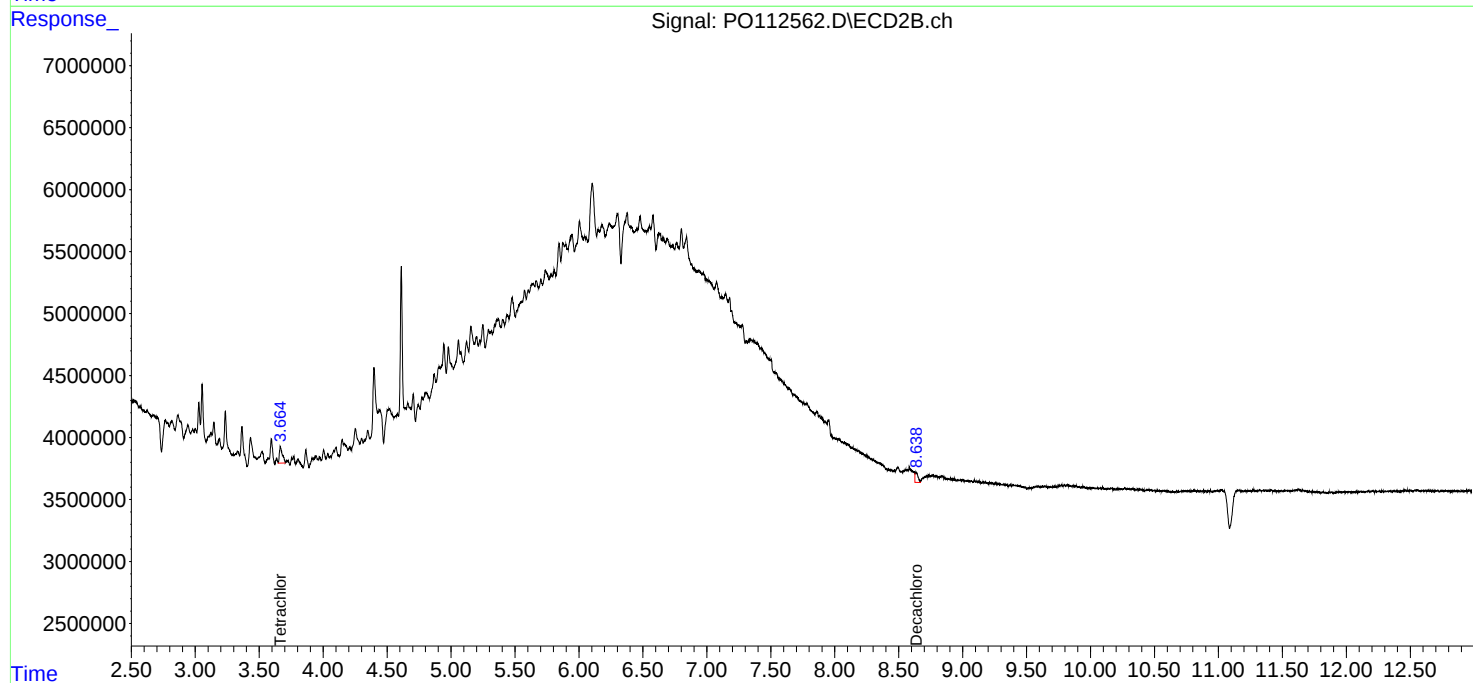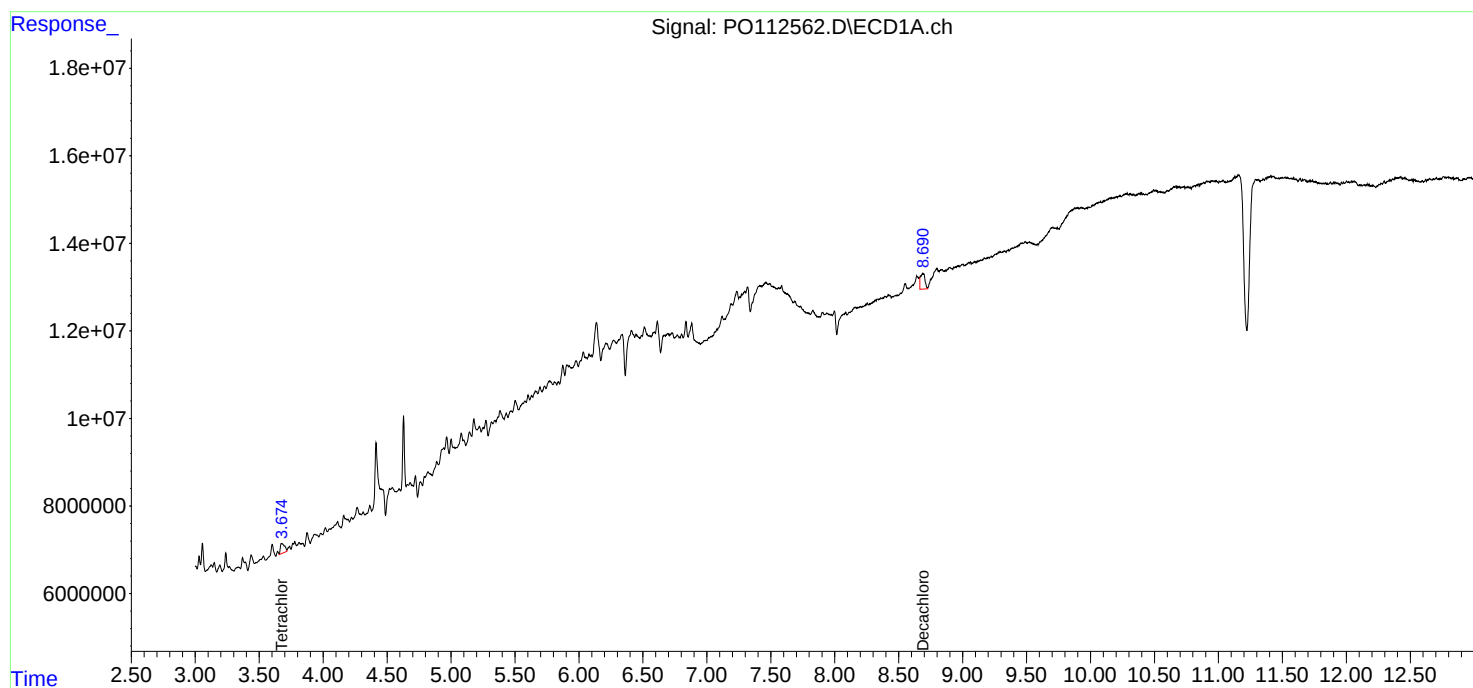

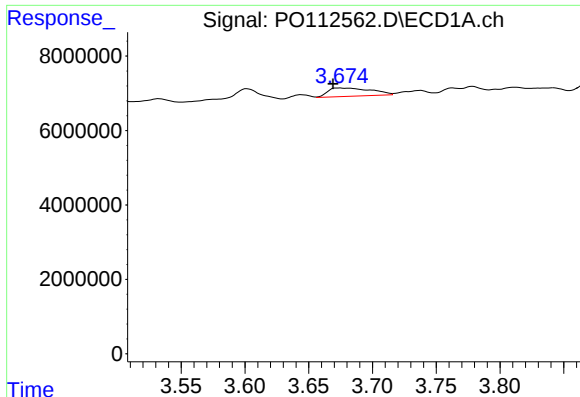


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: 0.005 min
Response: 5249663
Conc: 0.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
OILY-LIQUID


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2025
Supervised By :mohammad ahmed 07/30/2025

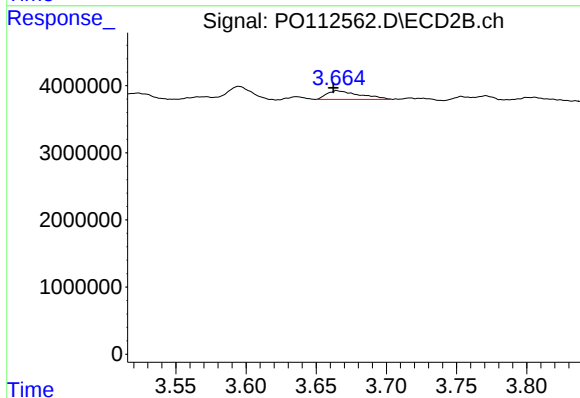


#1 Tetrachloro-m-xylene

R.T.: 3.664 min
Delta R.T.: 0.002 min
Response: 2137337
Conc: 0.43 ng/ml m

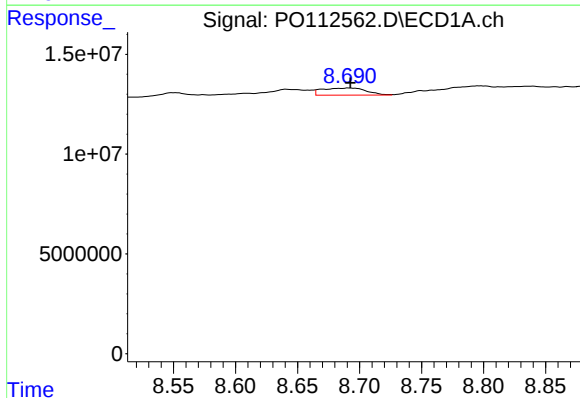

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.003 min
Response: 8732538
Conc: 1.19 ng/ml m

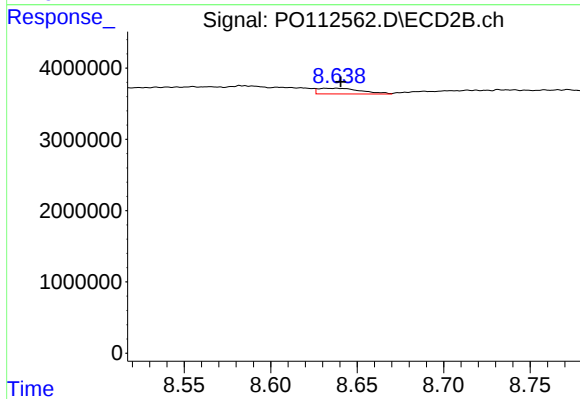

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: -0.002 min
Response: 1328751
Conc: 0.75 ng/ml m