

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072919\
 Data File : P0058482.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jul 2019 8:00
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 28 03:18:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 27 06:49:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.180	3.524	682627	653267	16.175	16.352
2)	SA Decachlor...	9.671	8.414	1008706	732552	18.626	18.558
Target Compounds							
35)	L7 AR-1260-5	0.000	7.079	0	21512	N.D.	3.994 #
37)	L8 AR-1262-2	0.000	7.079	0	21512	N.D.	3.810 #
38)	L8 AR-1262-3	0.000	7.359	0	1329	N.D.	0.538 #
39)	L8 AR-1262-4	0.000	7.420	0	10760	N.D.	2.534 #
41)	L9 AR-1268-1	0.000	7.359	0	1329	N.D.	0.163 #
42)	L9 AR-1268-2	0.000	7.420	0	10760	N.D.	1.420 #
43)	L9 AR-1268-3	0.000	7.621	0	6333	N.D.	0.991 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072919\
Data File : P0058482.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jul 2019 8:00
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 28 03:18:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072819.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 27 06:49:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

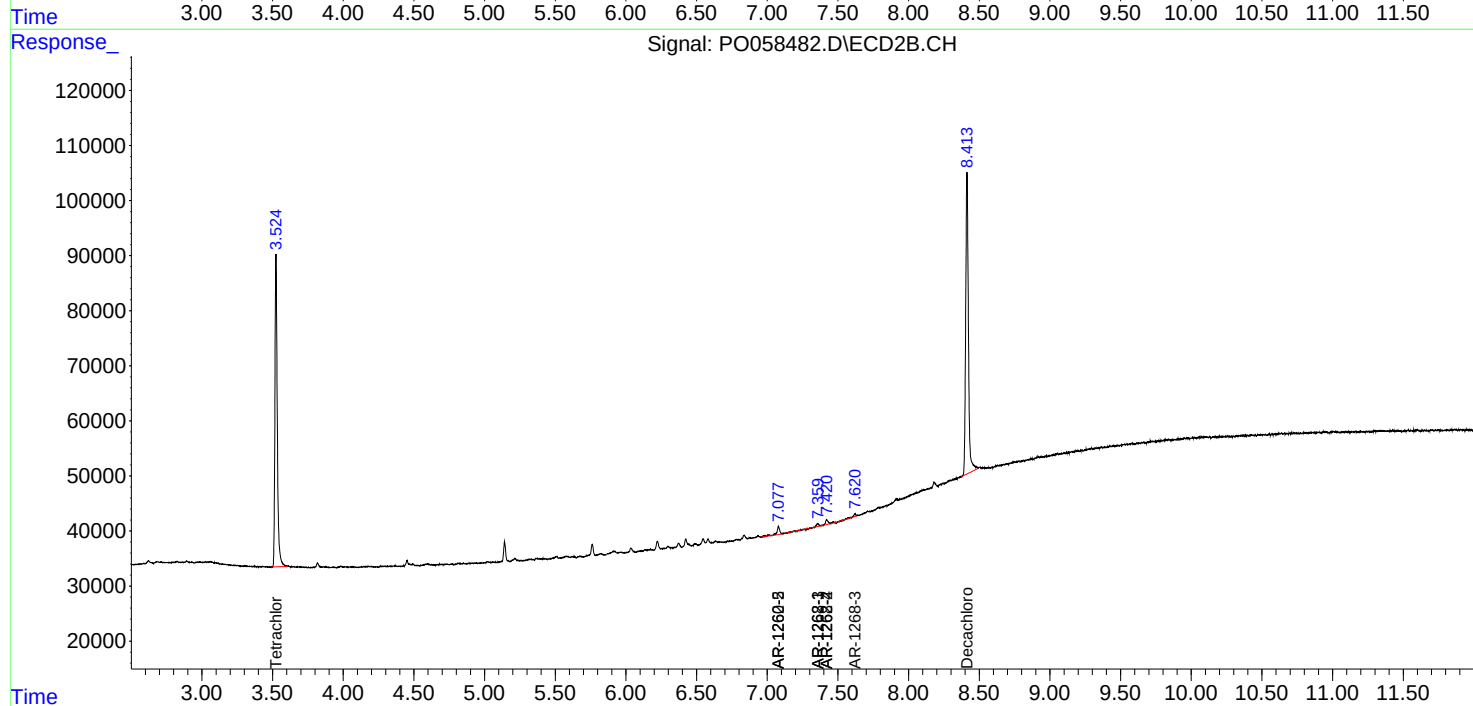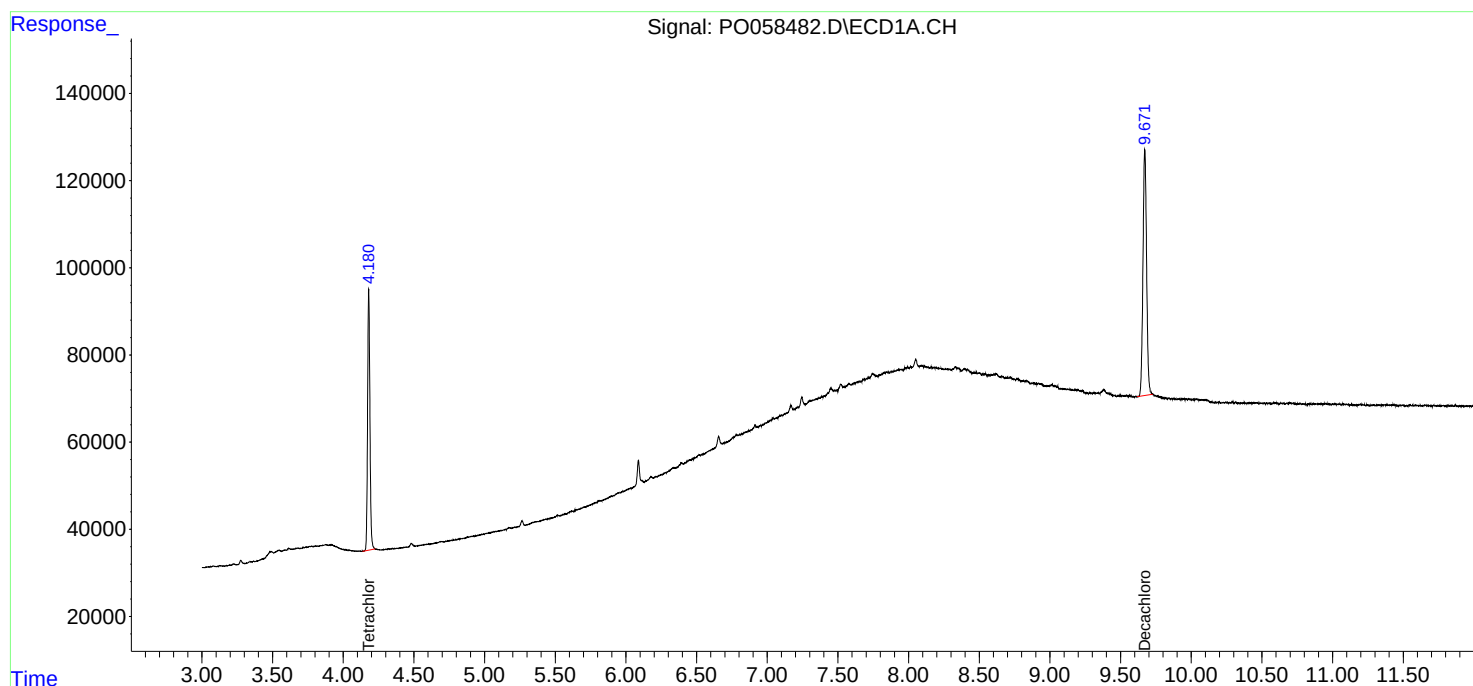


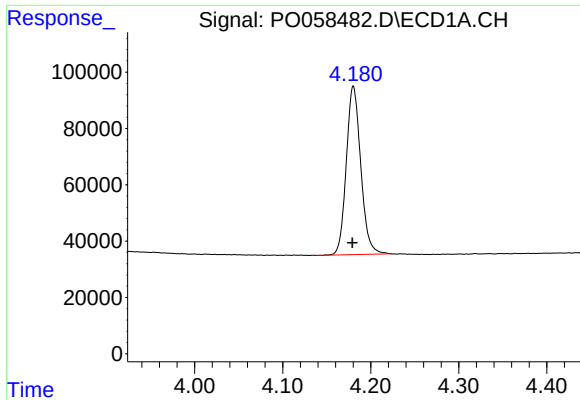

#1 Tetrachloro-m-xylene


R.T.: 4.180 min
Delta R.T.: 0.001 min
Response: 682627
Conc: 16.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

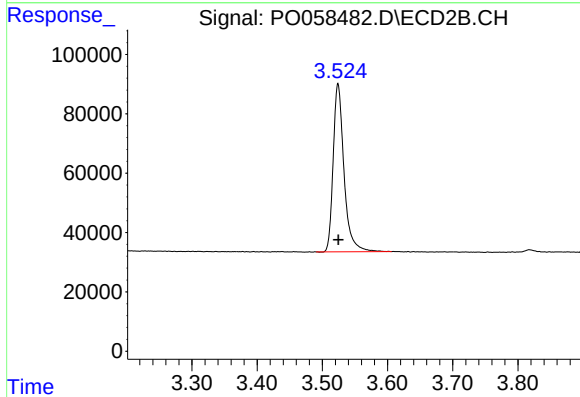


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: 0.000 min
Response: 653267
Conc: 16.35 ng/ml

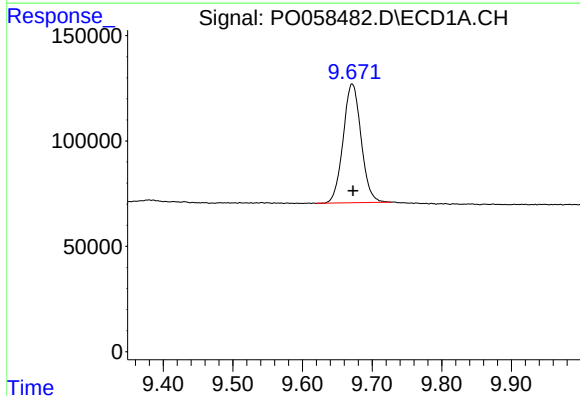


#2 Decachlorobiphenyl

R.T.: 9.671 min
Delta R.T.: -0.001 min
Response: 1008706
Conc: 18.63 ng/ml

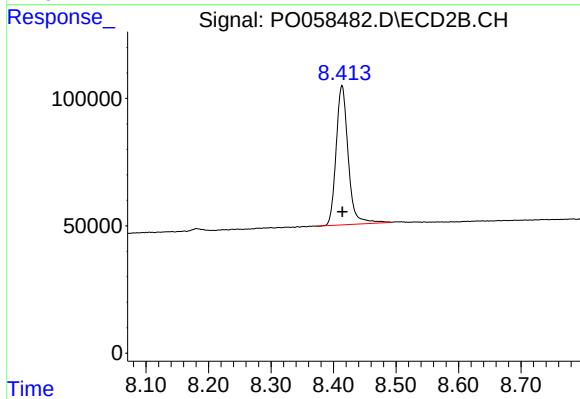

#2 Decachlorobiphenyl


R.T.: 8.414 min
Delta R.T.: 0.000 min
Response: 732552
Conc: 18.56 ng/ml

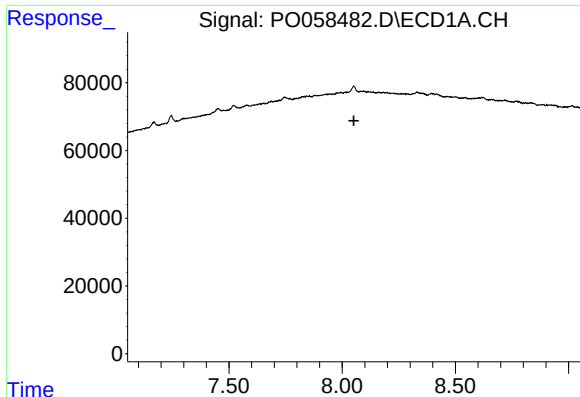

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.051 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

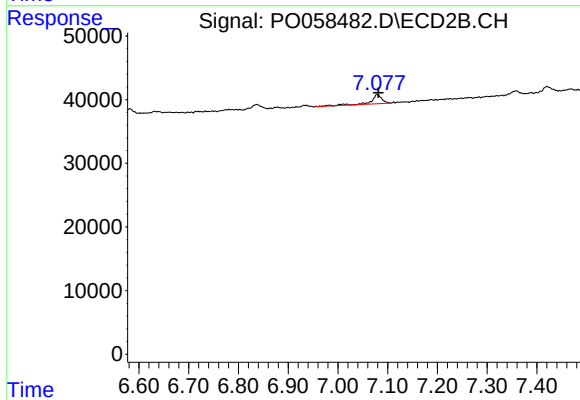


#35 AR-1260-5

R.T.: 7.079 min
Delta R.T.: -0.003 min
Response: 21512
Conc: 3.99 ng/ml

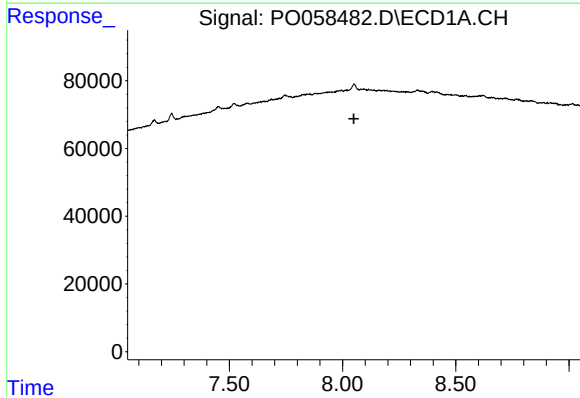


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.050 min
Response: 0
Conc: N.D.

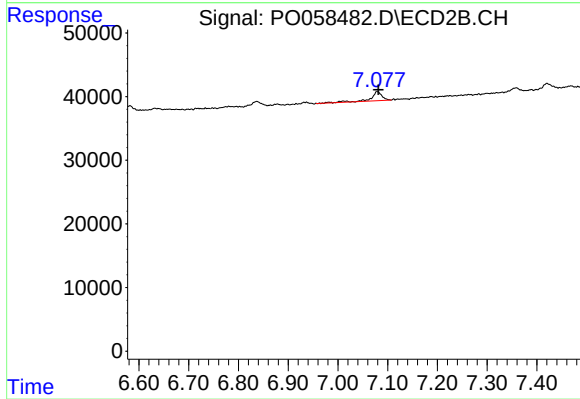

#37 AR-1262-2


R.T.: 7.079 min
Delta R.T.: -0.003 min
Response: 21512
Conc: 3.81 ng/ml

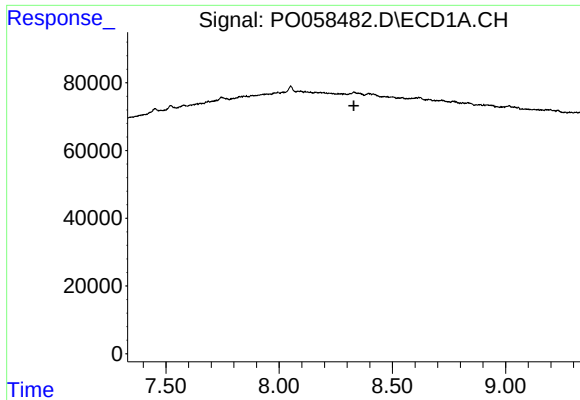

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.330 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

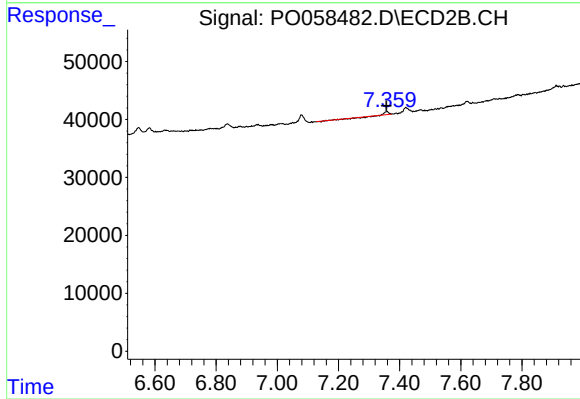


#38 AR-1262-3

R.T.: 7.359 min
Delta R.T.: 0.002 min
Response: 1329
Conc: 0.54 ng/ml

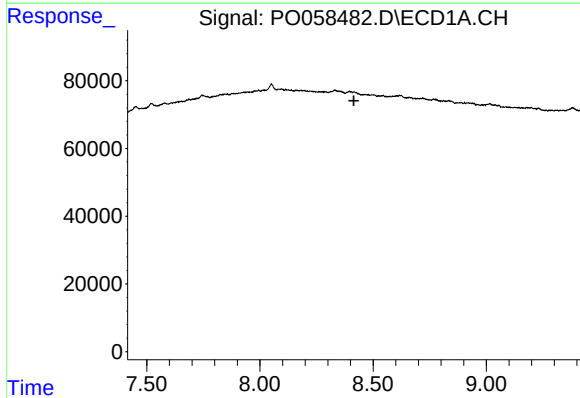


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.415 min
Response: 0
Conc: N.D.

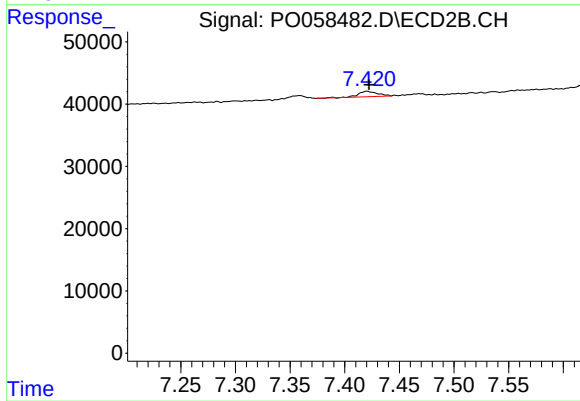

#39 AR-1262-4


R.T.: 7.420 min
Delta R.T.: -0.002 min
Response: 10760
Conc: 2.53 ng/ml

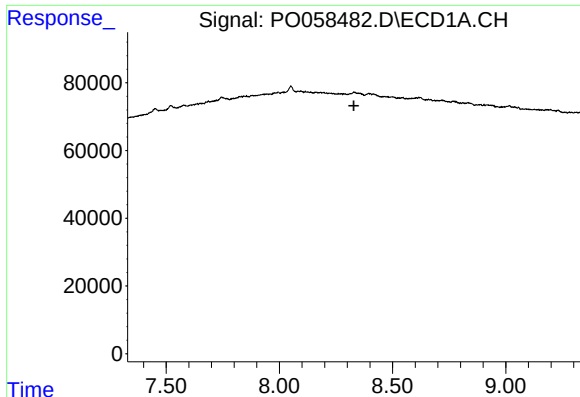

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.330 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

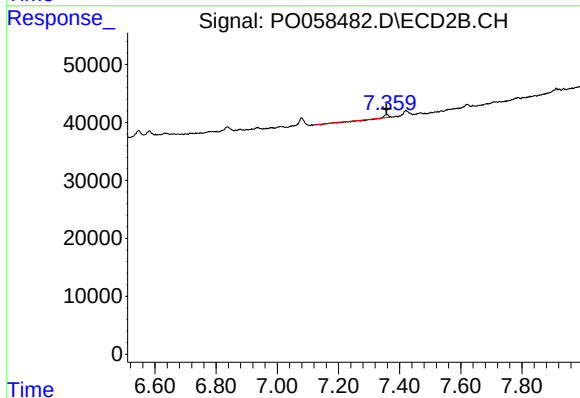


#41 AR-1268-1

R.T.: 7.359 min
Delta R.T.: 0.002 min
Response: 1329
Conc: 0.16 ng/ml

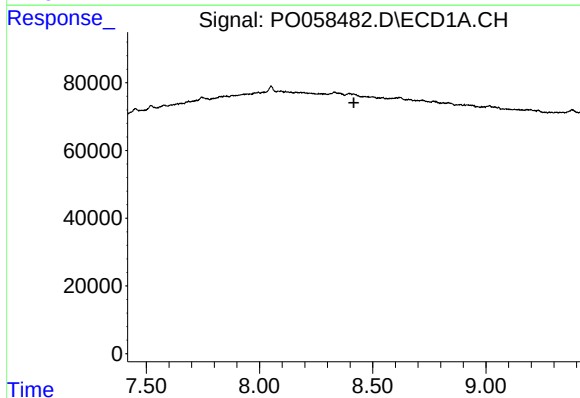


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.417 min
Response: 0
Conc: N.D.

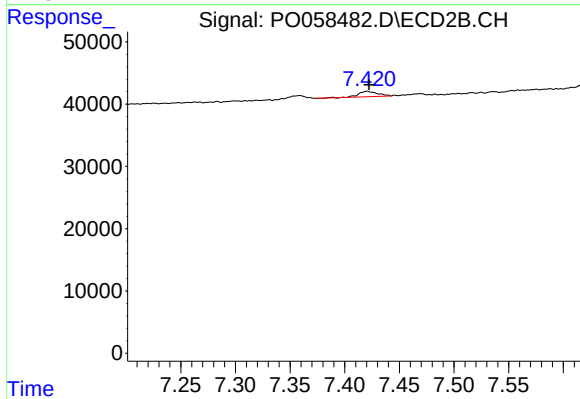

#42 AR-1268-2


R.T.: 7.420 min
Delta R.T.: -0.002 min
Response: 10760
Conc: 1.42 ng/ml

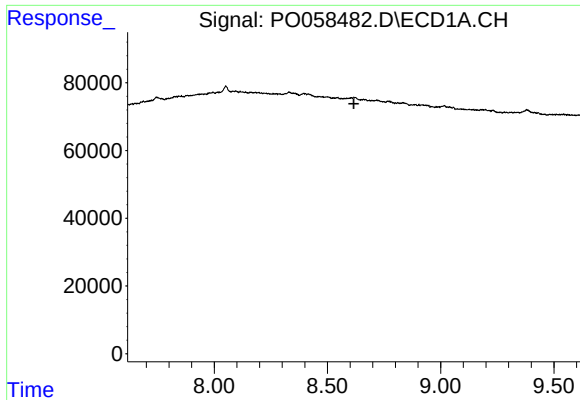

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.617 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

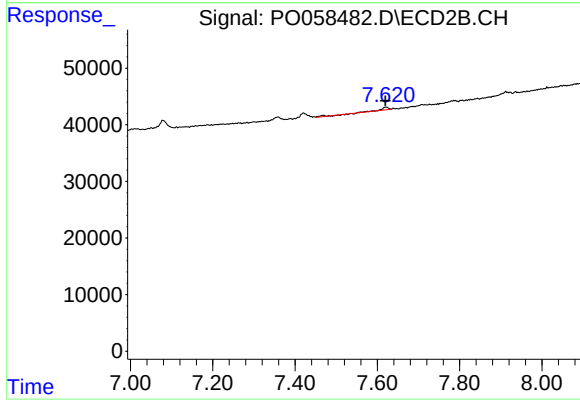

#43 AR-1268-3

R.T.: 7.621 min
Delta R.T.: 0.002 min
Response: 6333
Conc: 0.99 ng/ml